

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB093020\
 Data File : FB024983.D
 Signal(s) : FID2B.CH
 Acq On : 30 Sep 2020 15:36
 Operator : DD/AJ
 Sample : L4190-03MSD
 Misc : 5.05/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 01 01:01:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.801	396322	18.878 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.691	655361	21.792 ng/ml
2) t	2,2,4-Trimethylpentane	7.419	537344	17.581 ng/ml
3) t	n-Heptane	7.760	159912	5.257 ng/ml
4) t	Benzene	7.894	335202	8.998 ng/ml
6) t	Toluene	10.632	870792	24.944 ng/ml
7) t	Ethylbenzene	13.072	255603	7.885 ng/ml
8) t	m-Xylene	13.205	518480	16.322 ng/ml
9) t	O-Xylene	13.933	512896	16.878 ng/ml
10) t	1,2,4-Trimethylbenzene	16.211	393529	15.516 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

```
Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB093020\  
Data File : FB024983.D  
Signal(s) : FID2B.CH  
Acq On    : 30 Sep 2020 15:36  
Operator  : DD/AJ  
Sample    : L4190-03MSD  
Misc      : 5.05/5.00ml DI WATER  
ALS Vial  : 10 Sample Multiplier: 1
```

Integration File: Calibration.e
Quant Time: Oct 01 01:01:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

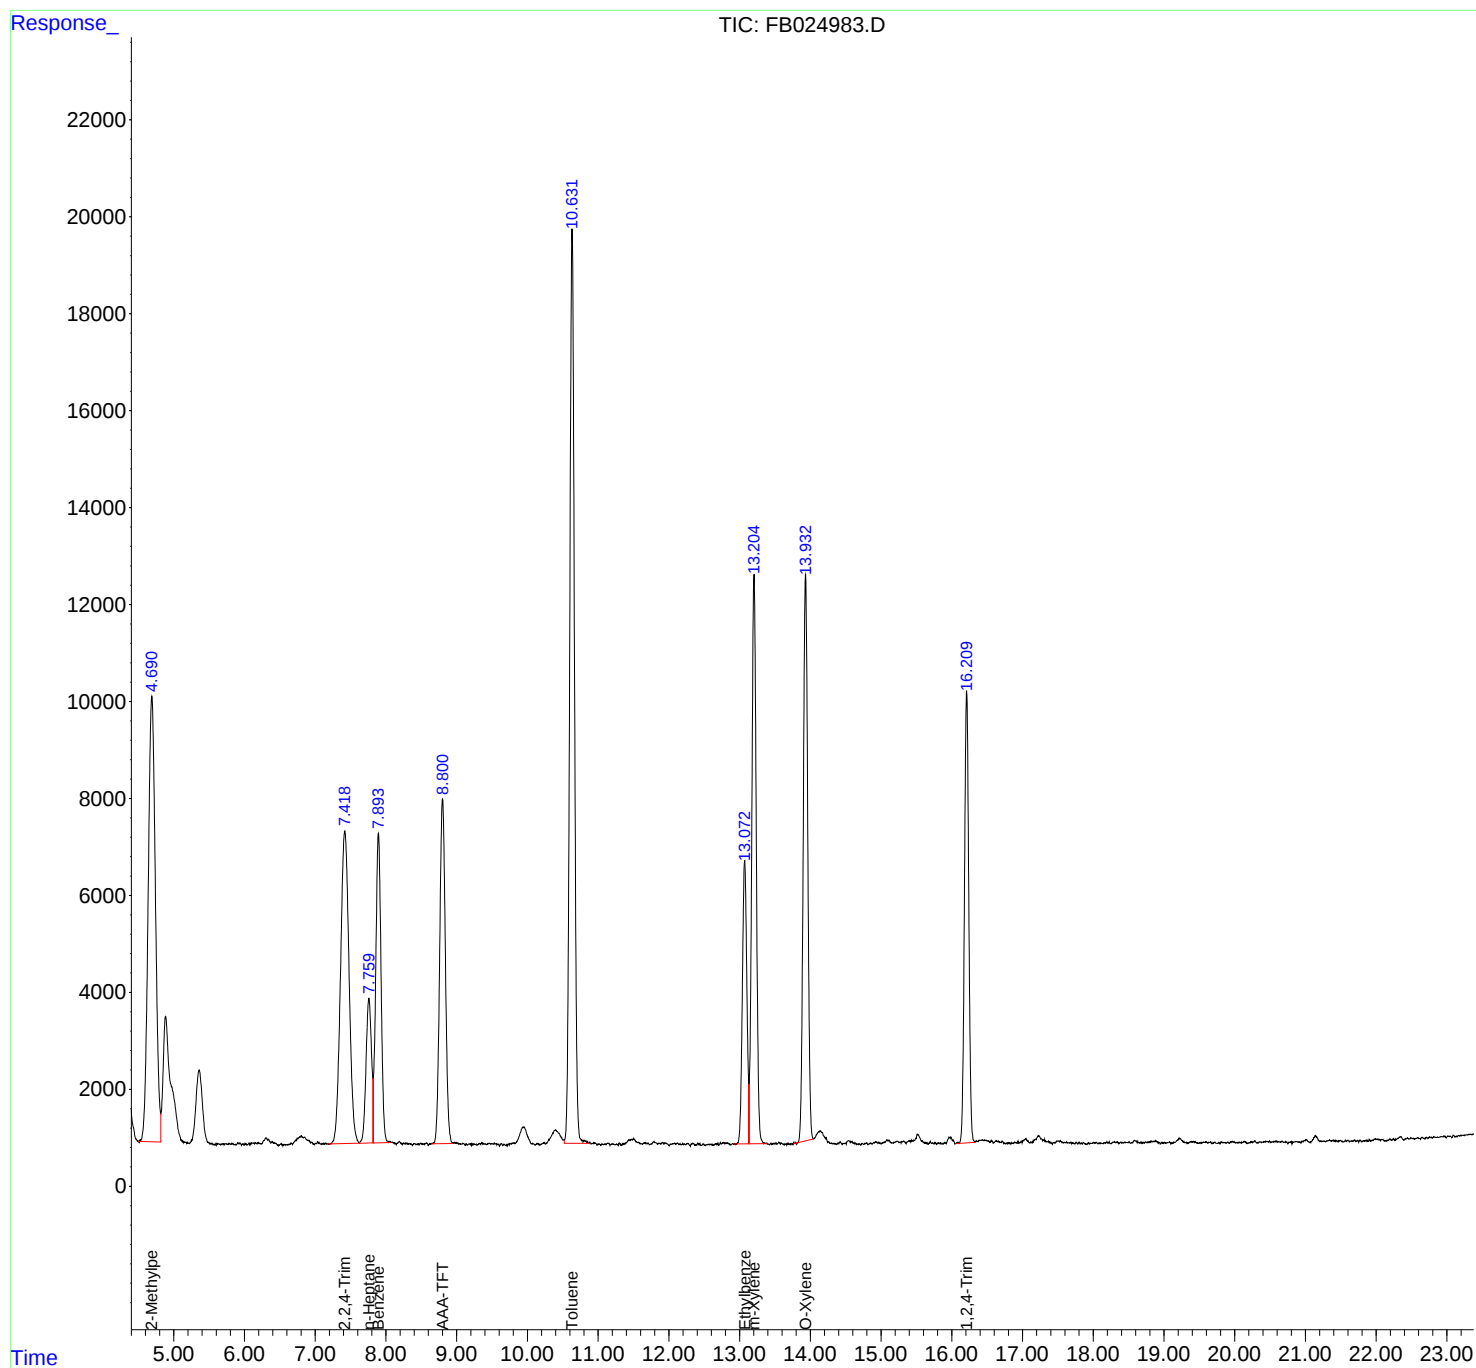

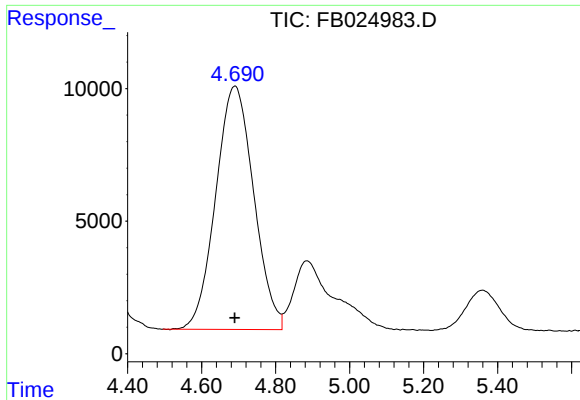


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.001 min
Response: 655361
Conc: 21.79 ng/ml

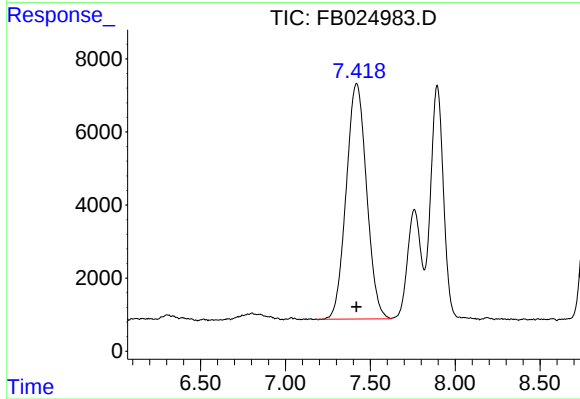


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.001 min
Response: 537344
Conc: 17.58 ng/ml

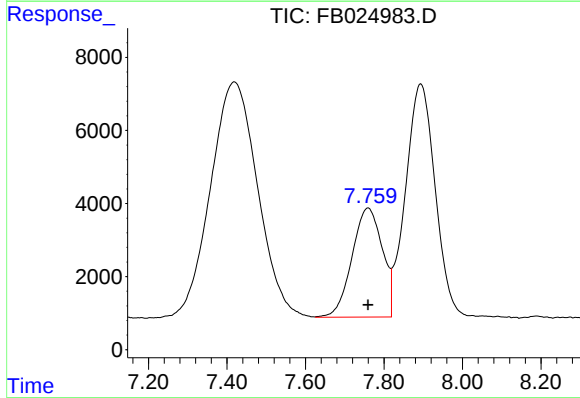


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 159912
Conc: 5.26 ng/ml

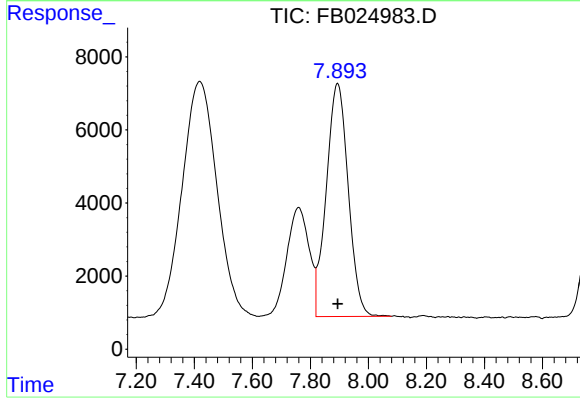


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 335202
Conc: 9.00 ng/ml

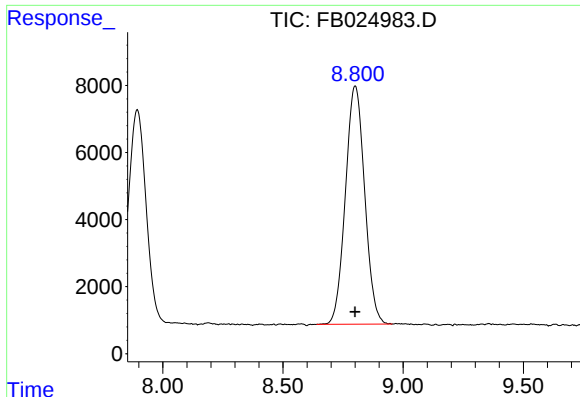


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 396322
Conc: 18.88 ng/ml

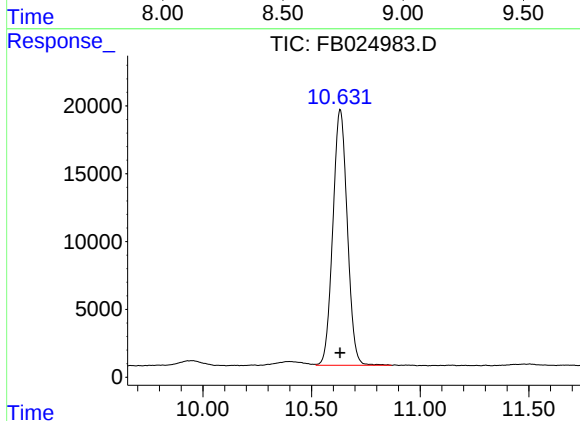


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 870792
Conc: 24.94 ng/ml

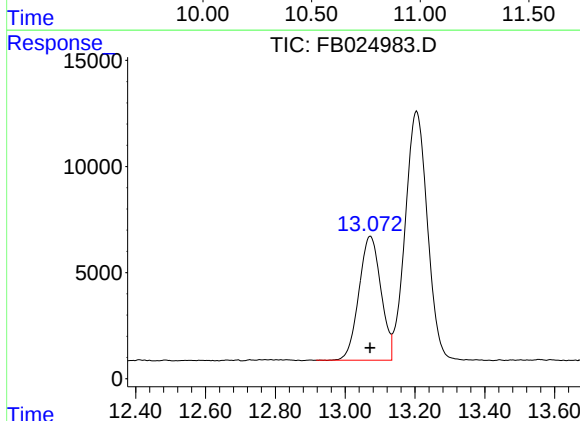


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 255603
Conc: 7.89 ng/ml

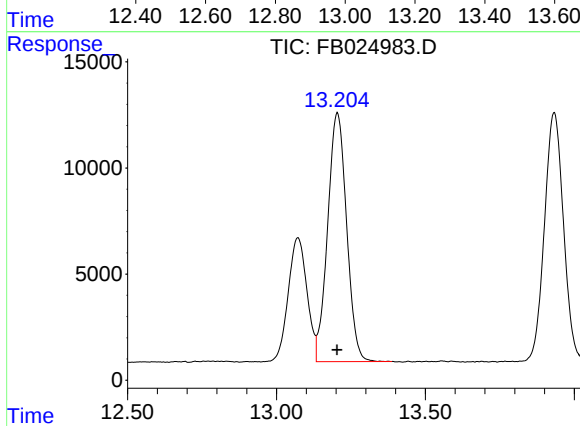


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 518480
Conc: 16.32 ng/ml

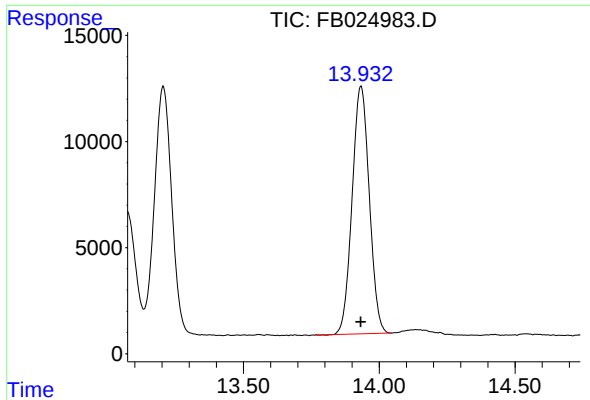

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.001 min
Response: 512896
Conc: 16.88 ng/ml

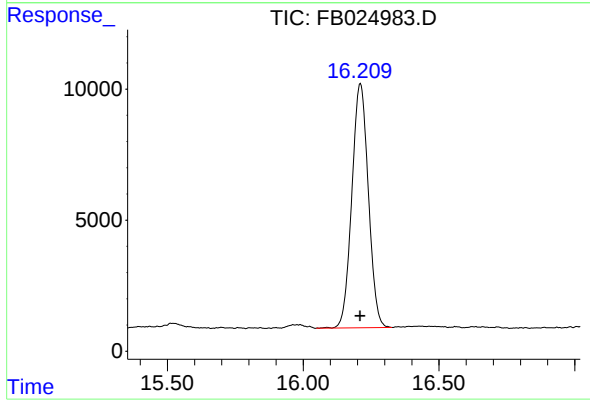

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.001 min
Response: 393529
Conc: 15.52 ng/ml