

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB093020\
 Data File : FB024982.D
 Signal(s) : FID2B.CH
 Acq On : 30 Sep 2020 15:06
 Operator : DD/AJ
 Sample : L4190-03MS
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 01 01:01:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.801	383625	18.273 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.690	690936	22.975 ng/ml
2) t	2,2,4-Trimethylpentane	7.419	621683	20.341 ng/ml
3) t	n-Heptane	7.760	192678	6.334 ng/ml
4) t	Benzene	7.895	336046	9.021 ng/ml
6) t	Toluene	10.632	904024	25.896 ng/ml
7) t	Ethylbenzene	13.072	272265	8.399 ng/ml
8) t	m-Xylene	13.205	546434	17.202 ng/ml
9) t	O-Xylene	13.933	537504	17.688 ng/ml
10) t	1,2,4-Trimethylbenzene	16.210	428992	16.914 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB093020\
Data File : FB024982.D
Signal(s) : FID2B.CH
Acq On : 30 Sep 2020 15:06
Operator : DD/AJ
Sample : L4190-03MS
Misc : 5.02/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 01 01:01:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

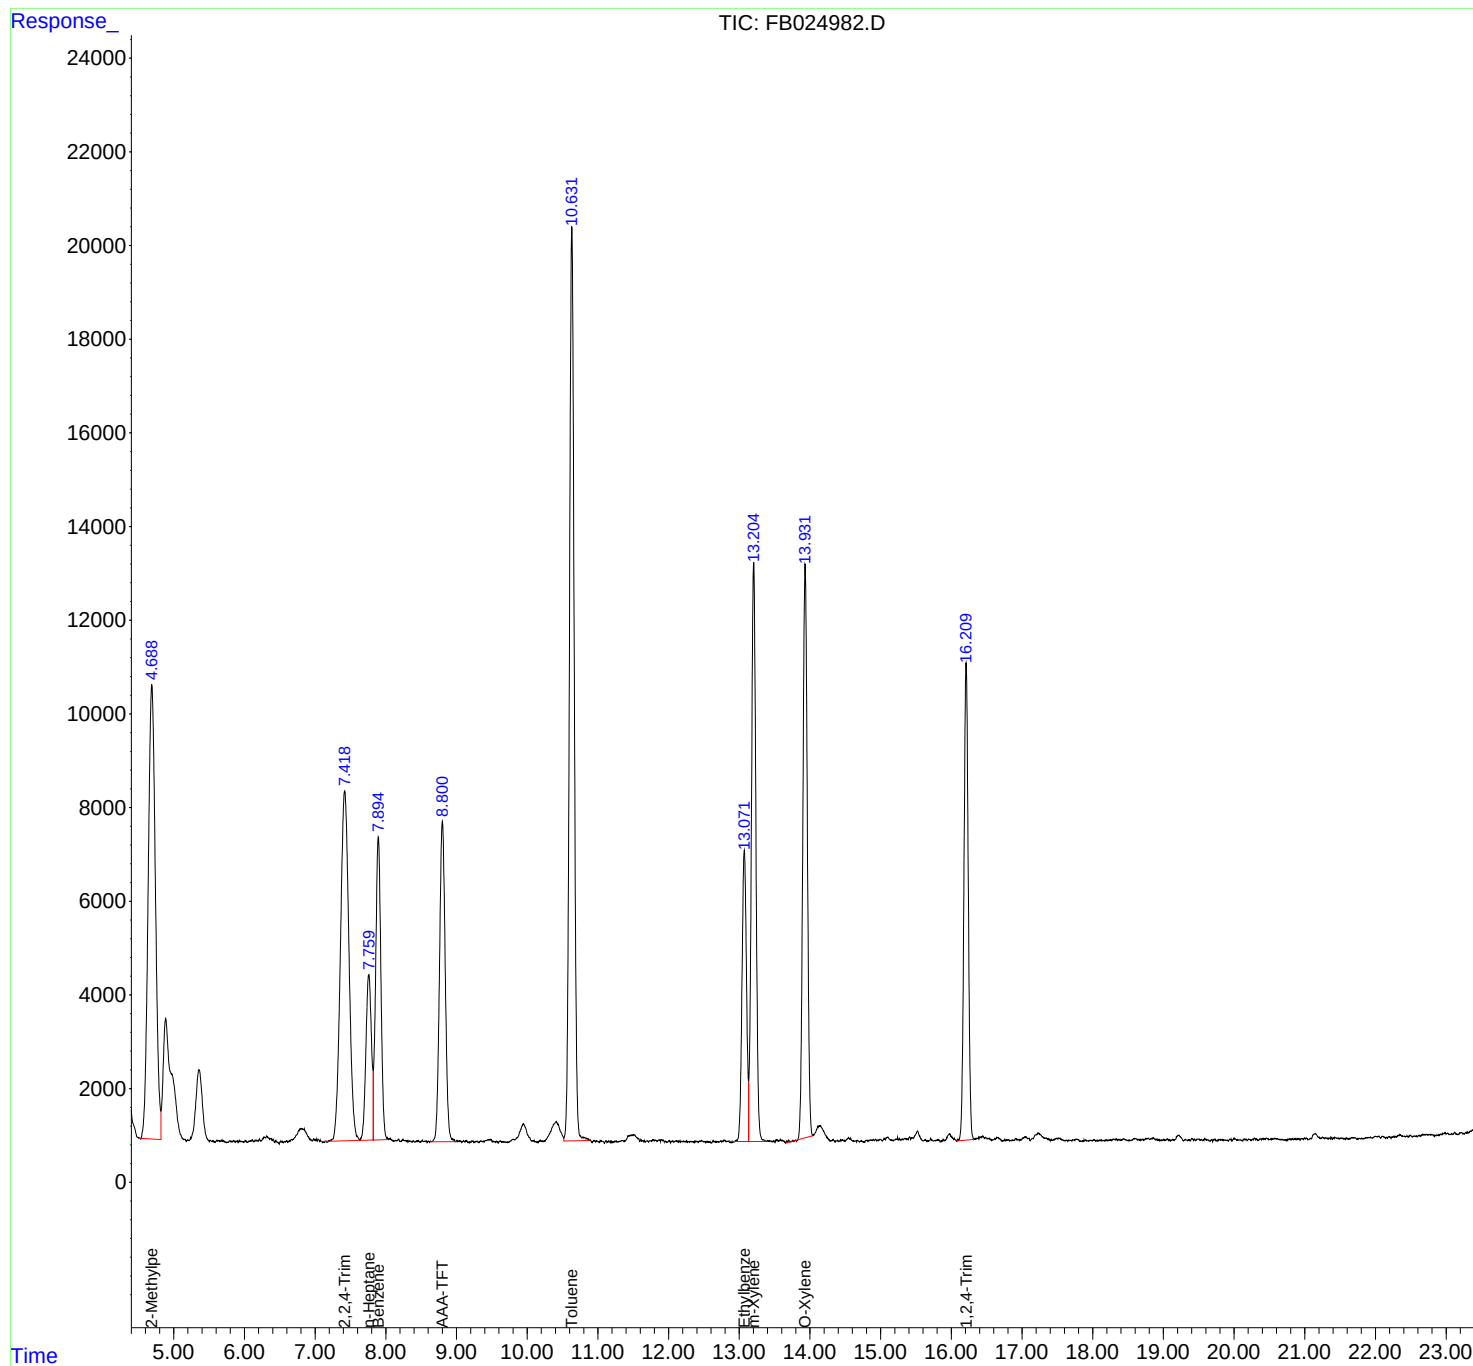

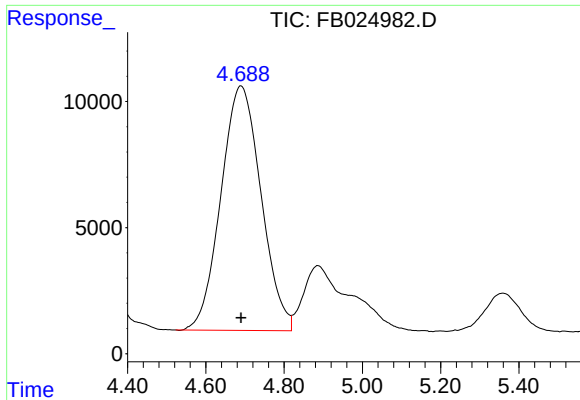


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 690936
Conc: 22.97 ng/ml

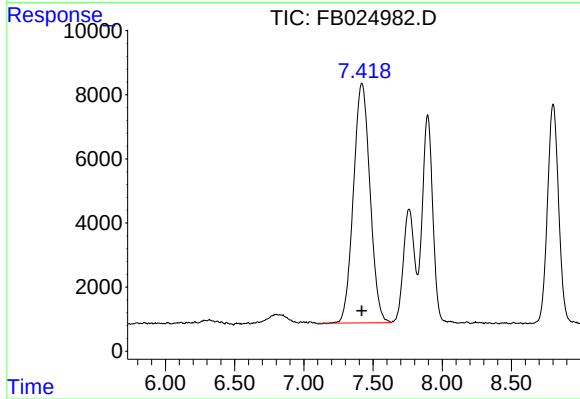


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.001 min
Response: 621683
Conc: 20.34 ng/ml

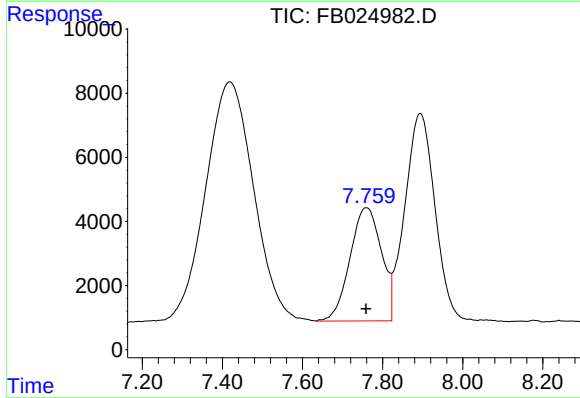


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.001 min
Response: 192678
Conc: 6.33 ng/ml

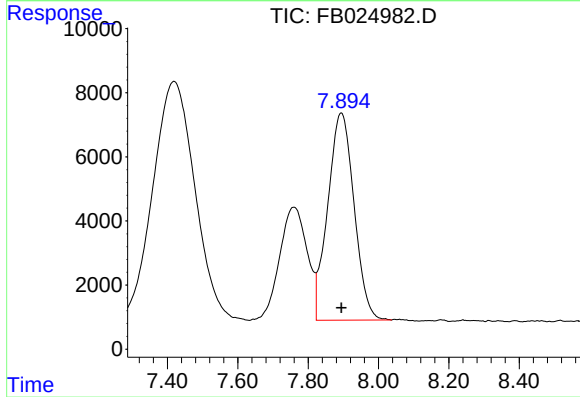


#4 Benzene

R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 336046
Conc: 9.02 ng/ml

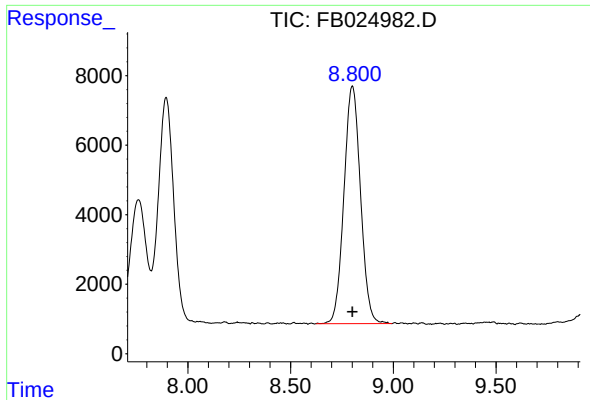


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 383625
Conc: 18.27 ng/ml

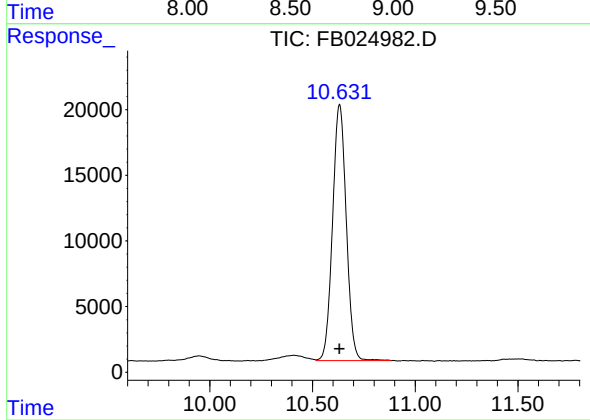


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 904024
Conc: 25.90 ng/ml

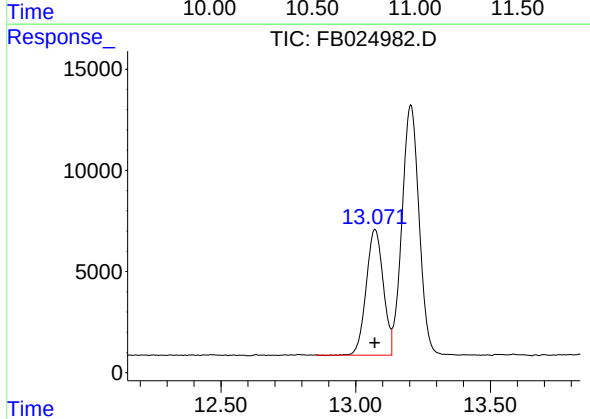


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 272265
Conc: 8.40 ng/ml

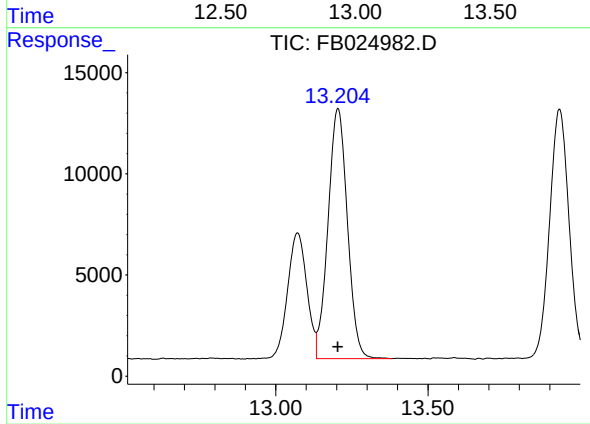


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 546434
Conc: 17.20 ng/ml

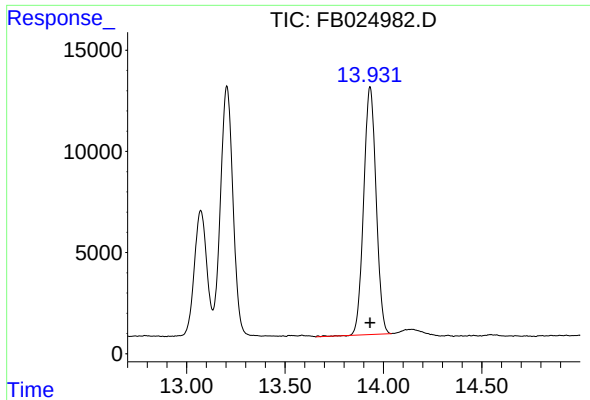

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 537504
Conc: 17.69 ng/ml

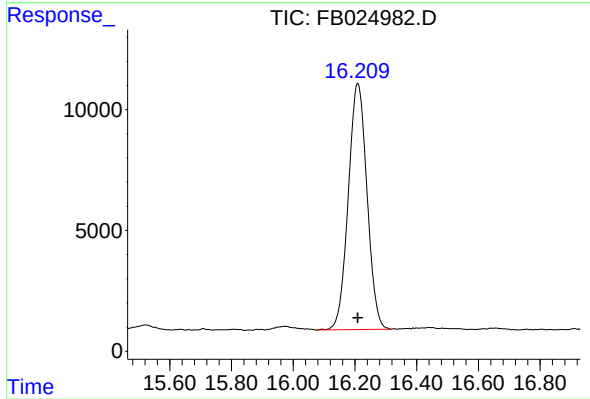

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 428992
Conc: 16.91 ng/ml