

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB093022\
 Data File : FB028498.D
 Signal(s) : FID2B.CH
 Acq On : 30 Sep 2022 12:28
 Operator : AJ/MA
 Sample : N4785-18
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 03 04:18:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.803	445389	37.212 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.392	235402	11.190 ng/ml
3) t n-Heptane	7.748	325979	15.164 ng/ml
4) t Benzene	7.878	74881	3.044 ng/ml
6) t Toluene	10.617	914824	39.294 ng/ml
7) t Ethylbenzene	13.053	290905	13.081 ng/ml
8) t m-Xylene	13.184	866756	39.718 ng/ml
9) t O-Xylene	13.913	351075	16.756 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	394531	19.621 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB093022\
Data File : FB028498.D
Signal(s) : FID2B.CH
Acq On : 30 Sep 2022 12:28
Operator : AJ/MA
Sample : N4785-18
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 03 04:18:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

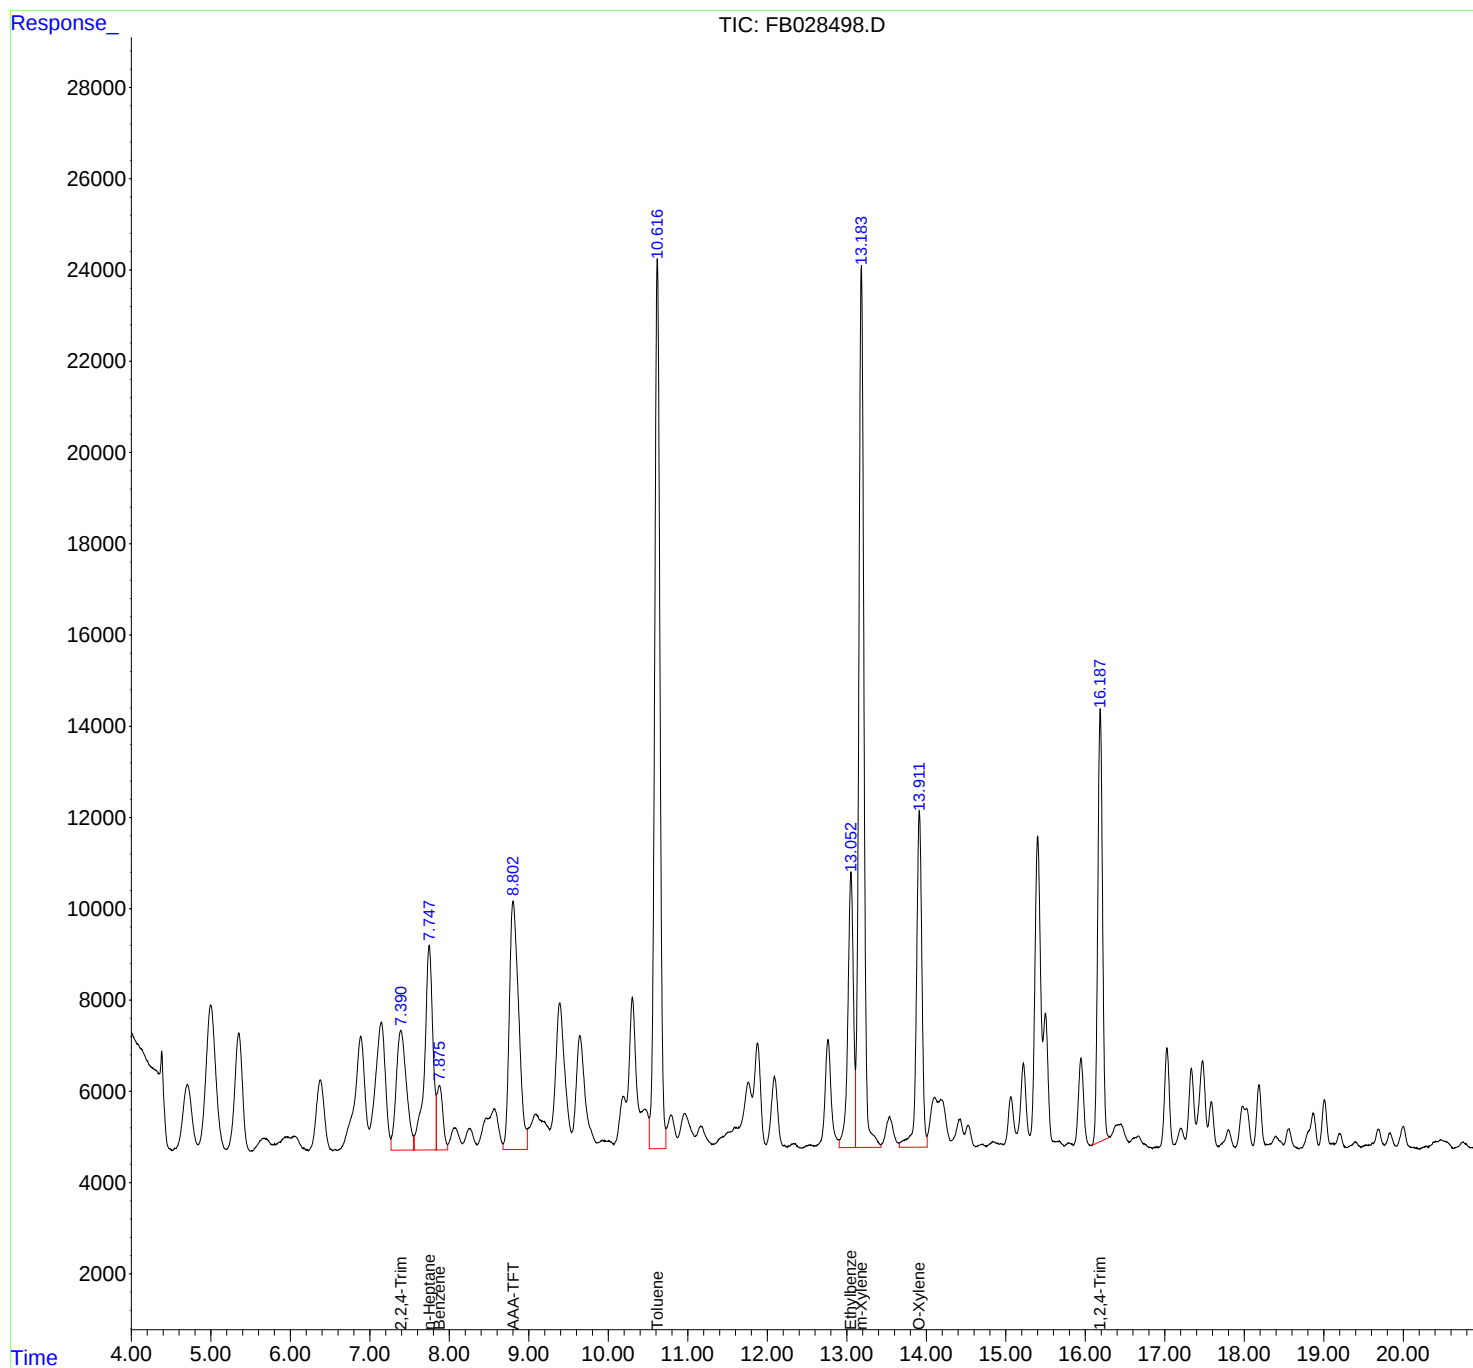


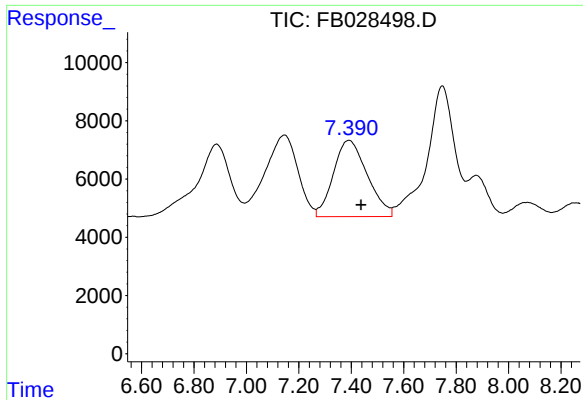

#2 2,2,4-Trimethylpentane


R.T.: 7.392 min
Delta R.T.: -0.045 min
Response: 235402
Conc: 11.19 ng/ml

Instrument :
FID_B
ClientSampleId :

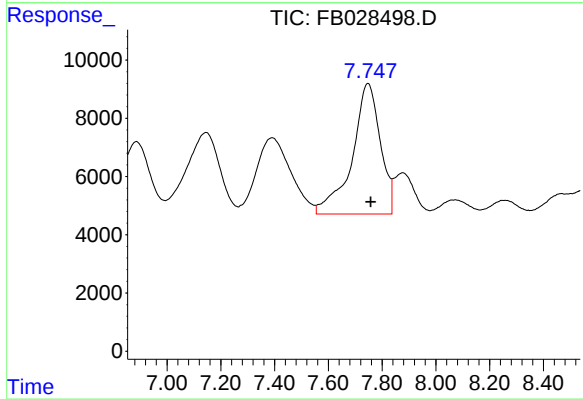


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.010 min
Response: 325979
Conc: 15.16 ng/ml

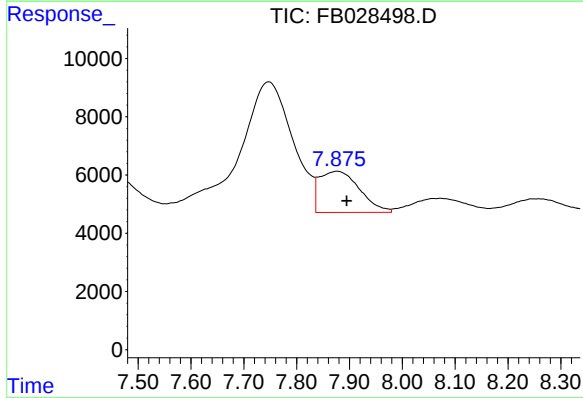


#4 Benzene

R.T.: 7.878 min
Delta R.T.: -0.017 min
Response: 74881
Conc: 3.04 ng/ml

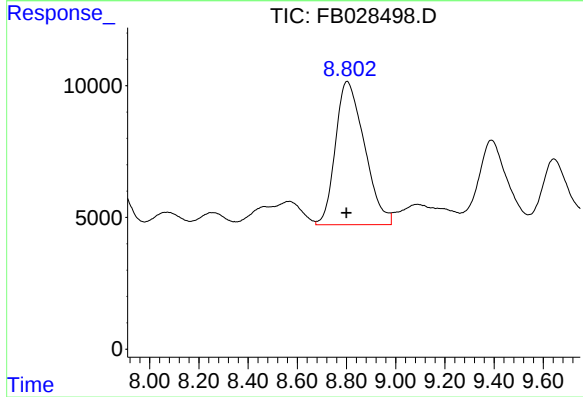

#5 AAA-TFT


R.T.: 8.803 min
Delta R.T.: 0.003 min
Response: 445389
Conc: 37.21 ng/ml

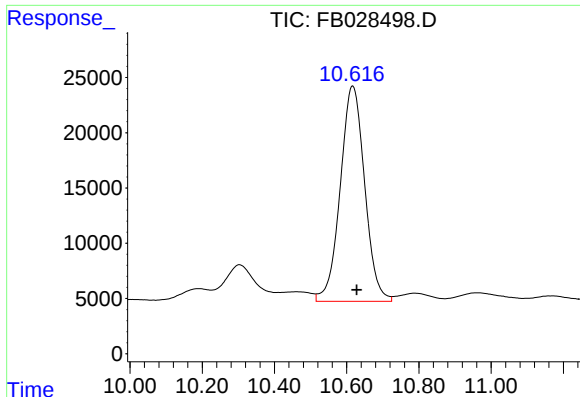

#6 Toluene


R.T.: 10.617 min
Delta R.T.: -0.011 min
Response: 914824
Conc: 39.29 ng/ml

Instrument :
FID_B
ClientSampleId :

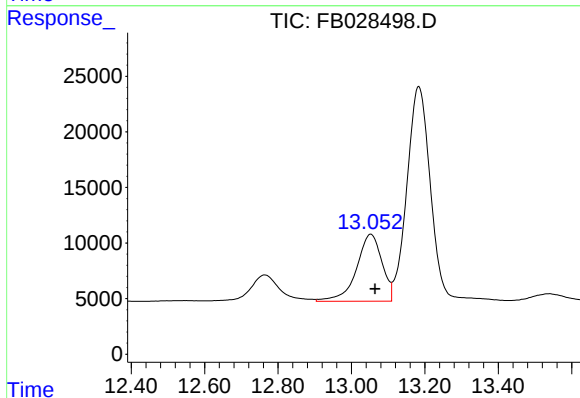


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.012 min
Response: 290905
Conc: 13.08 ng/ml

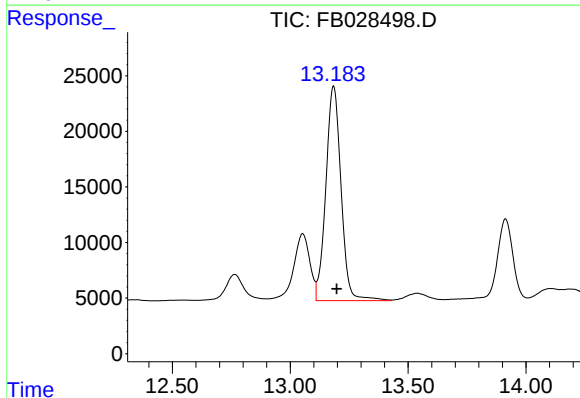


#8 m-Xylene

R.T.: 13.184 min
Delta R.T.: -0.013 min
Response: 866756
Conc: 39.72 ng/ml

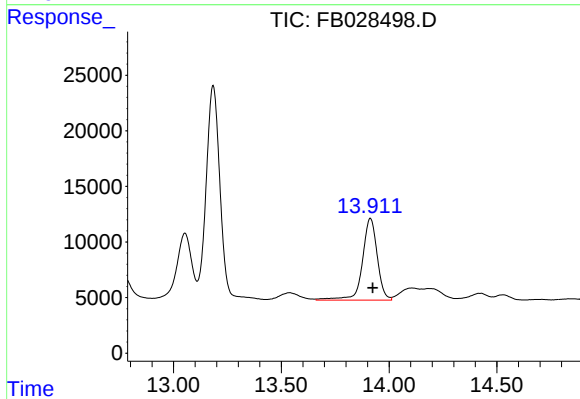

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.011 min
Response: 351075
Conc: 16.76 ng/ml

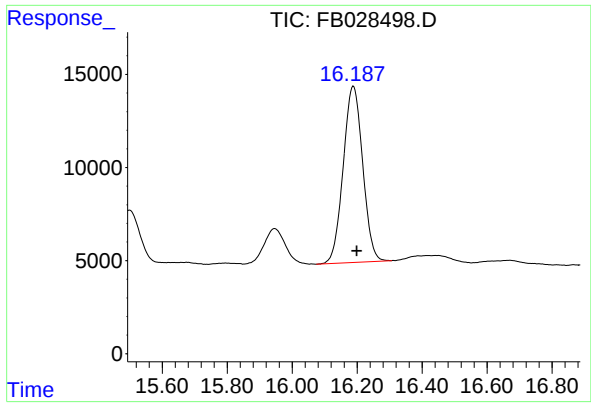

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.011 min
Response: 394531
Conc: 19.62 ng/ml

Instrument :
FID_B
ClientSampleId :