

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100118\
 Data File : FB018019.D
 Signal(s) : FID2B.CH
 Acq On : 1 Oct 2018 10:26
 Operator : MJ/SJ
 Sample : BSF1001S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 01 14:31:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
 Quant Title :
 QLast Update : Fri Sep 14 13:09:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.107	158661	18.757 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.958	392366	24.638 ng/ml
2) t	2,2,4-Trimethylpentane	7.722	409058	25.705 ng/ml
3) t	n-Heptane	8.062	130739	8.484 ng/ml
4) t	Benzene	8.201	165554	8.697 ng/ml
6) t	Toluene	10.955	428736	27.090 ng/ml
7) t	Ethylbenzene	13.405	148981	9.118 ng/ml
8) t	m-Xylene	13.538	319337	18.459 ng/ml
9) t	O-Xylene	14.269	332786	18.313 ng/ml
10) t	1,2,4-Trimethylbenzene	16.552	378008	17.770 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100118\
Data File : FB018019.D
Signal(s) : FID2B.CH
Acq On : 1 Oct 2018 10:26
Operator : MJ/SJ
Sample : BSF1001S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 01 14:31:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

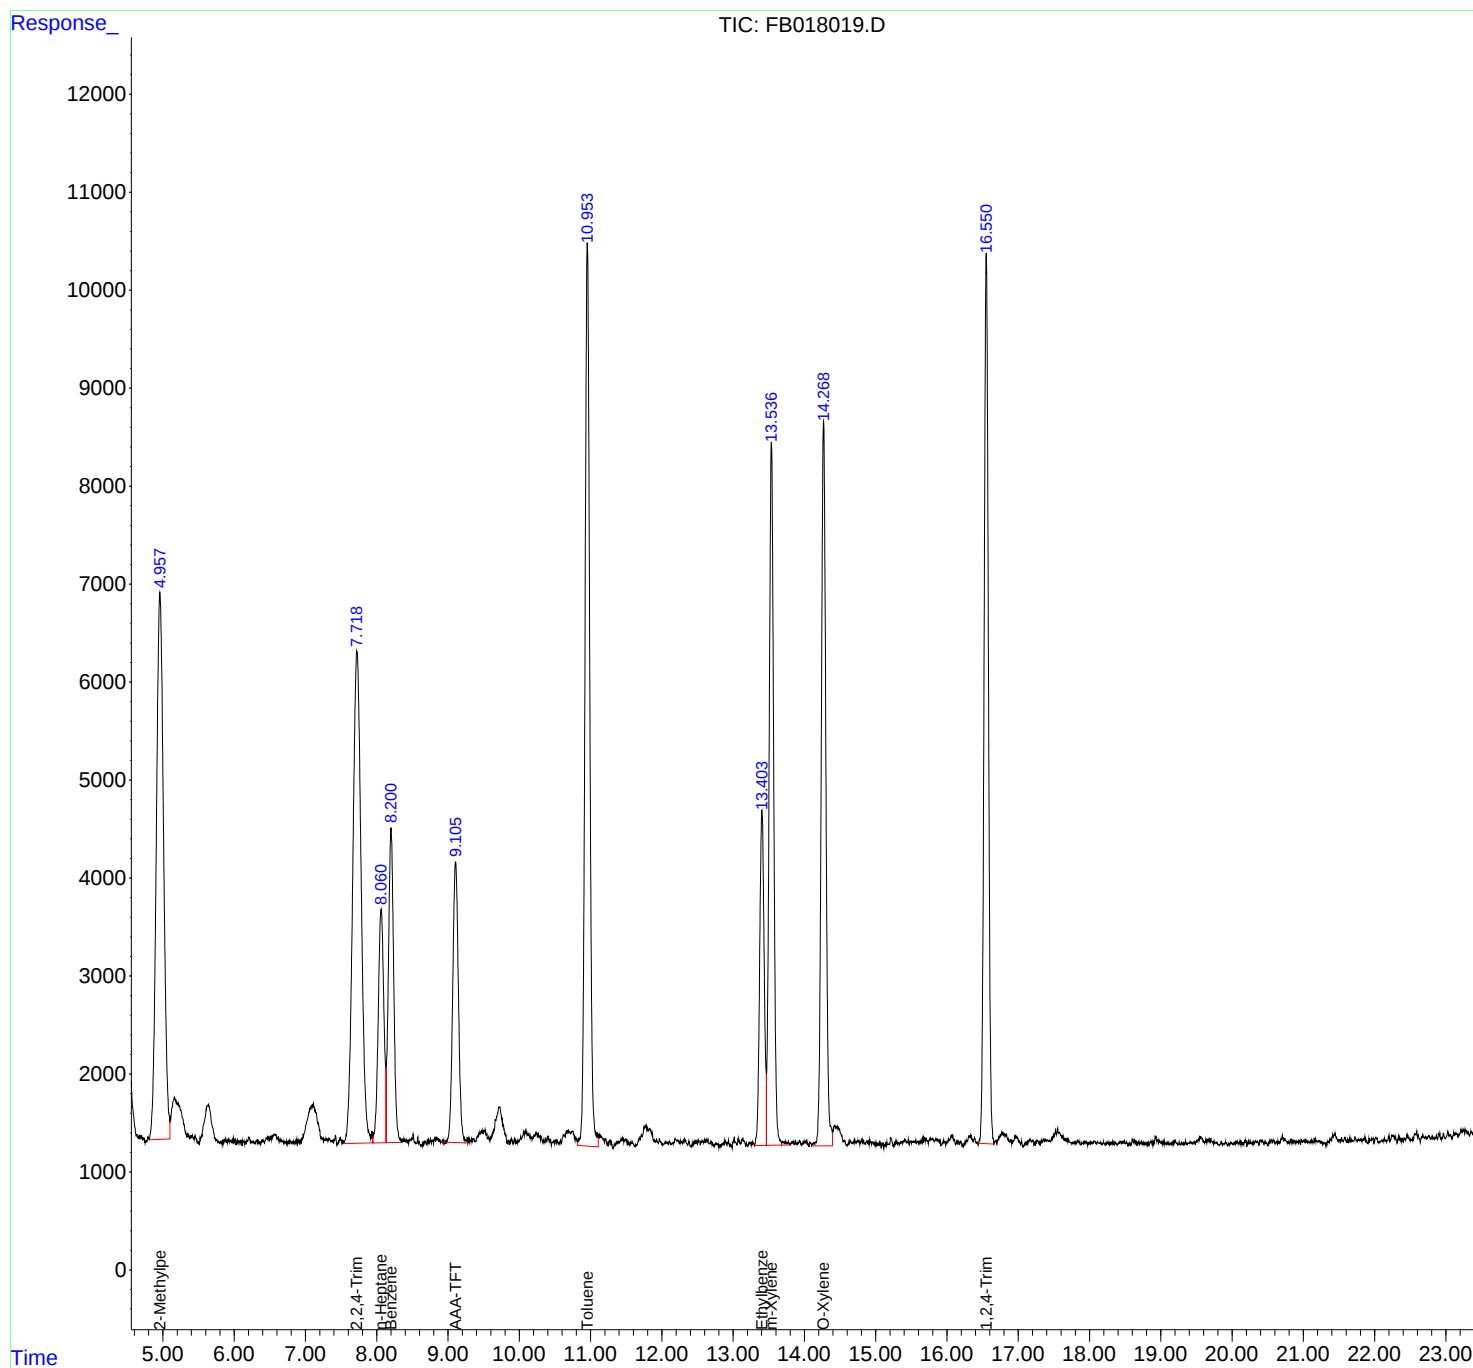

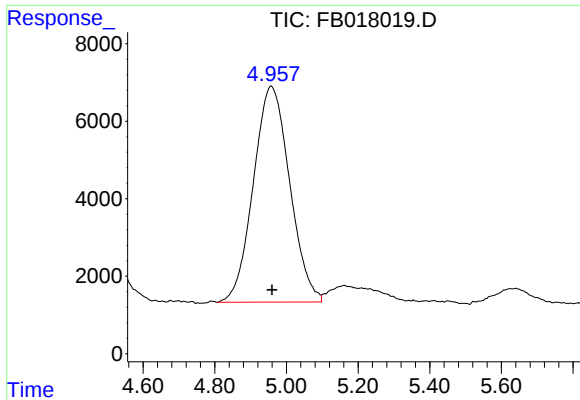


#1 2-Methylpentane

R.T.: 4.958 min
Delta R.T.: -0.002 min
Response: 392366
Conc: 24.64 ng/ml

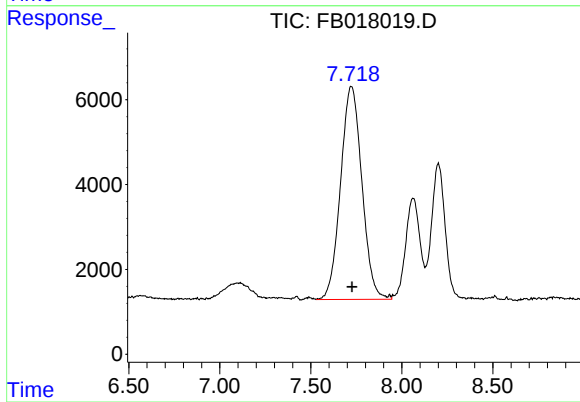


#2 2,2,4-Trimethylpentane

R.T.: 7.722 min
Delta R.T.: -0.005 min
Response: 409058
Conc: 25.70 ng/ml

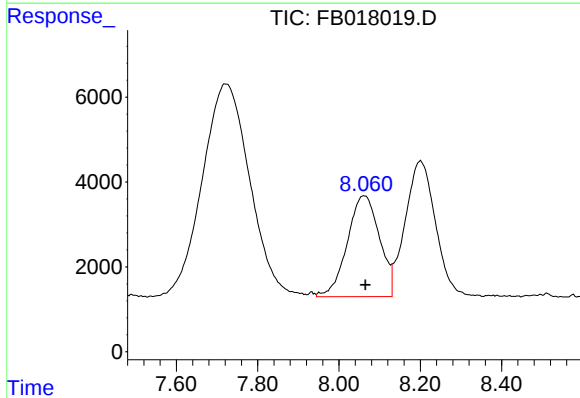


#3 n-Heptane

R.T.: 8.062 min
Delta R.T.: -0.003 min
Response: 130739
Conc: 8.48 ng/ml

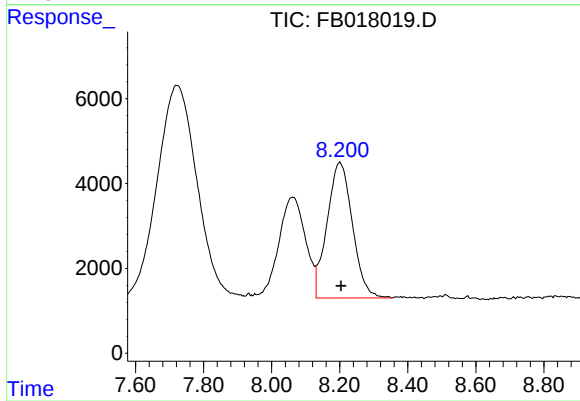


#4 Benzene

R.T.: 8.201 min
Delta R.T.: -0.004 min
Response: 165554
Conc: 8.70 ng/ml

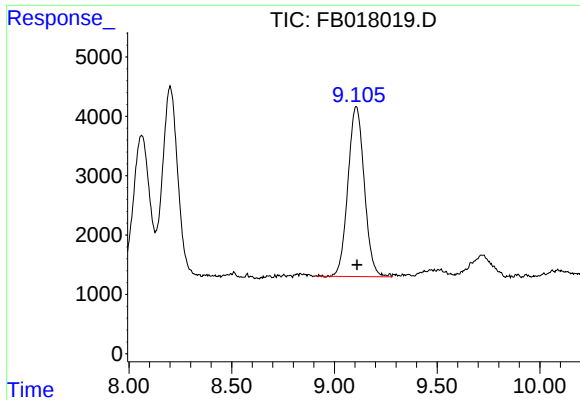


#5 AAA-TFT

R.T.: 9.107 min
Delta R.T.: -0.004 min
Response: 158661
Conc: 18.76 ng/ml

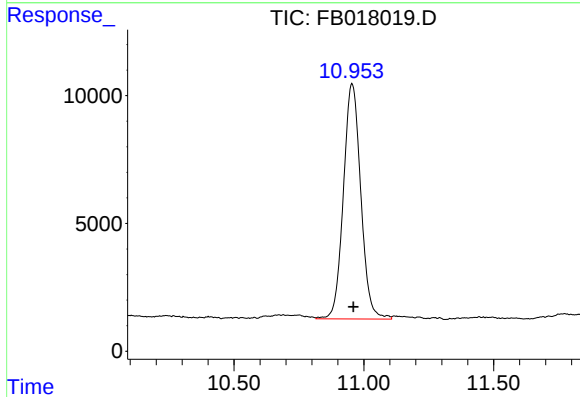


#6 Toluene

R.T.: 10.955 min
Delta R.T.: -0.004 min
Response: 428736
Conc: 27.09 ng/ml

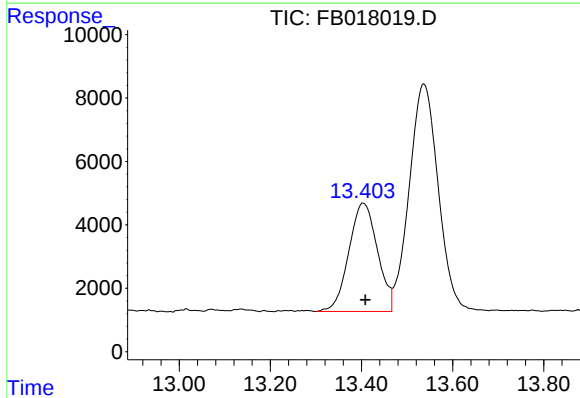


#7 Ethylbenzene

R.T.: 13.405 min
Delta R.T.: -0.004 min
Response: 148981
Conc: 9.12 ng/ml

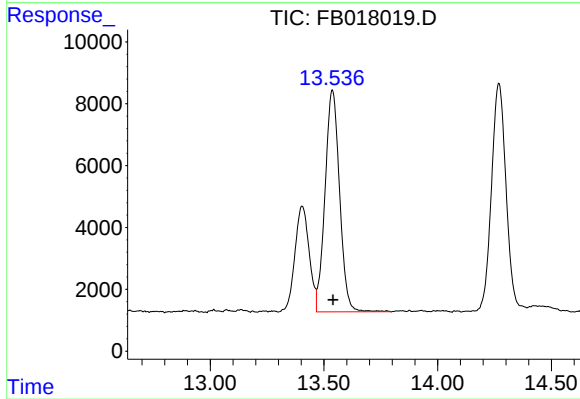


#8 m-Xylene

R.T.: 13.538 min
Delta R.T.: -0.004 min
Response: 319337
Conc: 18.46 ng/ml

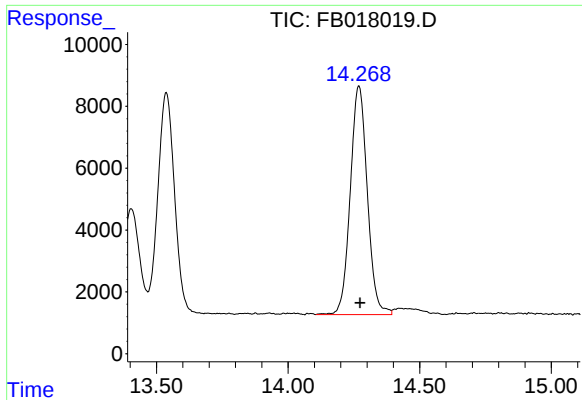

#9 O-Xylene

R.T.: 14.269 min
Delta R.T.: -0.004 min
Response: 332786
Conc: 18.31 ng/ml

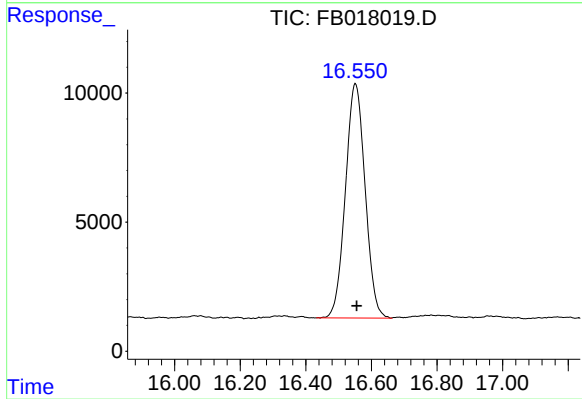

#10 1,2,4-Trimethylbenzene

R.T.: 16.552 min
Delta R.T.: -0.004 min
Response: 378008
Conc: 17.77 ng/ml