

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100118\
Data File : FB018025.D
Signal(s) : FID2B.CH
Acq On : 1 Oct 2018 13:31
Operator : MJ/SJ
Sample : J5171-02MSD
Misc : 5.02g/5.00mL DI Water
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 01 14:31:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.107	180910	21.387 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.959	452045	28.385 ng/ml
2) t	2,2,4-Trimethylpentane	7.723	408404	25.664 ng/ml
3) t	n-Heptane	8.062	129091	8.377 ng/ml
4) t	Benzene	8.201	194220	10.202 ng/ml
6) t	Toluene	10.955	477912	30.198 ng/ml
7) t	Ethylbenzene	13.406	164817	10.087 ng/ml
8) t	m-Xylene	13.538	348652	20.153 ng/ml
9) t	O-Xylene	14.270	373076	20.530 ng/ml
10) t	1,2,4-Trimethylbenzene	16.552	415183	19.518 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100118\
Data File : FB018025.D
Signal(s) : FID2B.CH
Acq On : 1 Oct 2018 13:31
Operator : MJ/SJ
Sample : J5171-02MSD
Misc : 5.02g/5.00mL DI Water
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 01 14:31:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

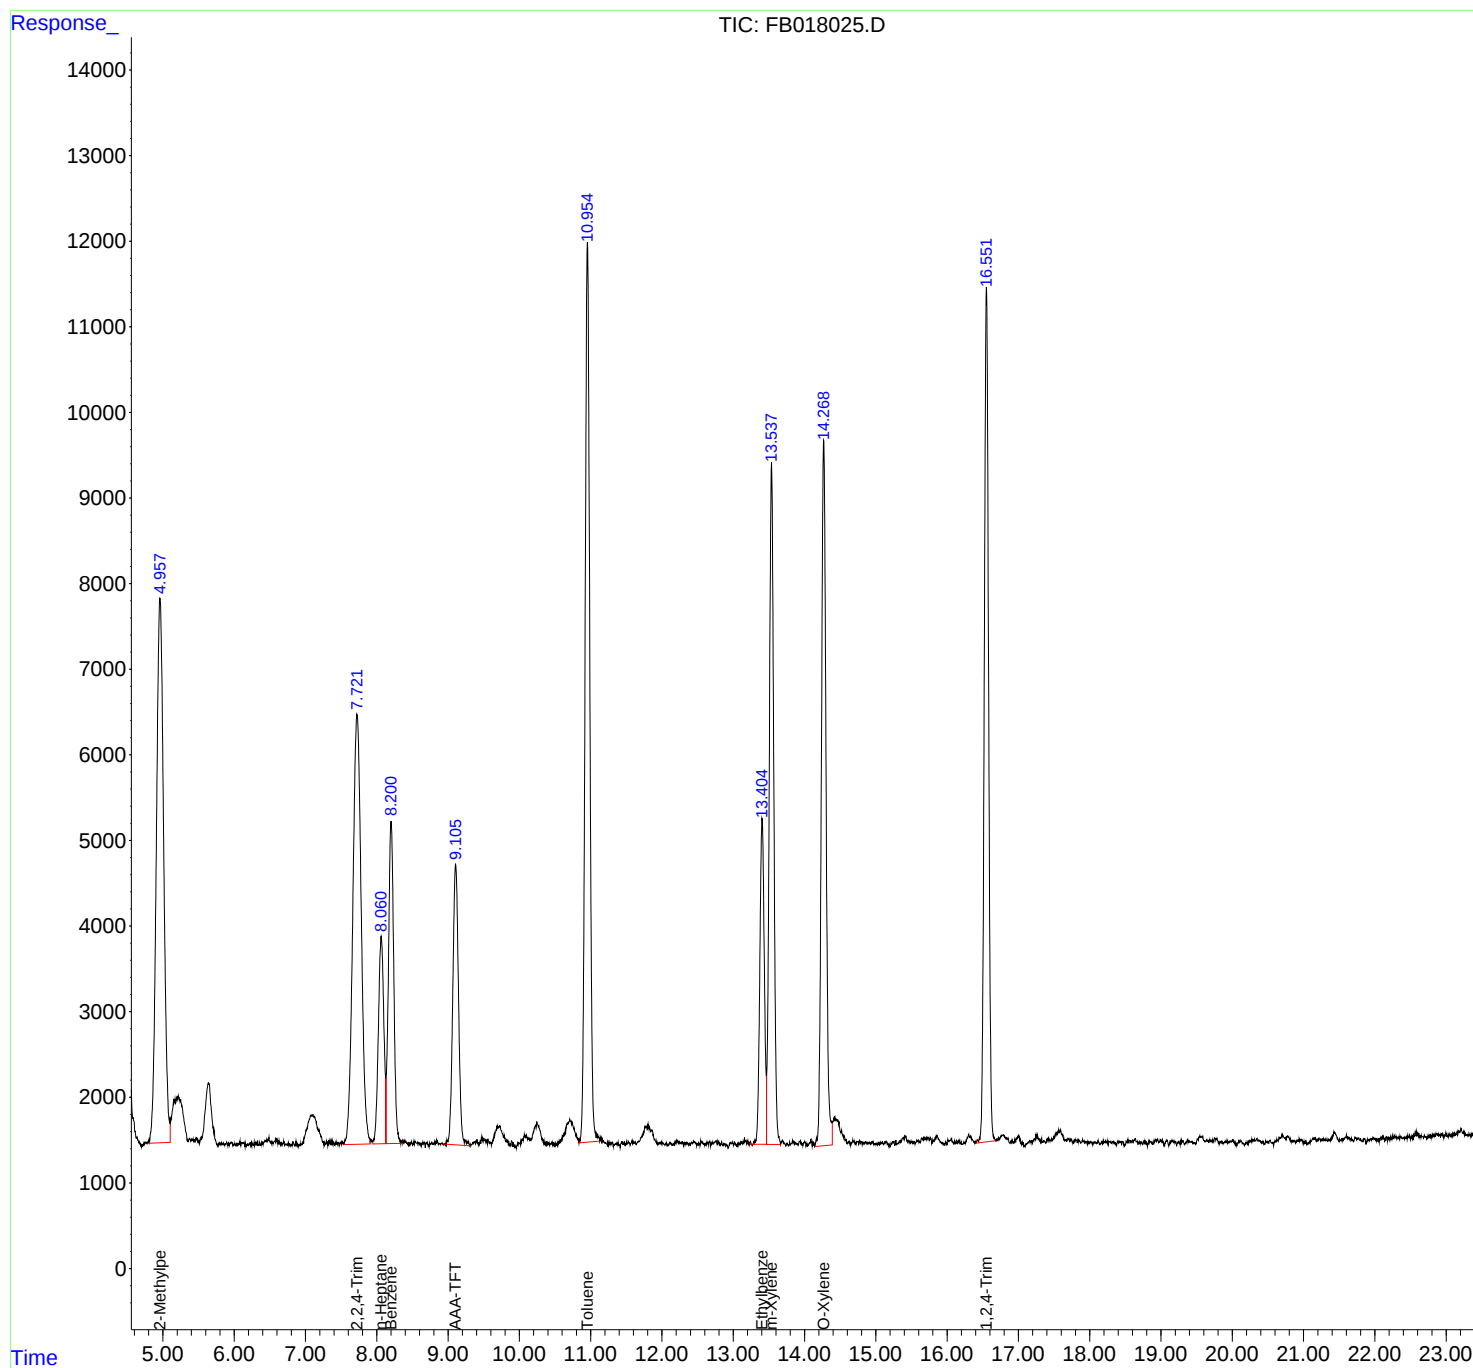

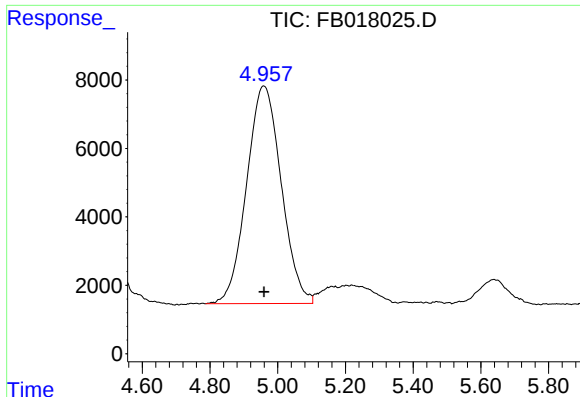


#1 2-Methylpentane

R.T.: 4.959 min
Delta R.T.: 0.000 min
Response: 452045
Conc: 28.39 ng/ml

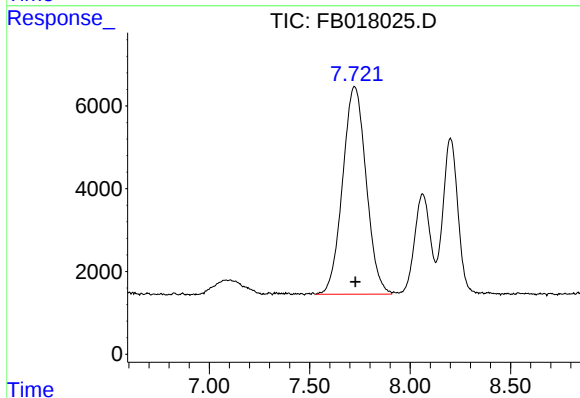


#2 2,2,4-Trimethylpentane

R.T.: 7.723 min
Delta R.T.: -0.004 min
Response: 408404
Conc: 25.66 ng/ml

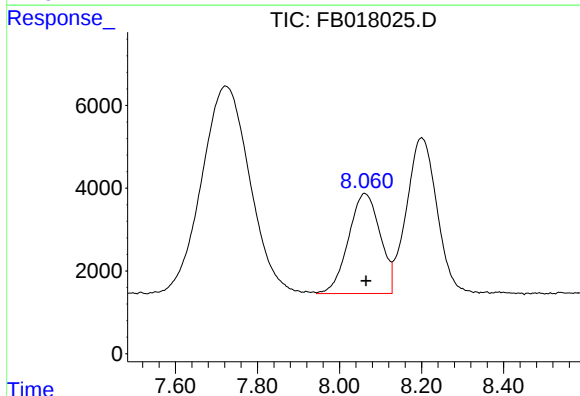


#3 n-Heptane

R.T.: 8.062 min
Delta R.T.: -0.003 min
Response: 129091
Conc: 8.38 ng/ml

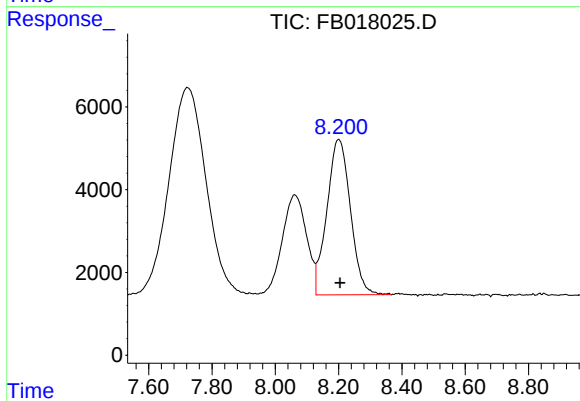


#4 Benzene

R.T.: 8.201 min
Delta R.T.: -0.004 min
Response: 194220
Conc: 10.20 ng/ml

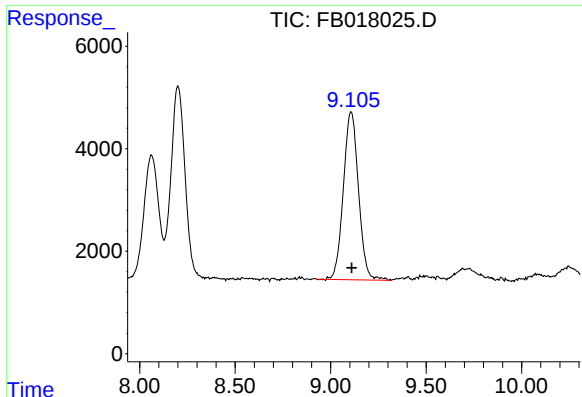


#5 AAA-TFT

R.T.: 9.107 min
Delta R.T.: -0.003 min
Response: 180910
Conc: 21.39 ng/ml

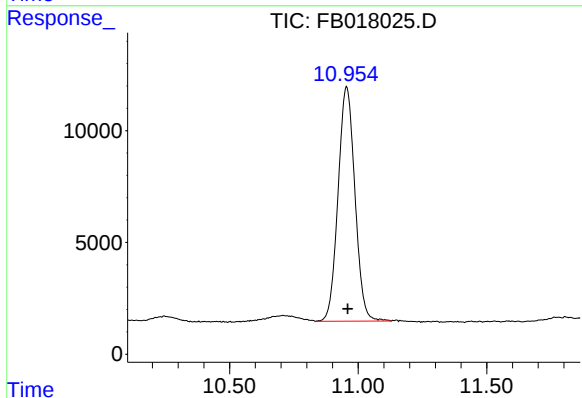


#6 Toluene

R.T.: 10.955 min
Delta R.T.: -0.004 min
Response: 477912
Conc: 30.20 ng/ml

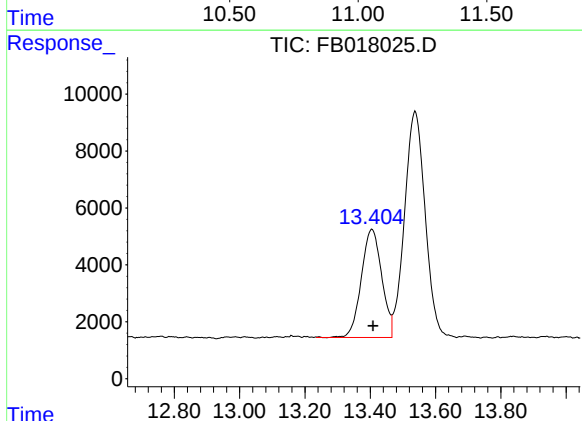


#7 Ethylbenzene

R.T.: 13.406 min
Delta R.T.: -0.003 min
Response: 164817
Conc: 10.09 ng/ml

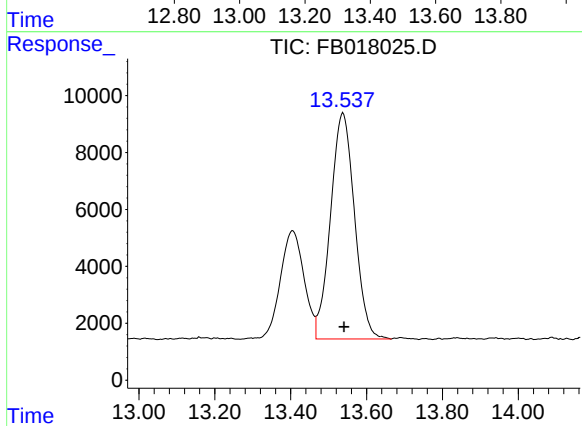


#8 m-Xylene

R.T.: 13.538 min
Delta R.T.: -0.003 min
Response: 348652
Conc: 20.15 ng/ml

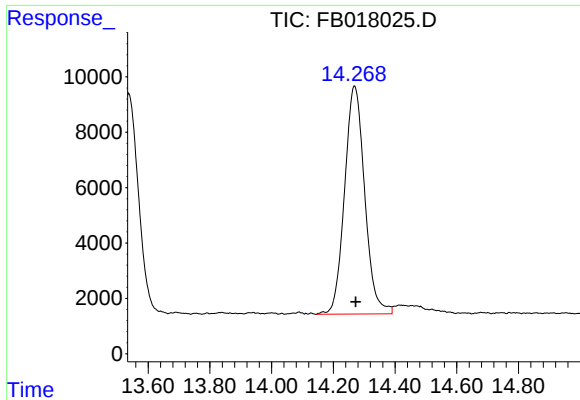

#9 O-Xylene

R.T.: 14.270 min
Delta R.T.: -0.004 min
Response: 373076
Conc: 20.53 ng/ml

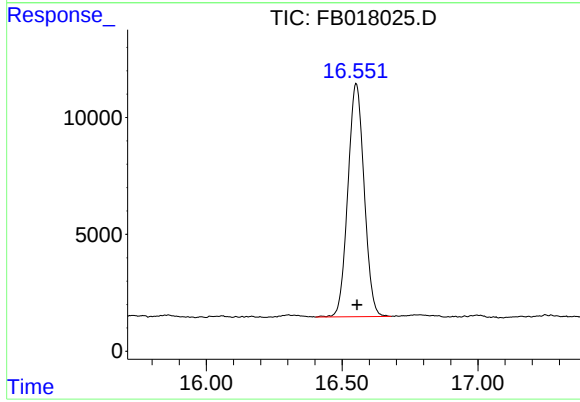

#10 1,2,4-Trimethylbenzene

R.T.: 16.552 min
Delta R.T.: -0.003 min
Response: 415183
Conc: 19.52 ng/ml