

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100120\
 Data File : FB024987.D
 Signal(s) : FID2B.CH
 Acq On : 1 Oct 2020 10:12
 Operator : DD/AJ
 Sample : BSF1001S1
 Misc : 5.00/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 02 02:35:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.801	433591	20.653 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.690	931515	30.975 ng/ml
2) t	2,2,4-Trimethylpentane	7.419	996662	32.609 ng/ml
3) t	n-Heptane	7.759	330371	10.860 ng/ml
4) t	Benzene	7.894	390874	10.493 ng/ml
6) t	Toluene	10.632	1094584	31.355 ng/ml
7) t	Ethylbenzene	13.072	337845	10.422 ng/ml
8) t	m-Xylene	13.205	664136	20.907 ng/ml
9) t	O-Xylene	13.932	648258	21.333 ng/ml
10) t	1,2,4-Trimethylbenzene	16.210	534359	21.069 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100120\
Data File : FB024987.D
Signal(s) : FID2B.CH
Acq On : 1 Oct 2020 10:12
Operator : DD/AJ
Sample : BSF1001S1
Misc : 5.00/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 02 02:35:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

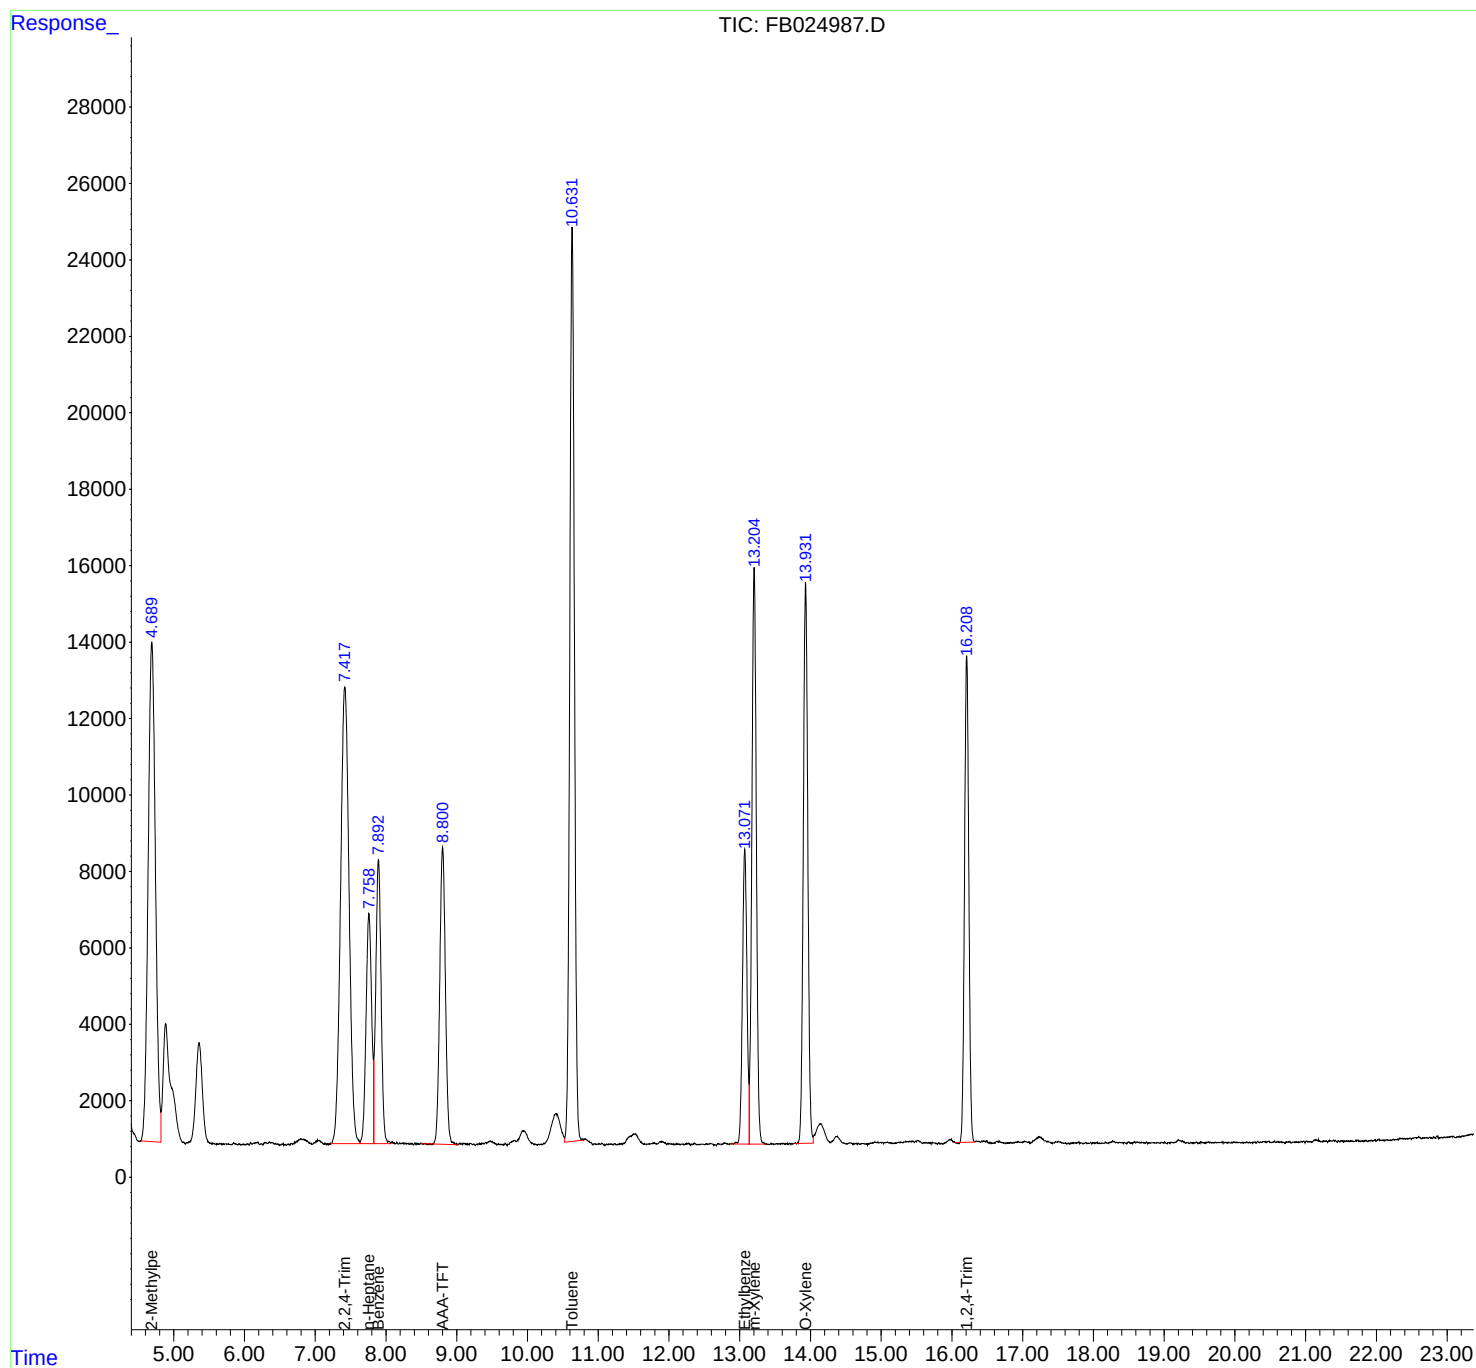

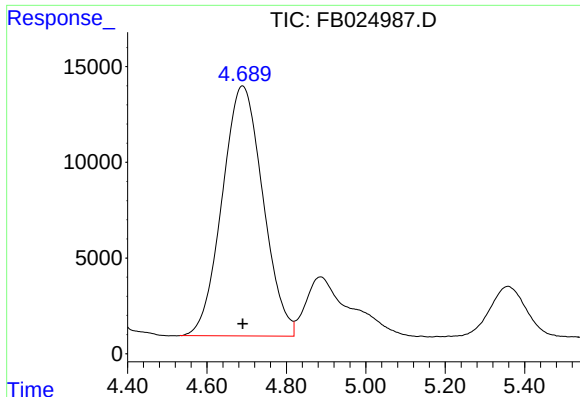


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 931515
Conc: 30.97 ng/ml

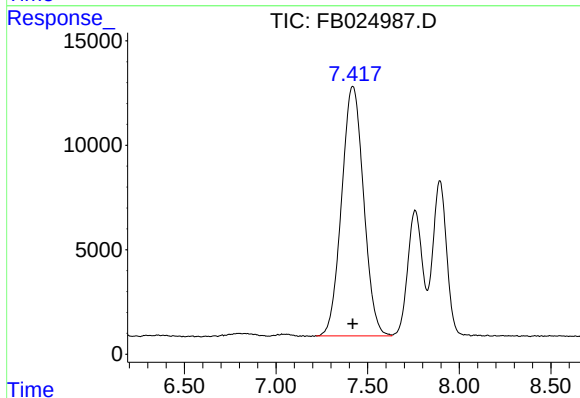


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 996662
Conc: 32.61 ng/ml

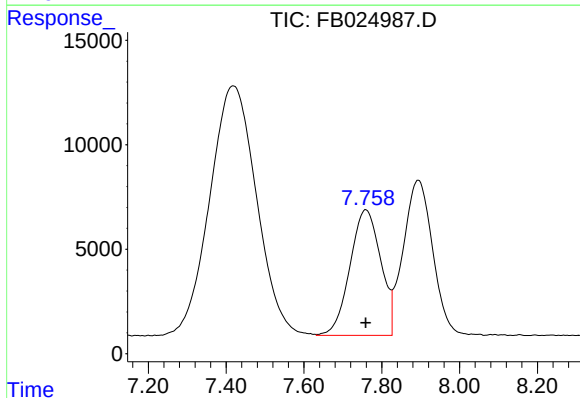


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 330371
Conc: 10.86 ng/ml

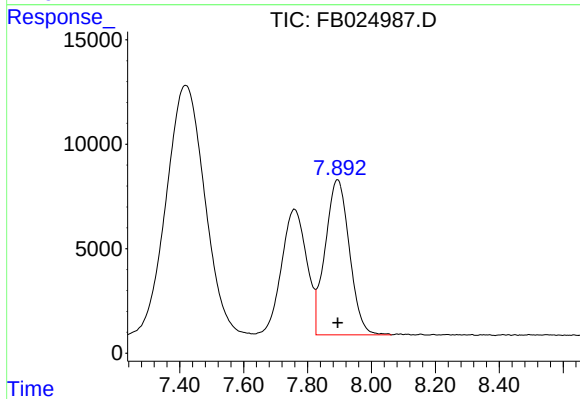


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 390874
Conc: 10.49 ng/ml

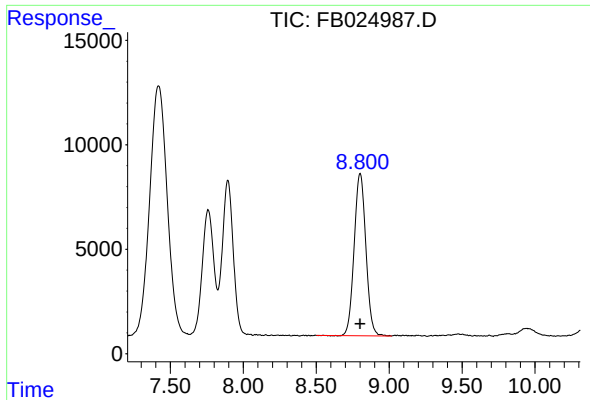


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 433591
Conc: 20.65 ng/ml

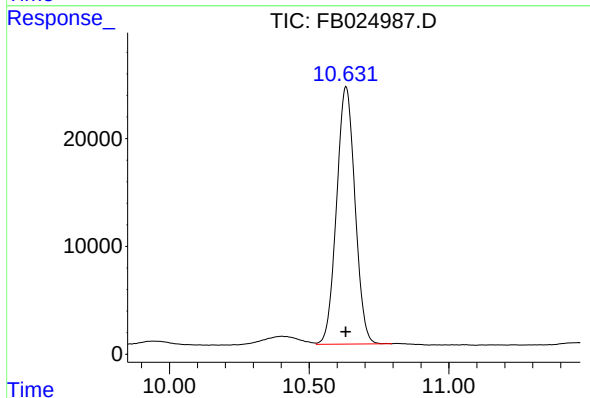


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 1094584
Conc: 31.35 ng/ml

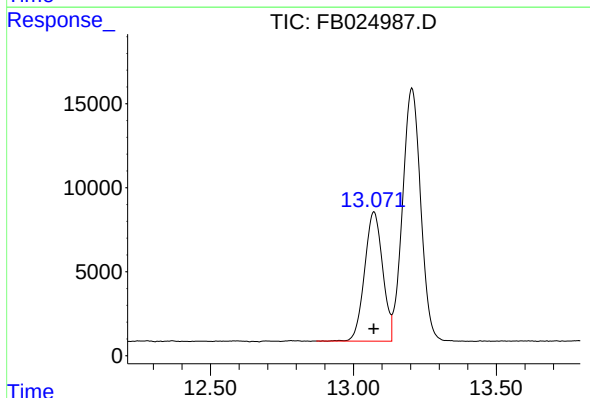


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 337845
Conc: 10.42 ng/ml

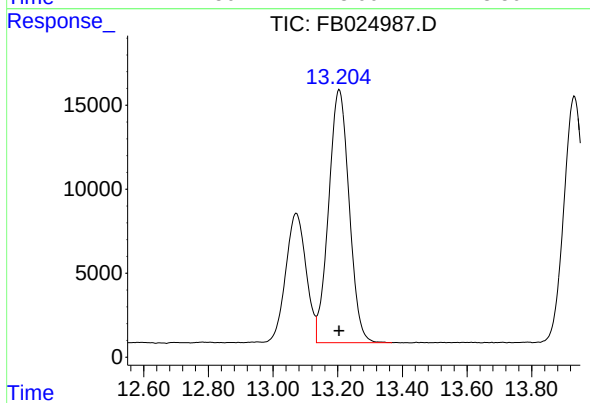


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 664136
Conc: 20.91 ng/ml

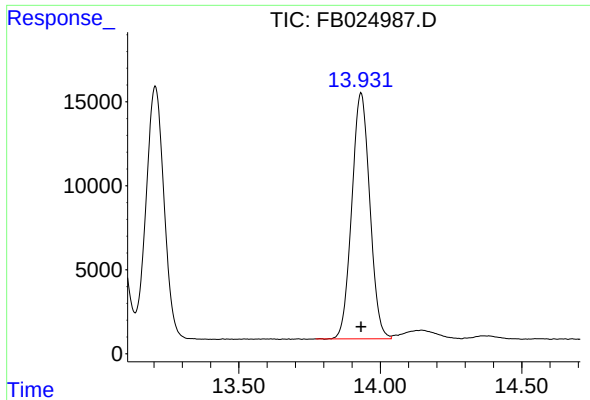

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 648258
Conc: 21.33 ng/ml

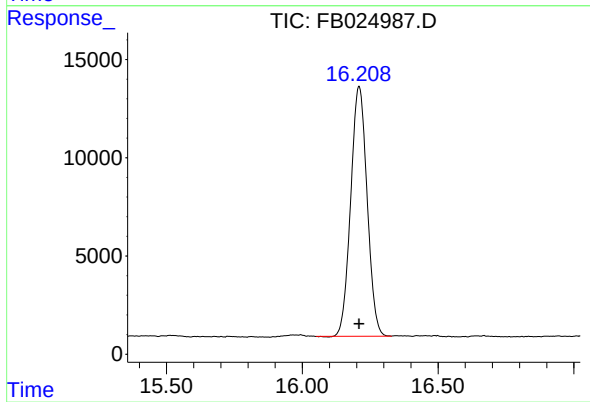

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 534359
Conc: 21.07 ng/ml