

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100120\
 Data File : FB024993.D
 Signal(s) : FID2B.CH
 Acq On : 1 Oct 2020 13:17
 Operator : DD/AJ
 Sample : L3863-10MS
 Misc : 5.00/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 02 02:36:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.800	433998	20.672 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.690	762625	25.359 ng/ml
2) t	2,2,4-Trimethylpentane	7.419	750220	24.546 ng/ml
3) t	n-Heptane	7.760	247228	8.127 ng/ml
4) t	Benzene	7.893	347873	9.339 ng/ml
6) t	Toluene	10.632	951012	27.242 ng/ml
7) t	Ethylbenzene	13.072	280667	8.658 ng/ml
8) t	m-Xylene	13.205	562387	17.704 ng/ml
9) t	O-Xylene	13.932	545105	17.938 ng/ml
10) t	1,2,4-Trimethylbenzene	16.210	425840	16.790 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100120\
Data File : FB024993.D
Signal(s) : FID2B.CH
Acq On : 1 Oct 2020 13:17
Operator : DD/AJ
Sample : L3863-10MS
Misc : 5.00/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 02 02:36:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

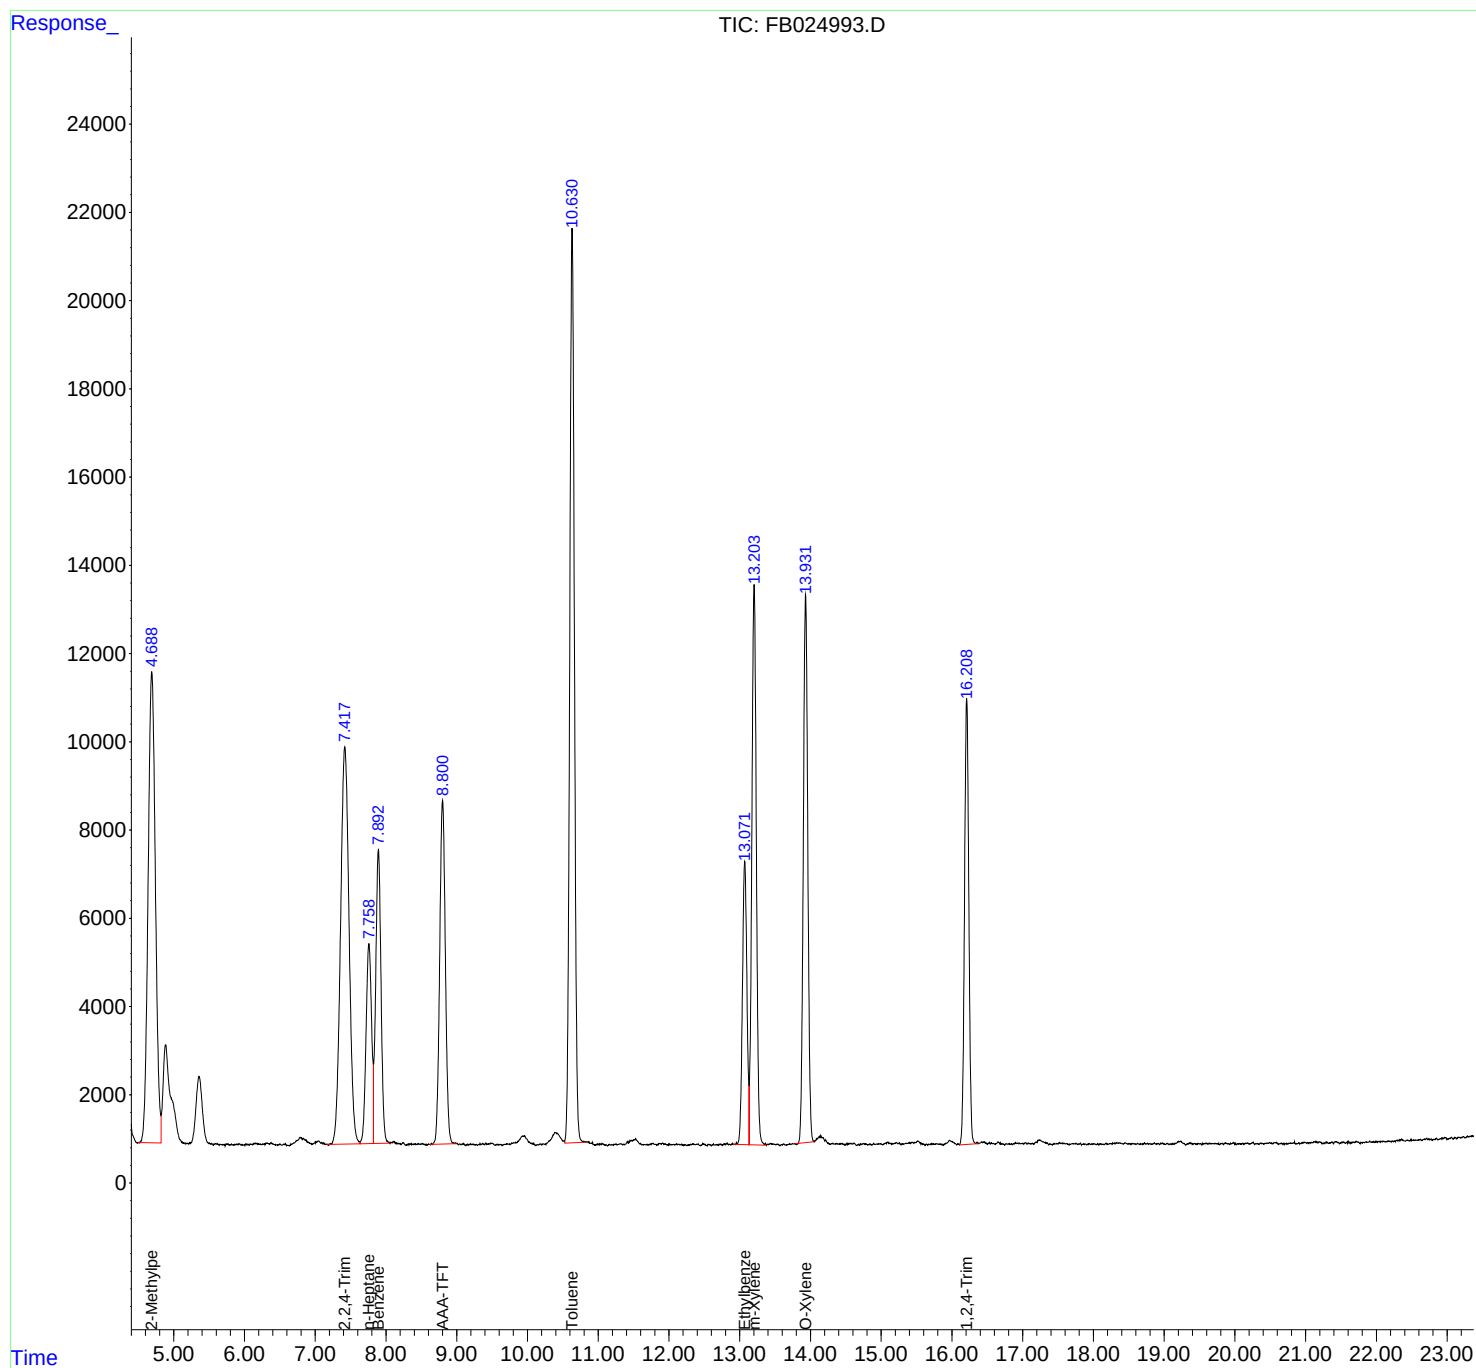

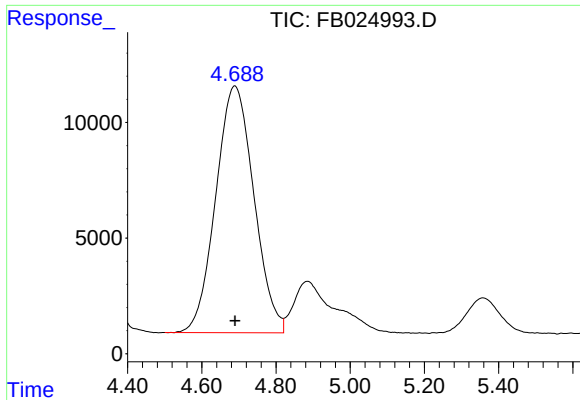


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 762625
Conc: 25.36 ng/ml

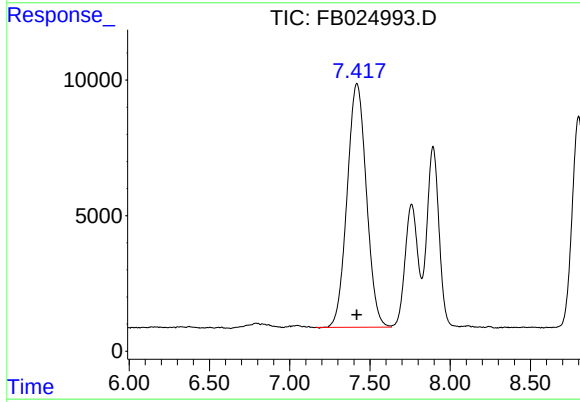


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 750220
Conc: 24.55 ng/ml

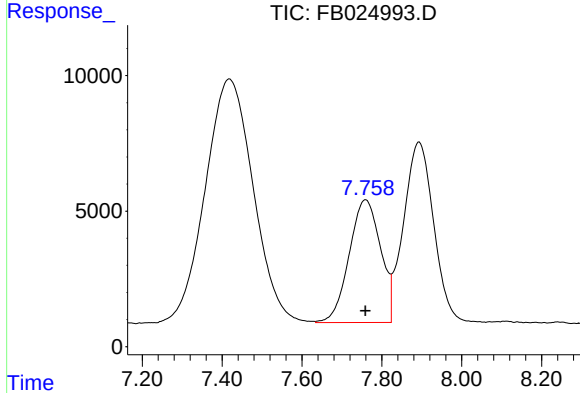


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 247228
Conc: 8.13 ng/ml

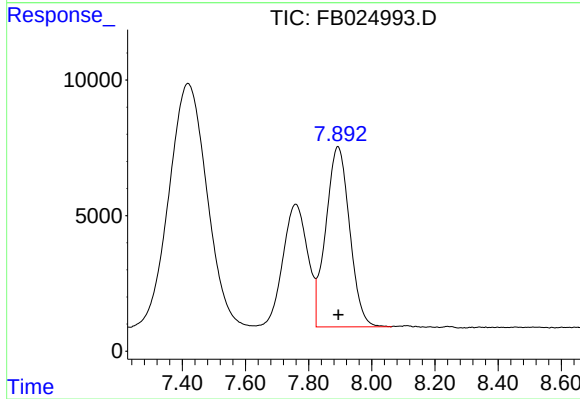


#4 Benzene

R.T.: 7.893 min
Delta R.T.: -0.001 min
Response: 347873
Conc: 9.34 ng/ml

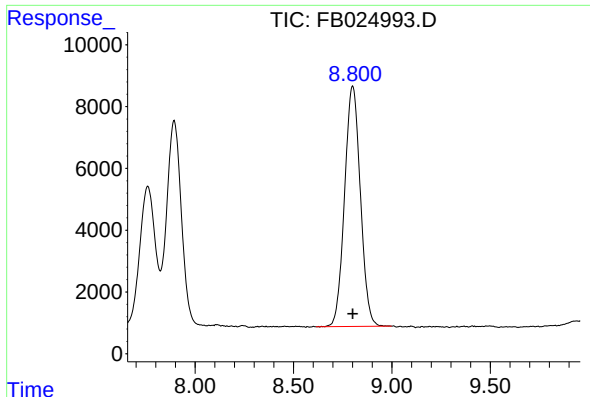


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 433998
Conc: 20.67 ng/ml

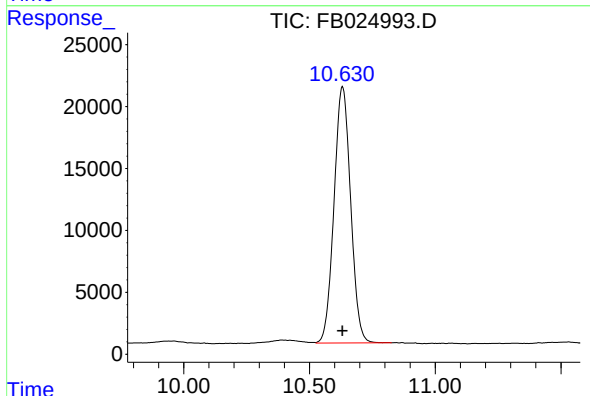


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 951012
Conc: 27.24 ng/ml

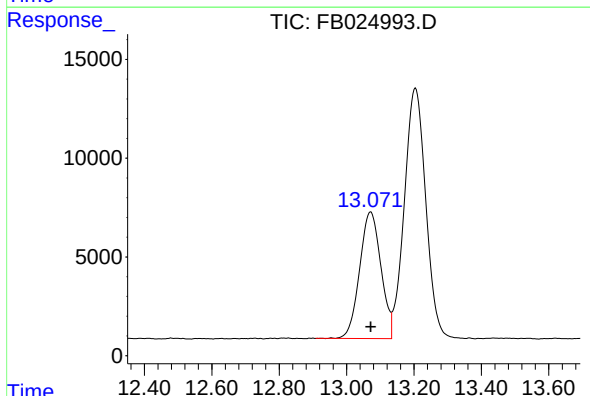


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 280667
Conc: 8.66 ng/ml

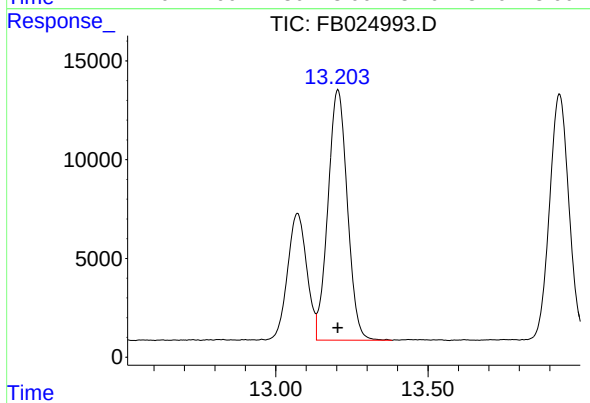


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 562387
Conc: 17.70 ng/ml

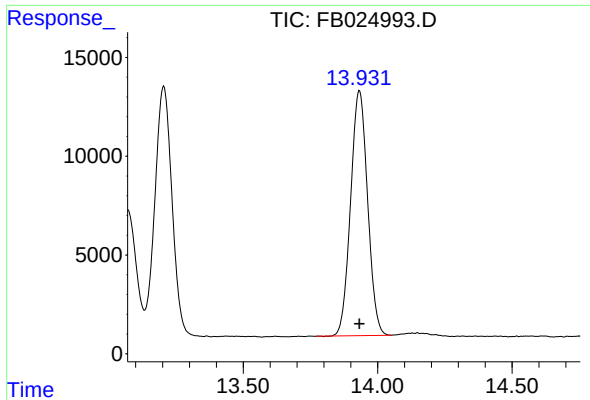

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 545105
Conc: 17.94 ng/ml

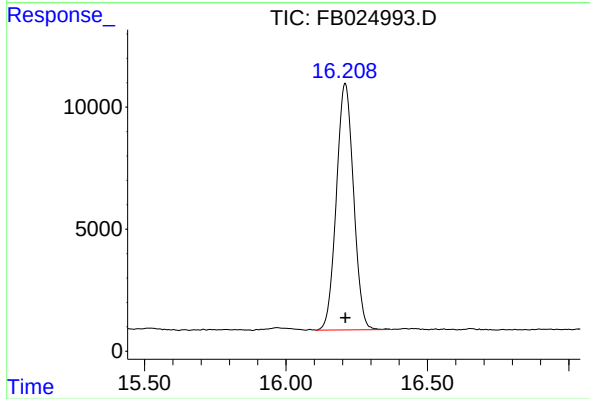

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 425840
Conc: 16.79 ng/ml