

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100120\
 Data File : FB024994.D
 Signal(s) : FID2B.CH
 Acq On : 1 Oct 2020 13:47
 Operator : DD/AJ
 Sample : L3863-10MSD
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 02 02:36:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	469445	22.361 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	776223	25.811 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	766501	25.079 ng/ml
3) t n-Heptane	7.758	251016	8.251 ng/ml
4) t Benzene	7.893	377799	10.142 ng/ml
6) t Toluene	10.631	1017784	29.155 ng/ml
7) t Ethylbenzene	13.071	291557	8.994 ng/ml
8) t m-Xylene	13.204	581357	18.301 ng/ml
9) t O-Xylene	13.932	568626	18.712 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	446874	17.619 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100120\
Data File : FB024994.D
Signal(s) : FID2B.CH
Acq On : 1 Oct 2020 13:47
Operator : DD/AJ
Sample : L3863-10MSD
Misc : 5.01/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 02 02:36:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

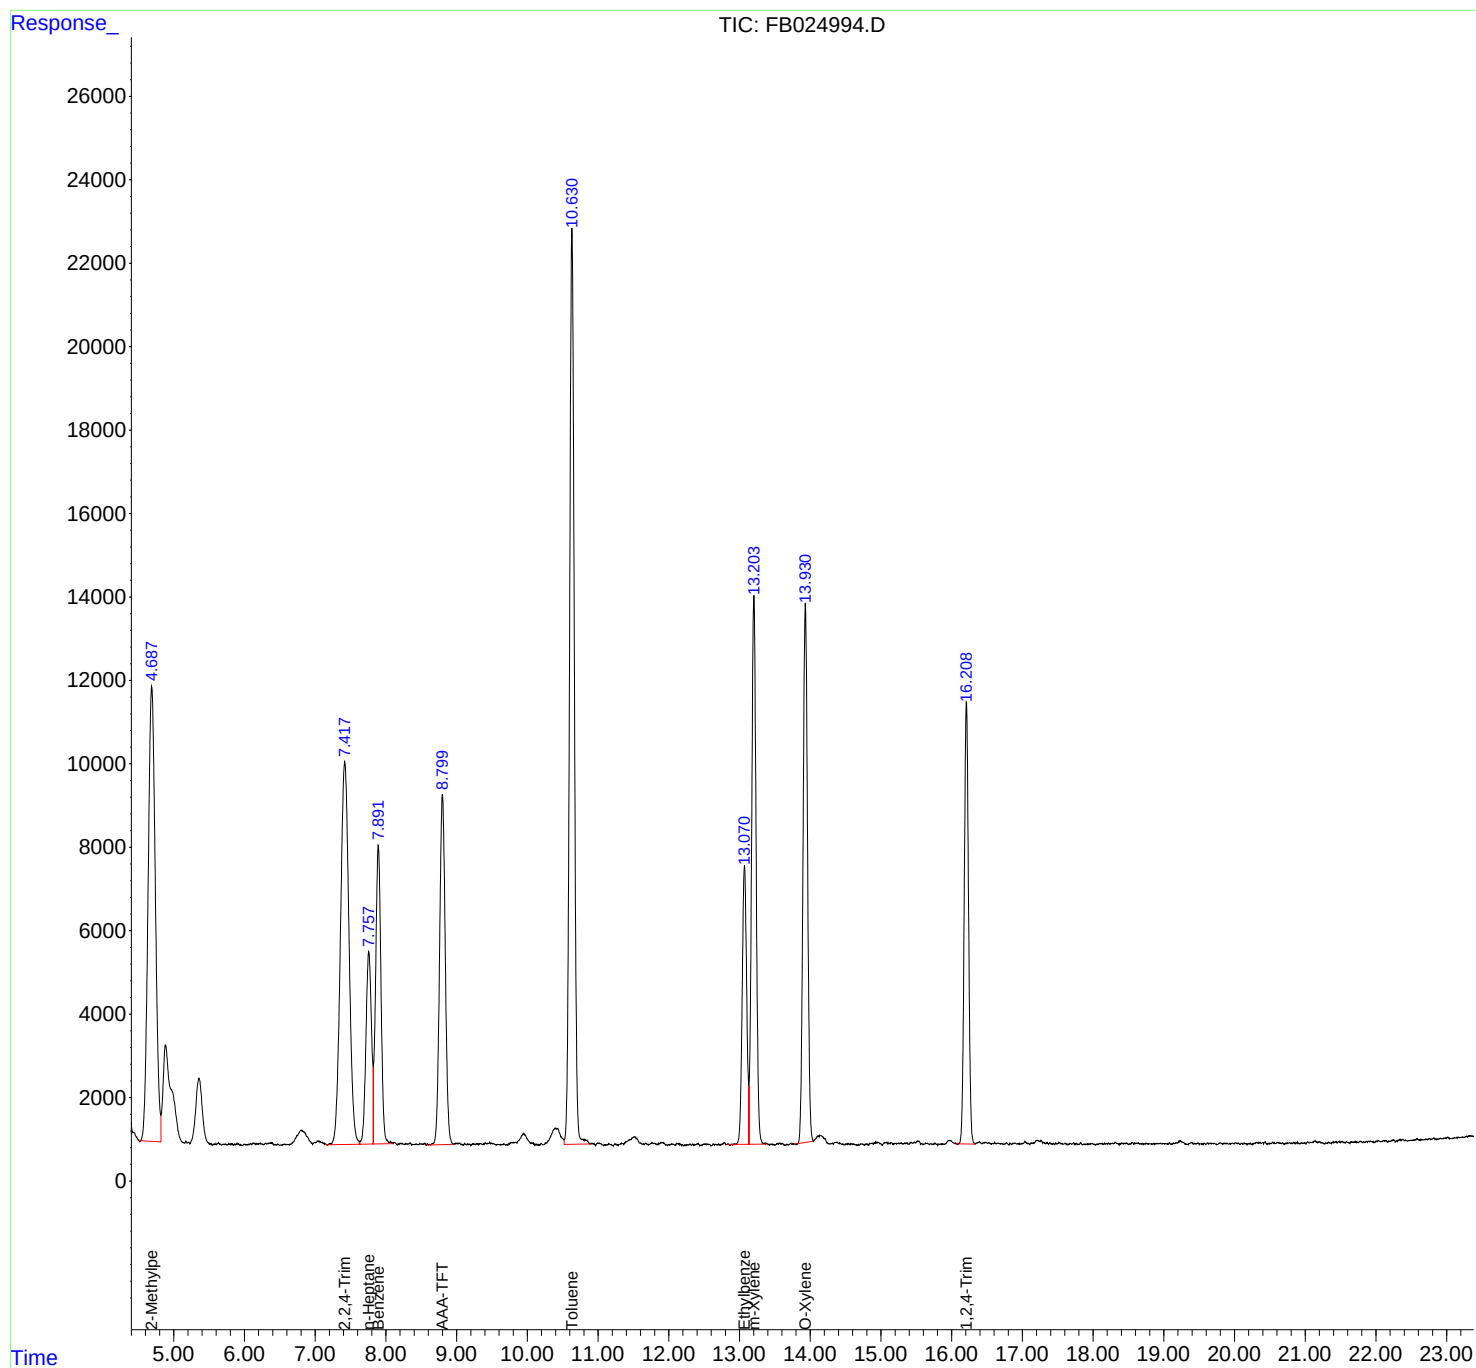

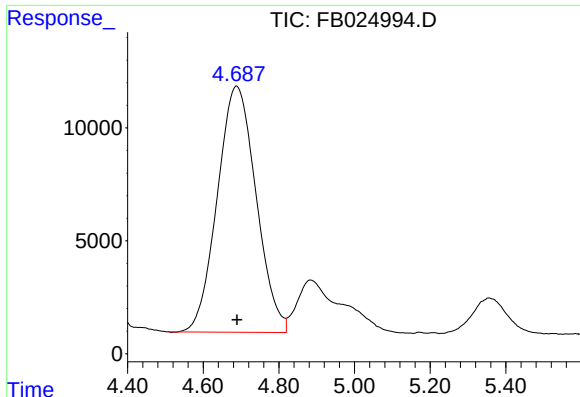


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: -0.001 min
Response: 776223
Conc: 25.81 ng/ml

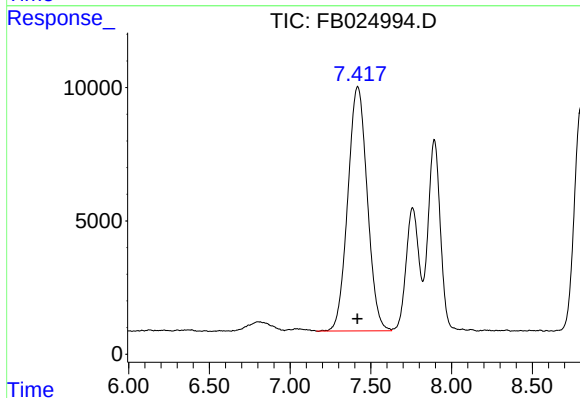


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 766501
Conc: 25.08 ng/ml

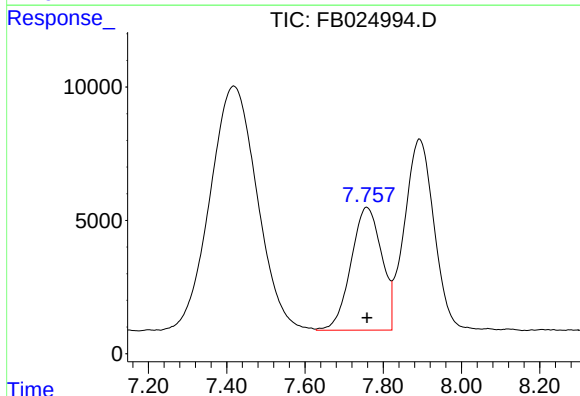


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.001 min
Response: 251016
Conc: 8.25 ng/ml

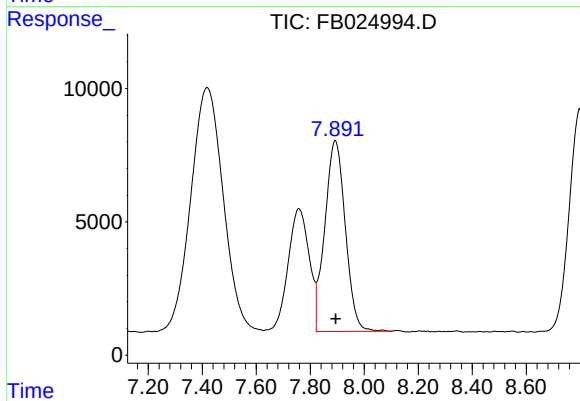


#4 Benzene

R.T.: 7.893 min
Delta R.T.: -0.002 min
Response: 377799
Conc: 10.14 ng/ml

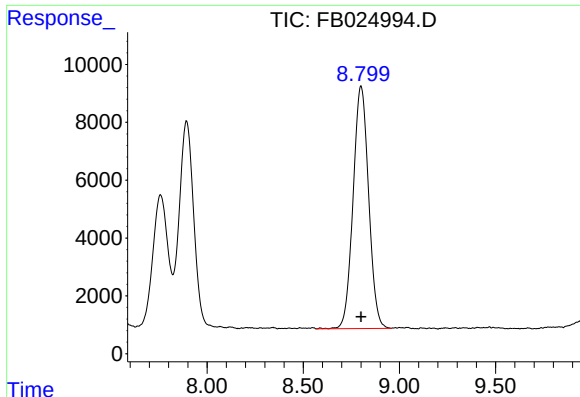


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 469445
Conc: 22.36 ng/ml

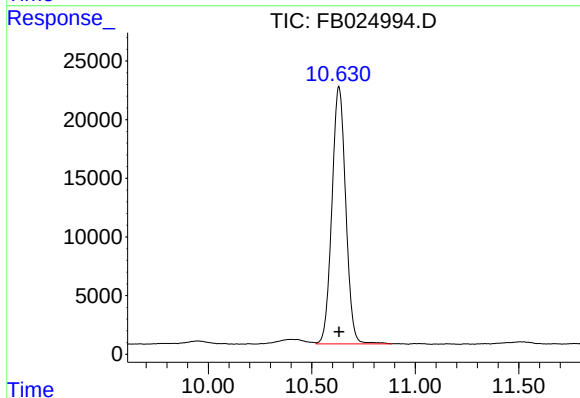


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1017784
Conc: 29.15 ng/ml

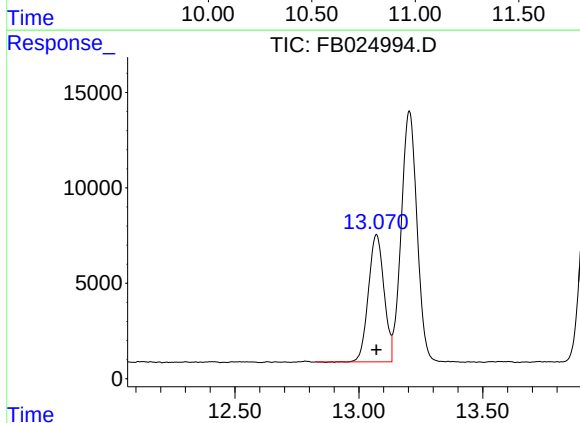


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 291557
Conc: 8.99 ng/ml

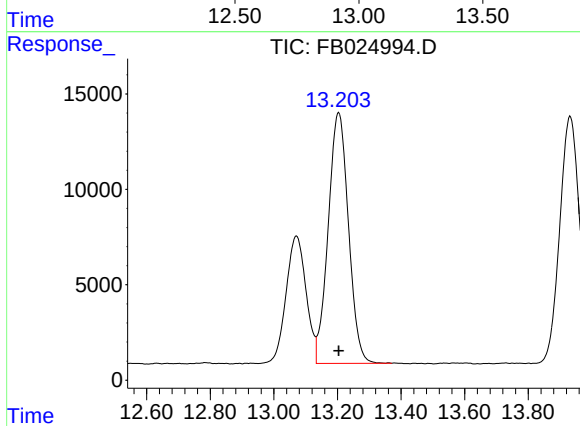

#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 581357
Conc: 18.30 ng/ml

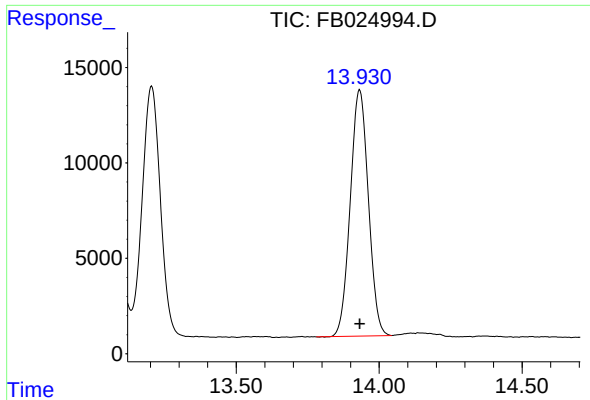


#9 O-Xylene

R.T.: 13.932 min

Delta R.T.: 0.000 min

Response: 568626

Conc: 18.71 ng/ml

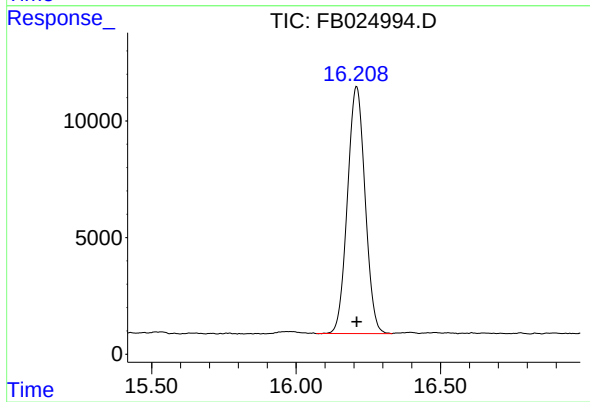

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min

Delta R.T.: 0.000 min

Response: 446874

Conc: 17.62 ng/ml