

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100218\
Data File : FB018077.D
Signal(s) : FID2B.CH
Acq On : 2 Oct 2018 20:26
Operator : MJ/SJ
Sample : J5218-05
Misc : 5.02g/5.00mL DI Water
ALS Vial : 22 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 03 08:22:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.107	149352	17.656 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.956	1871	0.118 ng/ml
4) t Benzene	8.218	8062	0.423 ng/ml
6) t Toluene	10.955	6744	0.426 ng/ml
8) t m-Xylene	13.535	2238	0.129 ng/ml
9) t O-Xylene	14.333	12806	0.705 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100218\
Data File : FB018077.D
Signal(s) : FID2B.CH
Acq On : 2 Oct 2018 20:26
Operator : MJ/SJ
Sample : J5218-05
Misc : 5.02g/5.00mL DI Water
ALS Vial : 22 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 03 08:22:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

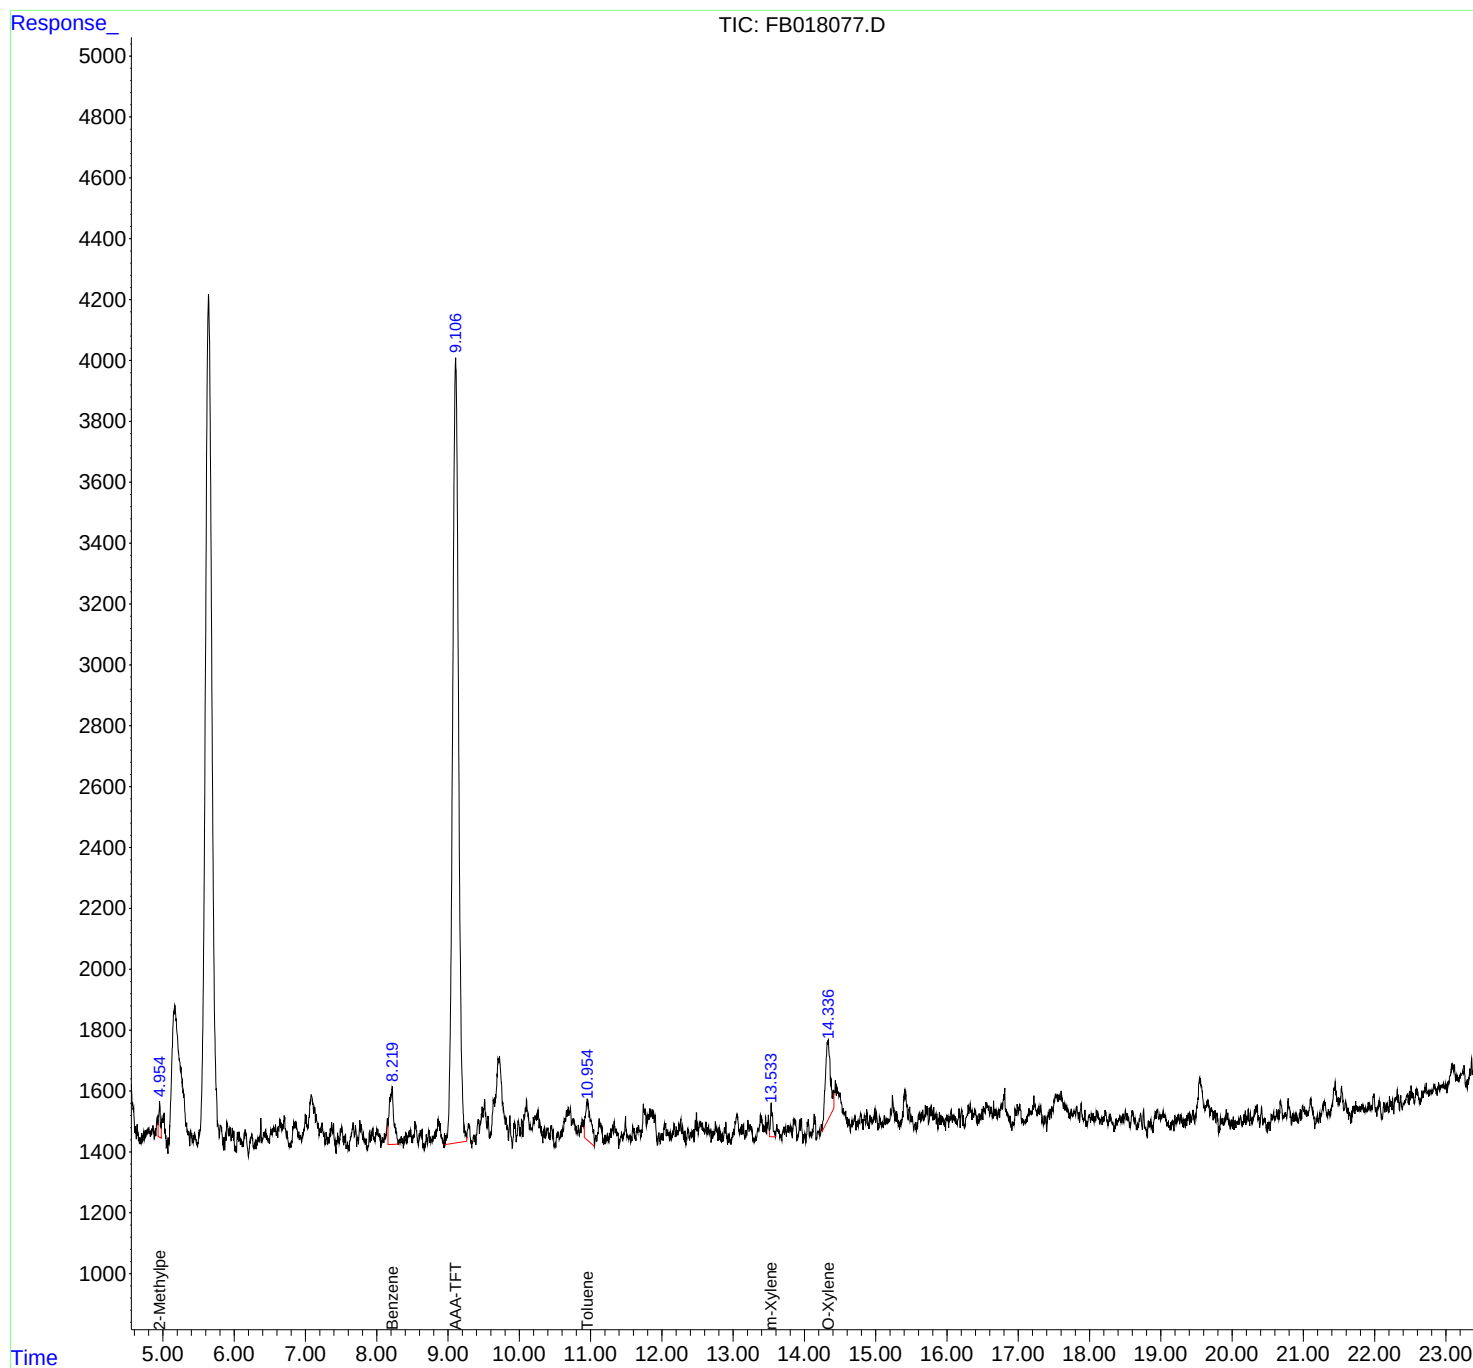

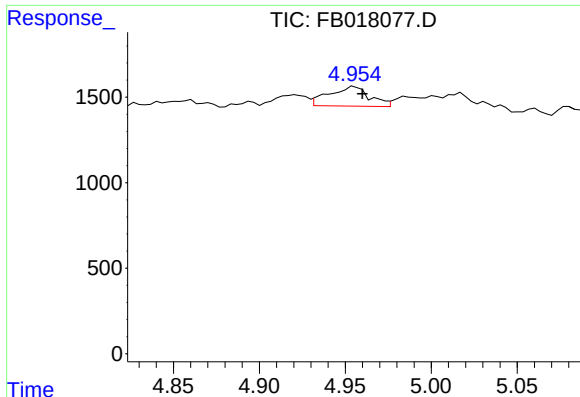

#1 2-Methylpentane

R.T.: 4.956 min
Delta R.T.: -0.004 min
Response: 1871
Conc: 0.12 ng/ml

#4 Benzene


R.T.: 8.218 min
Delta R.T.: 0.014 min
Response: 8062
Conc: 0.42 ng/ml

#5 AAA-TFT

R.T.: 9.107 min
Delta R.T.: -0.003 min
Response: 149352
Conc: 17.66 ng/ml


#6 Toluene

R.T.: 10.955 min
Delta R.T.: -0.004 min
Response: 6744
Conc: 0.43 ng/ml

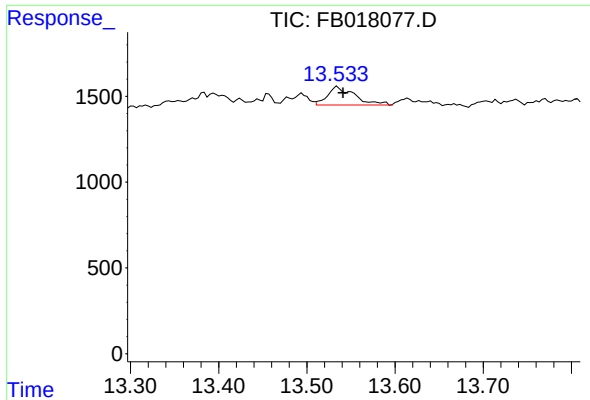

#8 m-Xylene

R.T.: 13.535 min
Delta R.T.: -0.006 min
Response: 2238
Conc: 0.13 ng/ml

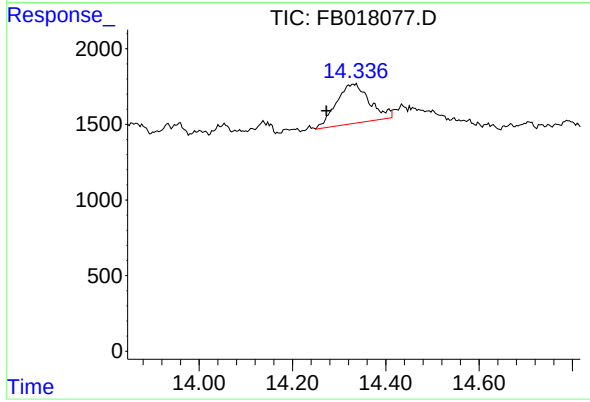

#9 O-Xylene

R.T.: 14.333 min
Delta R.T.: 0.059 min
Response: 12806
Conc: 0.70 ng/ml