

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100218\
 Data File : FB018058.D
 Signal(s) : FID2B.CH
 Acq On : 2 Oct 2018 9:05
 Operator : MJ/SJ
 Sample : BSF1002S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 03 08:19:58 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
 Quant Title :
 QLast Update : Fri Sep 14 13:09:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.108	176592	20.877 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.957	459705	28.866 ng/ml
2) t 2,2,4-Trimethylpentane	7.724	466209	29.296 ng/ml
3) t n-Heptane	8.063	149078	9.674 ng/ml
4) t Benzene	8.202	186512	9.798 ng/ml
6) t Toluene	10.957	469100	29.641 ng/ml
7) t Ethylbenzene	13.407	156497	9.578 ng/ml
8) t m-Xylene	13.539	337807	19.527 ng/ml
9) t O-Xylene	14.271	355950	19.588 ng/ml
10) t 1,2,4-Trimethylbenzene	16.554	415271	19.522 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100218\
Data File : FB018058.D
Signal(s) : FID2B.CH
Acq On : 2 Oct 2018 9:05
Operator : MJ/SJ
Sample : BSF1002S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 03 08:19:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

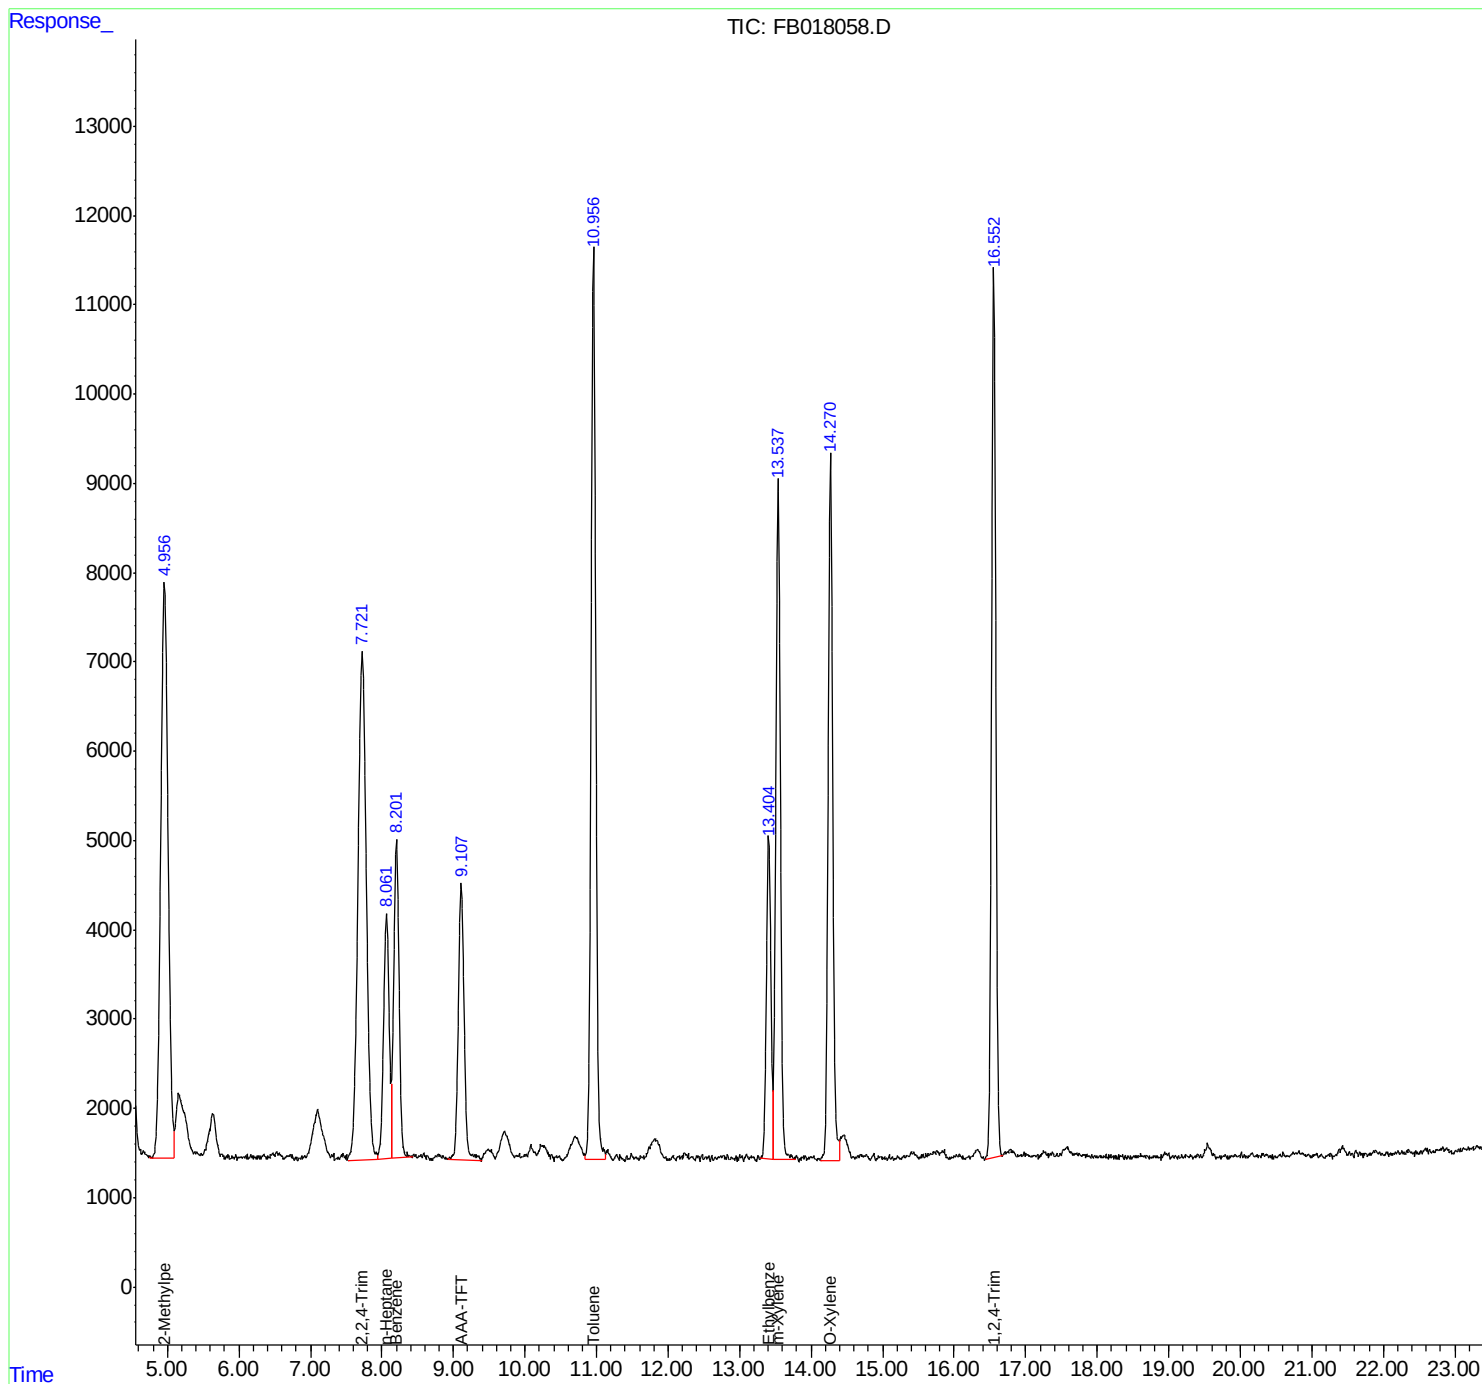

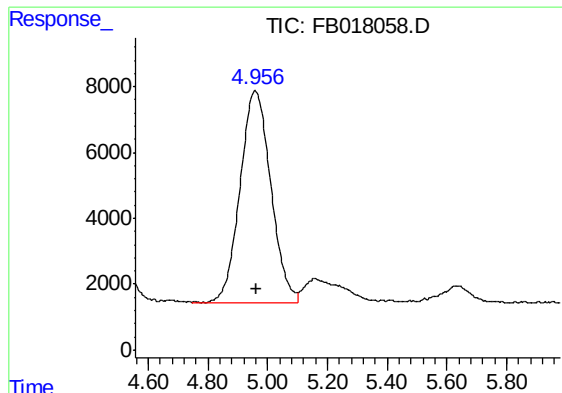


#1 2-Methylpentane

R.T.: 4.957 min
Delta R.T.: -0.003 min
Response: 459705
Conc: 28.87 ng/ml

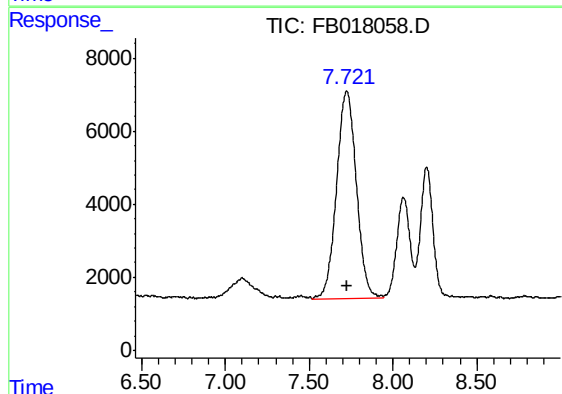


#2 2,2,4-Trimethylpentane

R.T.: 7.724 min
Delta R.T.: -0.003 min
Response: 466209
Conc: 29.30 ng/ml

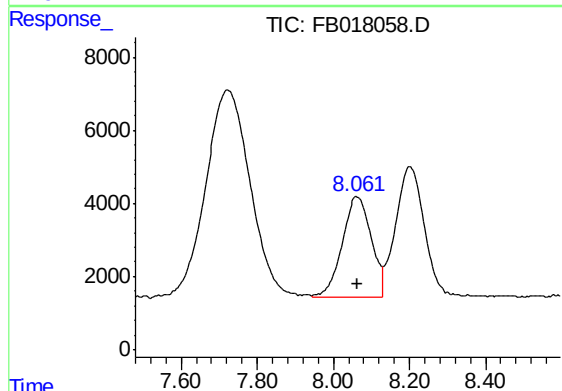


#3 n-Heptane

R.T.: 8.063 min
Delta R.T.: -0.002 min
Response: 149078
Conc: 9.67 ng/ml

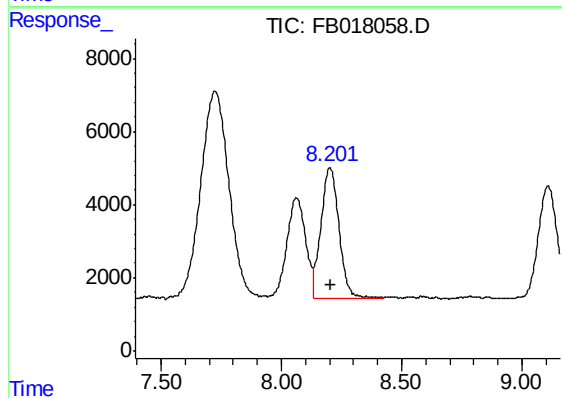


#4 Benzene

R.T.: 8.202 min
Delta R.T.: -0.002 min
Response: 186512
Conc: 9.80 ng/ml

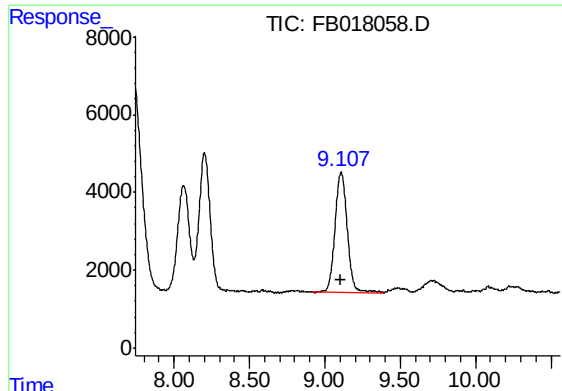


#5 AAA-TFT

R.T.: 9.108 min
Delta R.T.: -0.002 min
Response: 176592
Conc: 20.88 ng/ml

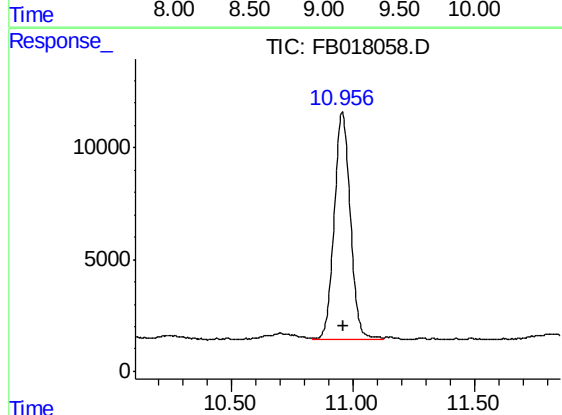


#6 Toluene

R.T.: 10.957 min
Delta R.T.: -0.002 min
Response: 469100
Conc: 29.64 ng/ml

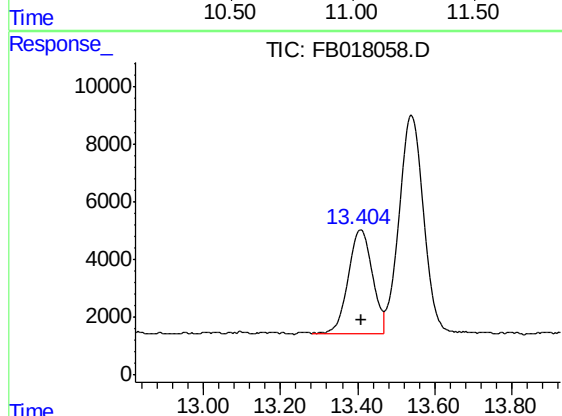


#7 Ethylbenzene

R.T.: 13.407 min
Delta R.T.: -0.002 min
Response: 156497
Conc: 9.58 ng/ml

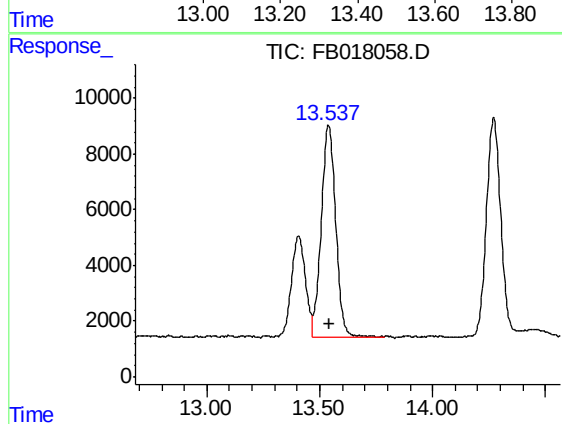


#8 m-Xylene

R.T.: 13.539 min
Delta R.T.: -0.002 min
Response: 337807
Conc: 19.53 ng/ml

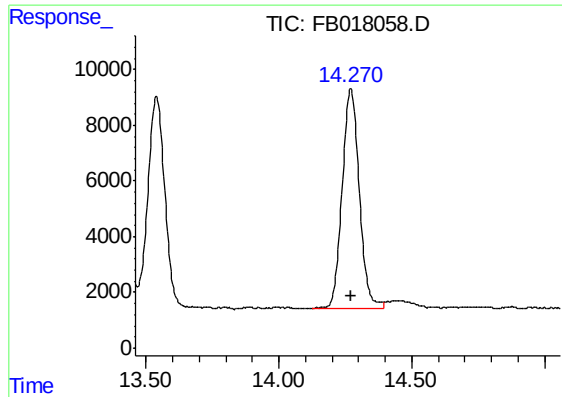

#9 O-Xylene

R.T.: 14.271 min
Delta R.T.: -0.002 min
Response: 355950
Conc: 19.59 ng/ml

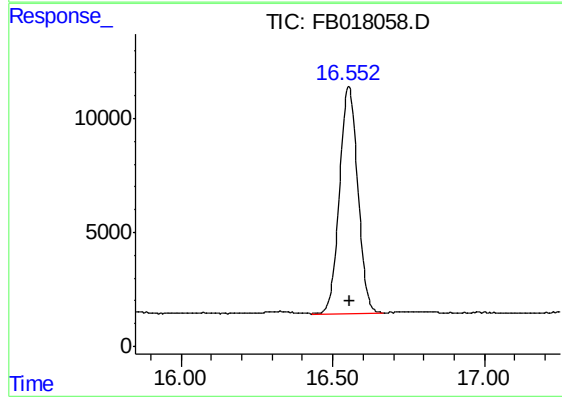

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min
Delta R.T.: -0.002 min
Response: 415271
Conc: 19.52 ng/ml