

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100218\
 Data File : FB018062.D
 Signal(s) : FID2B.CH
 Acq On : 2 Oct 2018 11:49
 Operator : MJ/SJ
 Sample : J5200-03MSD
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 03 08:20:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
 Quant Title :
 QLast Update : Fri Sep 14 13:09:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.106	156440	18.494 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.962	322053	20.223 ng/ml
2) t 2,2,4-Trimethylpentane	7.724	331504	20.831 ng/ml
3) t n-Heptane	8.066	31895	2.070 ng/ml
4) t Benzene	8.204	160646	8.439 ng/ml
6) t Toluene	10.957	412646	26.074 ng/ml
7) t Ethylbenzene	13.406	138104	8.452 ng/ml
8) t m-Xylene	13.539	274082	15.843 ng/ml
9) t O-Xylene	14.270	311041	17.116 ng/ml
10) t 1,2,4-Trimethylbenzene	16.554	268360	12.616 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100218\
Data File : FB018062.D
Signal(s) : FID2B.CH
Acq On : 2 Oct 2018 11:49
Operator : MJ/SJ
Sample : J5200-03MSD
Misc : 5.01g/5.00mL DI Water
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 03 08:20:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

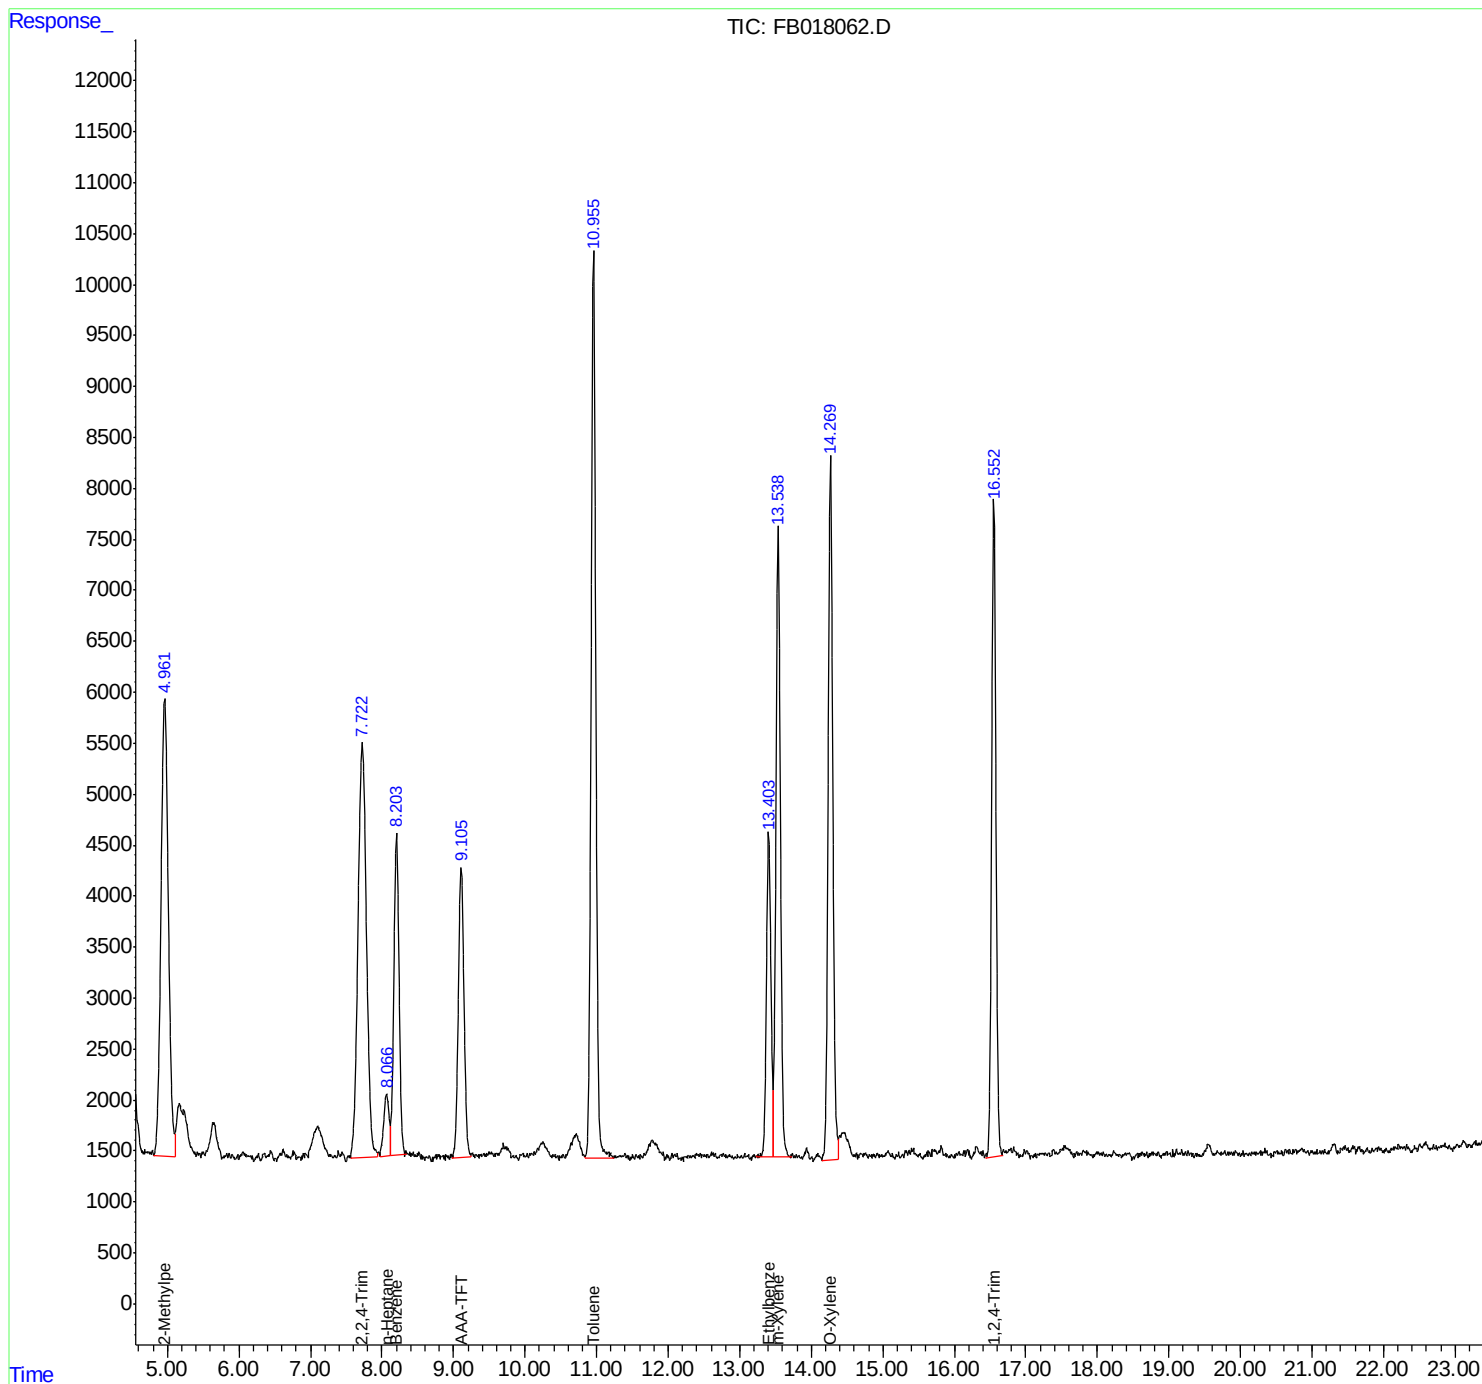

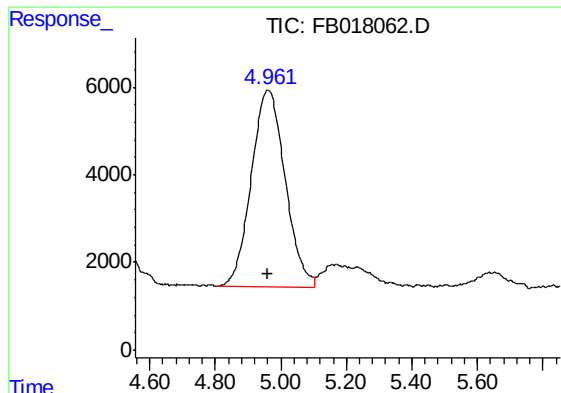


#1 2-Methylpentane

R.T.: 4.962 min
Delta R.T.: 0.002 min
Response: 322053
Conc: 20.22 ng/ml

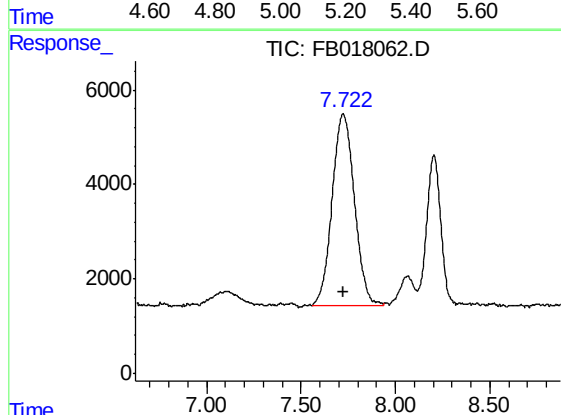


#2 2,2,4-Trimethylpentane

R.T.: 7.724 min
Delta R.T.: -0.003 min
Response: 331504
Conc: 20.83 ng/ml

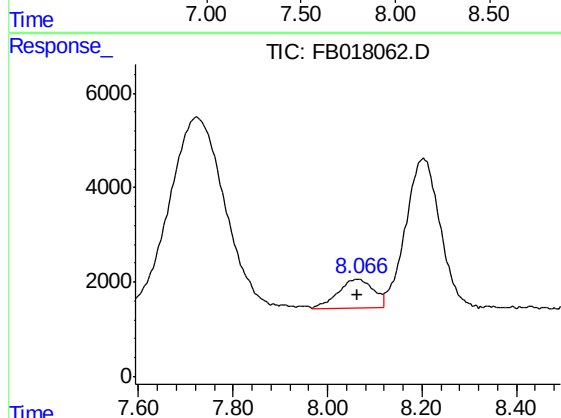


#3 n-Heptane

R.T.: 8.066 min
Delta R.T.: 0.000 min
Response: 31895
Conc: 2.07 ng/ml

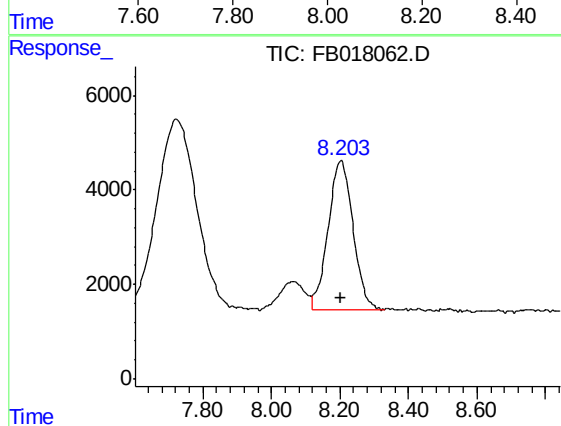


#4 Benzene

R.T.: 8.204 min
Delta R.T.: 0.000 min
Response: 160646
Conc: 8.44 ng/ml

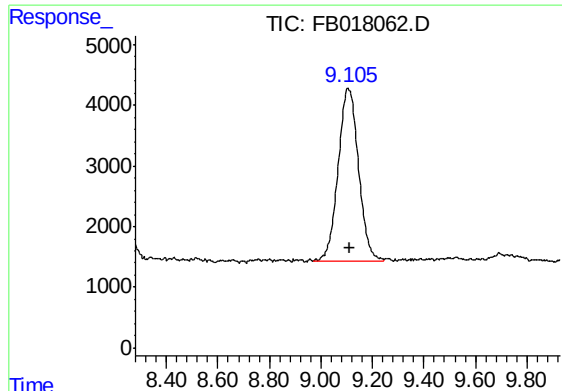


#5 AAA-TFT

R.T.: 9.106 min
Delta R.T.: -0.004 min
Response: 156440
Conc: 18.49 ng/ml

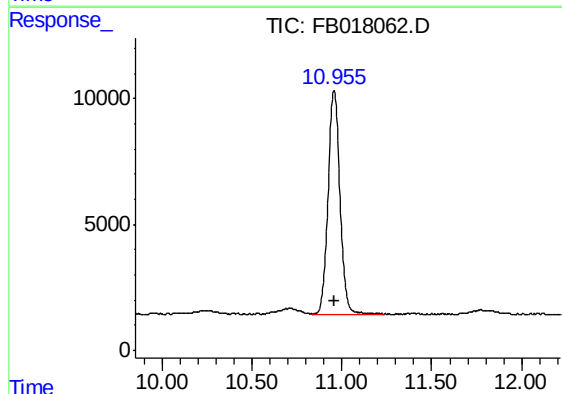


#6 Toluene

R.T.: 10.957 min
Delta R.T.: -0.003 min
Response: 412646
Conc: 26.07 ng/ml

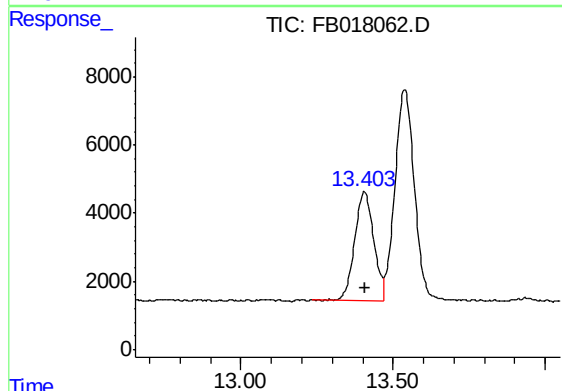


#7 Ethylbenzene

R.T.: 13.406 min
Delta R.T.: -0.003 min
Response: 138104
Conc: 8.45 ng/ml

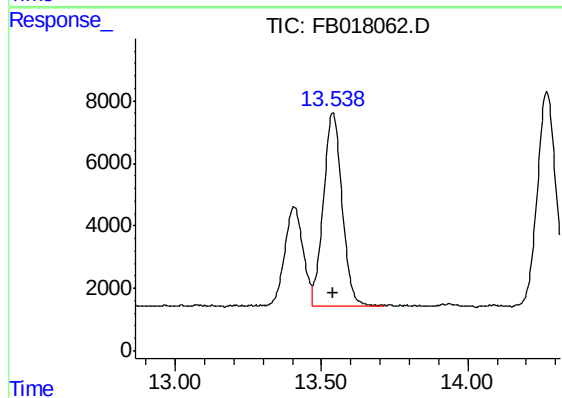

#8 m-Xylene

R.T.: 13.539 min
Delta R.T.: -0.002 min
Response: 274082
Conc: 15.84 ng/ml

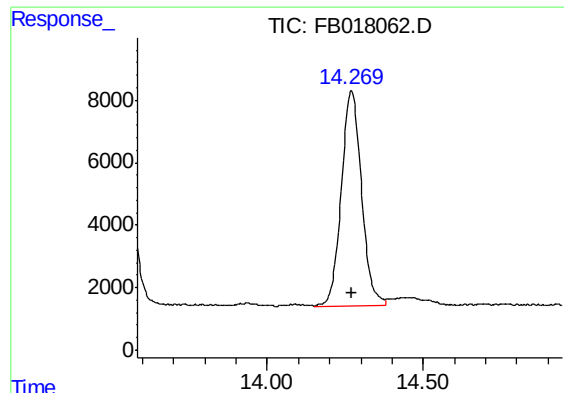


#9 O-Xylene

R.T.: 14.270 min

Delta R.T.: -0.003 min

Response: 311041

Conc: 17.12 ng/ml

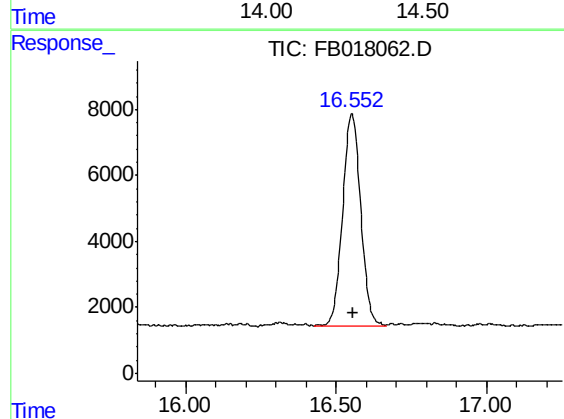

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min

Delta R.T.: -0.002 min

Response: 268360

Conc: 12.62 ng/ml