

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100219\
 Data File : FB022661.D
 Signal(s) : FID2B.CH
 Acq On : 2 Oct 2019 13:40
 Operator : DD/AJ
 Sample : VBF1002S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 VBF1002S1

Integration File: Calibration.e
 Quant Time: Oct 03 02:02:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
 Quant Title :
 QLast Update : Wed Oct 02 06:15:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.970	494084	20.506 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.823	25124	0.753 ng/ml
2) t 2,2,4-Trimethylpentane	7.585	48767	1.406 ng/ml
3) t n-Heptane	7.925	7759	0.229 ng/ml
4) t Benzene	8.090	4549	0.109 ng/ml
6) t Toluene	10.812	25465	0.629 ng/ml
8) t m-Xylene	13.387	4875	0.131 ng/ml
9) t O-Xylene	14.121	6341	0.182 ng/ml
10) t 1,2,4-Trimethylbenzene	16.419	9041	0.365 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100219\
Data File : FB022661.D
Signal(s) : FID2B.CH
Acq On : 2 Oct 2019 13:40
Operator : DD/AJ
Sample : VBF1002S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampled :
VBF1002S1

Integration File: Calibration.e
Quant Time: Oct 03 02:02:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
Quant Title :
QLast Update : Wed Oct 02 06:15:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

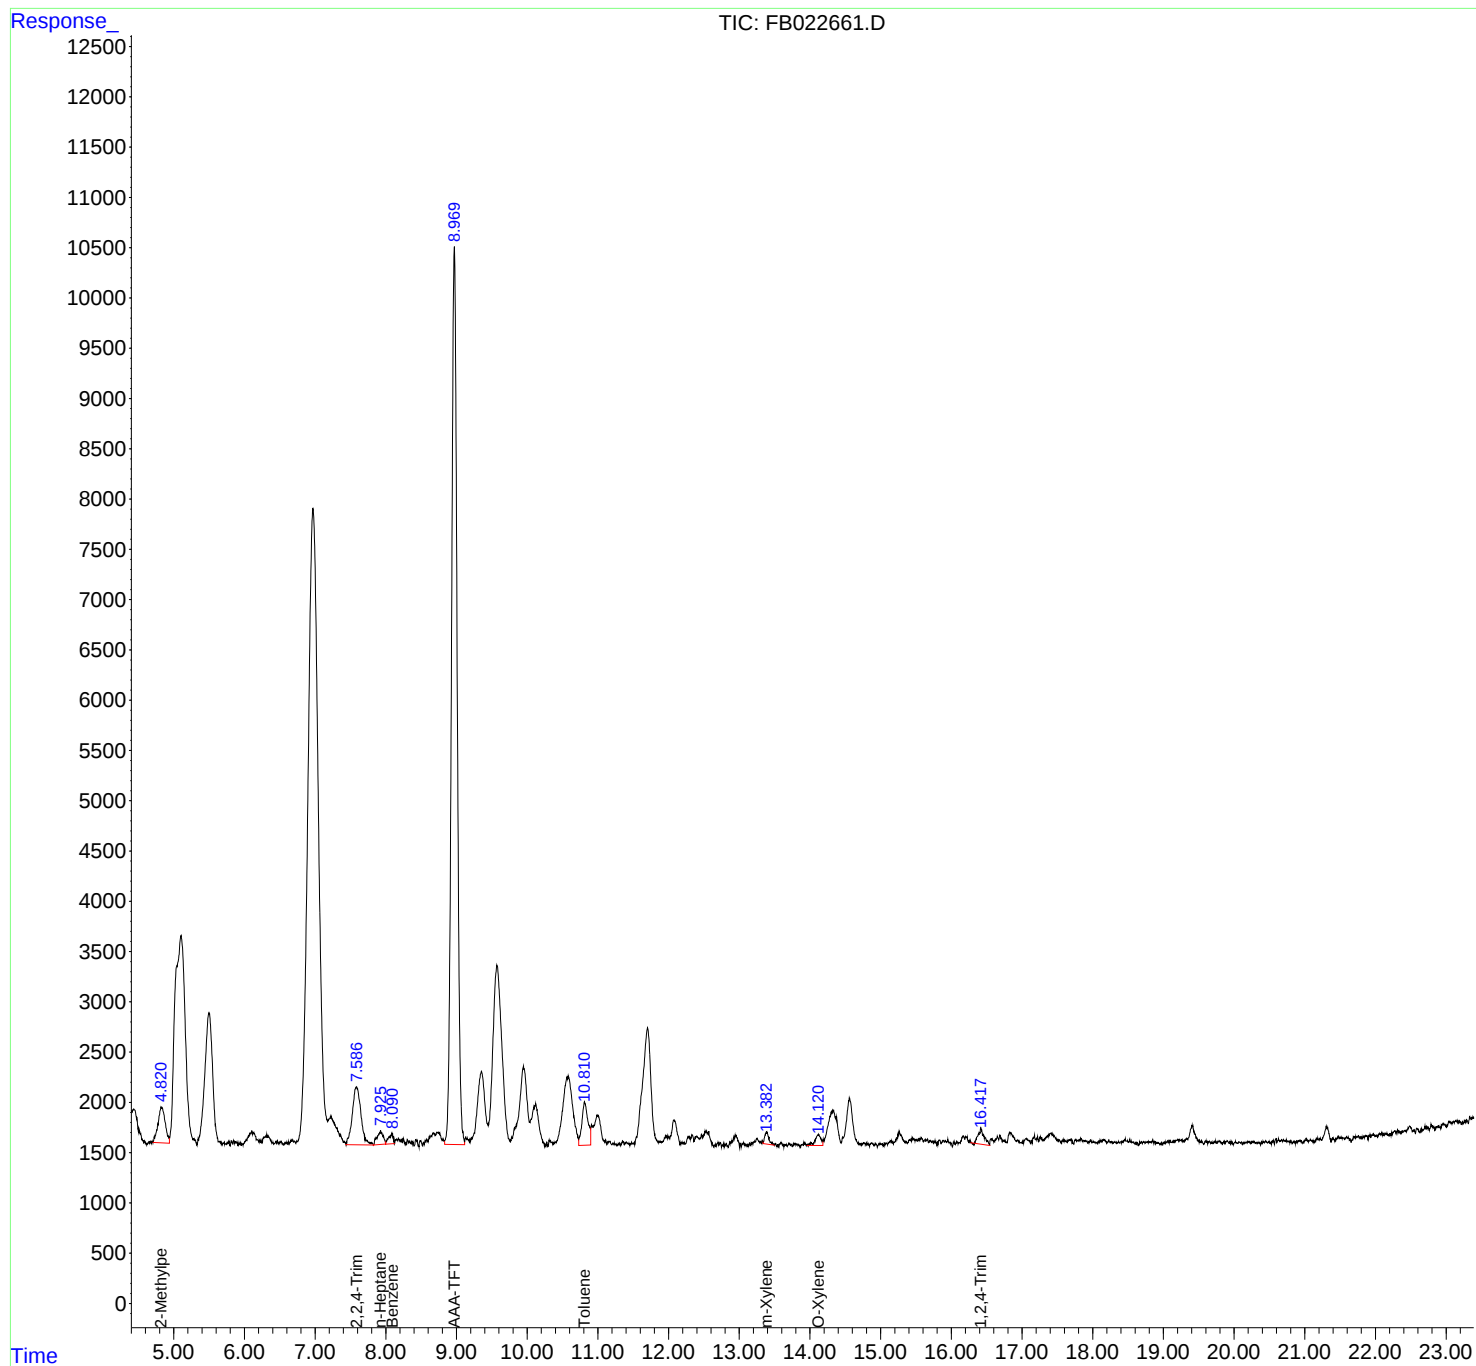


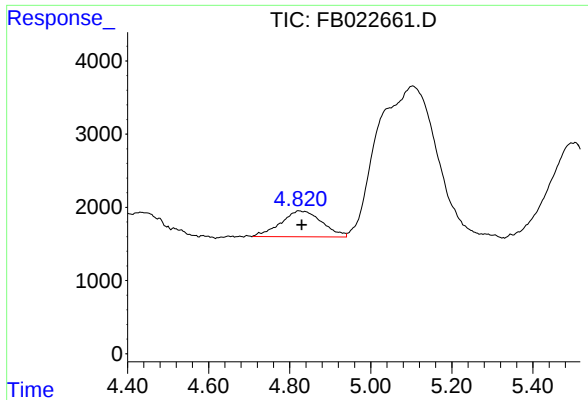

#1 2-Methylpentane


R.T.: 4.823 min
Delta R.T.: -0.007 min
Response: 25124
Conc: 0.75 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF1002S1

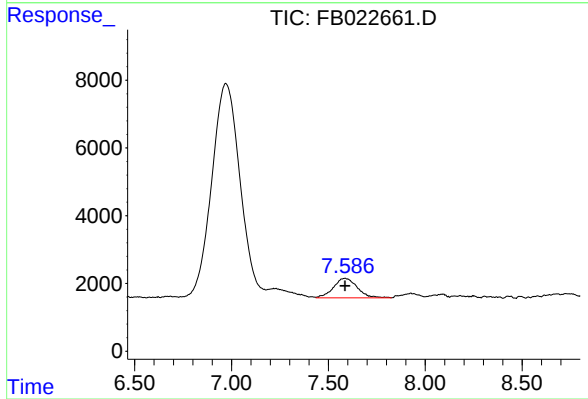


#2 2,2,4-Trimethylpentane

R.T.: 7.585 min
Delta R.T.: 0.000 min
Response: 48767
Conc: 1.41 ng/ml

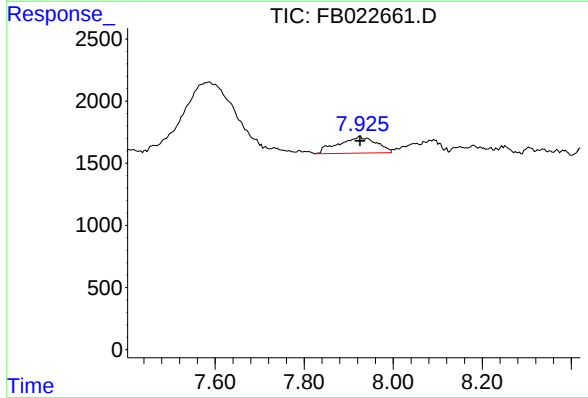


#3 n-Heptane

R.T.: 7.925 min
Delta R.T.: 0.000 min
Response: 7759
Conc: 0.23 ng/ml

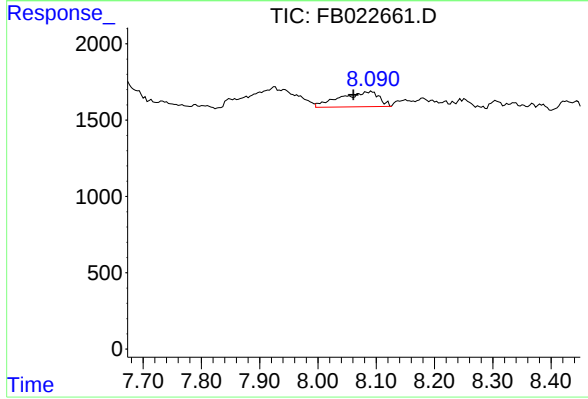

#4 Benzene


R.T.: 8.090 min
Delta R.T.: 0.029 min
Response: 4549
Conc: 0.11 ng/ml

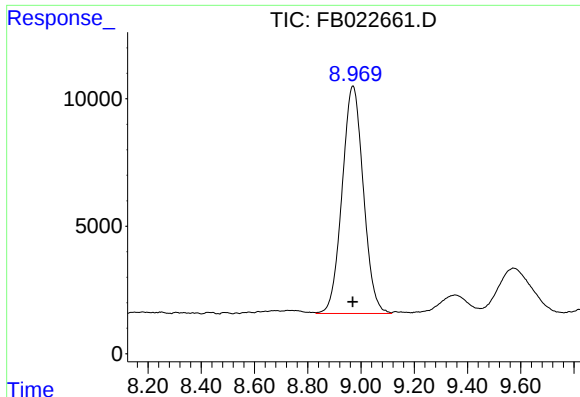

#5 AAA-TFT


R.T.: 8.970 min
Delta R.T.: 0.002 min
Response: 494084
Conc: 20.51 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF1002S1

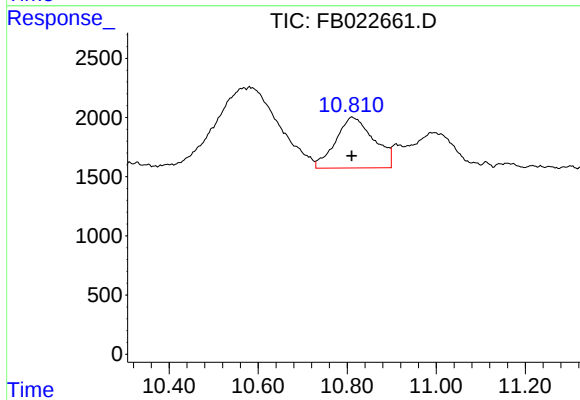


#6 Toluene

R.T.: 10.812 min
Delta R.T.: 0.003 min
Response: 25465
Conc: 0.63 ng/ml

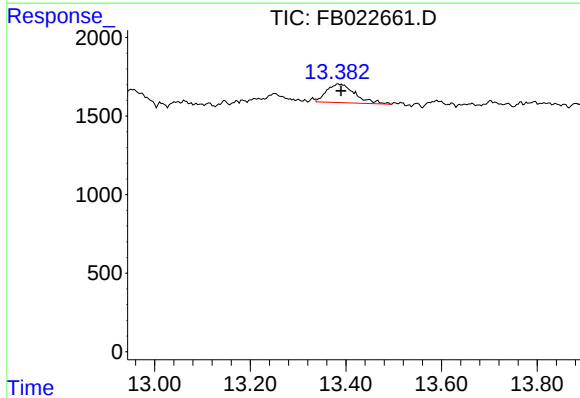


#8 m-Xylene

R.T.: 13.387 min
Delta R.T.: -0.003 min
Response: 4875
Conc: 0.13 ng/ml

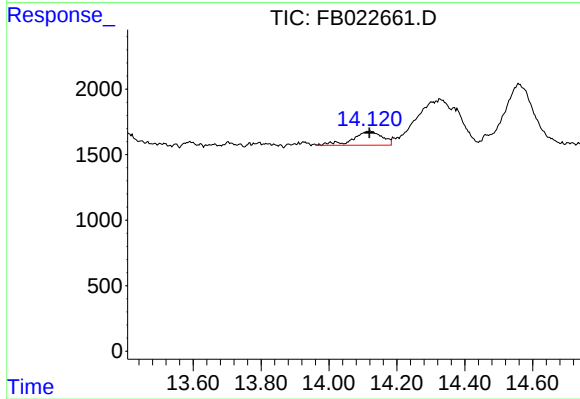

#9 O-Xylene

R.T.: 14.121 min
Delta R.T.: 0.002 min
Response: 6341
Conc: 0.18 ng/ml

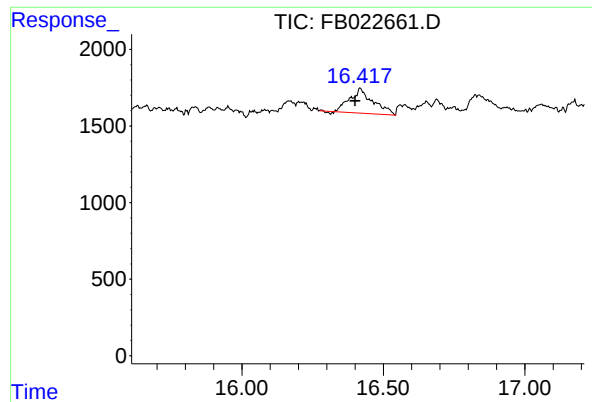

#10 1,2,4-Trimethylbenzene

R.T.: 16.419 min
Delta R.T.: 0.019 min
Response: 9041
Conc: 0.36 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF1002S1