

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100219\
 Data File : FB022671.D
 Signal(s) : FID2B.CH
 Acq On : 2 Oct 2019 18:43
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO STD

Integration File: Calibration.e
 Quant Time: Oct 03 02:04:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
 Quant Title :
 QLast Update : Wed Oct 02 06:15:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.971	507400	21.059 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.835	1037812	31.120 ng/ml
2) t 2,2,4-Trimethylpentane	7.589	1103902	31.825 ng/ml
3) t n-Heptane	7.929	360893	10.658 ng/ml
4) t Benzene	8.064	438995	10.541 ng/ml
6) t Toluene	10.813	1252595	30.945 ng/ml
7) t Ethylbenzene	13.259	397009	10.258 ng/ml
8) t m-Xylene	13.392	749155	20.204 ng/ml
9) t O-Xylene	14.122	708016	20.279 ng/ml
10) t 1,2,4-Trimethylbenzene	16.404	510337	20.597 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100219\
Data File : FB022671.D
Signal(s) : FID2B.CH
Acq On : 2 Oct 2019 18:43
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

Integration File: Calibration.e
Quant Time: Oct 03 02:04:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
Quant Title :
QLast Update : Wed Oct 02 06:15:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

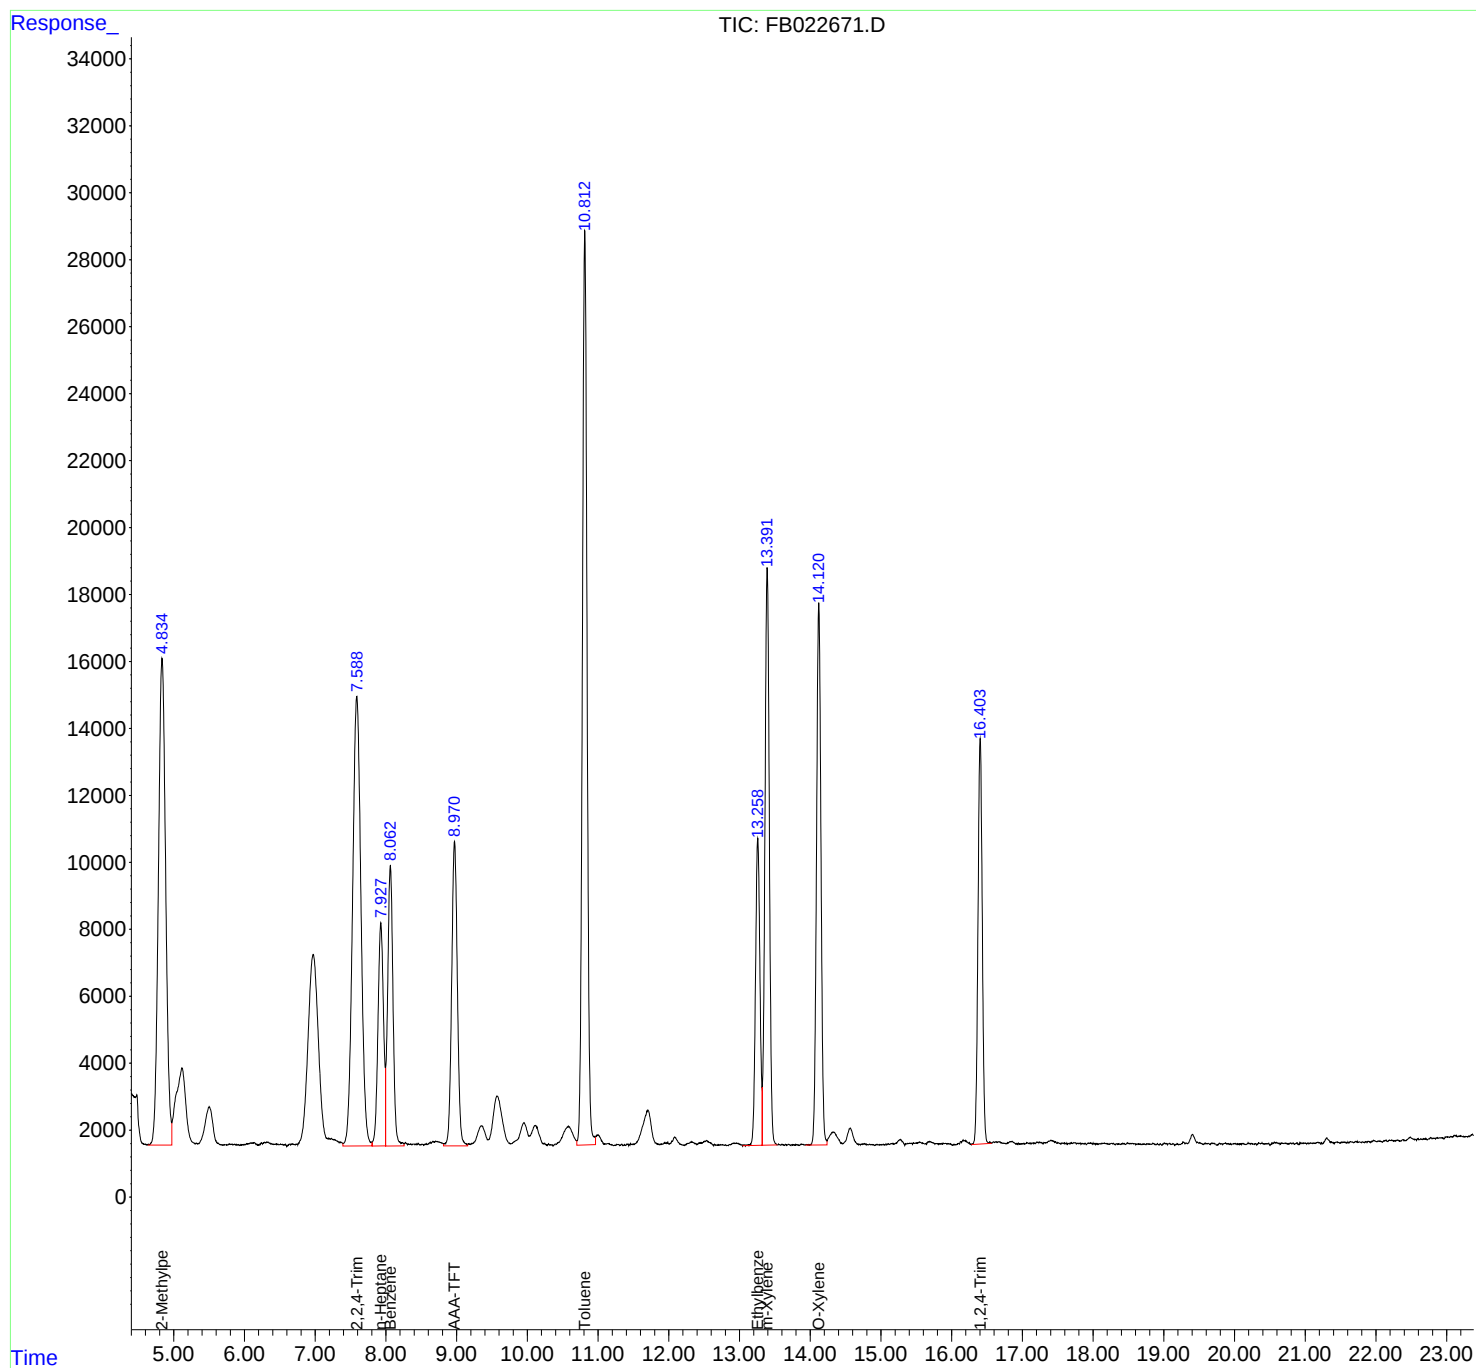


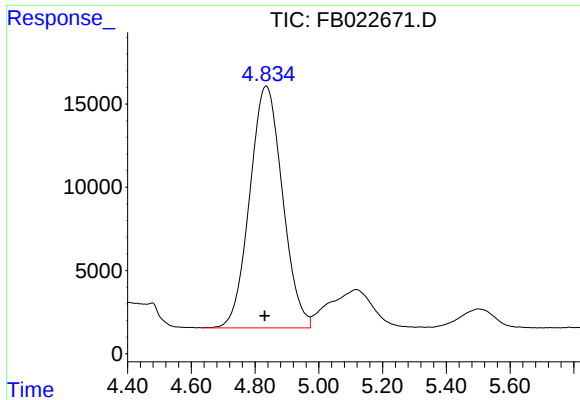

#1 2-Methylpentane


R.T.: 4.835 min
Delta R.T.: 0.005 min
Response: 1037812
Conc: 31.12 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

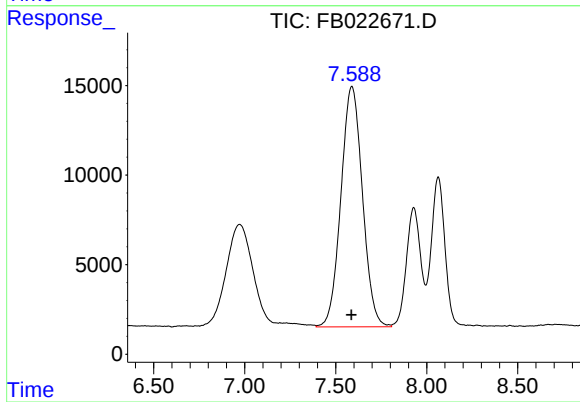


#2 2,2,4-Trimethylpentane

R.T.: 7.589 min
Delta R.T.: 0.003 min
Response: 1103902
Conc: 31.83 ng/ml

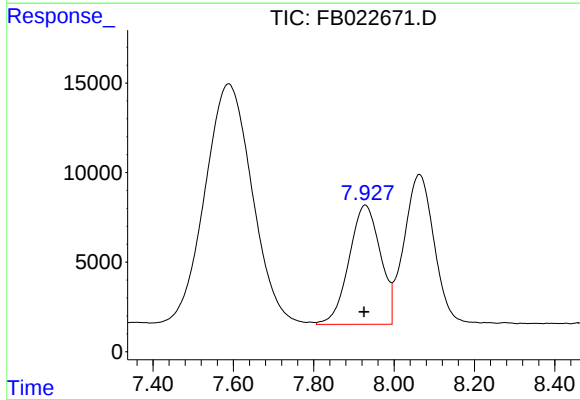


#3 n-Heptane

R.T.: 7.929 min
Delta R.T.: 0.003 min
Response: 360893
Conc: 10.66 ng/ml

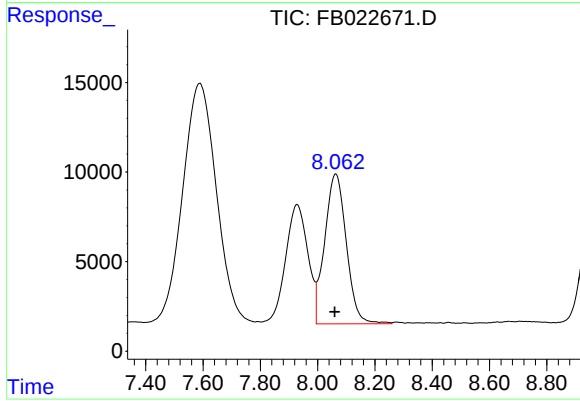

#4 Benzene


R.T.: 8.064 min
Delta R.T.: 0.003 min
Response: 438995
Conc: 10.54 ng/ml

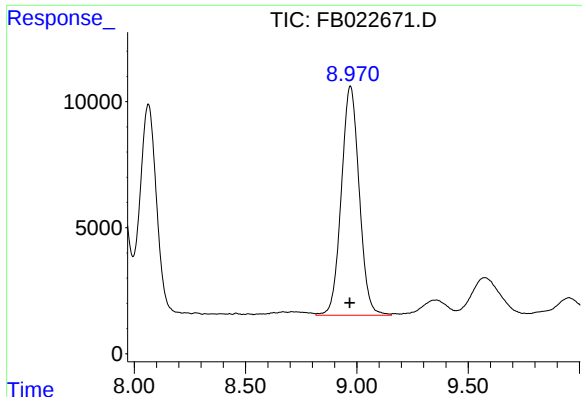

#5 AAA-TFT


R.T.: 8.971 min
Delta R.T.: 0.003 min
Response: 507400
Conc: 21.06 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

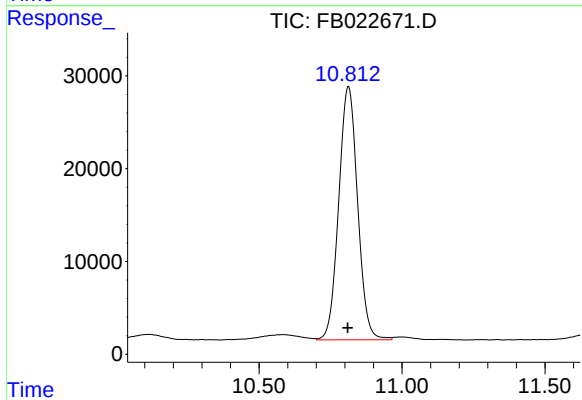


#6 Toluene

R.T.: 10.813 min
Delta R.T.: 0.003 min
Response: 1252595
Conc: 30.95 ng/ml

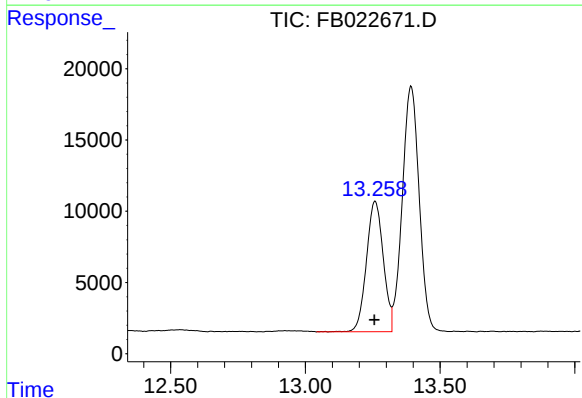


#7 Ethylbenzene

R.T.: 13.259 min
Delta R.T.: 0.003 min
Response: 397009
Conc: 10.26 ng/ml

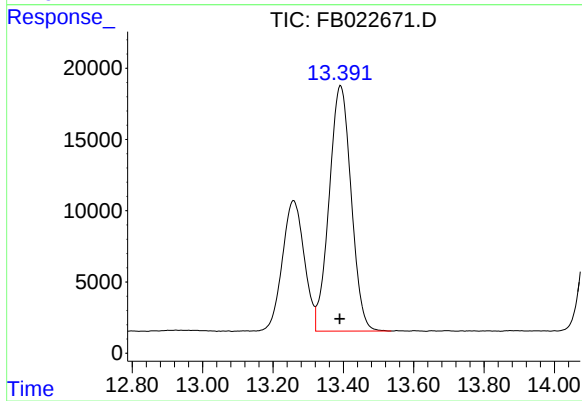

#8 m-Xylene


R.T.: 13.392 min
Delta R.T.: 0.003 min
Response: 749155
Conc: 20.20 ng/ml

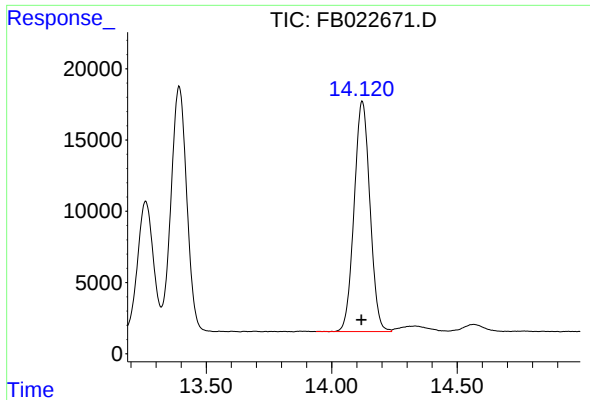

#9 O-Xylene

R.T.: 14.122 min
Delta R.T.: 0.003 min
Response: 708016
Conc: 20.28 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

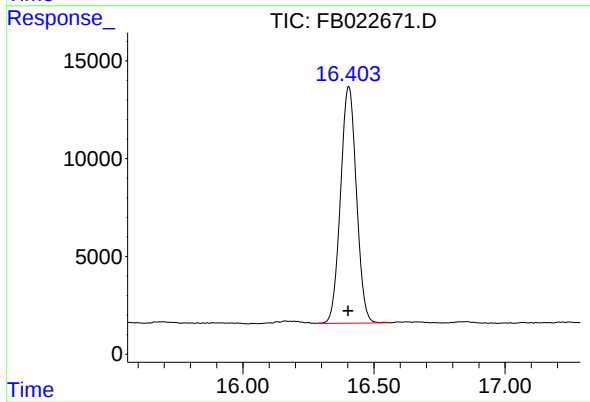

#10 1,2,4-Trimethylbenzene

R.T.: 16.404 min
Delta R.T.: 0.004 min
Response: 510337
Conc: 20.60 ng/ml