

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100219\
 Data File : FB022662.D
 Signal(s) : FID2B.CH
 Acq On : 2 Oct 2019 14:11
 Operator : DD/AJ
 Sample : BSF1002S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1002S1

Integration File: Calibration.e
 Quant Time: Oct 03 02:02:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
 Quant Title :
 QLast Update : Wed Oct 02 06:15:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.970	515799	21.408 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.832	1046215	31.372 ng/ml
2) t 2,2,4-Trimethylpentane	7.587	1156403	33.339 ng/ml
3) t n-Heptane	7.927	373031	11.016 ng/ml
4) t Benzene	8.061	435126	10.448 ng/ml
6) t Toluene	10.811	1254766	30.999 ng/ml
7) t Ethylbenzene	13.258	399509	10.323 ng/ml
8) t m-Xylene	13.391	747271	20.153 ng/ml
9) t O-Xylene	14.120	697870	19.988 ng/ml
10) t 1,2,4-Trimethylbenzene	16.402	519593	20.971 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100219\
Data File : FB022662.D
Signal(s) : FID2B.CH
Acq On : 2 Oct 2019 14:11
Operator : DD/AJ
Sample : BSF1002S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1002S1

Integration File: Calibration.e
Quant Time: Oct 03 02:02:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
Quant Title :
QLast Update : Wed Oct 02 06:15:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

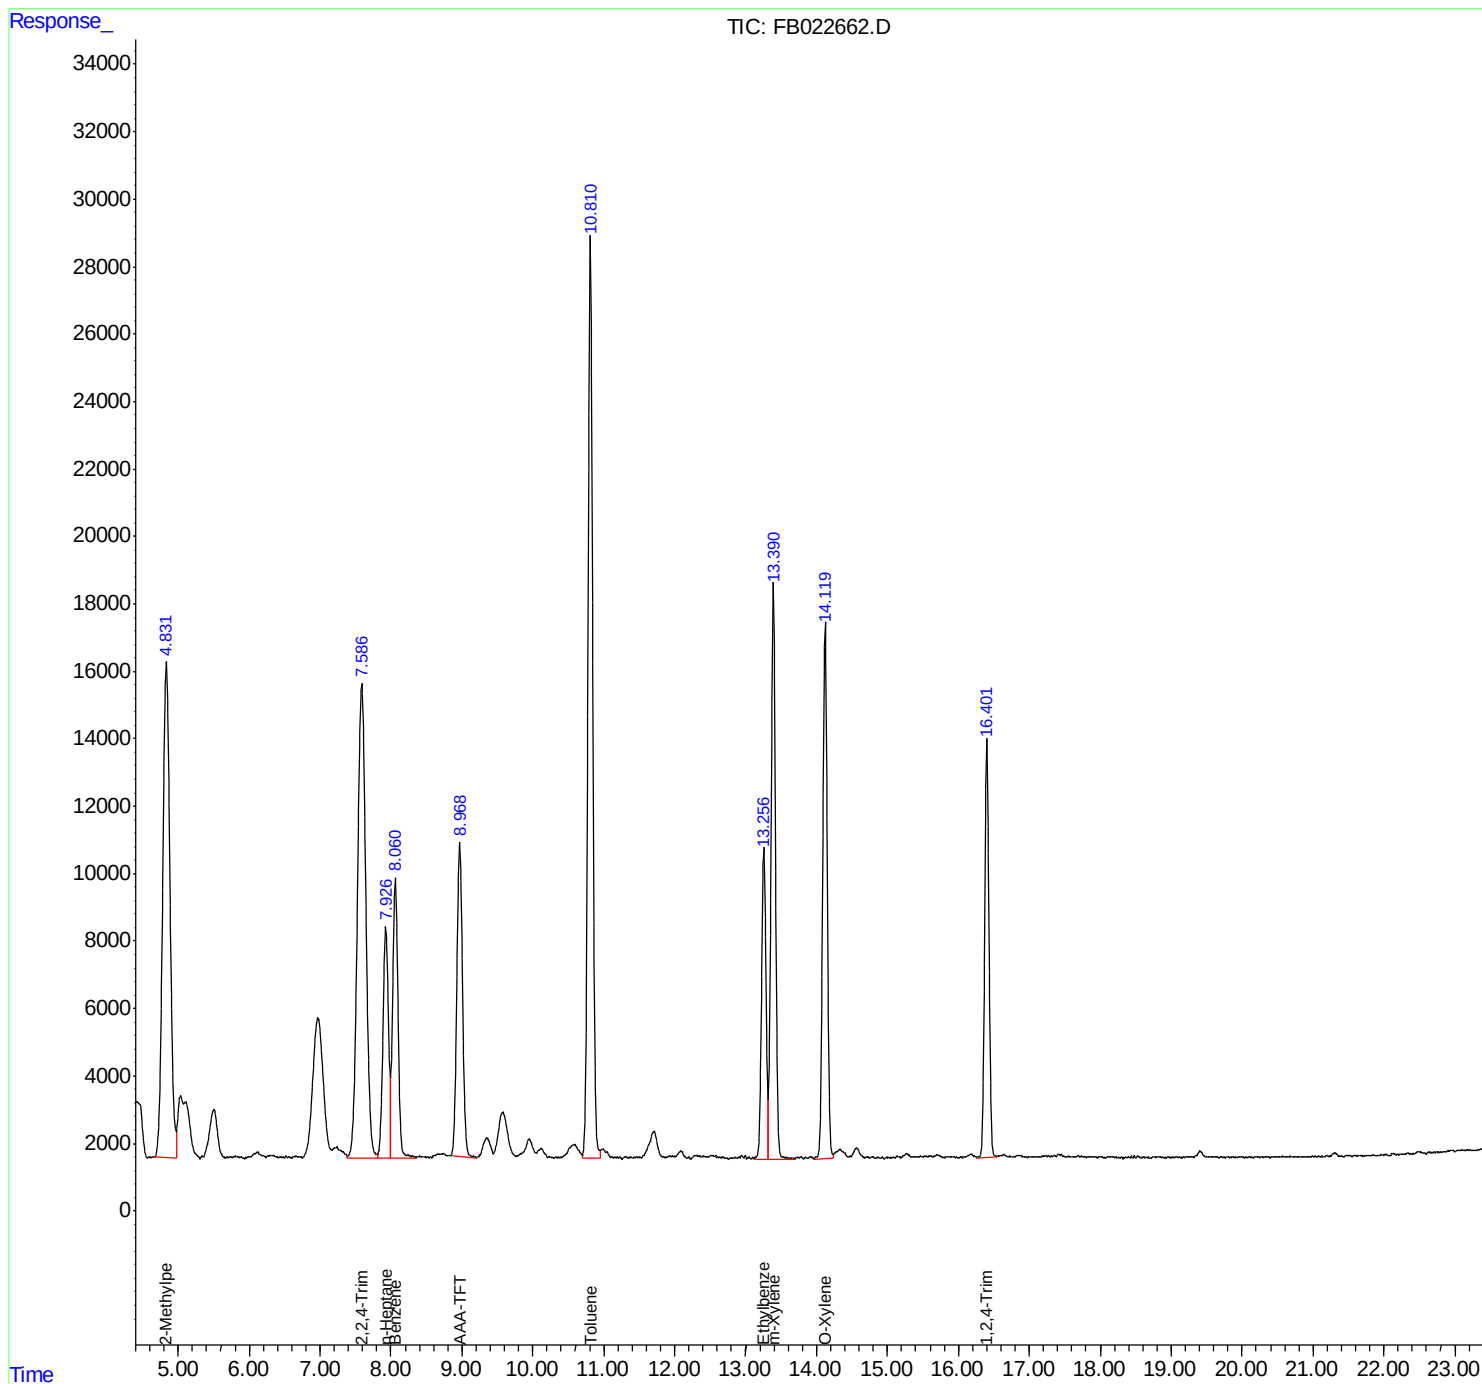


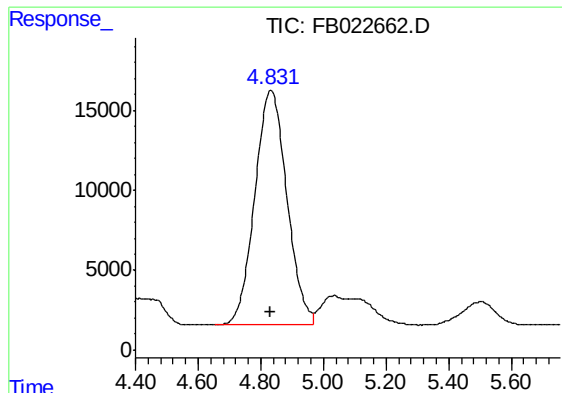

#1 2-Methylpentane


R.T.: 4.832 min
Delta R.T.: 0.002 min
Response: 1046215
Conc: 31.37 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1002S1

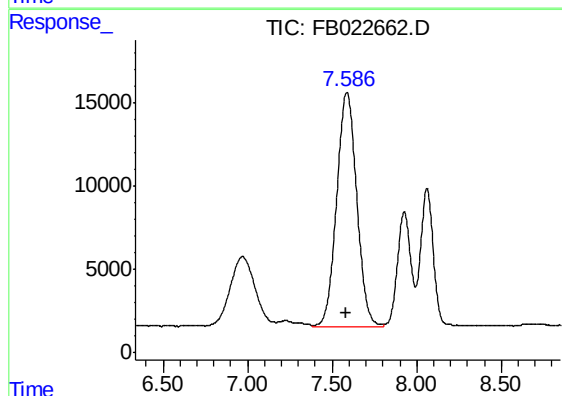


#2 2,2,4-Trimethylpentane

R.T.: 7.587 min
Delta R.T.: 0.001 min
Response: 1156403
Conc: 33.34 ng/ml

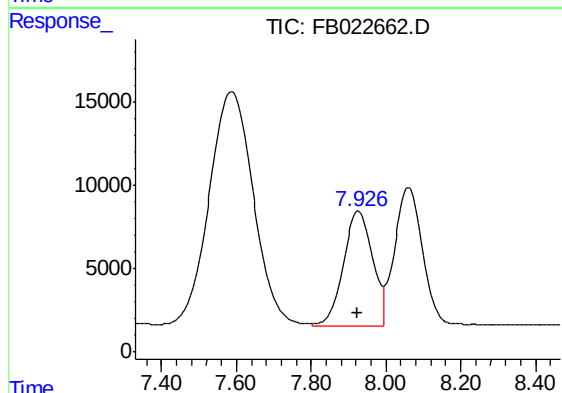


#3 n-Heptane

R.T.: 7.927 min
Delta R.T.: 0.001 min
Response: 373031
Conc: 11.02 ng/ml

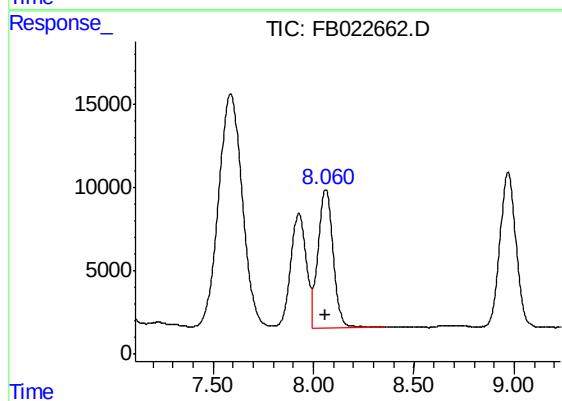

#4 Benzene


R.T.: 8.061 min
Delta R.T.: 0.000 min
Response: 435126
Conc: 10.45 ng/ml

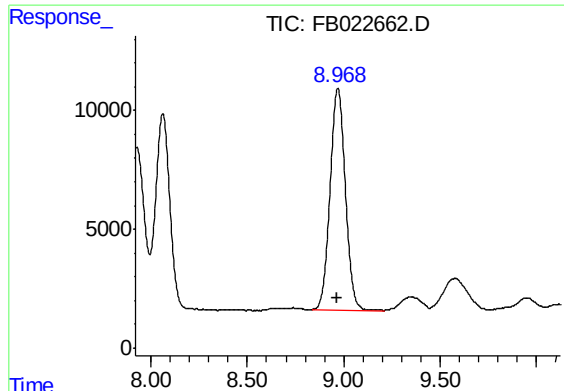

#5 AAA-TFT


R.T.: 8.970 min
Delta R.T.: 0.001 min
Response: 515799
Conc: 21.41 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1002S1

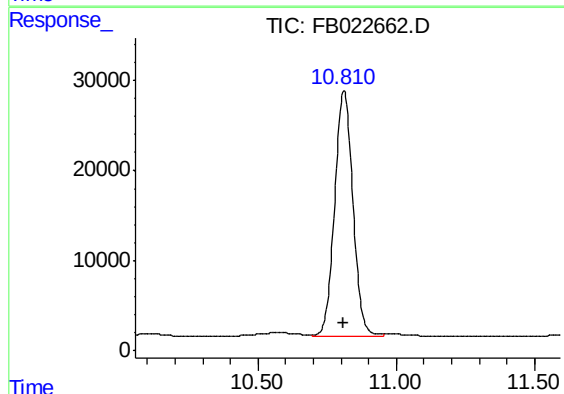


#6 Toluene

R.T.: 10.811 min
Delta R.T.: 0.001 min
Response: 1254766
Conc: 31.00 ng/ml

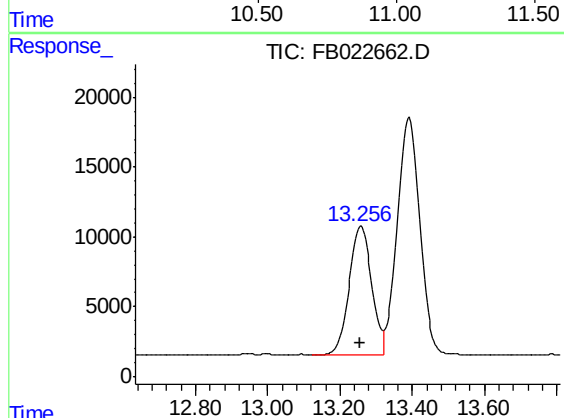


#7 Ethylbenzene

R.T.: 13.258 min
Delta R.T.: 0.002 min
Response: 399509
Conc: 10.32 ng/ml

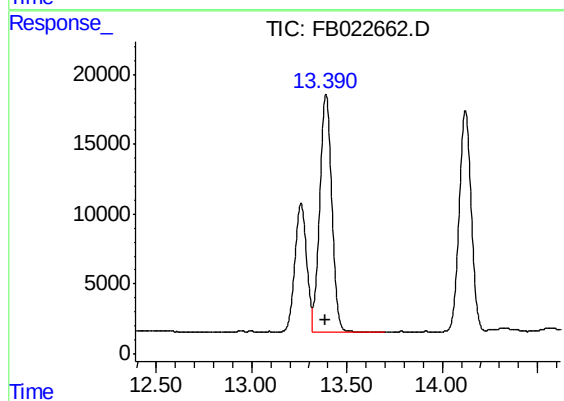

#8 m-Xylene


R.T.: 13.391 min
Delta R.T.: 0.002 min
Response: 747271
Conc: 20.15 ng/ml

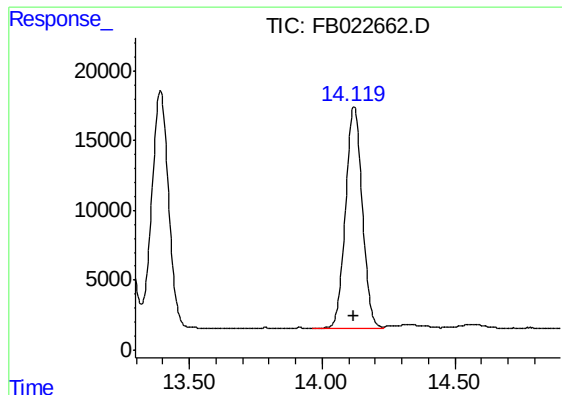

#9 O-Xylene

R.T.: 14.120 min
Delta R.T.: 0.001 min
Response: 697870
Conc: 19.99 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1002S1

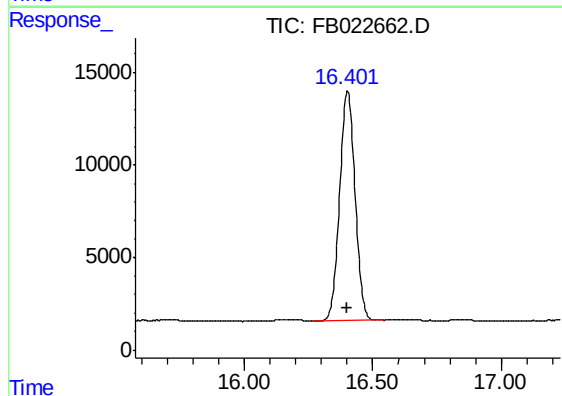

#10 1,2,4-Trimethylbenzene

R.T.: 16.402 min
Delta R.T.: 0.002 min
Response: 519593
Conc: 20.97 ng/ml