

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100220\
 Data File : FB025003.D
 Signal(s) : FID2B.CH
 Acq On : 2 Oct 2020 11:11
 Operator : DD/AJ
 Sample : L4221-02MS
 Misc : 5.05/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 03 01:07:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	395704	18.848 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	745596	24.792 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	738796	24.172 ng/ml
3) t n-Heptane	7.758	240288	7.899 ng/ml
4) t Benzene	7.892	347988	9.342 ng/ml
6) t Toluene	10.631	966036	27.673 ng/ml
7) t Ethylbenzene	13.070	293584	9.057 ng/ml
8) t m-Xylene	13.203	580240	18.266 ng/ml
9) t O-Xylene	13.931	560830	18.456 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	454961	17.938 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100220\
Data File : FB025003.D
Signal(s) : FID2B.CH
Acq On : 2 Oct 2020 11:11
Operator : DD/AJ
Sample : L4221-02MS
Misc : 5.05/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 03 01:07:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

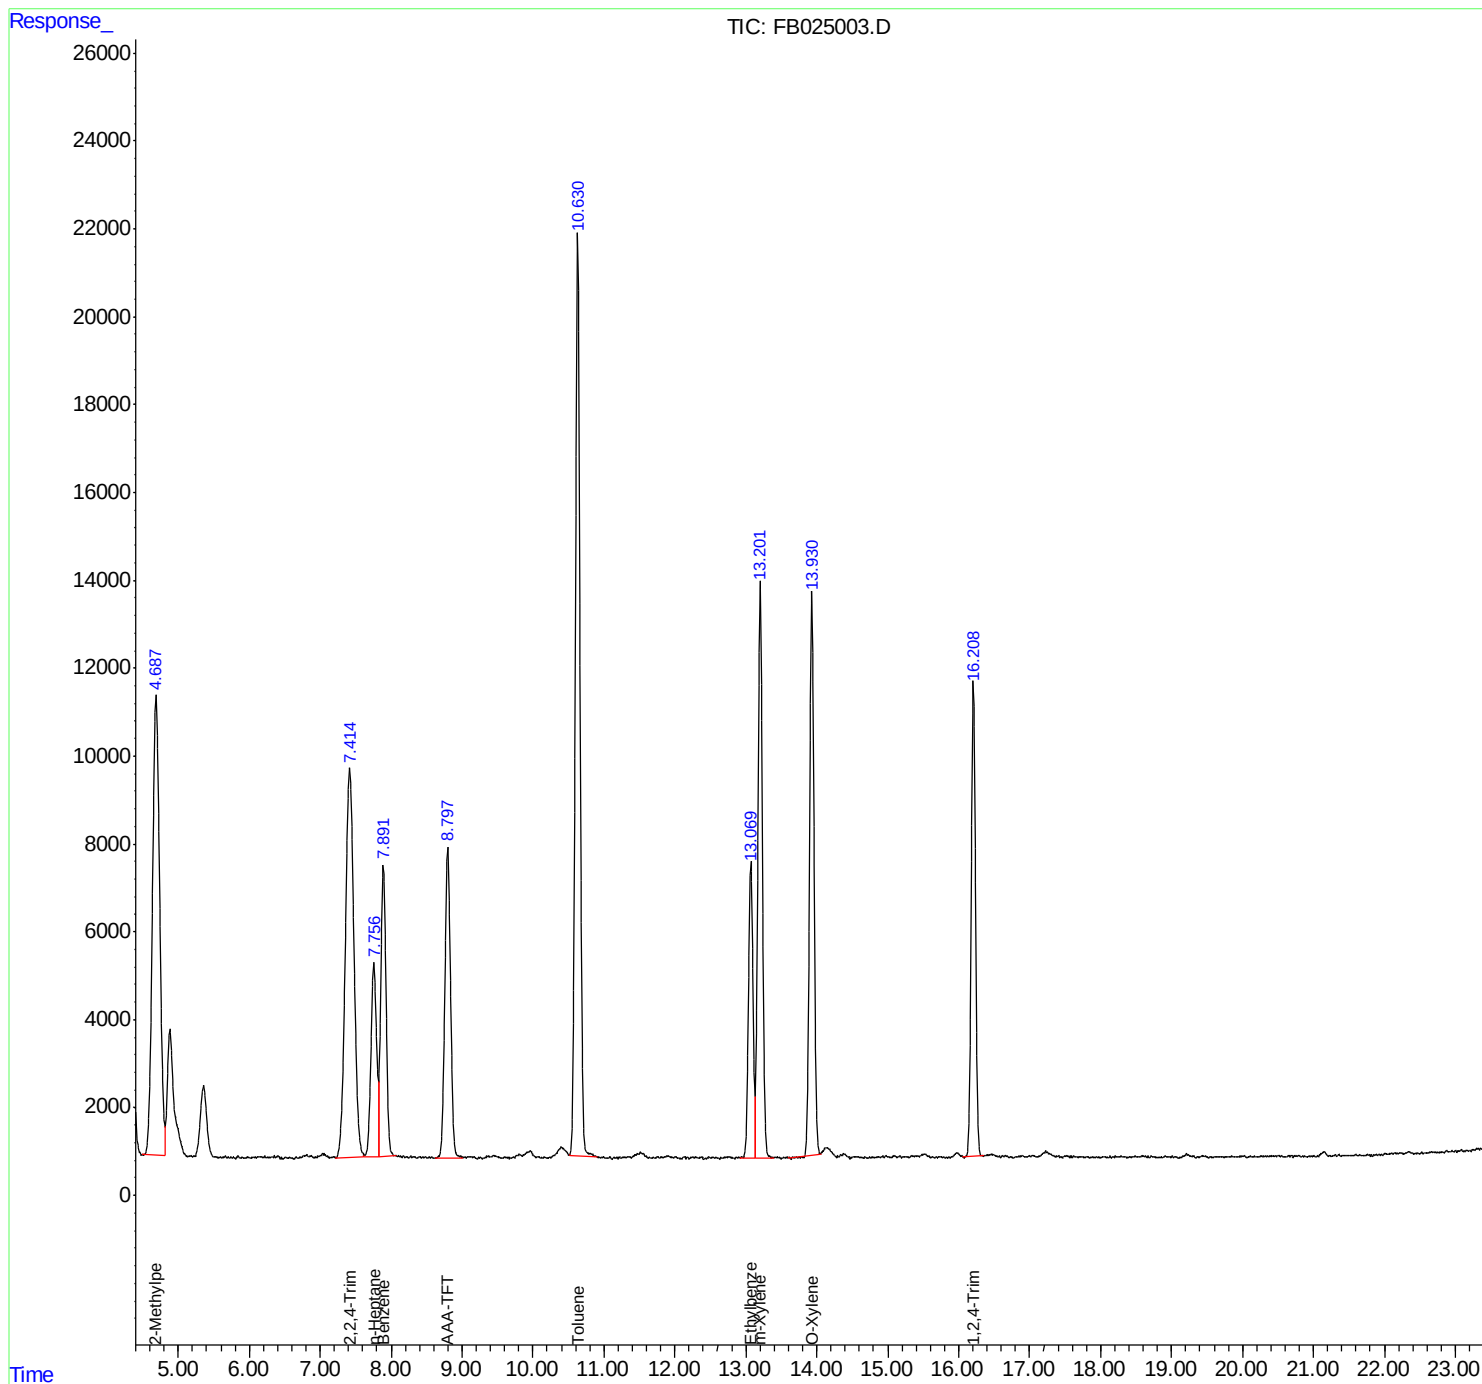

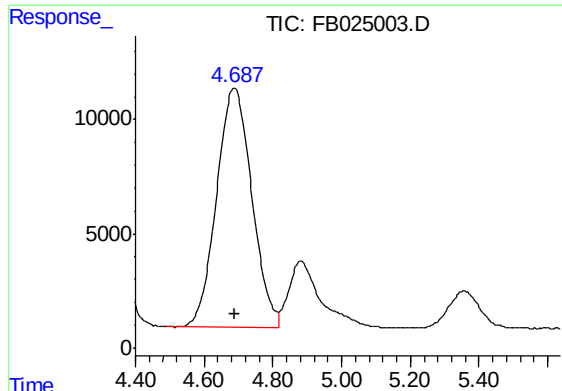


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: -0.001 min
Response: 745596
Conc: 24.79 ng/ml

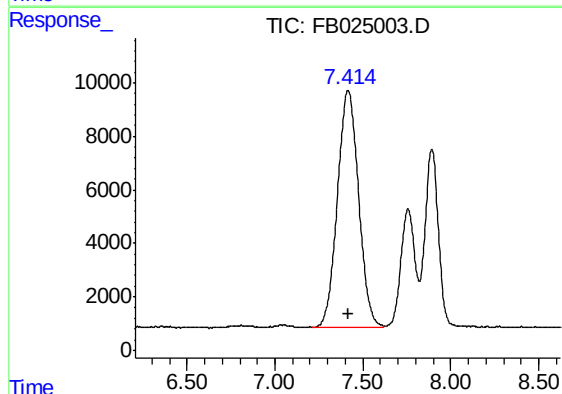


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 738796
Conc: 24.17 ng/ml

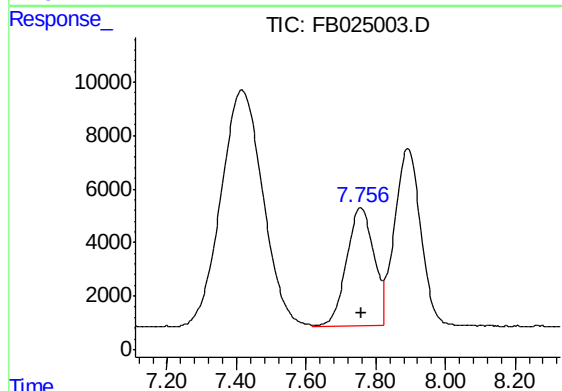


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.001 min
Response: 240288
Conc: 7.90 ng/ml

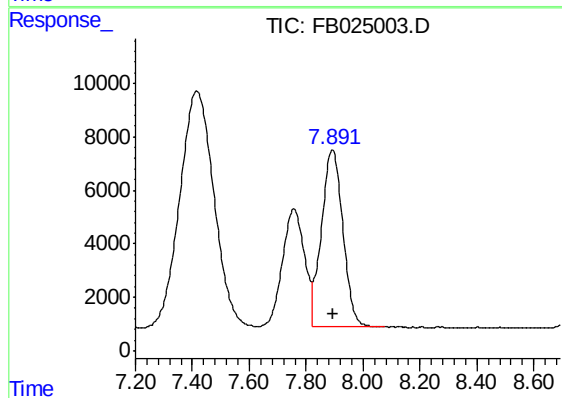


#4 Benzene

R.T.: 7.892 min
Delta R.T.: -0.002 min
Response: 347988
Conc: 9.34 ng/ml

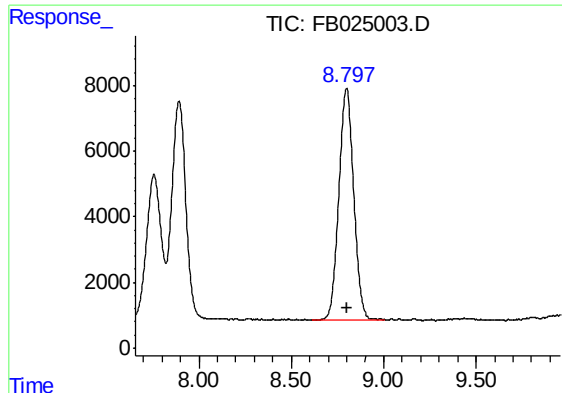


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: -0.002 min
Response: 395704
Conc: 18.85 ng/ml

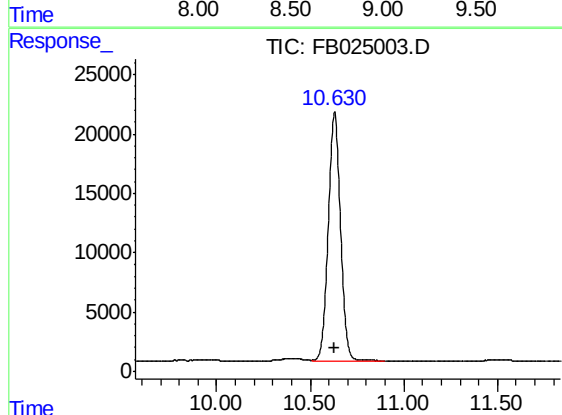


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 966036
Conc: 27.67 ng/ml

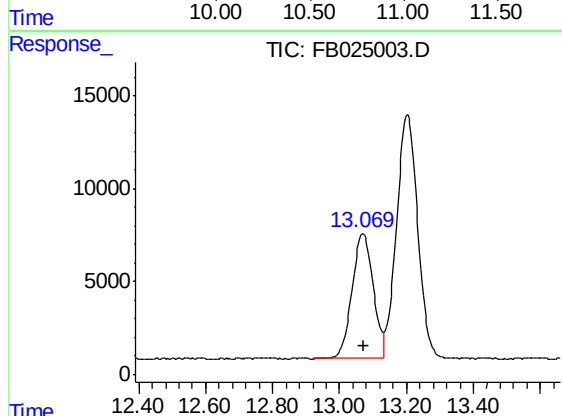


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 293584
Conc: 9.06 ng/ml

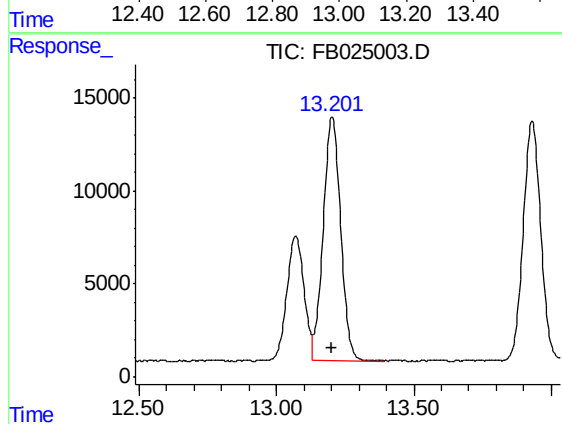


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: -0.001 min
Response: 580240
Conc: 18.27 ng/ml

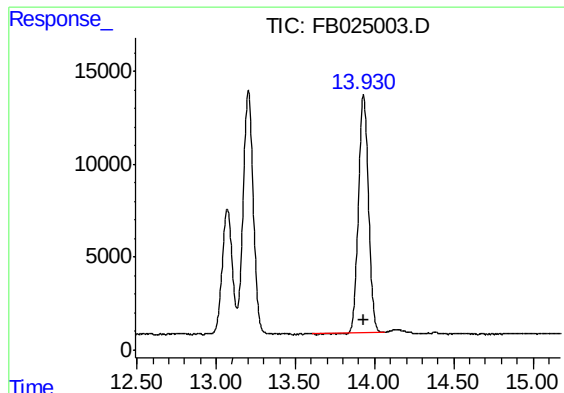

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: -0.001 min
Response: 560830
Conc: 18.46 ng/ml

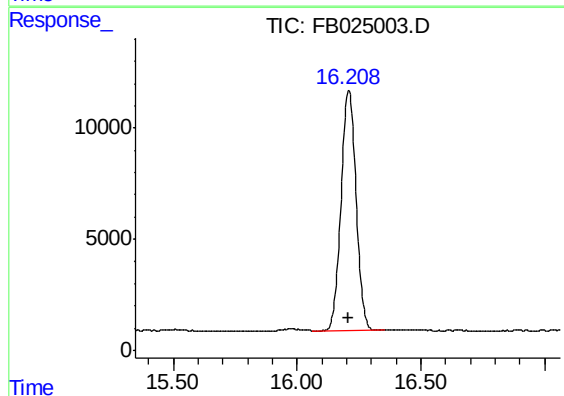

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 454961
Conc: 17.94 ng/ml