

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100220\
 Data File : FB025000.D
 Signal(s) : FID2B.CH
 Acq On : 2 Oct 2020 9:39
 Operator : DD/AJ
 Sample : BSF1002S1
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 03 01:06:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	405382	19.309 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	826605	27.486 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	886542	29.006 ng/ml
3) t n-Heptane	7.757	289962	9.531 ng/ml
4) t Benzene	7.892	354513	9.517 ng/ml
6) t Toluene	10.631	993445	28.458 ng/ml
7) t Ethylbenzene	13.071	315577	9.735 ng/ml
8) t m-Xylene	13.204	620670	19.539 ng/ml
9) t O-Xylene	13.931	609194	20.047 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	505718	19.939 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100220\
Data File : FB025000.D
Signal(s) : FID2B.CH
Acq On : 2 Oct 2020 9:39
Operator : DD/AJ
Sample : BSF1002S1
Misc : 5.02/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 03 01:06:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

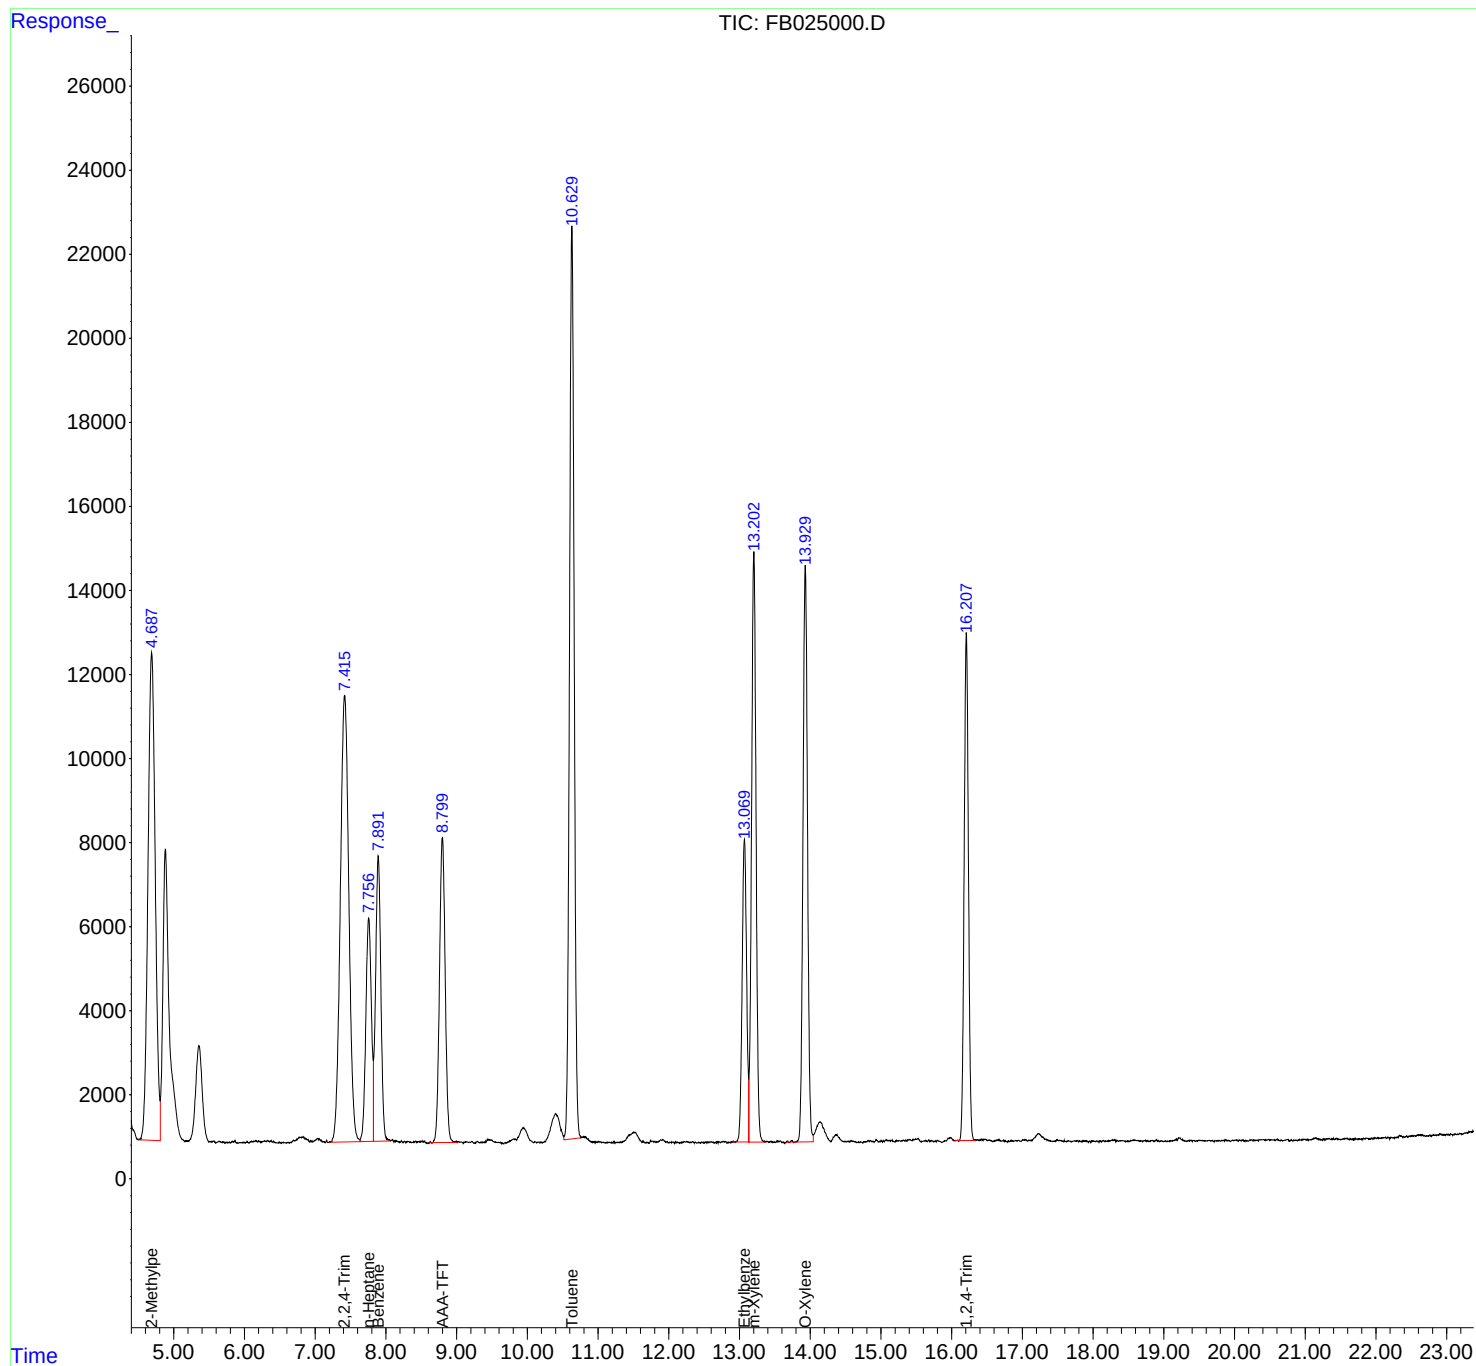

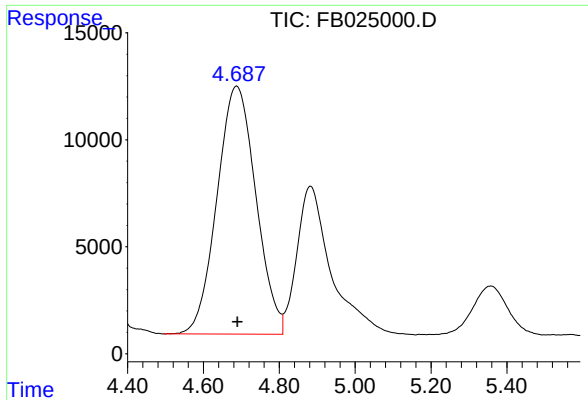


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.002 min
Response: 826605
Conc: 27.49 ng/ml

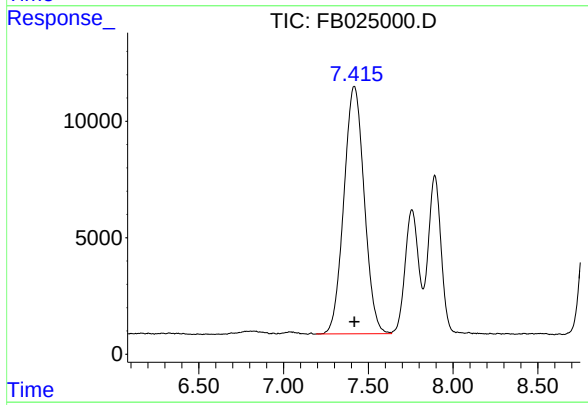


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.001 min
Response: 886542
Conc: 29.01 ng/ml

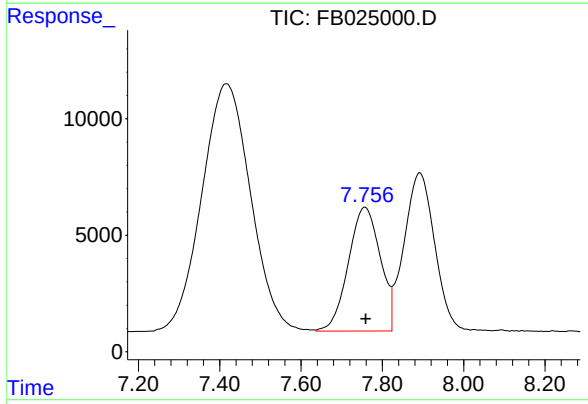


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.002 min
Response: 289962
Conc: 9.53 ng/ml

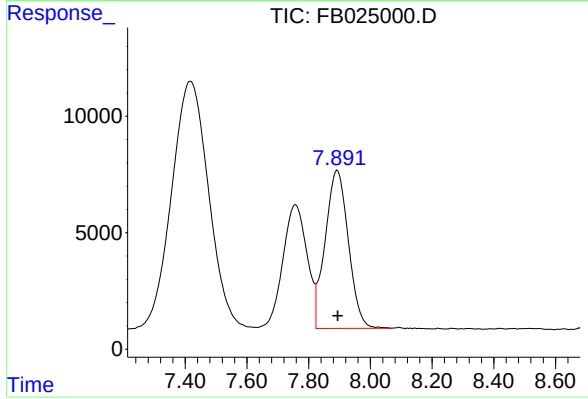


#4 Benzene

R.T.: 7.892 min
Delta R.T.: -0.002 min
Response: 354513
Conc: 9.52 ng/ml

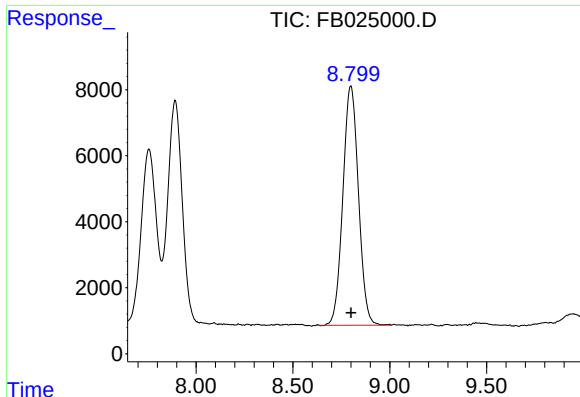


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: -0.001 min
Response: 405382
Conc: 19.31 ng/ml

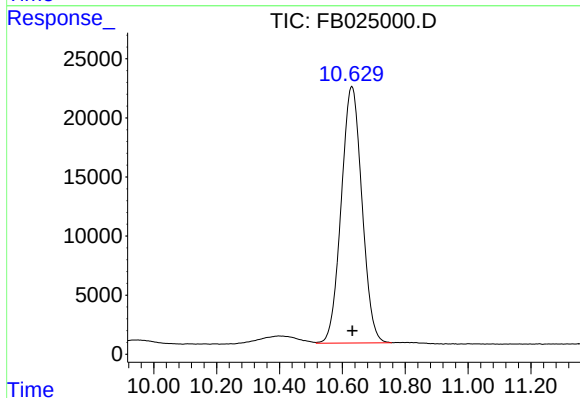


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 993445
Conc: 28.46 ng/ml

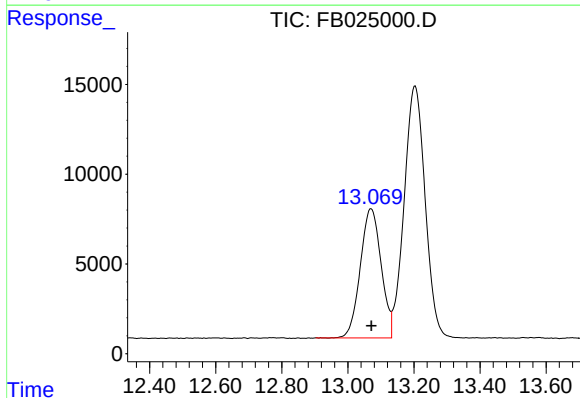


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 315577
Conc: 9.74 ng/ml

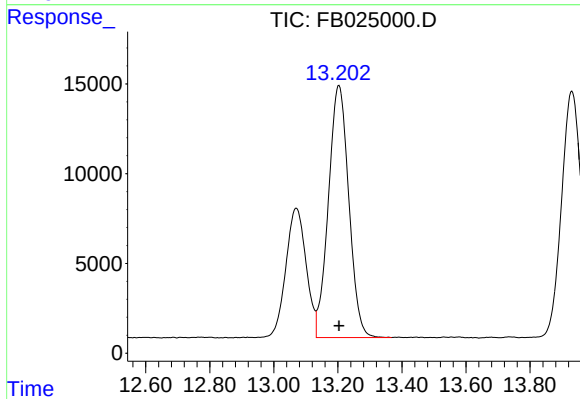


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 620670
Conc: 19.54 ng/ml

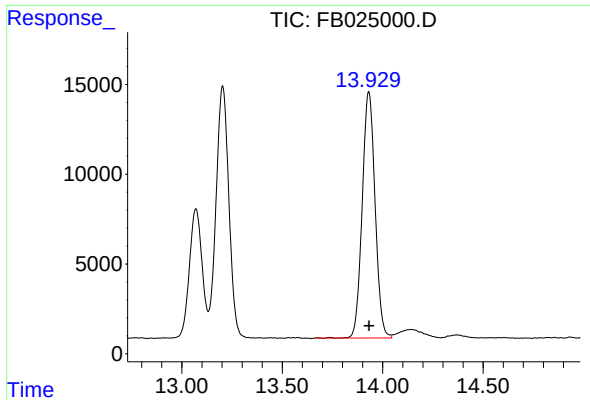

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 609194
Conc: 20.05 ng/ml

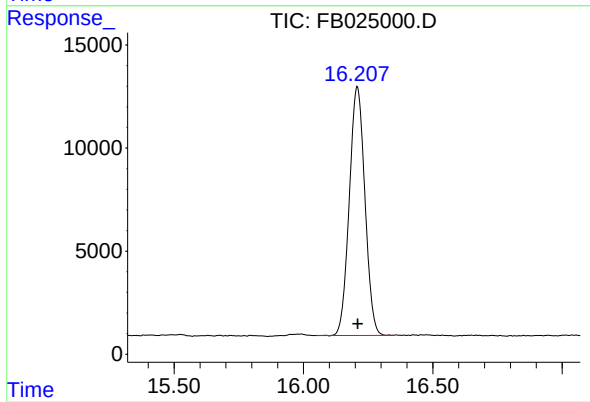

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.001 min
Response: 505718
Conc: 19.94 ng/ml