

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100220\
 Data File : FB025004.D
 Signal(s) : FID2B.CH
 Acq On : 2 Oct 2020 11:42
 Operator : DD/AJ
 Sample : L4221-02MSD
 Misc : 5.04/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 03 01:07:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	443664	21.133 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	715312	23.785 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	620359	20.297 ng/ml
3) t n-Heptane	7.759	199942	6.572 ng/ml
4) t Benzene	7.893	349778	9.390 ng/ml
6) t Toluene	10.631	943792	27.035 ng/ml
7) t Ethylbenzene	13.071	282245	8.707 ng/ml
8) t m-Xylene	13.204	555646	17.492 ng/ml
9) t O-Xylene	13.931	542118	17.840 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	417459	16.459 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100220\
Data File : FB025004.D
Signal(s) : FID2B.CH
Acq On : 2 Oct 2020 11:42
Operator : DD/AJ
Sample : L4221-02MSD
Misc : 5.04/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 03 01:07:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

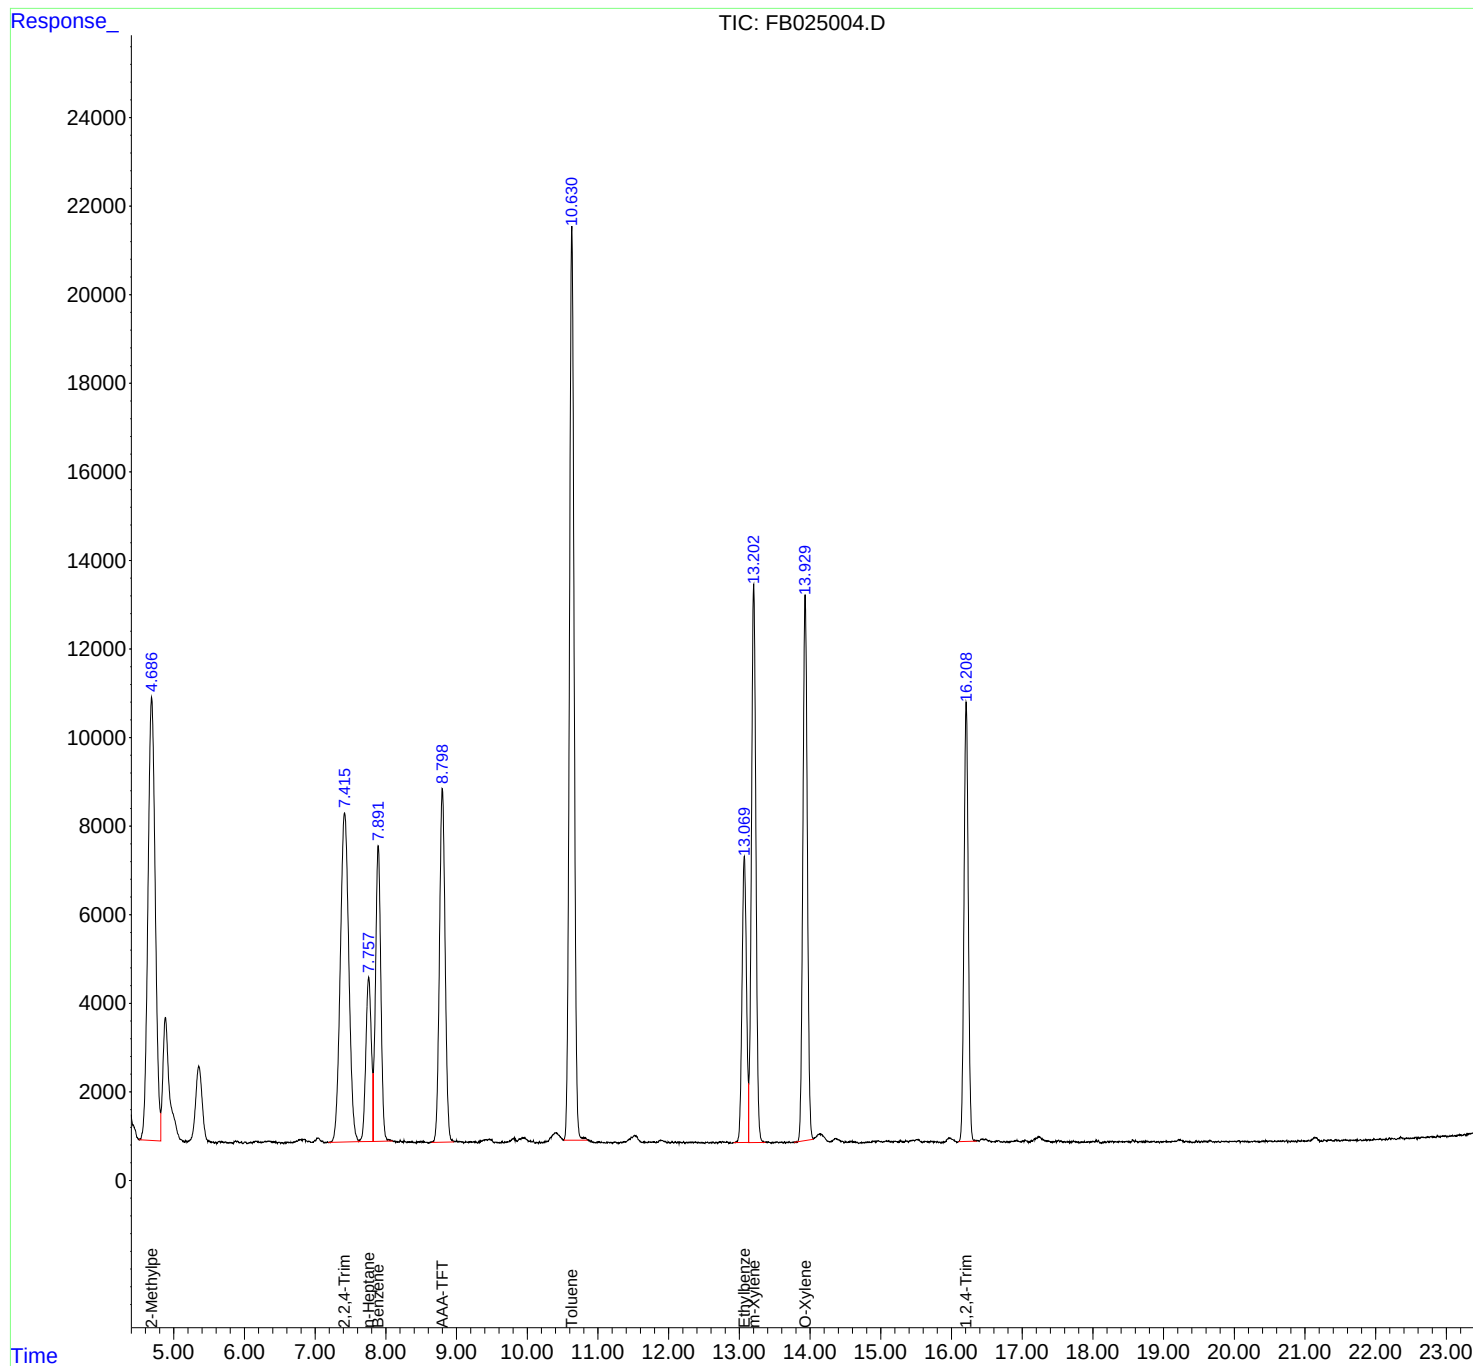

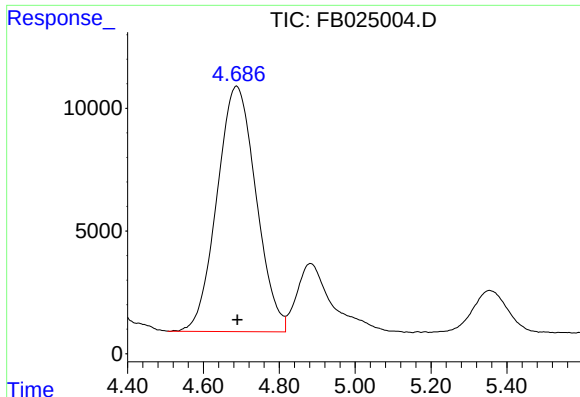


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.002 min
Response: 715312
Conc: 23.79 ng/ml

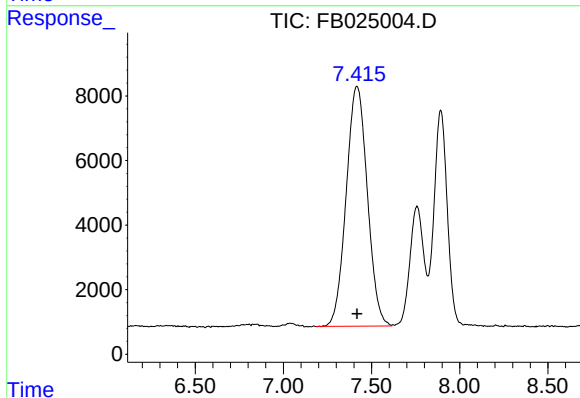


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 620359
Conc: 20.30 ng/ml

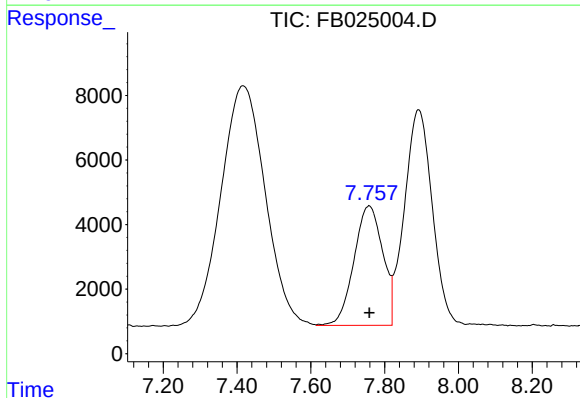


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 199942
Conc: 6.57 ng/ml

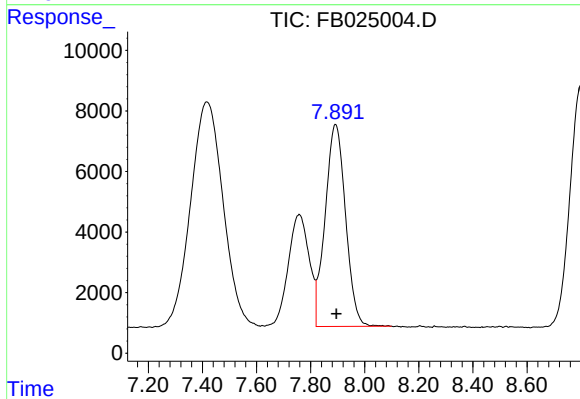


#4 Benzene

R.T.: 7.893 min
Delta R.T.: -0.002 min
Response: 349778
Conc: 9.39 ng/ml

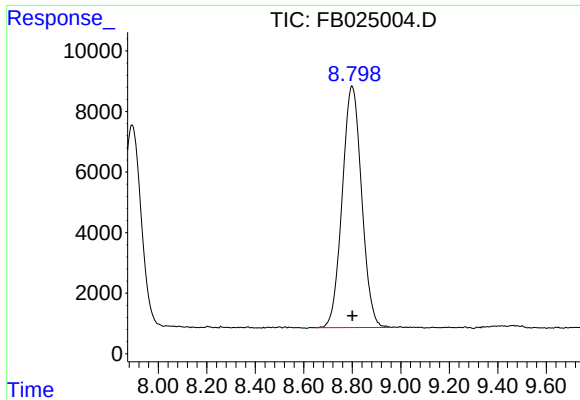


#5 AAA-TFT

R.T.: 8.799 min
 Delta R.T.: -0.001 min
 Response: 443664
 Conc: 21.13 ng/ml

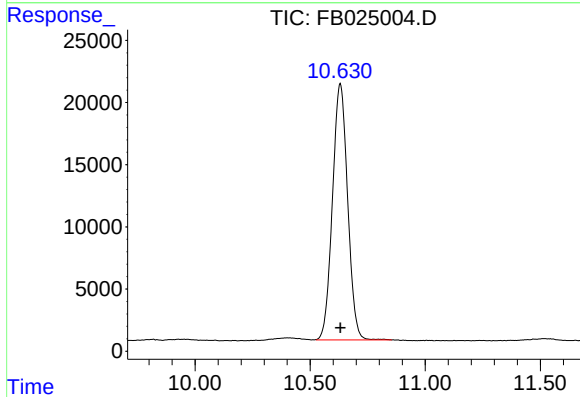


#6 Toluene

R.T.: 10.631 min
 Delta R.T.: 0.000 min
 Response: 943792
 Conc: 27.04 ng/ml

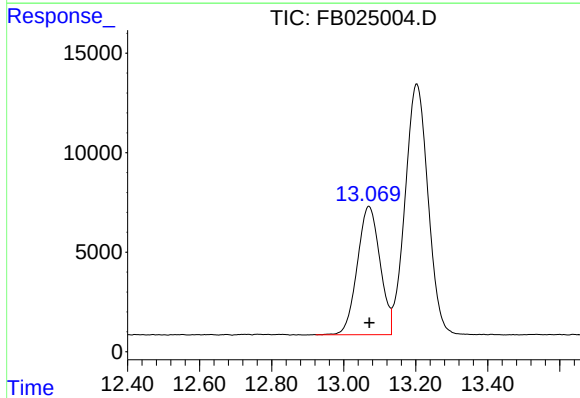


#7 Ethylbenzene

R.T.: 13.071 min
 Delta R.T.: 0.000 min
 Response: 282245
 Conc: 8.71 ng/ml

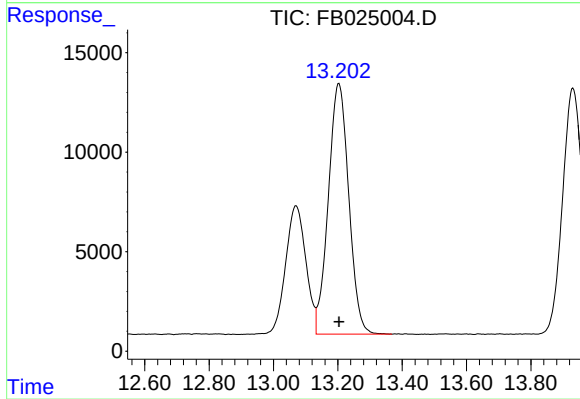

#8 m-Xylene

R.T.: 13.204 min
 Delta R.T.: 0.000 min
 Response: 555646
 Conc: 17.49 ng/ml

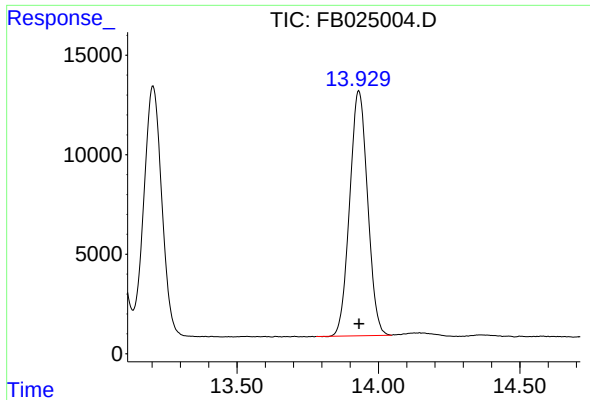


#9 O-Xylene

R.T.: 13.931 min

Delta R.T.: 0.000 min

Response: 542118

Conc: 17.84 ng/ml

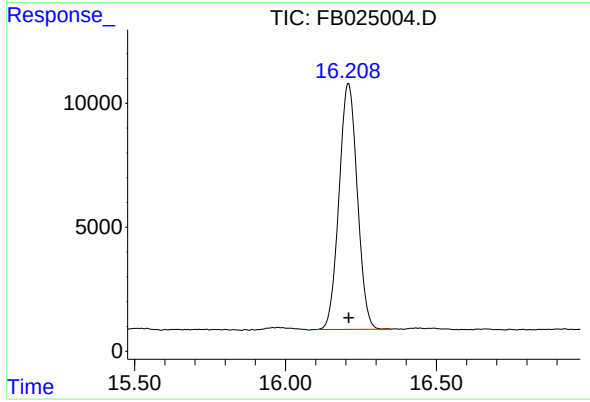

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min

Delta R.T.: 0.000 min

Response: 417459

Conc: 16.46 ng/ml