

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100223\
Data File : FB030363.D
Signal(s) : FID2B.CH
Acq On : 2 Oct 2023 15:00
Operator : YP/AJ
Sample : BSF1002S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1002S2

Integration File: Calibration.e
Quant Time: Oct 03 00:29:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
Quant Title :
QLast Update : Mon Sep 18 13:44:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	277209	20.041 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	542720	29.649 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	619716	30.633 ng/ml
3) t n-Heptane	7.750	209320	9.852 ng/ml
4) t Benzene	7.886	258335	10.148 ng/ml
6) t Toluene	10.618	750956	30.298 ng/ml
7) t Ethylbenzene	13.054	235845	10.131 ng/ml
8) t m-Xylene	13.187	466614	20.344 ng/ml
9) t O-Xylene	13.913	449771	20.256 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	423246	19.316 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100223\
Data File : FB030363.D
Signal(s) : FID2B.CH
Acq On : 2 Oct 2023 15:00
Operator : YP/AJ
Sample : BSF1002S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1002S2

Integration File: Calibration.e
Quant Time: Oct 03 00:29:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
Quant Title :
QLast Update : Mon Sep 18 13:44:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

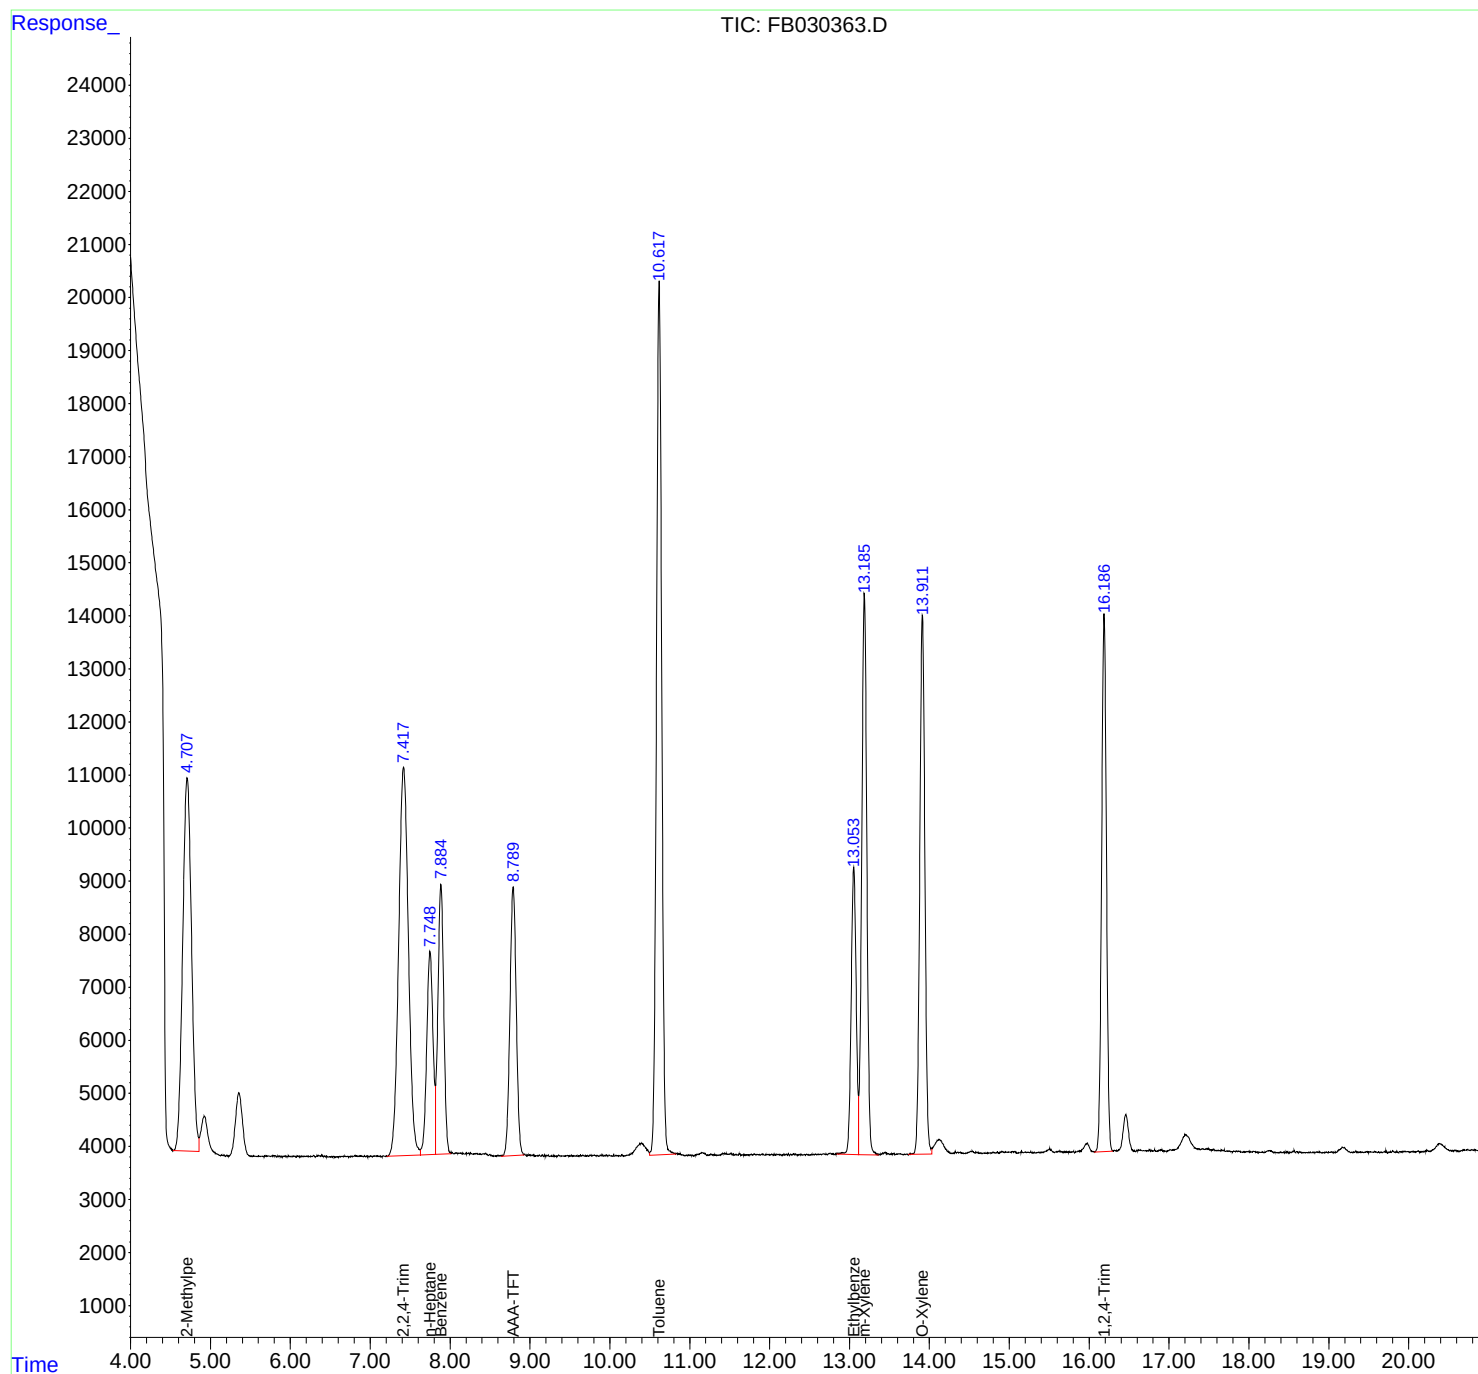


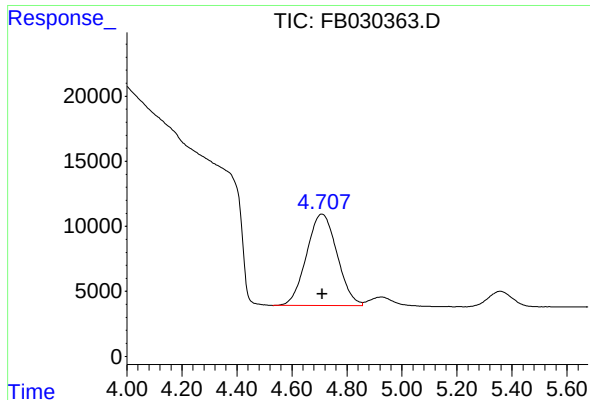

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: -0.002 min
Response: 542720
Conc: 29.65 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1002S2

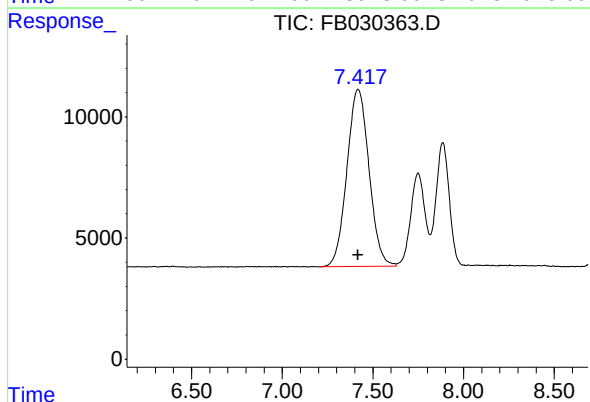


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 619716
Conc: 30.63 ng/ml

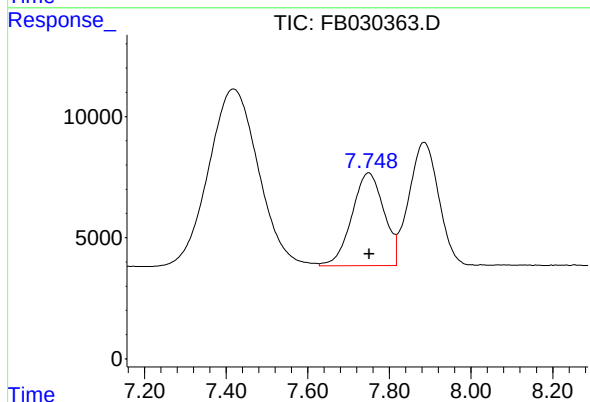


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 209320
Conc: 9.85 ng/ml

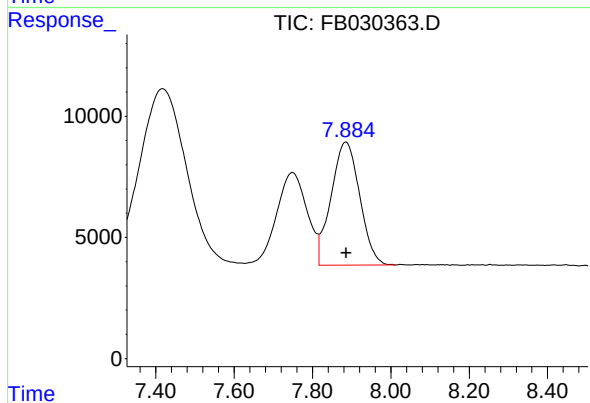

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.001 min
Response: 258335
Conc: 10.15 ng/ml

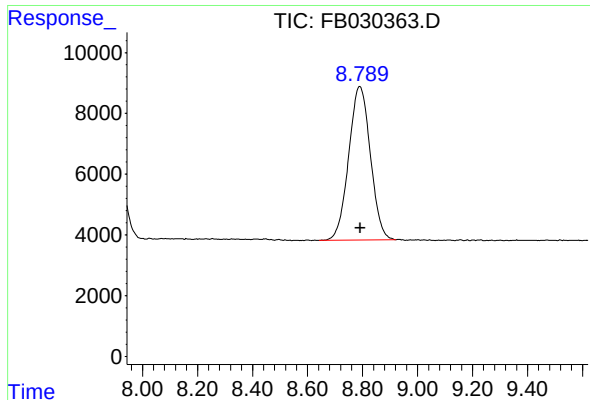

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.002 min
Response: 277209
Conc: 20.04 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1002S2

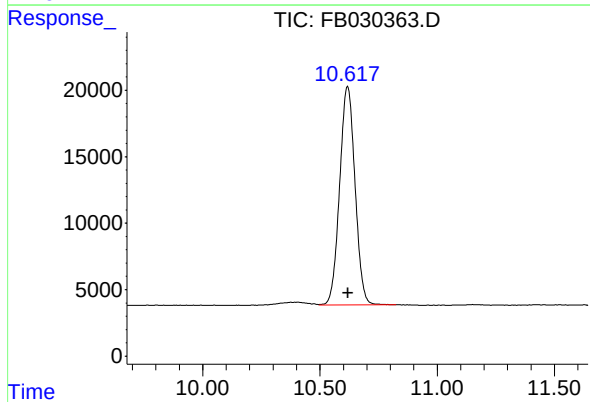


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.002 min
Response: 750956
Conc: 30.30 ng/ml

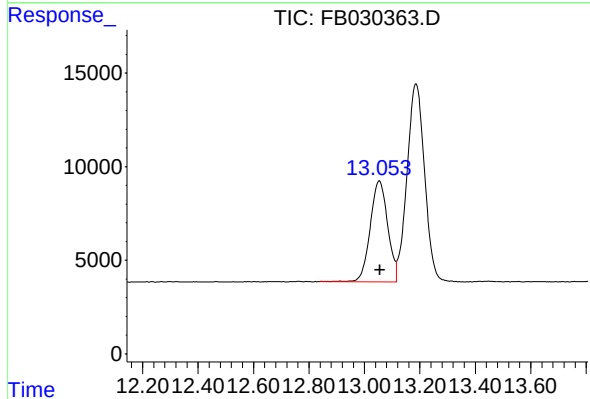


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.002 min
Response: 235845
Conc: 10.13 ng/ml

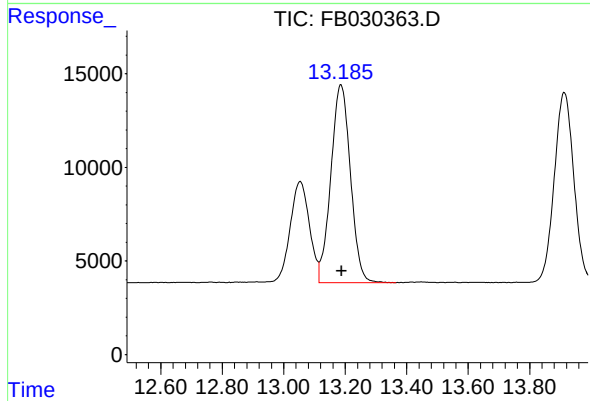

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.002 min
Response: 466614
Conc: 20.34 ng/ml

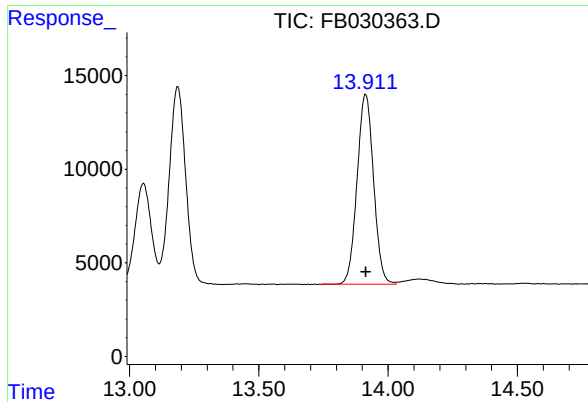

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.002 min
Response: 449771
Conc: 20.26 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1002S2

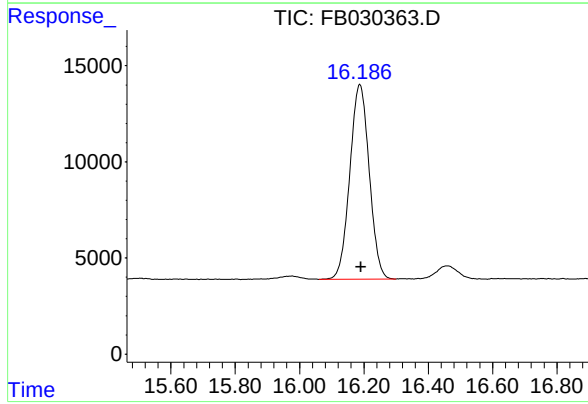

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.003 min
Response: 423246
Conc: 19.32 ng/ml