

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100223\
 Data File : FB030367.D
 Signal(s) : FID2B.CH
 Acq On : 2 Oct 2023 18:56
 Operator : YP/AJ
 Sample : 04686-01MS 50X
 Misc : 5.04G/5.00 ML DI MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 WASTEMS

Integration File: Calibration.e
 Quant Time: Oct 03 00:29:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
 Quant Title :
 QLast Update : Mon Sep 18 13:44:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	263976	19.085 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	460071	25.134 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	566198	27.987 ng/ml
3) t n-Heptane	7.746	181703	8.552 ng/ml
4) t Benzene	7.884	246235	9.673 ng/ml
6) t Toluene	10.618	705965	28.483 ng/ml
7) t Ethylbenzene	13.055	217821	9.357 ng/ml
8) t m-Xylene	13.188	433759	18.911 ng/ml
9) t O-Xylene	13.915	423978	19.094 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	385930	17.613 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100223\
Data File : FB030367.D
Signal(s) : FID2B.CH
Acq On : 2 Oct 2023 18:56
Operator : YP/AJ
Sample : 04686-01MS 50X
Misc : 5.04G/5.00 ML DI MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
WASTEMS

Integration File: Calibration.e
Quant Time: Oct 03 00:29:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
Quant Title :
QLast Update : Mon Sep 18 13:44:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

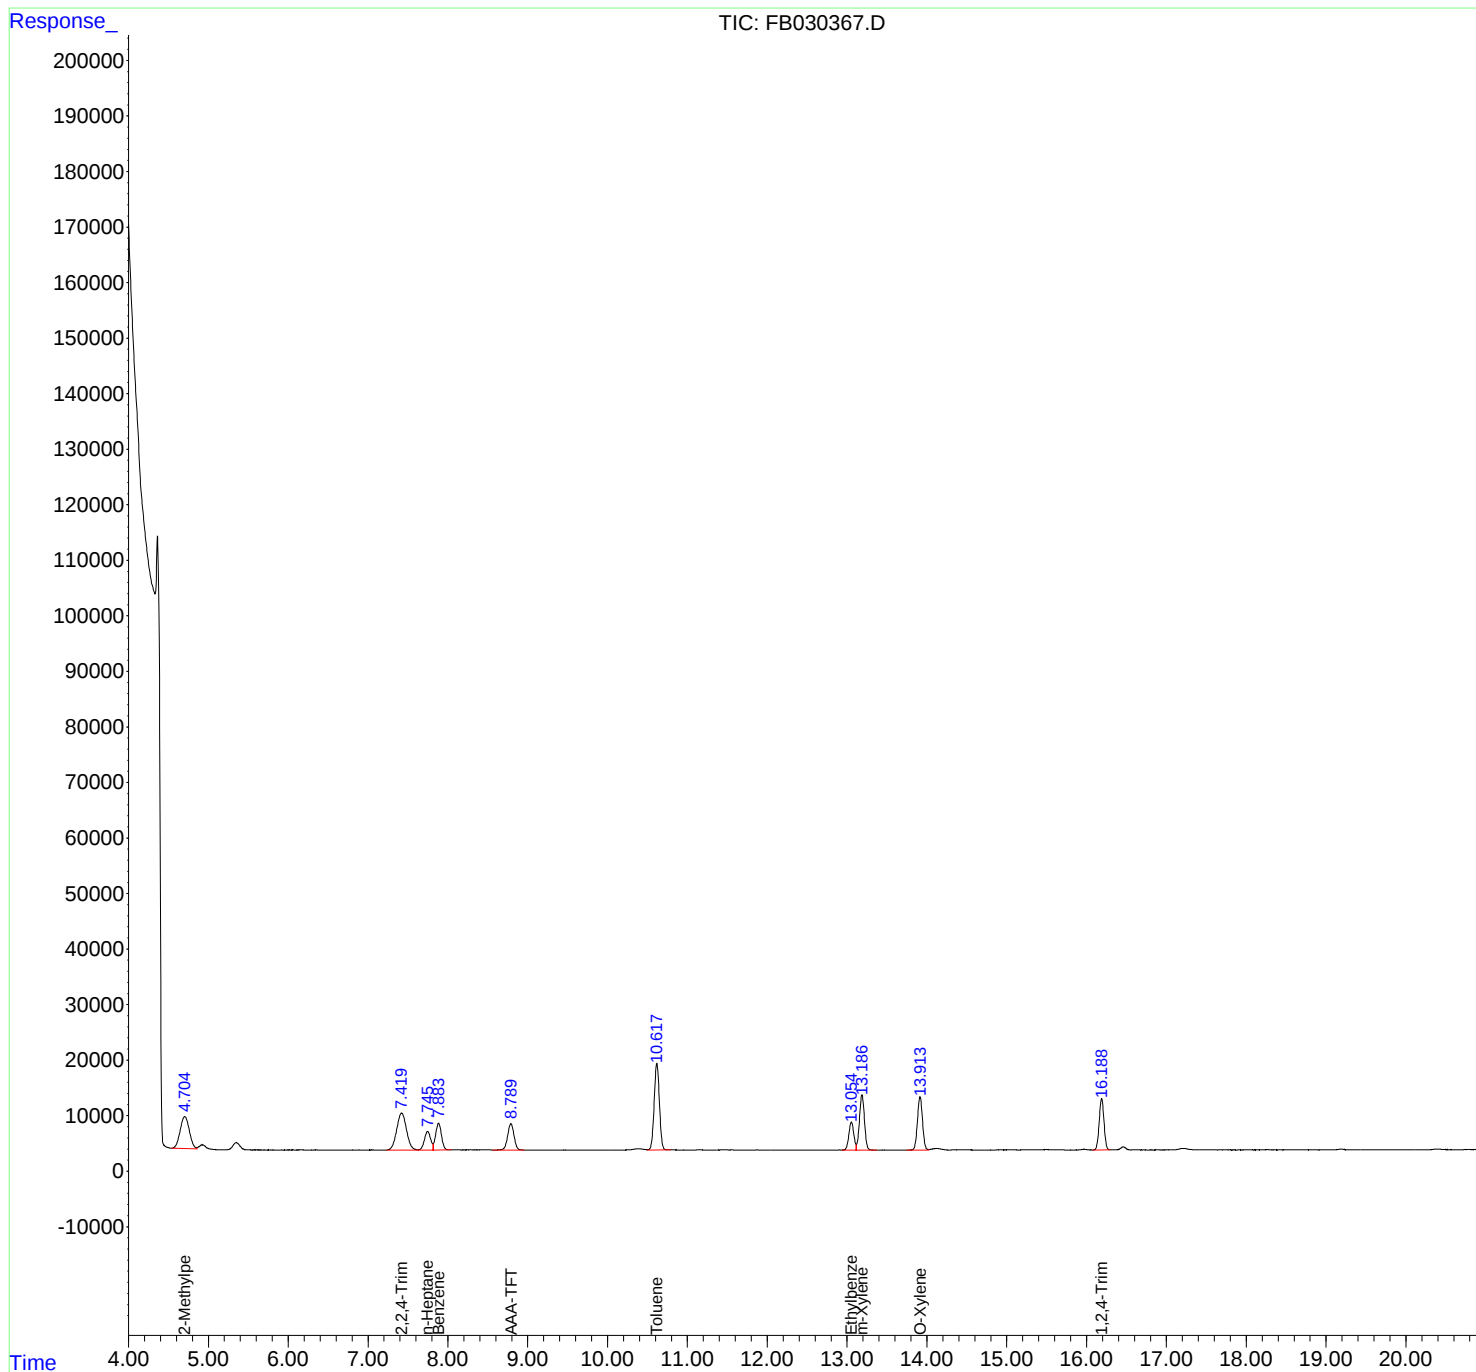


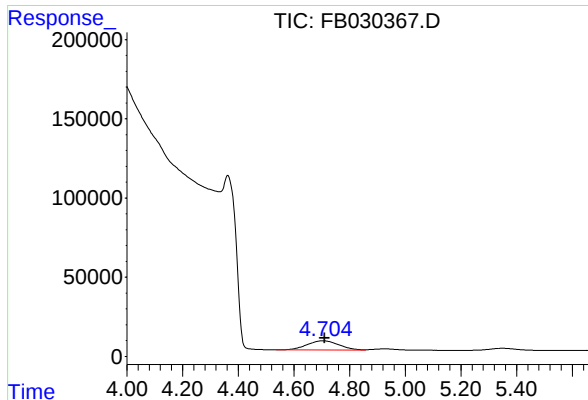

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.005 min
Response: 460071
Conc: 25.13 ng/ml

Instrument :
FID_B
ClientSampleId :
WASTEMS

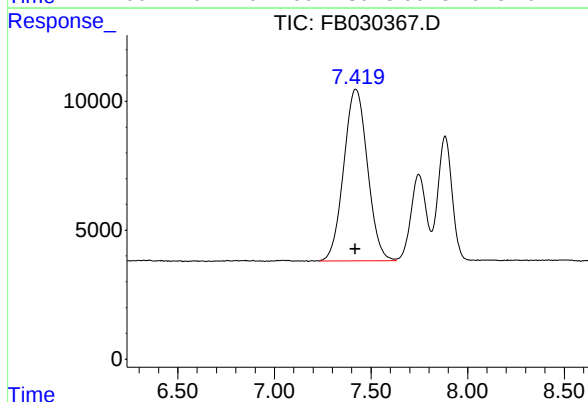


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.002 min
Response: 566198
Conc: 27.99 ng/ml

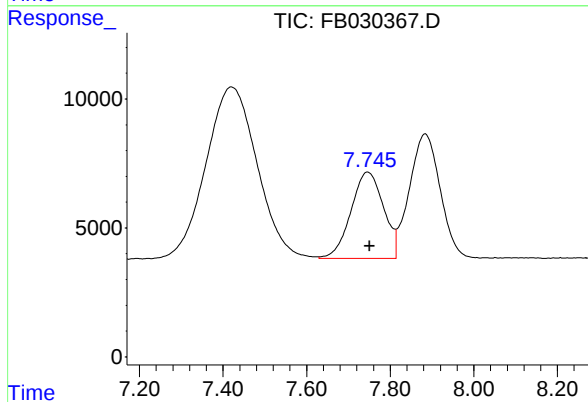


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.004 min
Response: 181703
Conc: 8.55 ng/ml

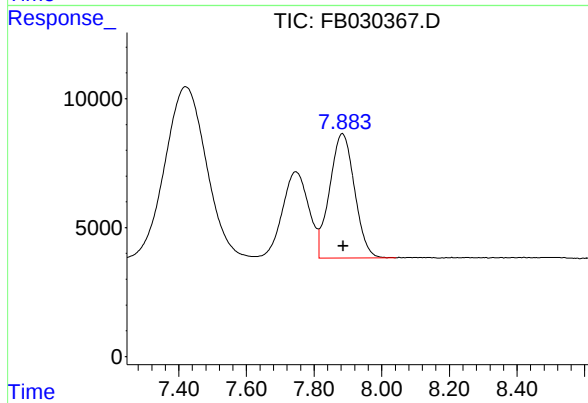

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.002 min
Response: 246235
Conc: 9.67 ng/ml

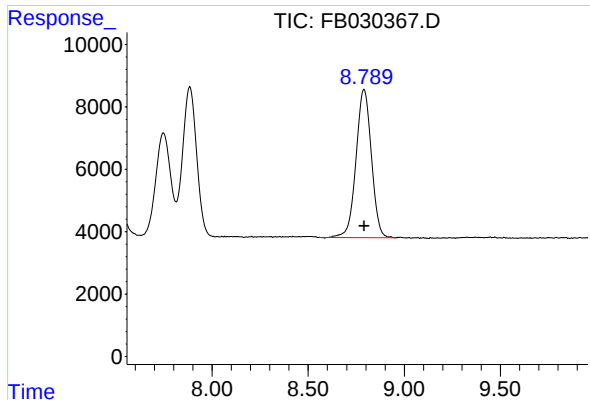

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.002 min
Response: 263976
Conc: 19.08 ng/ml

Instrument :
FID_B
ClientSampleId :
WASTEMS

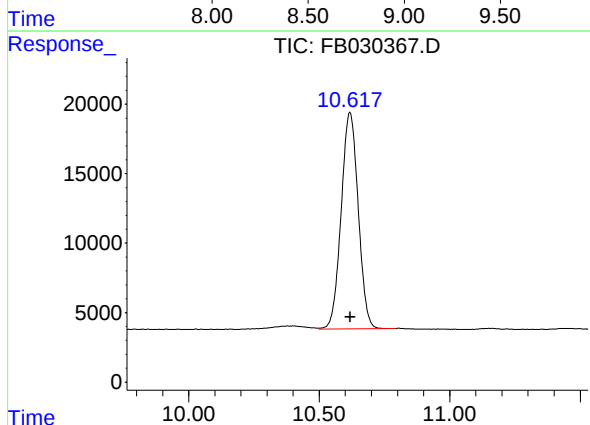


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.001 min
Response: 705965
Conc: 28.48 ng/ml

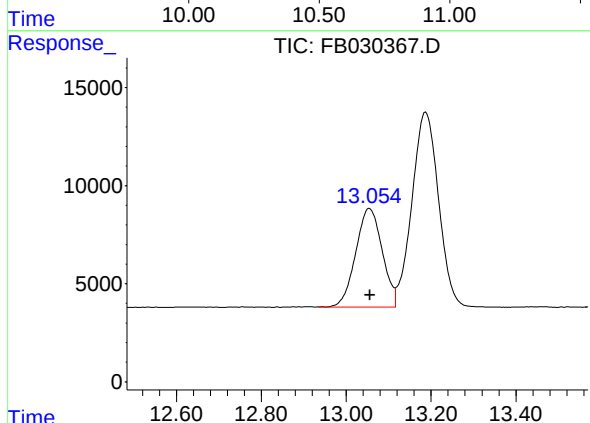


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: 0.000 min
Response: 217821
Conc: 9.36 ng/ml

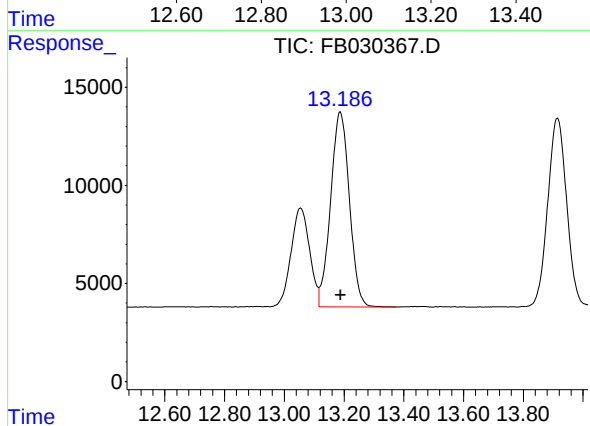

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: 0.000 min
Response: 433759
Conc: 18.91 ng/ml

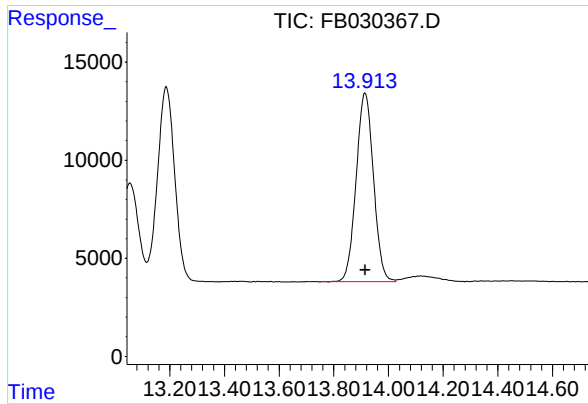

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: 0.000 min
Response: 423978
Conc: 19.09 ng/ml

Instrument :
FID_B
ClientSampleId :
WASTEMS

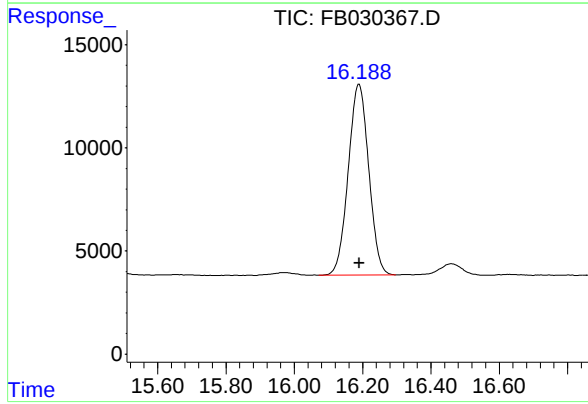

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.001 min
Response: 385930
Conc: 17.61 ng/ml