

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100223\
 Data File : FB030369.D
 Signal(s) : FID2B.CH
 Acq On : 2 Oct 2023 20:14
 Operator : YP/AJ
 Sample : BSF1002S3
 Misc : 5.00G/5.00 ML DI MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1002S3

Integration File: Calibration.e
 Quant Time: Oct 03 00:29:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
 Quant Title :
 QLast Update : Mon Sep 18 13:44:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	274864	19.872 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	499423	27.283 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	585611	28.947 ng/ml
3) t n-Heptane	7.752	194115	9.136 ng/ml
4) t Benzene	7.887	240730	9.457 ng/ml
6) t Toluene	10.620	713791	28.798 ng/ml
7) t Ethylbenzene	13.056	220360	9.466 ng/ml
8) t m-Xylene	13.189	438377	19.113 ng/ml
9) t O-Xylene	13.915	421176	18.968 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	399429	18.229 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100223\
Data File : FB030369.D
Signal(s) : FID2B.CH
Acq On : 2 Oct 2023 20:14
Operator : YP/AJ
Sample : BSF1002S3
Misc : 5.00G/5.00 ML DI MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1002S3

Integration File: Calibration.e
Quant Time: Oct 03 00:29:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
Quant Title :
QLast Update : Mon Sep 18 13:44:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

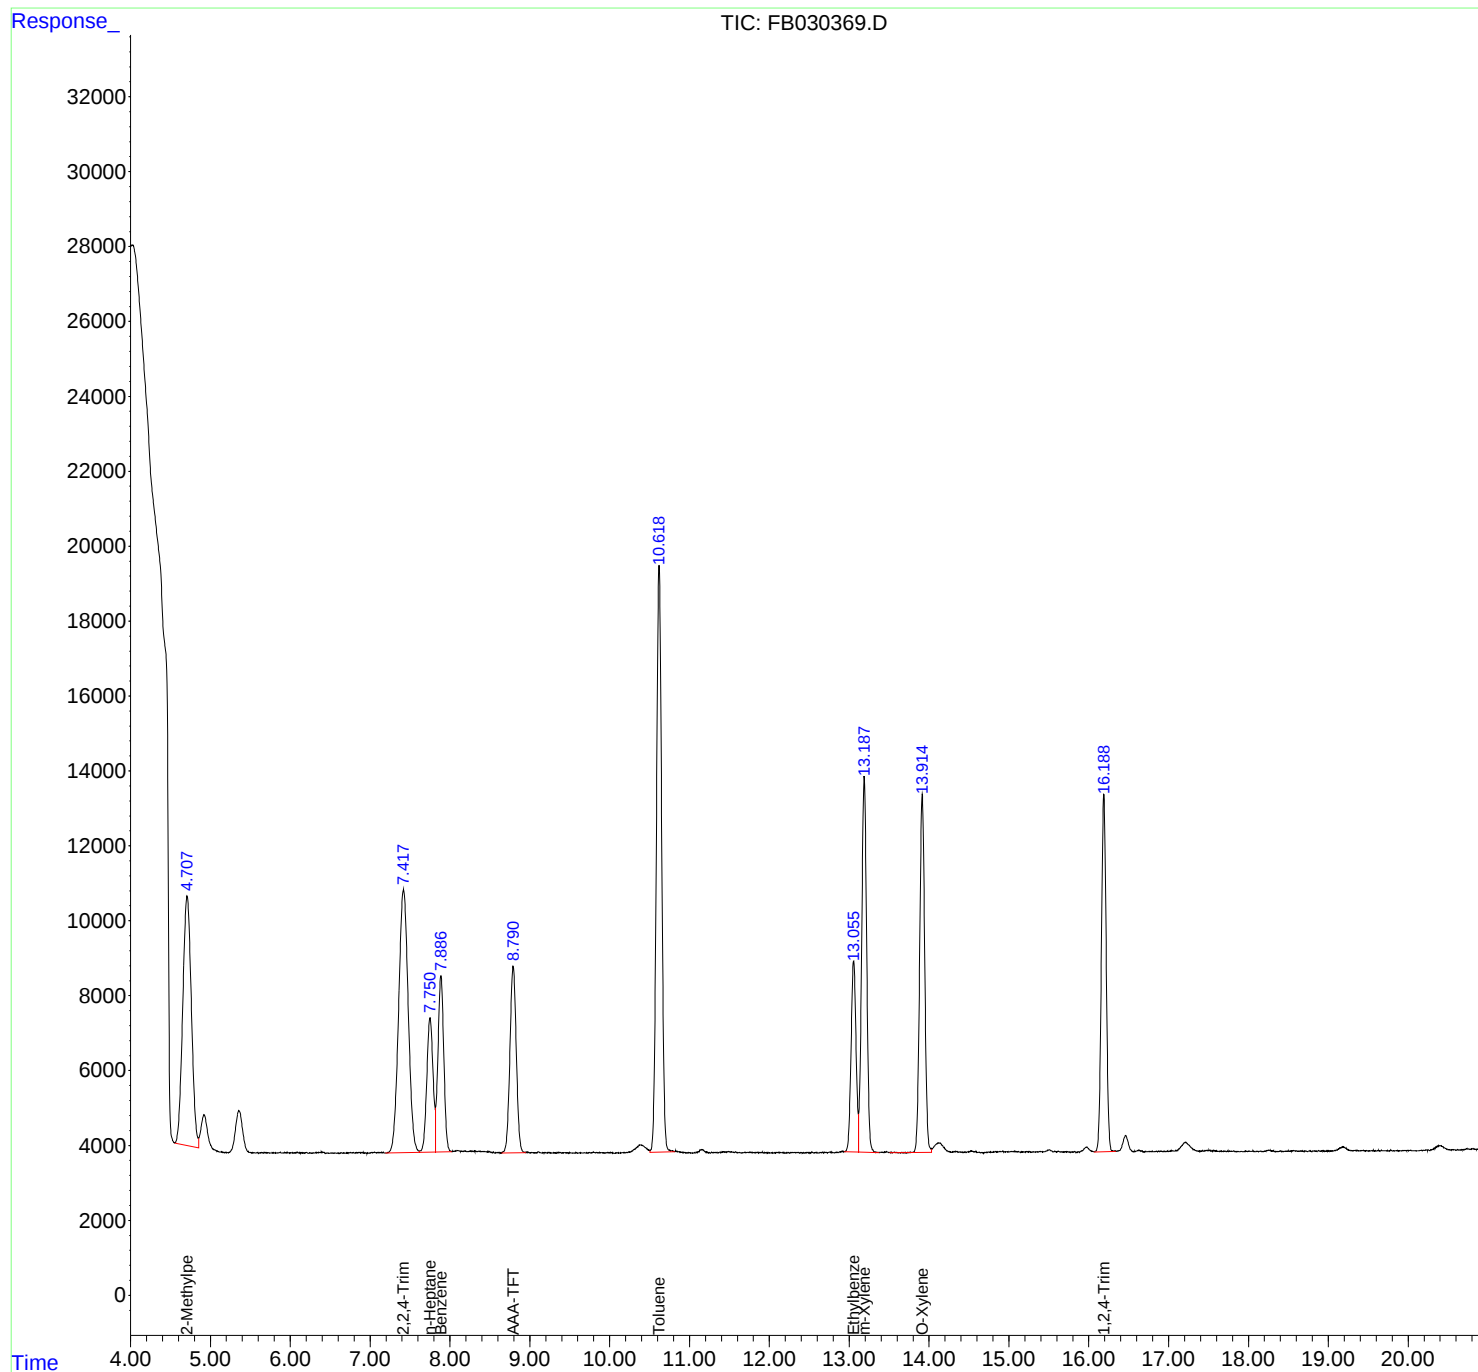


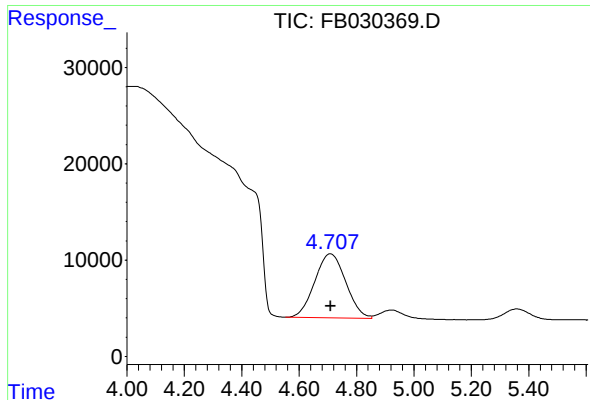

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: -0.002 min
Response: 499423
Conc: 27.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1002S3

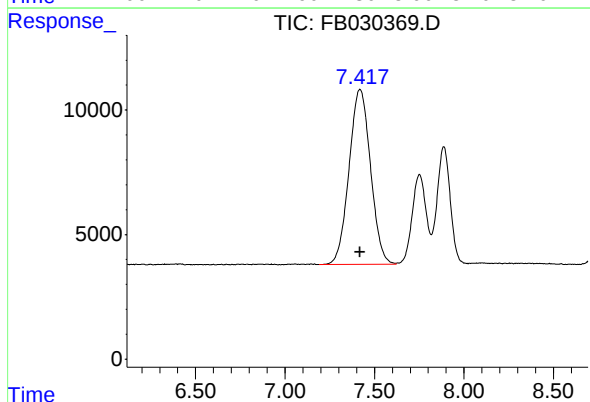


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 585611
Conc: 28.95 ng/ml

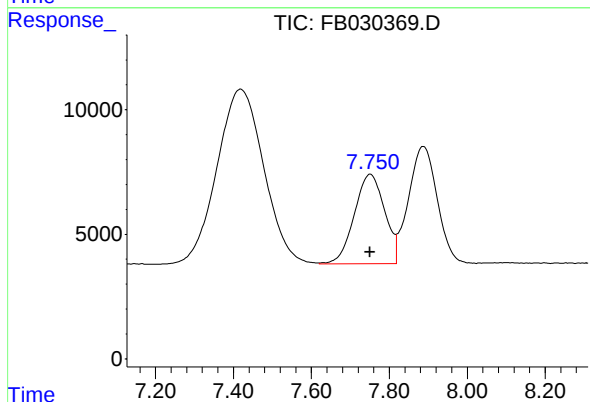


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.001 min
Response: 194115
Conc: 9.14 ng/ml

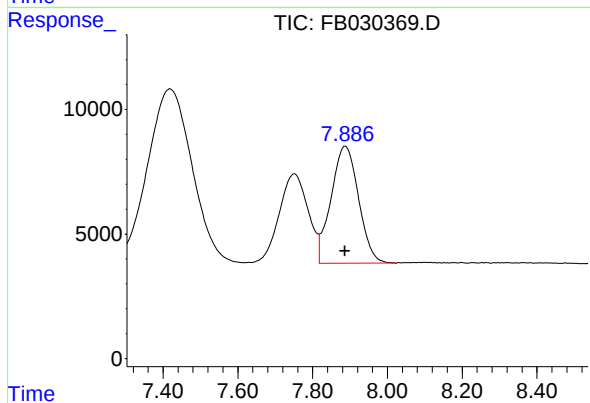

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.000 min
Response: 240730
Conc: 9.46 ng/ml

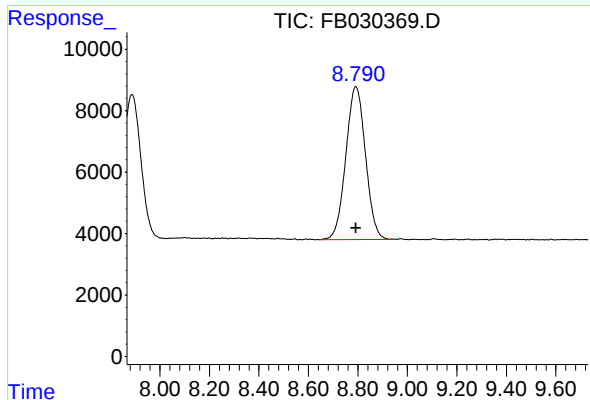

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 274864
Conc: 19.87 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1002S3

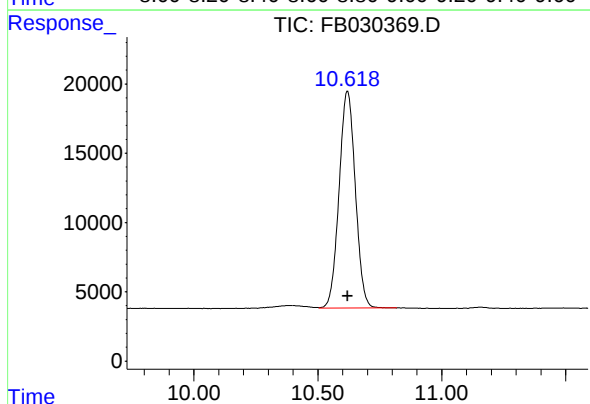


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.000 min
Response: 713791
Conc: 28.80 ng/ml

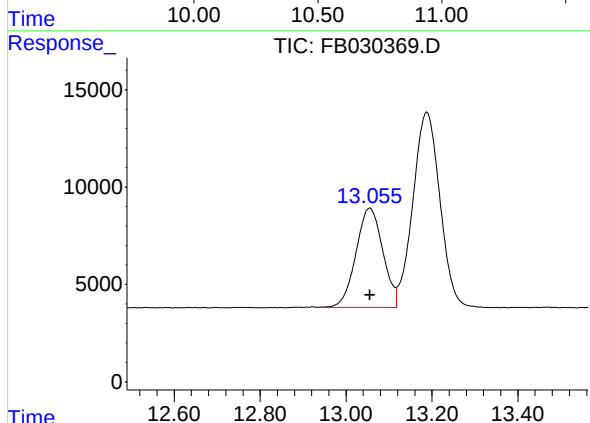


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 220360
Conc: 9.47 ng/ml

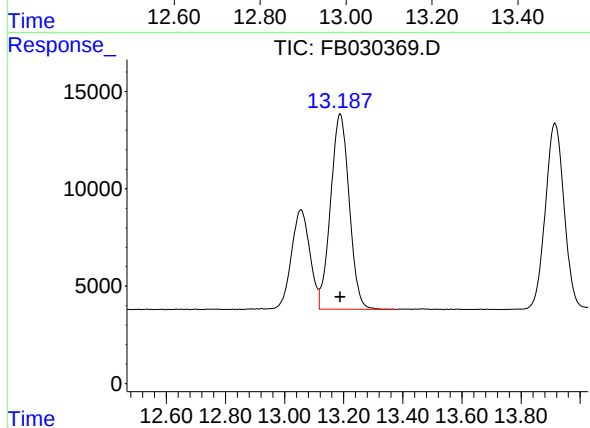

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 438377
Conc: 19.11 ng/ml

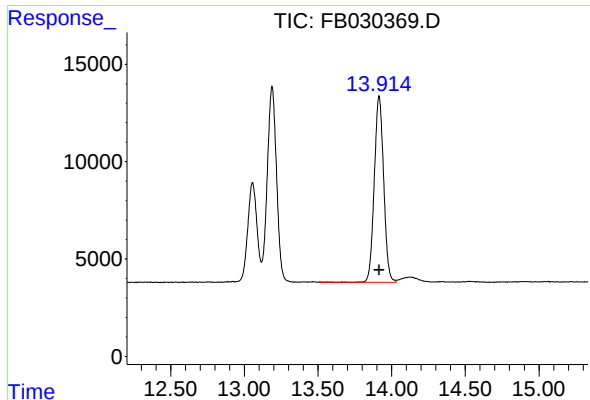

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: 0.000 min
Response: 421176
Conc: 18.97 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1002S3

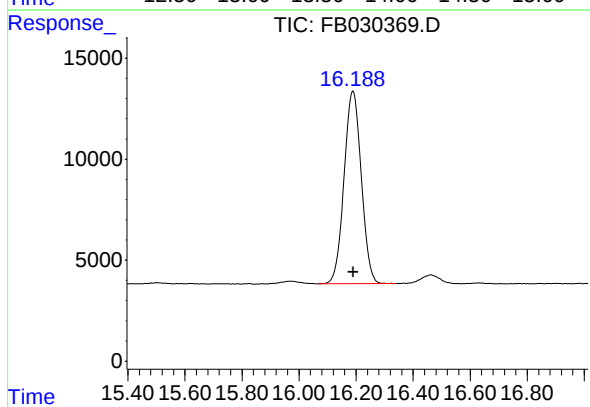

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.001 min
Response: 399429
Conc: 18.23 ng/ml