

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB100318\  
Data File : FB018086.D  
Signal(s) : FID2B.CH  
Acq On : 3 Oct 2018 18:39  
Operator : MJ/SJ  
Sample : J5194-03  
Misc : 5.03g/5.00mL DI Water  
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Oct 04 07:28:19 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB091418.M  
Quant Title :  
QLast Update : Fri Sep 14 13:09:25 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 9.111  | 162456   | 19.205 ng/ml |
| Target Compounds             |        |          |              |
| 1) t 2-Methylpentane         | 4.943  | 3604     | 0.226 ng/ml  |
| 8) t m-Xylene                | 13.532 | 7271     | 0.420 ng/ml  |
| 9) t O-Xylene                | 14.275 | 10680    | 0.588 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.555 | 33930    | 1.595 ng/ml  |
| -----                        |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB100318\  
Data File : FB018086.D  
Signal(s) : FID2B.CH  
Acq On : 3 Oct 2018 18:39  
Operator : MJ/SJ  
Sample : J5194-03  
Misc : 5.03g/5.00mL DI Water  
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Oct 04 07:28:19 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB091418.M  
Quant Title :  
QLast Update : Fri Sep 14 13:09:25 2018  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

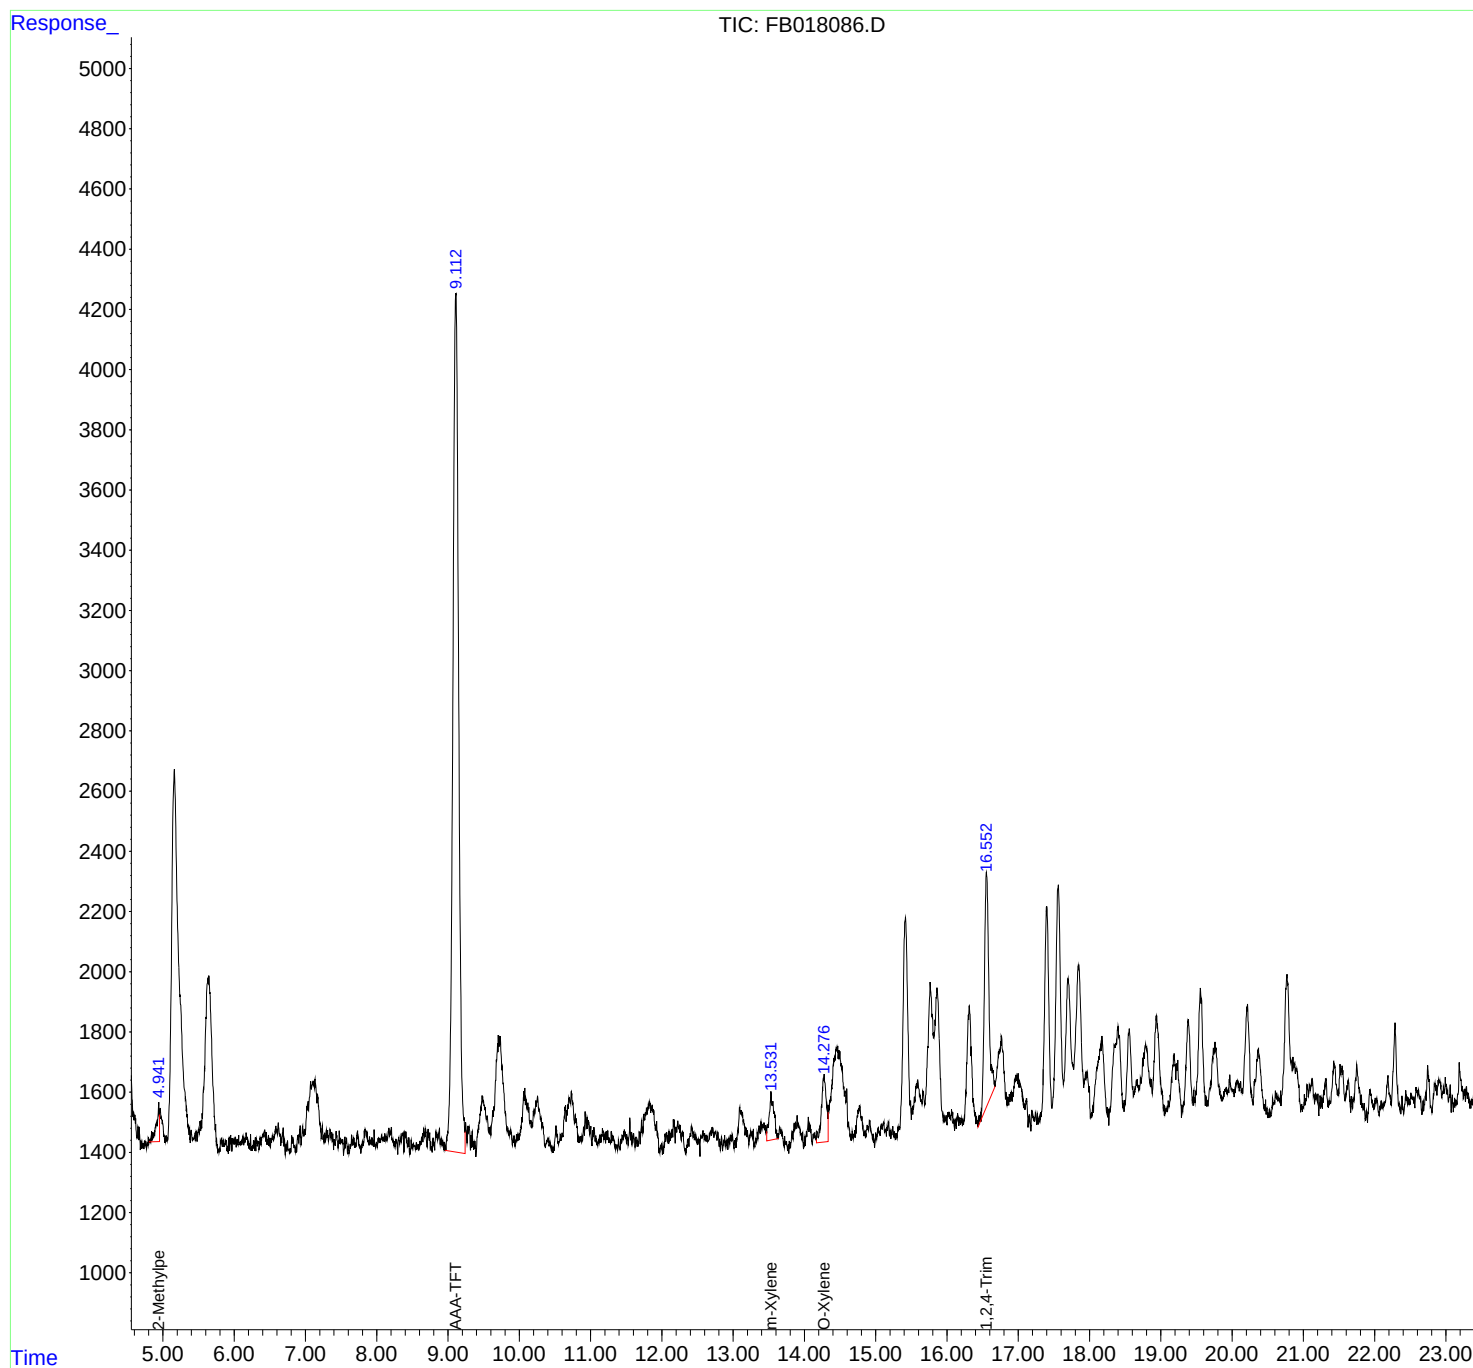

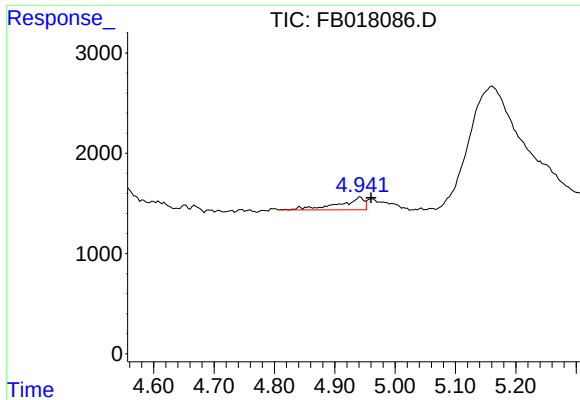


#1 2-Methylpentane

R.T.: 4.943 min  
Delta R.T.: -0.017 min  
Response: 3604  
Conc: 0.23 ng/ml

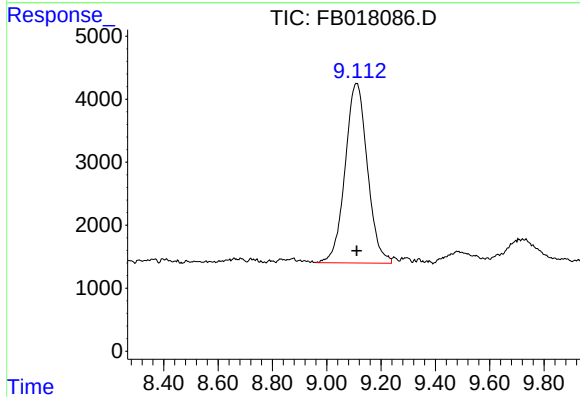


#5 AAA-TFT

R.T.: 9.111 min  
Delta R.T.: 0.000 min  
Response: 162456  
Conc: 19.21 ng/ml

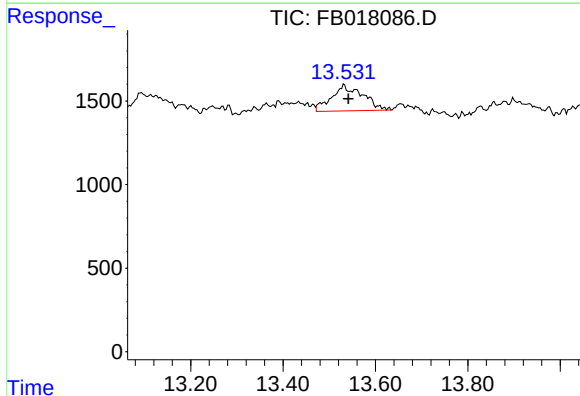


#8 m-Xylene

R.T.: 13.532 min  
Delta R.T.: -0.009 min  
Response: 7271  
Conc: 0.42 ng/ml

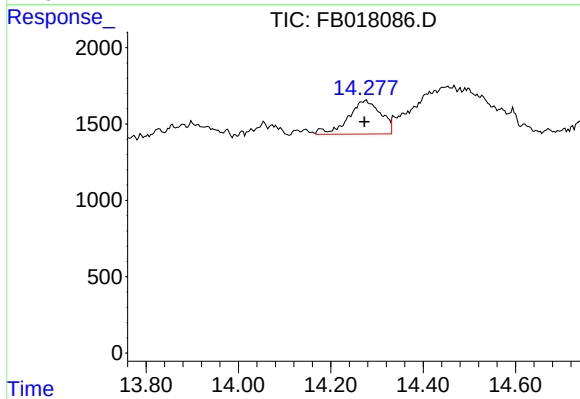

#9 O-Xylene

R.T.: 14.275 min  
Delta R.T.: 0.002 min  
Response: 10680  
Conc: 0.59 ng/ml

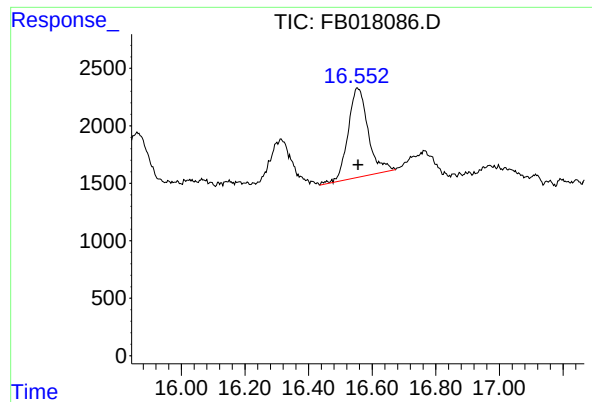

#10 1,2,4-Trimethylbenzene

R.T.: 16.555 min  
Delta R.T.: 0.000 min  
Response: 33930  
Conc: 1.60 ng/ml