

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100318\
 Data File : FB018087.D
 Signal(s) : FID2B.CH
 Acq On : 3 Oct 2018 19:09
 Operator : MJ/SJ
 Sample : J5194-03MS
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 04 07:28:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
 Quant Title :
 QLast Update : Fri Sep 14 13:09:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.108	167953	19.855 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.960	359243	22.558 ng/ml
2) t 2,2,4-Trimethylpentane	7.725	278448	17.497 ng/ml
3) t n-Heptane	8.065	89446	5.804 ng/ml
4) t Benzene	8.203	164717	8.653 ng/ml
6) t Toluene	10.958	405983	25.653 ng/ml
7) t Ethylbenzene	13.408	142814	8.740 ng/ml
8) t m-Xylene	13.540	285240	16.488 ng/ml
9) t O-Xylene	14.271	323448	17.799 ng/ml
10) t 1,2,4-Trimethylbenzene	16.554	328898	15.462 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100318\
Data File : FB018087.D
Signal(s) : FID2B.CH
Acq On : 3 Oct 2018 19:09
Operator : MJ/SJ
Sample : J5194-03MS
Misc : 5.01g/5.00mL DI Water
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 04 07:28:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

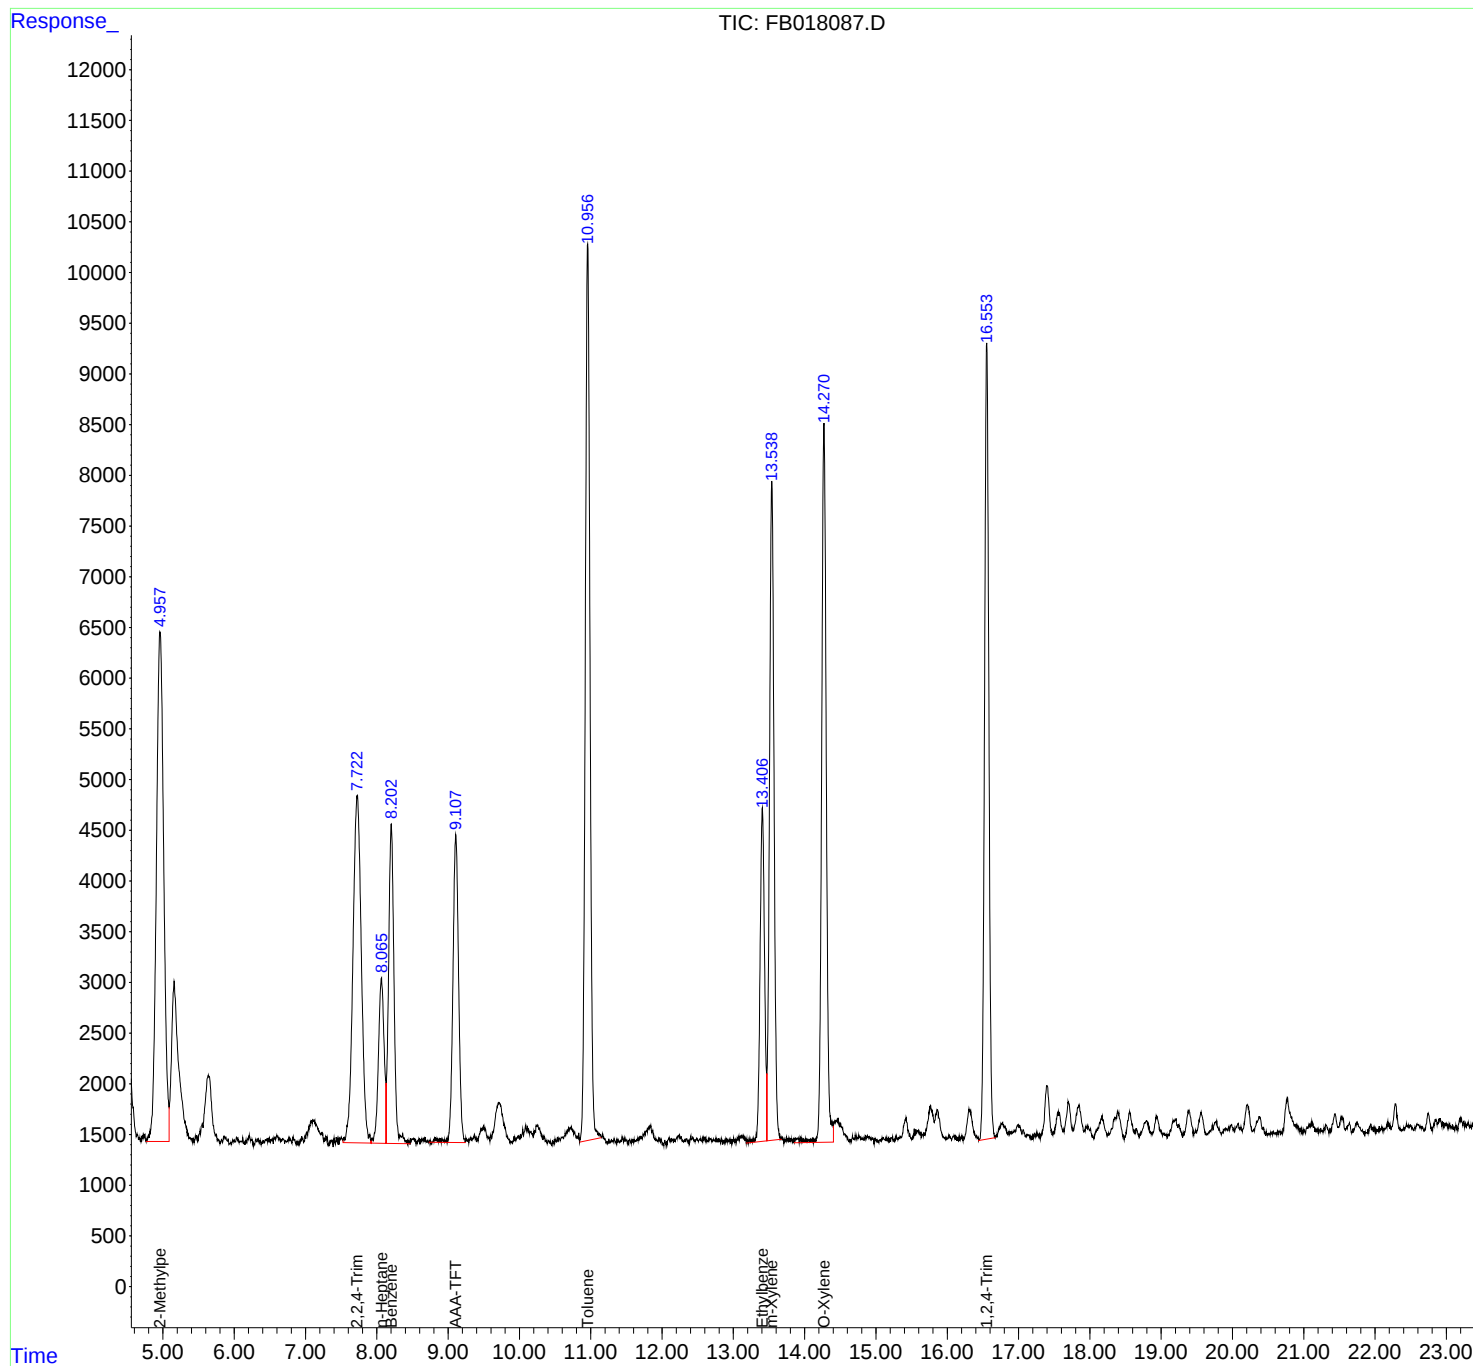

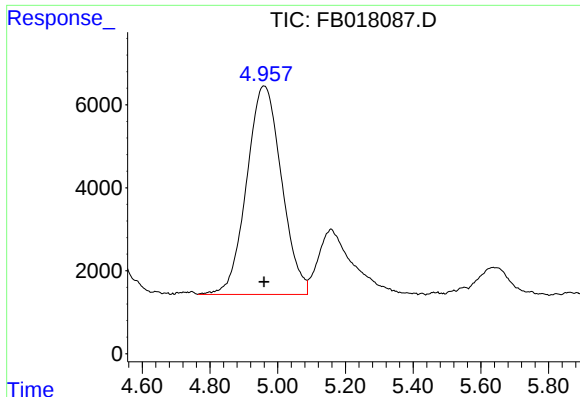


#1 2-Methylpentane

R.T.: 4.960 min
Delta R.T.: 0.000 min
Response: 359243
Conc: 22.56 ng/ml

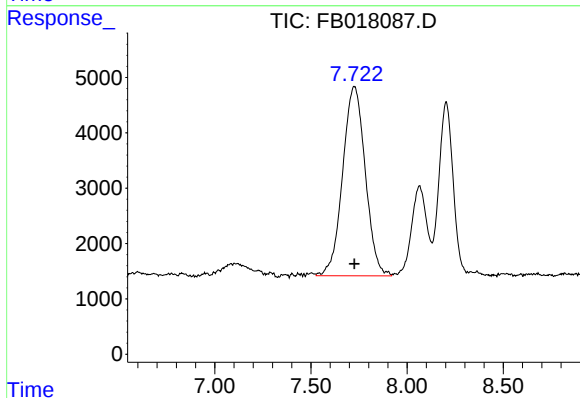


#2 2,2,4-Trimethylpentane

R.T.: 7.725 min
Delta R.T.: -0.002 min
Response: 278448
Conc: 17.50 ng/ml

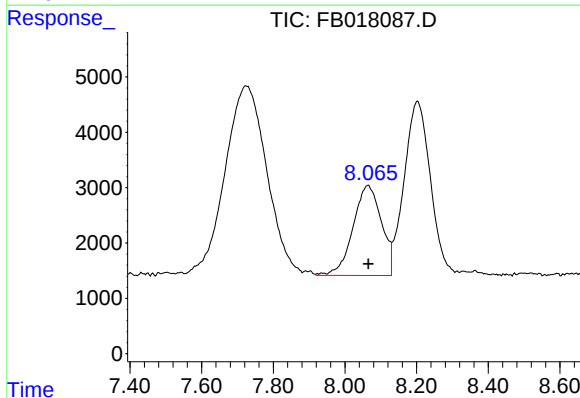


#3 n-Heptane

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 89446
Conc: 5.80 ng/ml

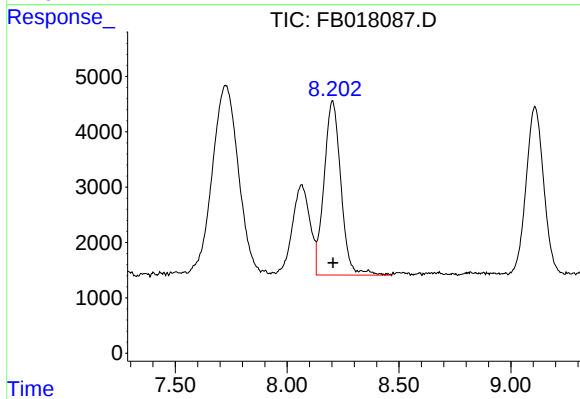


#4 Benzene

R.T.: 8.203 min
Delta R.T.: -0.002 min
Response: 164717
Conc: 8.65 ng/ml

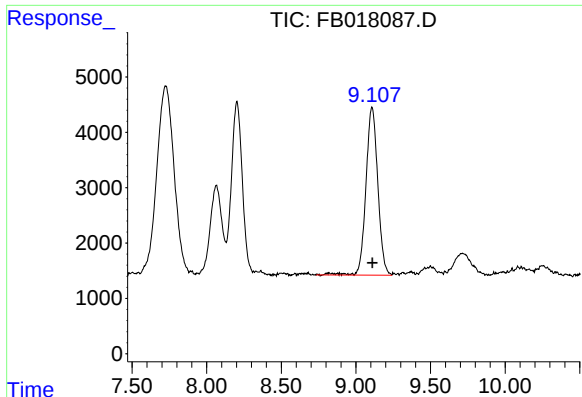


#5 AAA-TFT

R.T.: 9.108 min
Delta R.T.: -0.002 min
Response: 167953
Conc: 19.86 ng/ml

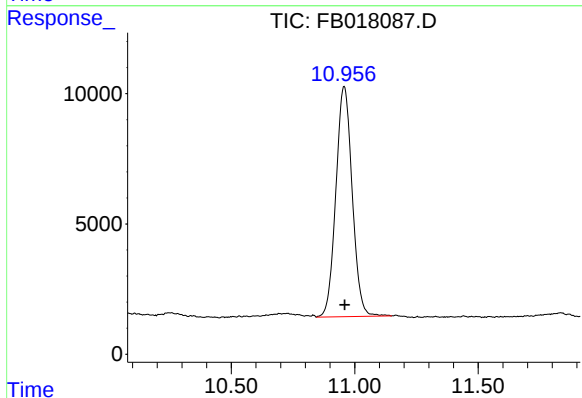


#6 Toluene

R.T.: 10.958 min
Delta R.T.: -0.002 min
Response: 405983
Conc: 25.65 ng/ml

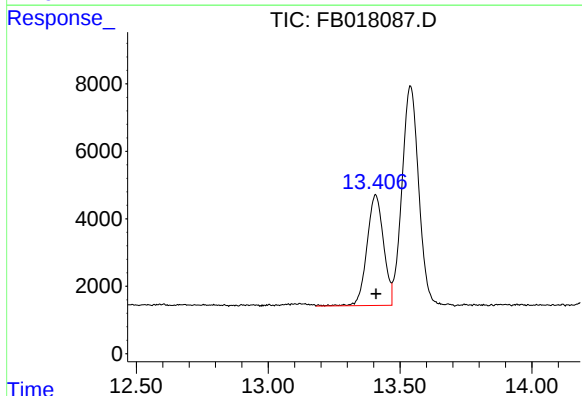


#7 Ethylbenzene

R.T.: 13.408 min
Delta R.T.: 0.000 min
Response: 142814
Conc: 8.74 ng/ml

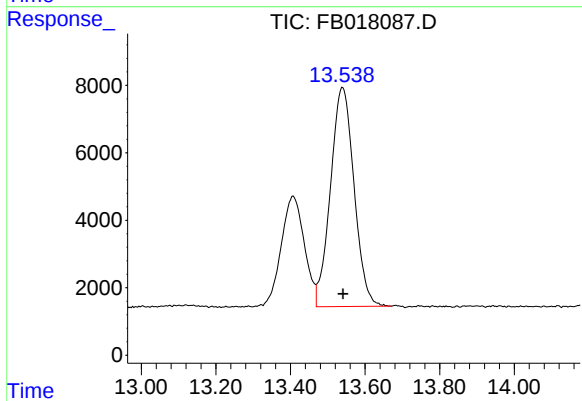


#8 m-Xylene

R.T.: 13.540 min
Delta R.T.: -0.001 min
Response: 285240
Conc: 16.49 ng/ml

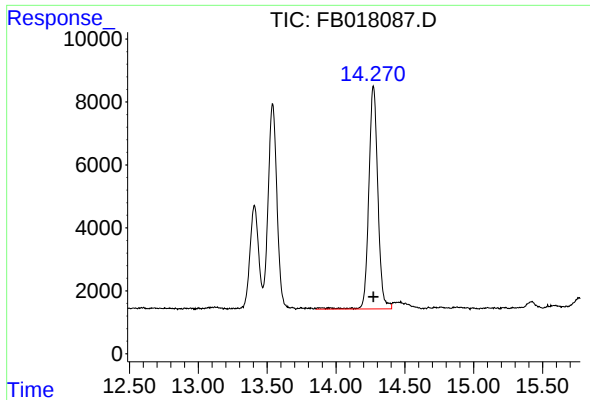

#9 O-Xylene

R.T.: 14.271 min
Delta R.T.: -0.002 min
Response: 323448
Conc: 17.80 ng/ml

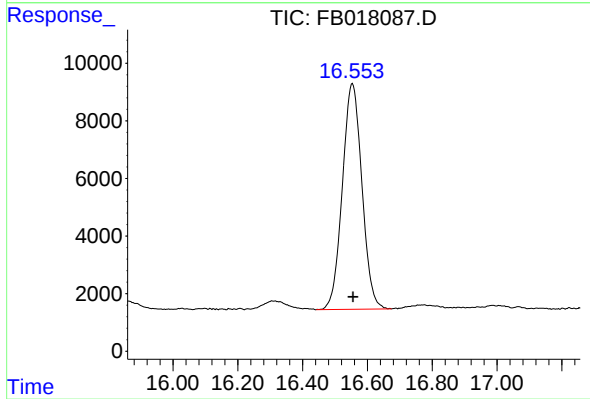

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min
Delta R.T.: -0.001 min
Response: 328898
Conc: 15.46 ng/ml