

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100319\
 Data File : FB022675.D
 Signal(s) : FID2B.CH
 Acq On : 3 Oct 2019 14:23
 Operator : DD/AJ
 Sample : K5140-02
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 04 01:06:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
 Quant Title :
 QLast Update : Wed Oct 02 06:15:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.026	1903925	79.020 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.827	11866	0.356 ng/ml
2) t 2,2,4-Trimethylpentane	7.562	66314	1.912 ng/ml
3) t n-Heptane	7.921	391956	11.575 ng/ml
6) t Toluene	10.804	1194806	29.518 ng/ml
7) t Ethylbenzene	13.230	8102004	209.351 ng/ml
8) t m-Xylene	13.380	6320304	170.451 ng/ml
9) t O-Xylene	14.113	4410069	126.311 ng/ml
10) t 1,2,4-Trimethylbenzene	16.394	5038815	203.367 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100319\
Data File : FB022675.D
Signal(s) : FID2B.CH
Acq On : 3 Oct 2019 14:23
Operator : DD/AJ
Sample : K5140-02
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 04 01:06:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
Quant Title :
QLast Update : Wed Oct 02 06:15:33 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

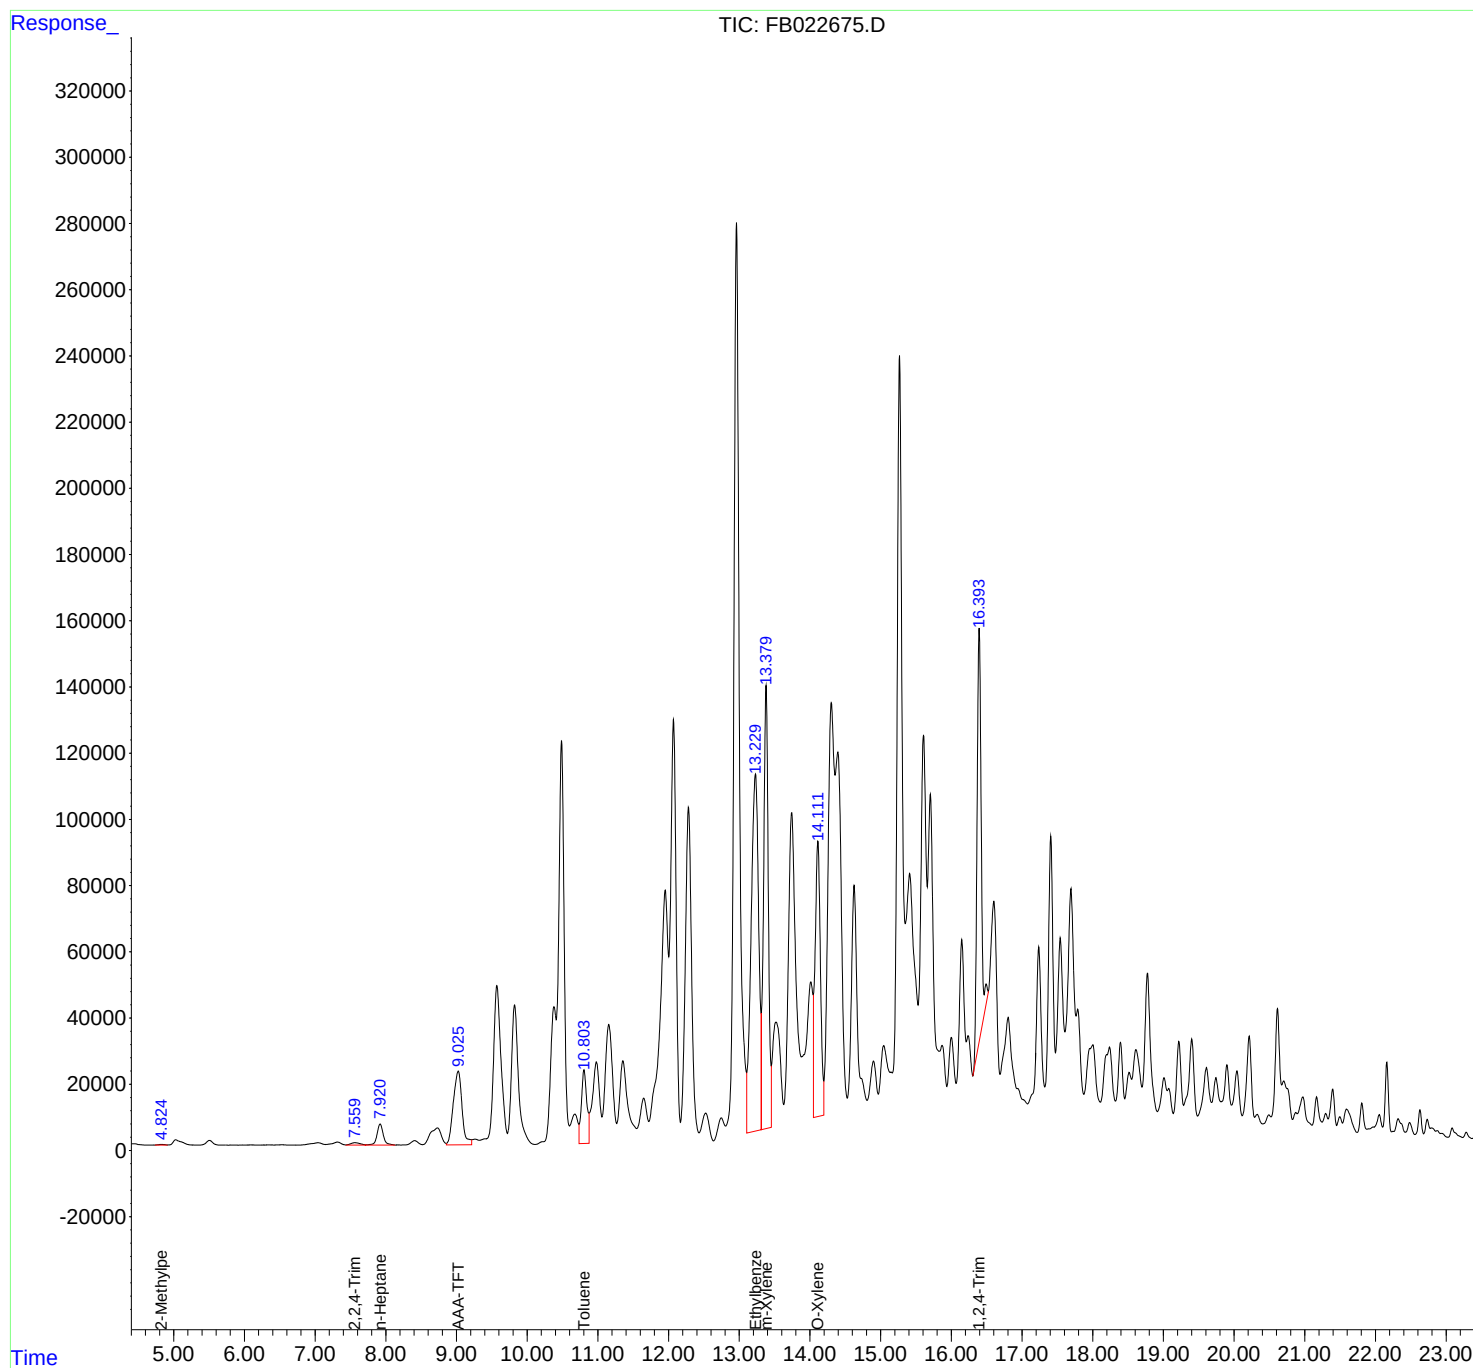

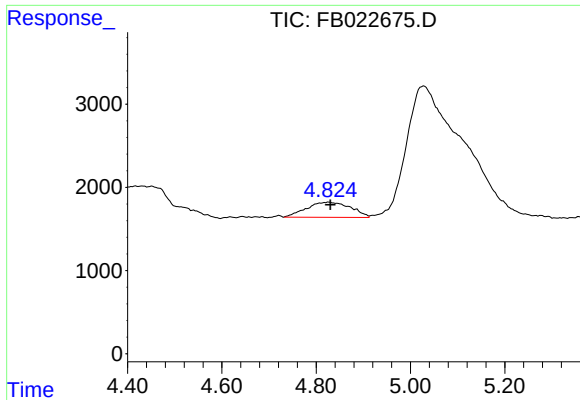


#1 2-Methylpentane

R.T.: 4.827 min
Delta R.T.: -0.003 min
Response: 11866
Conc: 0.36 ng/ml

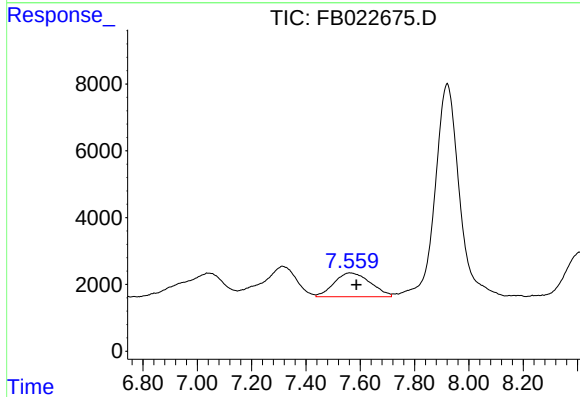


#2 2,2,4-Trimethylpentane

R.T.: 7.562 min
Delta R.T.: -0.024 min
Response: 66314
Conc: 1.91 ng/ml

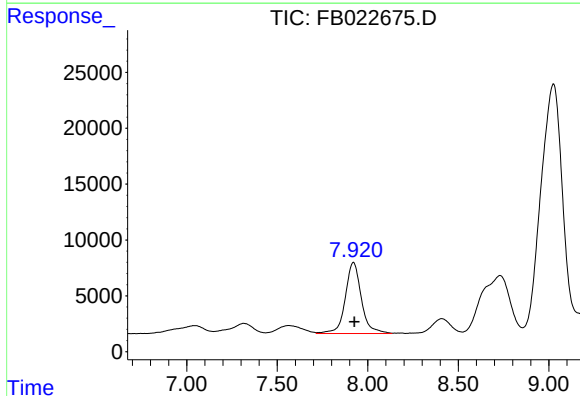


#3 n-Heptane

R.T.: 7.921 min
Delta R.T.: -0.005 min
Response: 391956
Conc: 11.57 ng/ml

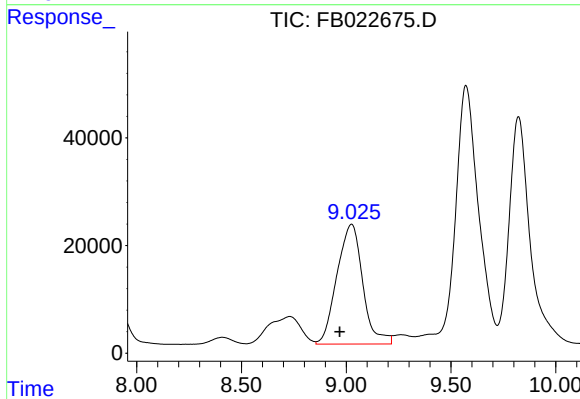


#5 AAA-TFT

R.T.: 9.026 min
Delta R.T.: 0.058 min
Response: 1903925
Conc: 79.02 ng/ml

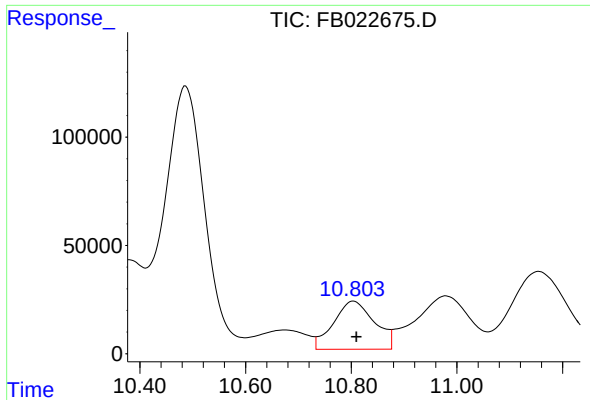


#6 Toluene

R.T.: 10.804 min
Delta R.T.: -0.006 min
Response: 1194806
Conc: 29.52 ng/ml

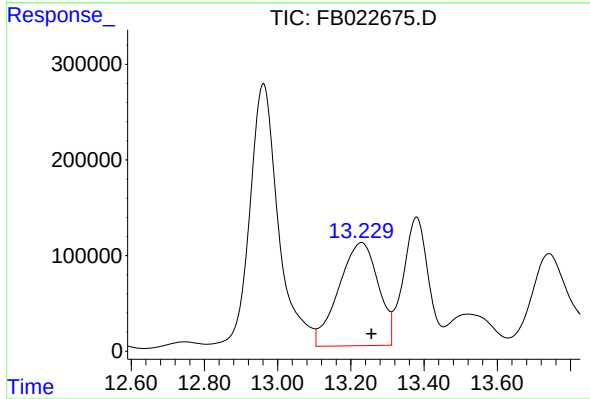


#7 Ethylbenzene

R.T.: 13.230 min
Delta R.T.: -0.027 min
Response: 8102004
Conc: 209.35 ng/ml

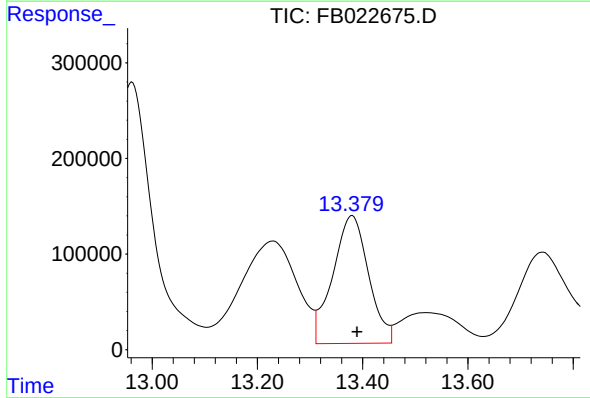


#8 m-Xylene

R.T.: 13.380 min
Delta R.T.: -0.009 min
Response: 6320304
Conc: 170.45 ng/ml

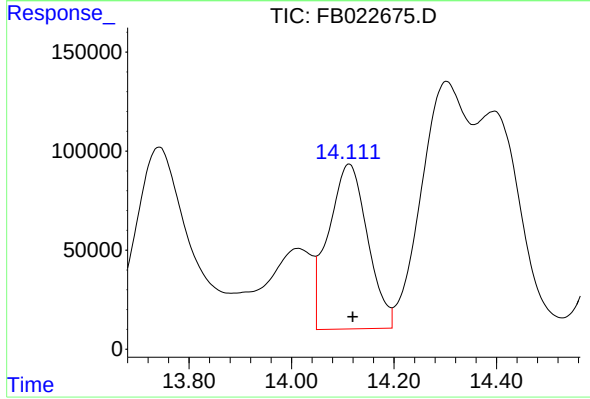

#9 O-Xylene

R.T.: 14.113 min
Delta R.T.: -0.007 min
Response: 4410069
Conc: 126.31 ng/ml

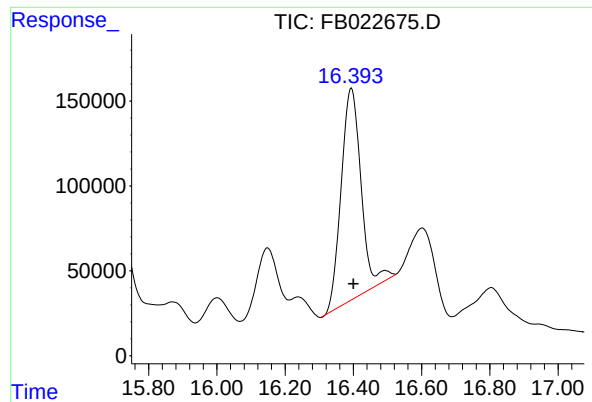

#10 1,2,4-Trimethylbenzene

R.T.: 16.394 min
Delta R.T.: -0.006 min
Response: 5038815
Conc: 203.37 ng/ml