

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100319\
 Data File : FB022679.D
 Signal(s) : FID2B.CH
 Acq On : 3 Oct 2019 16:22
 Operator : DD/AJ
 Sample : K5140-02 50X
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 04 01:07:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
 Quant Title :
 QLast Update : Wed Oct 02 06:15:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.968	579630	24.057 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.834	30944	0.928 ng/ml
2) t 2,2,4-Trimethylpentane	7.595	3334	0.096 ng/ml
3) t n-Heptane	7.916	19634	0.580 ng/ml
6) t Toluene	10.810	86267	2.131 ng/ml
7) t Ethylbenzene	13.229	1388104	35.868 ng/ml
8) t m-Xylene	13.384	915628	24.693 ng/ml
9) t O-Xylene	14.117	755612	21.642 ng/ml
10) t 1,2,4-Trimethylbenzene	16.397	1935546	78.119 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100319\
Data File : FB022679.D
Signal(s) : FID2B.CH
Acq On : 3 Oct 2019 16:22
Operator : DD/AJ
Sample : K5140-02 50X
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 04 01:07:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
Quant Title :
QLast Update : Wed Oct 02 06:15:33 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

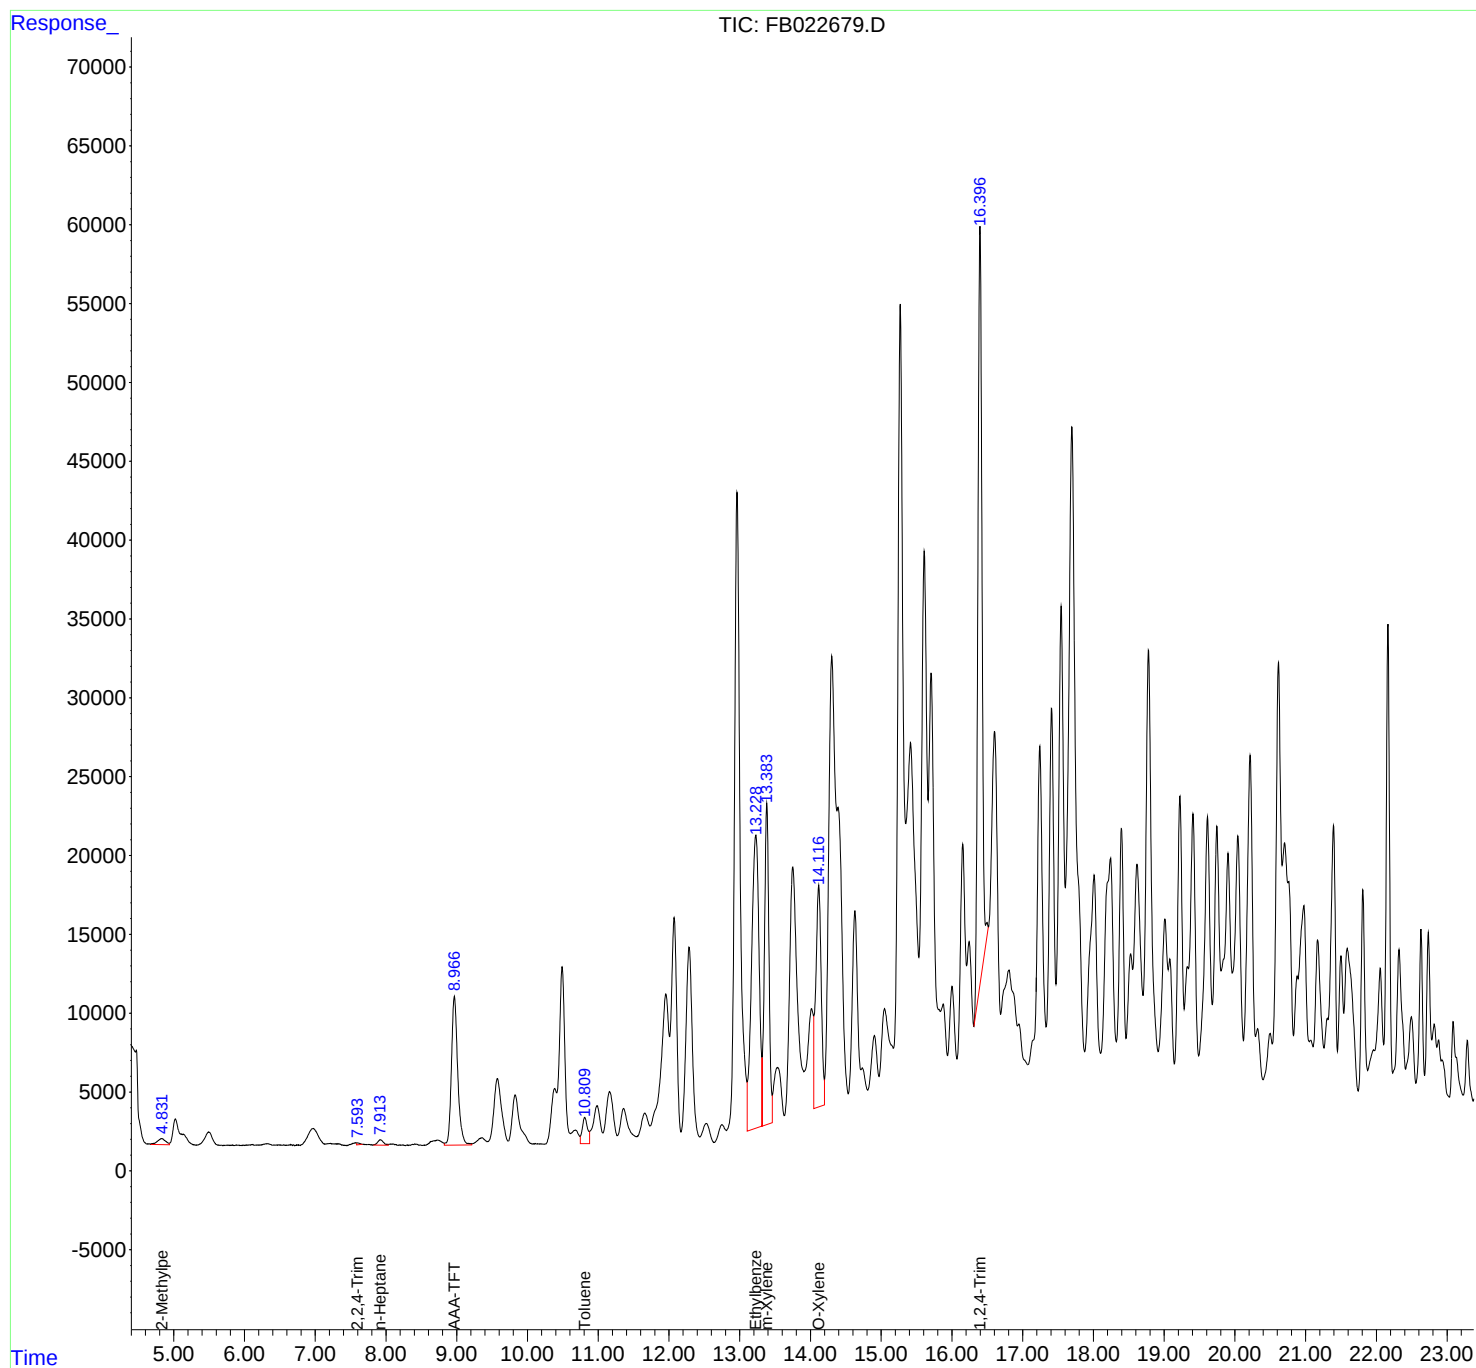

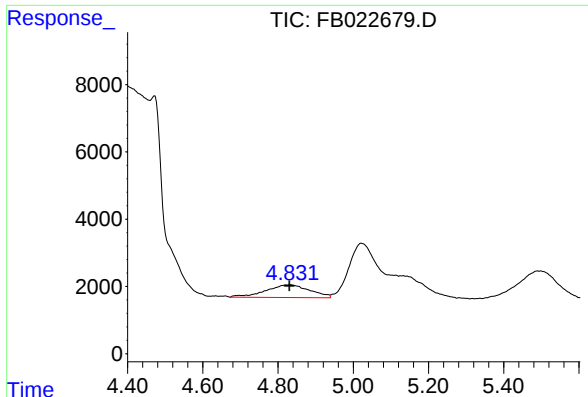


#1 2-Methylpentane

R.T.: 4.834 min
Delta R.T.: 0.004 min
Response: 30944
Conc: 0.93 ng/ml

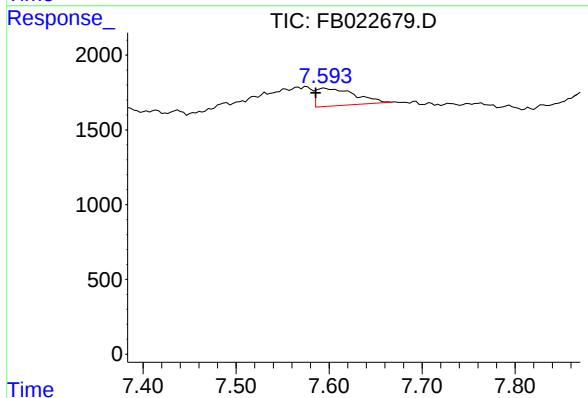


#2 2,2,4-Trimethylpentane

R.T.: 7.595 min
Delta R.T.: 0.010 min
Response: 3334
Conc: 0.10 ng/ml

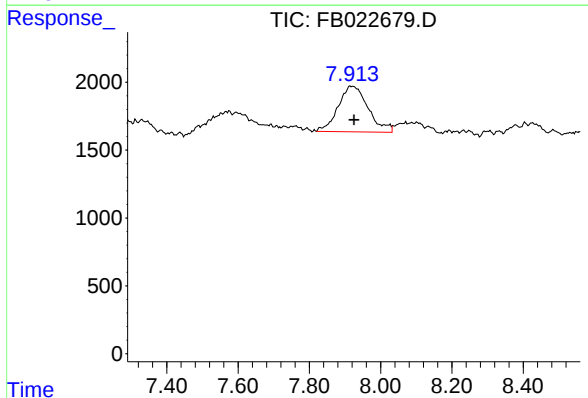


#3 n-Heptane

R.T.: 7.916 min
Delta R.T.: -0.010 min
Response: 19634
Conc: 0.58 ng/ml

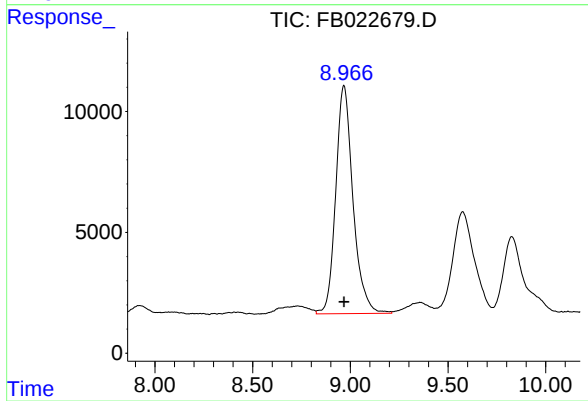


#5 AAA-TFT

R.T.: 8.968 min
Delta R.T.: 0.000 min
Response: 579630
Conc: 24.06 ng/ml

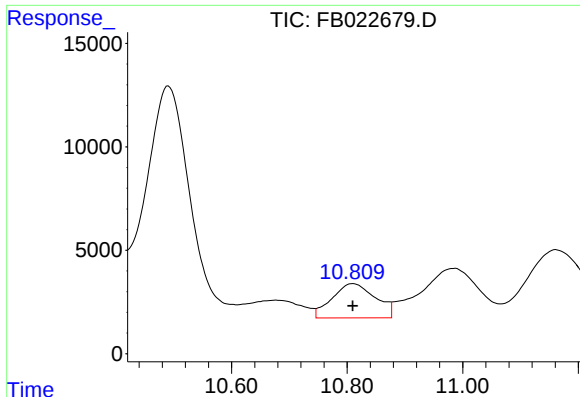


#6 Toluene

R.T.: 10.810 min
Delta R.T.: 0.000 min
Response: 86267
Conc: 2.13 ng/ml

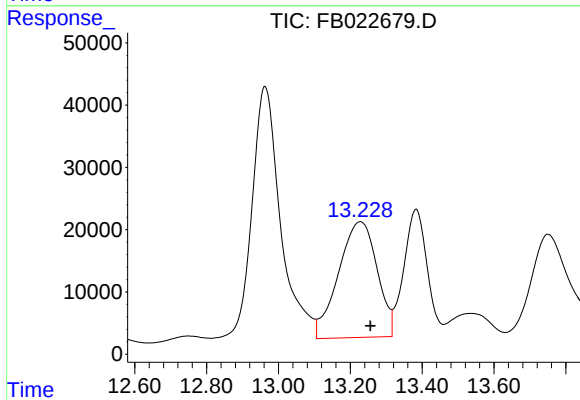


#7 Ethylbenzene

R.T.: 13.229 min
Delta R.T.: -0.028 min
Response: 1388104
Conc: 35.87 ng/ml

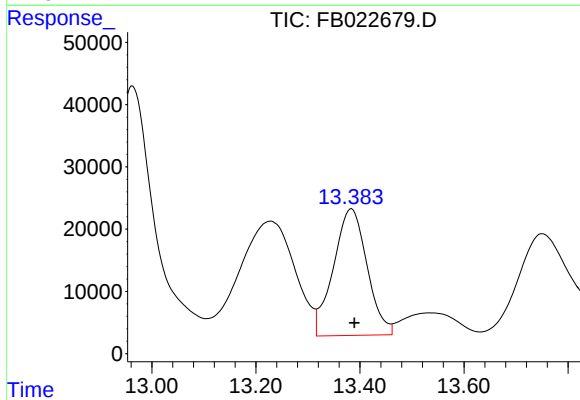


#8 m-Xylene

R.T.: 13.384 min
Delta R.T.: -0.006 min
Response: 915628
Conc: 24.69 ng/ml

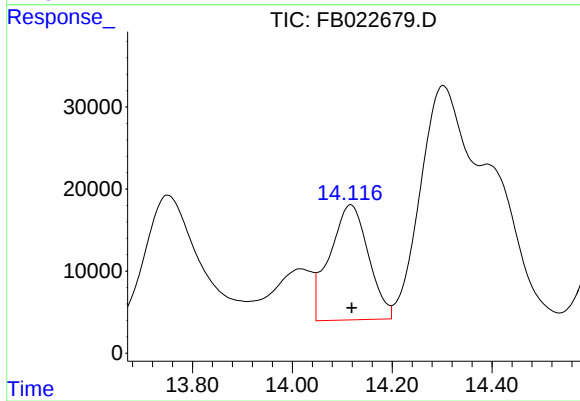

#9 O-Xylene

R.T.: 14.117 min
Delta R.T.: -0.002 min
Response: 755612
Conc: 21.64 ng/ml

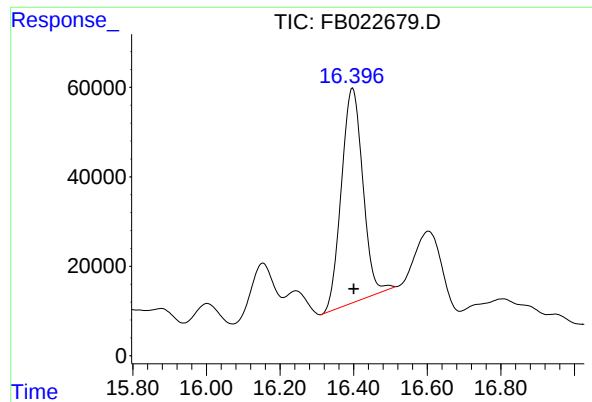

#10 1,2,4-Trimethylbenzene

R.T.: 16.397 min
Delta R.T.: -0.003 min
Response: 1935546
Conc: 78.12 ng/ml