

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100319\
 Data File : FB022674.D
 Signal(s) : FID2B.CH
 Acq On : 3 Oct 2019 12:49
 Operator : DD/AJ
 Sample : BSF1003S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 04 01:06:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
 Quant Title :
 QLast Update : Wed Oct 02 06:15:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.967	512132	21.255 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.836	1062881	31.872 ng/ml
2) t 2,2,4-Trimethylpentane	7.586	1090666	31.444 ng/ml
3) t n-Heptane	7.926	365002	10.779 ng/ml
4) t Benzene	8.059	434044	10.422 ng/ml
6) t Toluene	10.807	1259363	31.112 ng/ml
7) t Ethylbenzene	13.253	393972	10.180 ng/ml
8) t m-Xylene	13.386	733363	19.778 ng/ml
9) t O-Xylene	14.116	683034	19.563 ng/ml
10) t 1,2,4-Trimethylbenzene	16.397	513355	20.719 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100319\
Data File : FB022674.D
Signal(s) : FID2B.CH
Acq On : 3 Oct 2019 12:49
Operator : DD/AJ
Sample : BSF1003S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 04 01:06:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
Quant Title :
QLast Update : Wed Oct 02 06:15:33 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

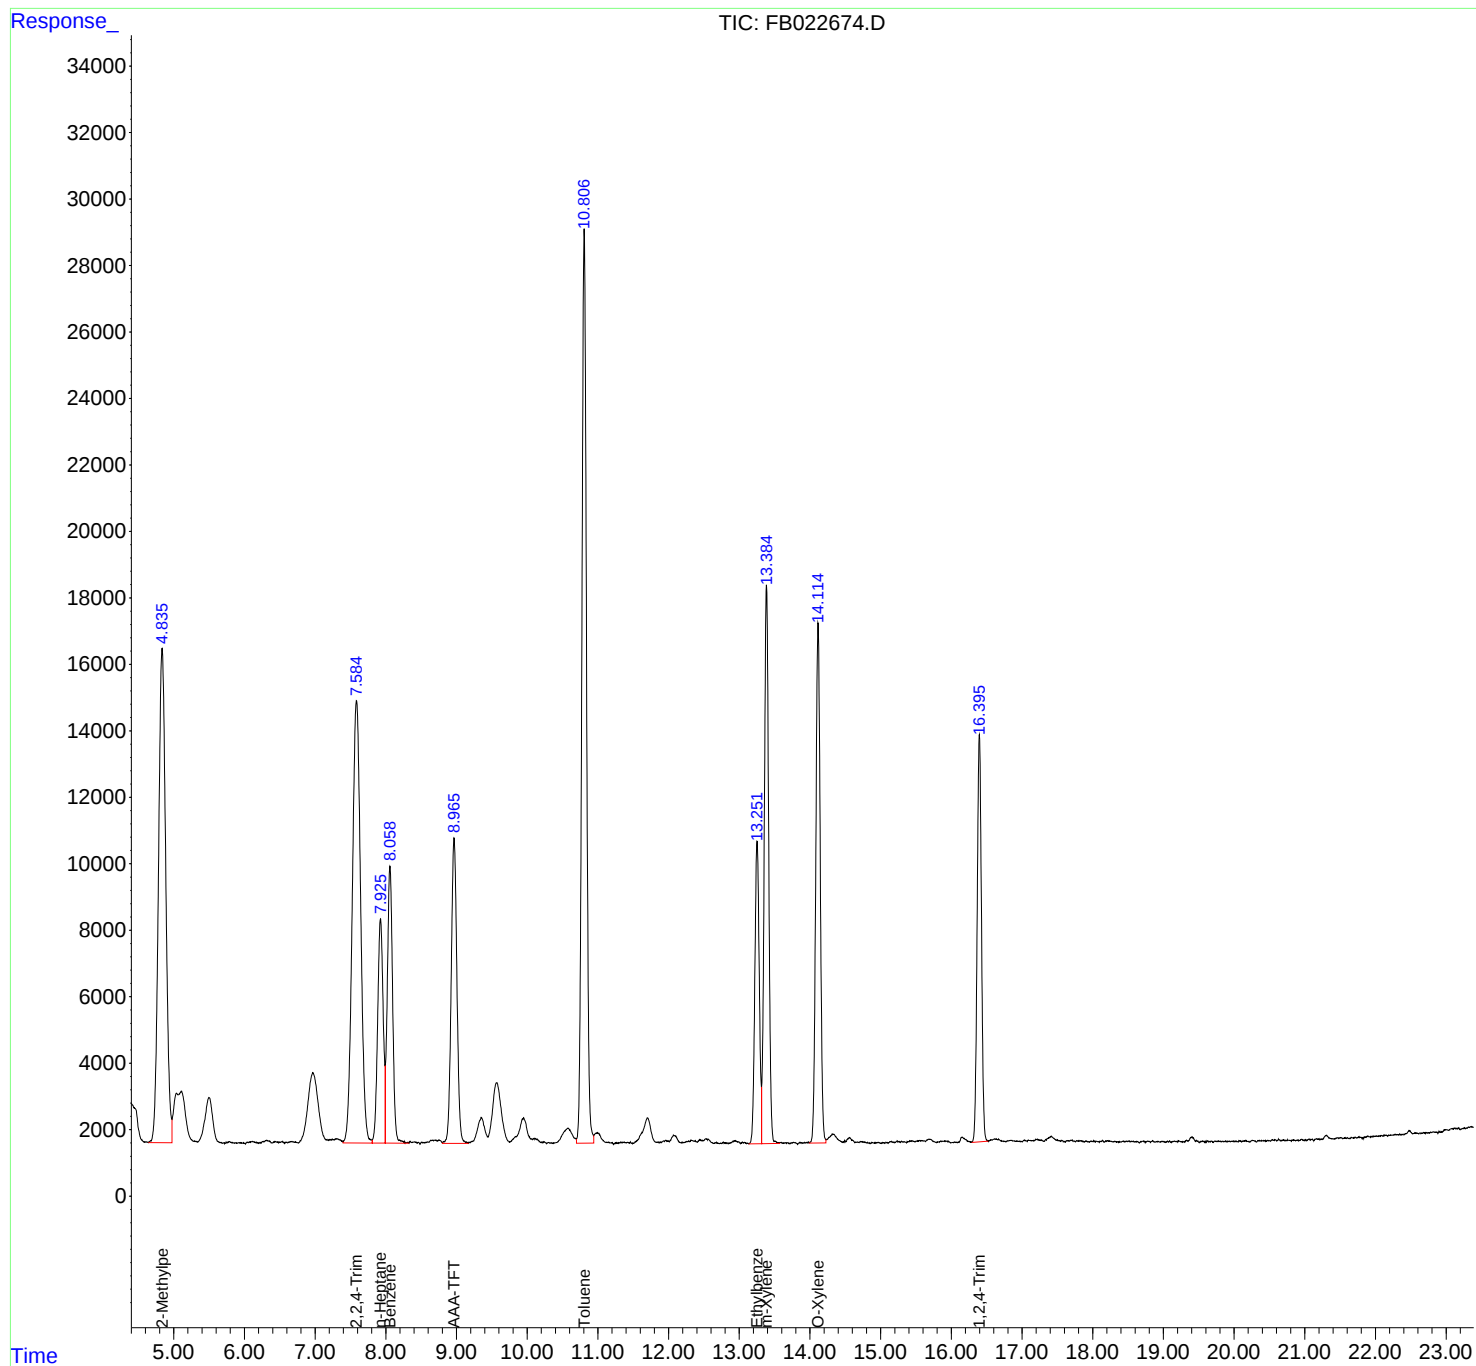

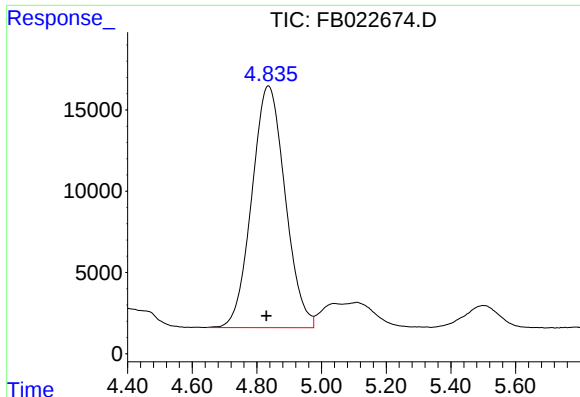


#1 2-Methylpentane

R.T.: 4.836 min
Delta R.T.: 0.006 min
Response: 1062881
Conc: 31.87 ng/ml

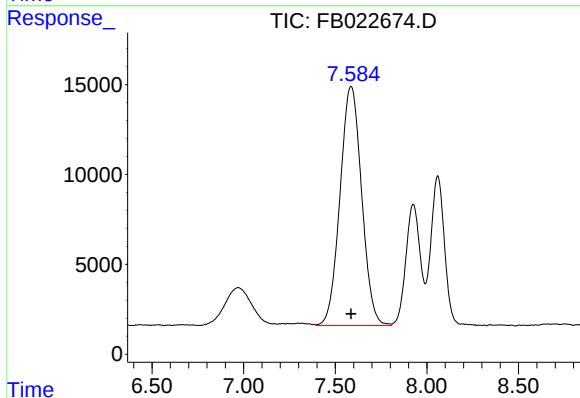


#2 2,2,4-Trimethylpentane

R.T.: 7.586 min
Delta R.T.: 0.000 min
Response: 1090666
Conc: 31.44 ng/ml

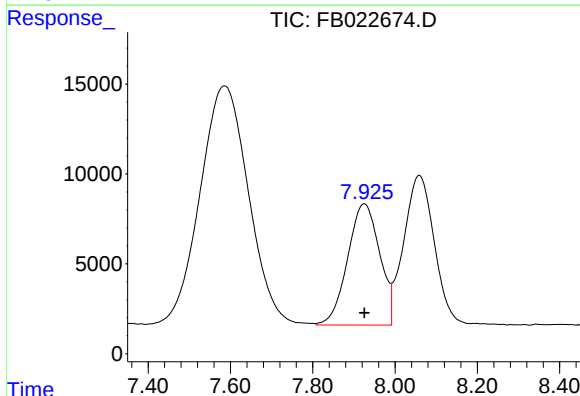


#3 n-Heptane

R.T.: 7.926 min
Delta R.T.: 0.000 min
Response: 365002
Conc: 10.78 ng/ml

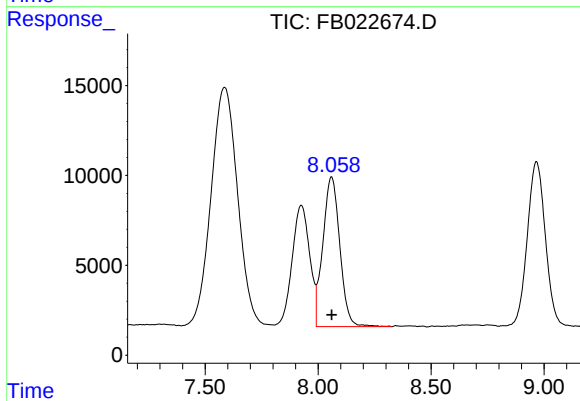


#4 Benzene

R.T.: 8.059 min
Delta R.T.: 0.000 min
Response: 434044
Conc: 10.42 ng/ml

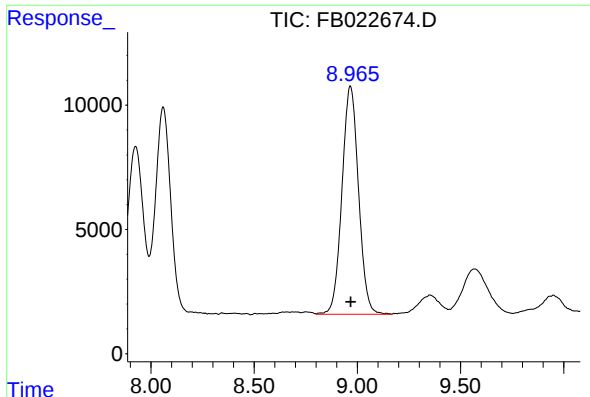


#5 AAA-TFT

R.T.: 8.967 min
Delta R.T.: -0.002 min
Response: 512132
Conc: 21.26 ng/ml

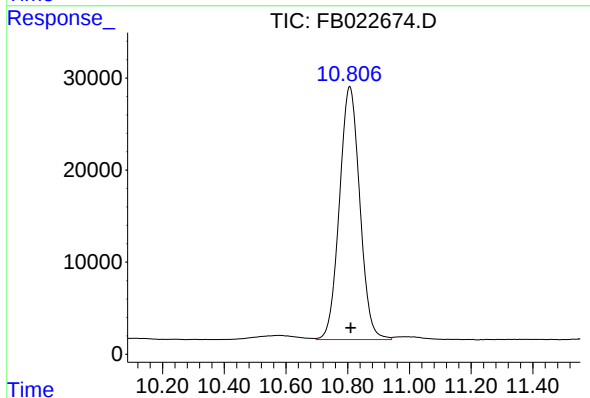


#6 Toluene

R.T.: 10.807 min
Delta R.T.: -0.003 min
Response: 1259363
Conc: 31.11 ng/ml

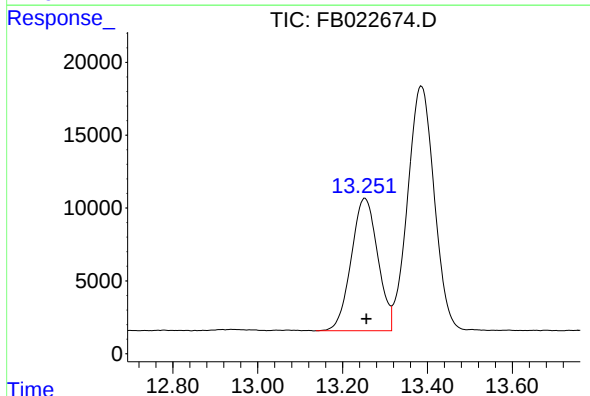


#7 Ethylbenzene

R.T.: 13.253 min
Delta R.T.: -0.003 min
Response: 393972
Conc: 10.18 ng/ml

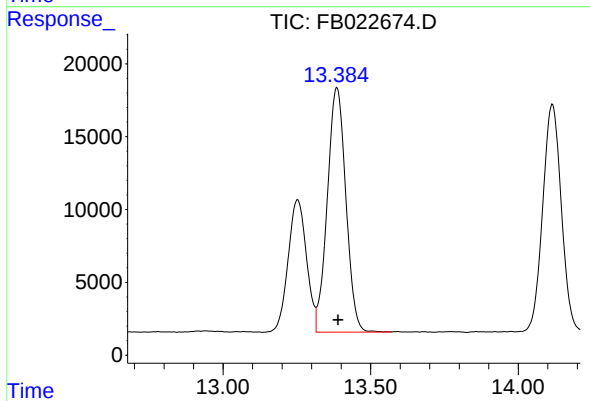


#8 m-Xylene

R.T.: 13.386 min
Delta R.T.: -0.003 min
Response: 733363
Conc: 19.78 ng/ml

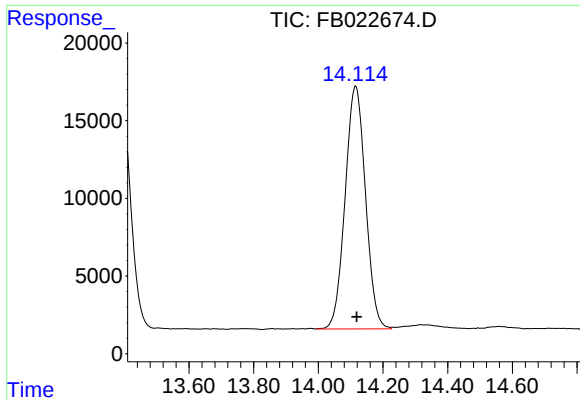

#9 O-Xylene

R.T.: 14.116 min
Delta R.T.: -0.003 min
Response: 683034
Conc: 19.56 ng/ml

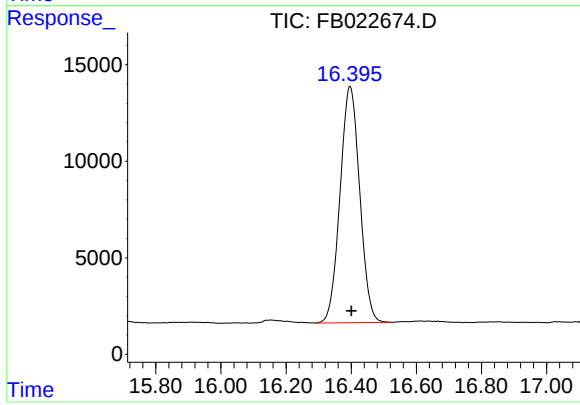

#10 1,2,4-Trimethylbenzene

R.T.: 16.397 min
Delta R.T.: -0.003 min
Response: 513355
Conc: 20.72 ng/ml