

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100319\
 Data File : FB022676.D
 Signal(s) : FID2B.CH
 Acq On : 3 Oct 2019 14:53
 Operator : DD/AJ
 Sample : K5140-02MS
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 04 01:06:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
 Quant Title :
 QLast Update : Wed Oct 02 06:15:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.031	1900462	78.876 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.837	825022	24.740 ng/ml
2) t 2,2,4-Trimethylpentane	7.584	782048	22.546 ng/ml
3) t n-Heptane	7.924	621072	18.341 ng/ml
4) t Benzene	8.057	400574	9.618 ng/ml
6) t Toluene	10.807	2470258	61.027 ng/ml
7) t Ethylbenzene	13.235	9149843	236.427 ng/ml
8) t m-Xylene	13.383	7373992	198.868 ng/ml
9) t O-Xylene	14.116	5326863	152.570 ng/ml
10) t 1,2,4-Trimethylbenzene	16.397	5031667	203.078 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100319\
Data File : FB022676.D
Signal(s) : FID2B.CH
Acq On : 3 Oct 2019 14:53
Operator : DD/AJ
Sample : K5140-02MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 04 01:06:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
Quant Title :
QLast Update : Wed Oct 02 06:15:33 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

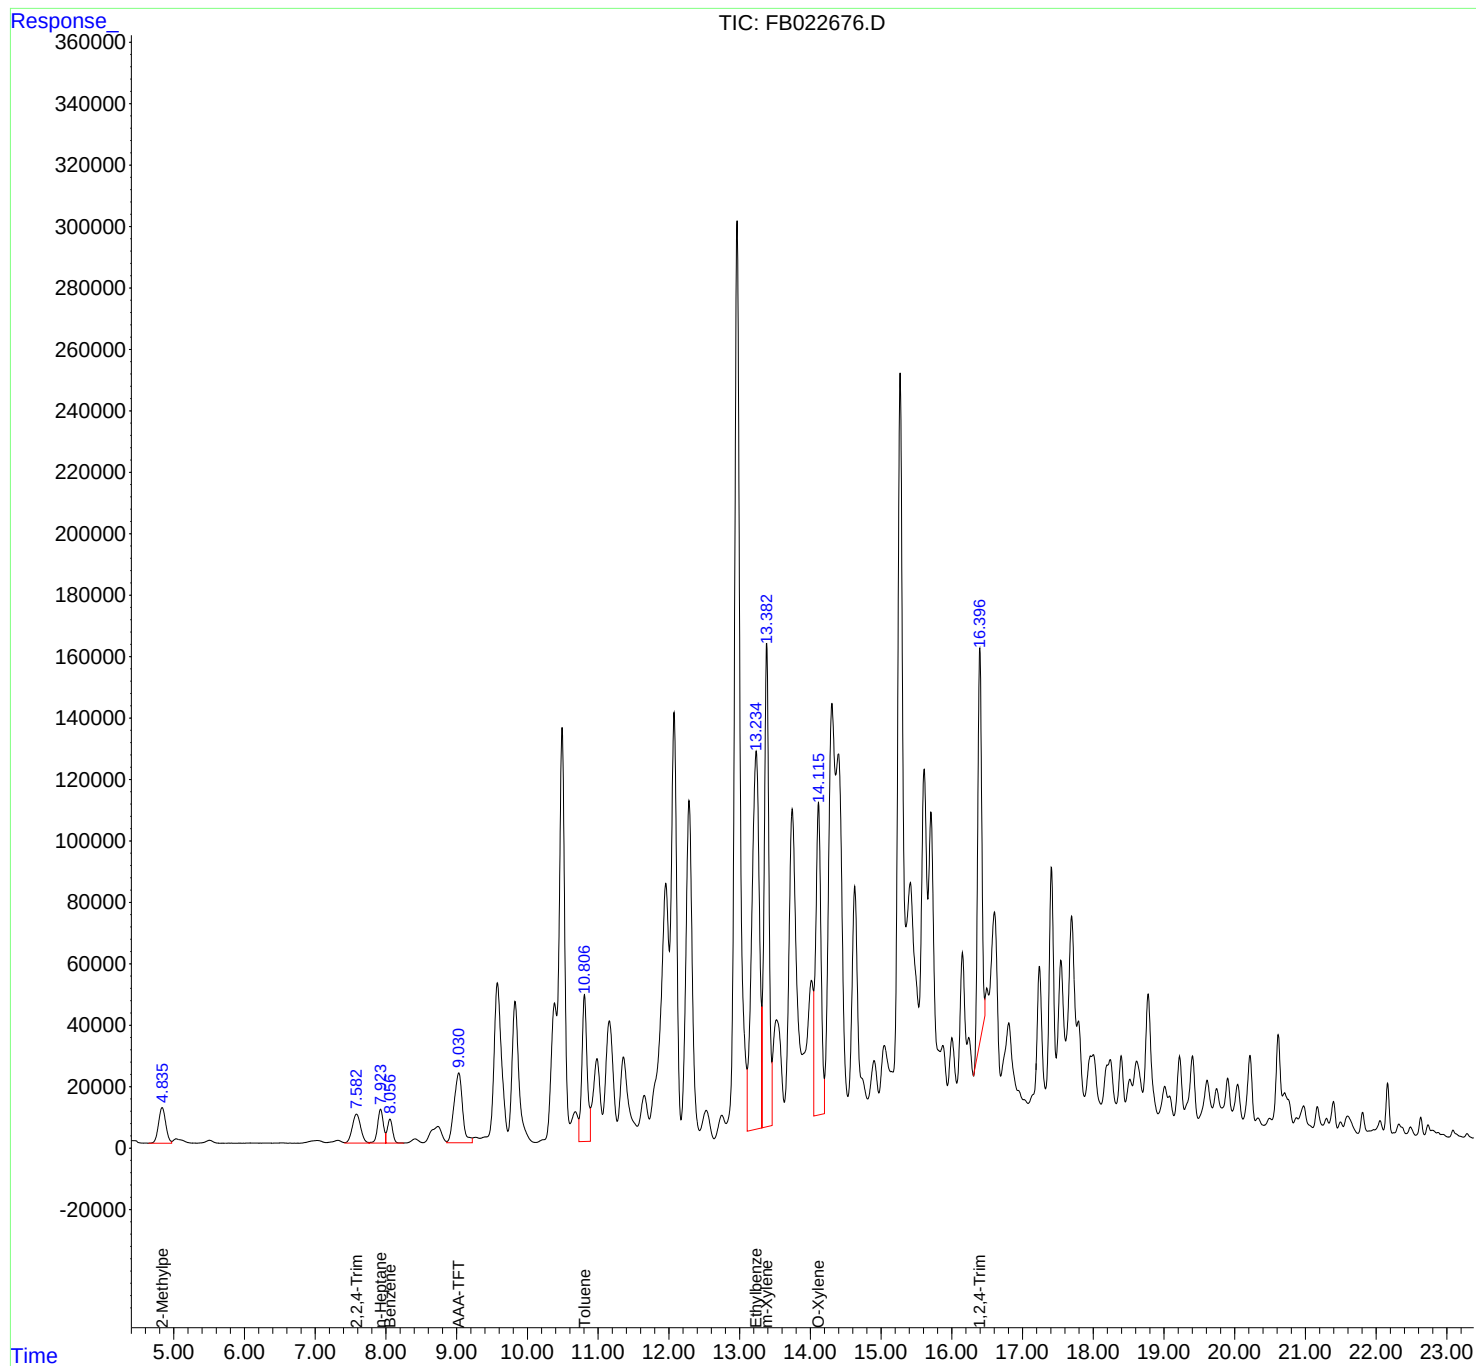

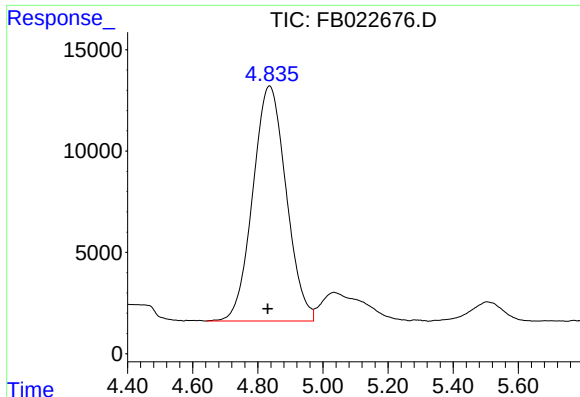


#1 2-Methylpentane

R.T.: 4.837 min
Delta R.T.: 0.007 min
Response: 825022
Conc: 24.74 ng/ml

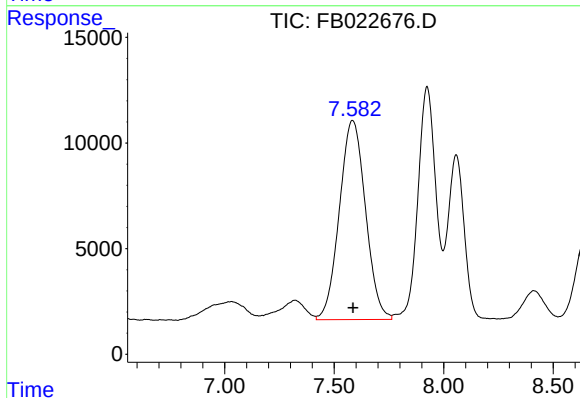


#2 2,2,4-Trimethylpentane

R.T.: 7.584 min
Delta R.T.: -0.002 min
Response: 782048
Conc: 22.55 ng/ml

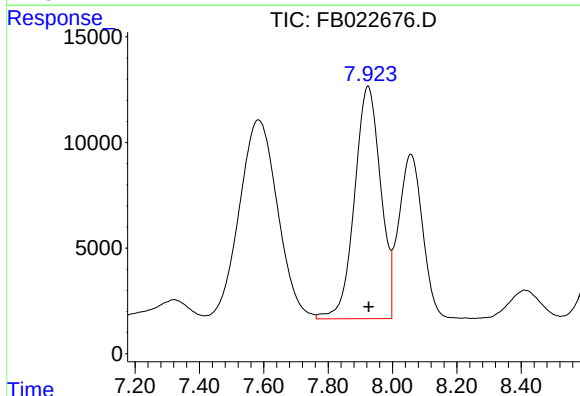


#3 n-Heptane

R.T.: 7.924 min
Delta R.T.: -0.001 min
Response: 621072
Conc: 18.34 ng/ml

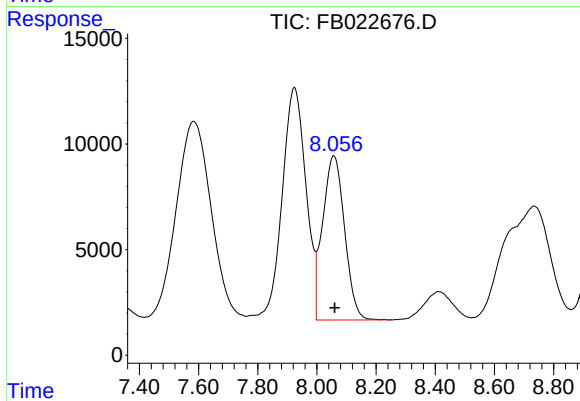


#4 Benzene

R.T.: 8.057 min
Delta R.T.: -0.003 min
Response: 400574
Conc: 9.62 ng/ml

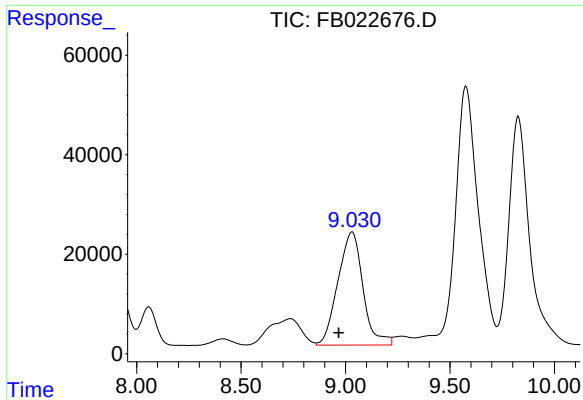


#5 AAA-TFT

R.T.: 9.031 min
Delta R.T.: 0.062 min
Response: 1900462
Conc: 78.88 ng/ml

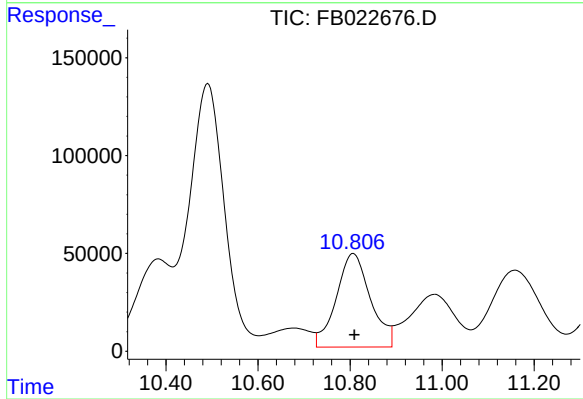


#6 Toluene

R.T.: 10.807 min
Delta R.T.: -0.003 min
Response: 2470258
Conc: 61.03 ng/ml

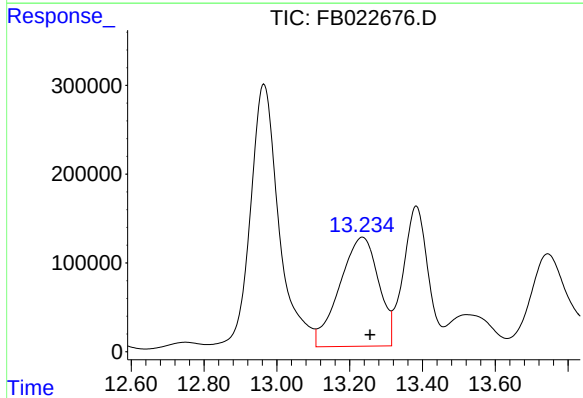


#7 Ethylbenzene

R.T.: 13.235 min
Delta R.T.: -0.021 min
Response: 9149843
Conc: 236.43 ng/ml

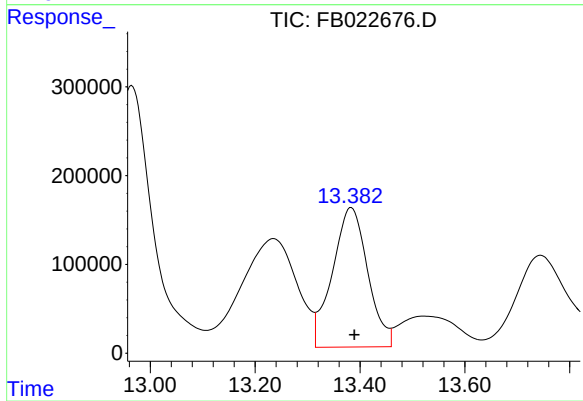


#8 m-Xylene

R.T.: 13.383 min
Delta R.T.: -0.006 min
Response: 7373992
Conc: 198.87 ng/ml

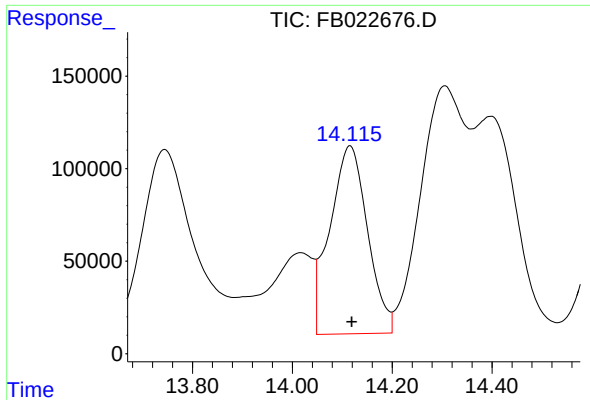

#9 O-Xylene

R.T.: 14.116 min
Delta R.T.: -0.004 min
Response: 5326863
Conc: 152.57 ng/ml

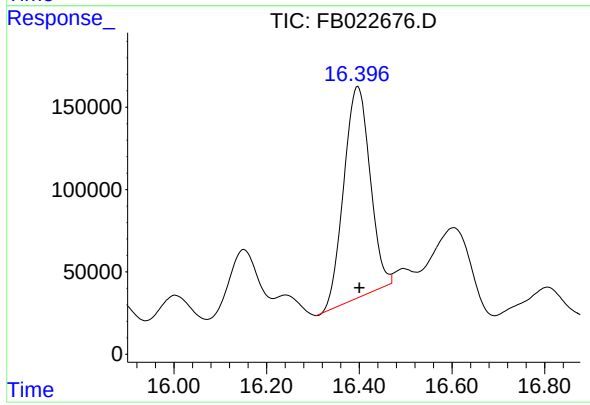

#10 1,2,4-Trimethylbenzene

R.T.: 16.397 min
Delta R.T.: -0.004 min
Response: 5031667
Conc: 203.08 ng/ml