

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100319\
 Data File : FB022677.D
 Signal(s) : FID2B.CH
 Acq On : 3 Oct 2019 15:22
 Operator : DD/AJ
 Sample : K5140-02MSD
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 04 01:06:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
 Quant Title :
 QLast Update : Wed Oct 02 06:15:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.029	1734147	71.974 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.837	771000	23.120 ng/ml
2) t 2,2,4-Trimethylpentane	7.584	701122	20.213 ng/ml
3) t n-Heptane	7.925	536591	15.846 ng/ml
4) t Benzene	8.058	394146	9.464 ng/ml
6) t Toluene	10.807	2294109	56.676 ng/ml
7) t Ethylbenzene	13.236	8555079	221.058 ng/ml
8) t m-Xylene	13.384	7079798	190.934 ng/ml
9) t O-Xylene	14.116	5179973	148.363 ng/ml
10) t 1,2,4-Trimethylbenzene	16.397	5225982	210.921 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100319\
Data File : FB022677.D
Signal(s) : FID2B.CH
Acq On : 3 Oct 2019 15:22
Operator : DD/AJ
Sample : K5140-02MSD
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 04 01:06:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
Quant Title :
QLast Update : Wed Oct 02 06:15:33 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

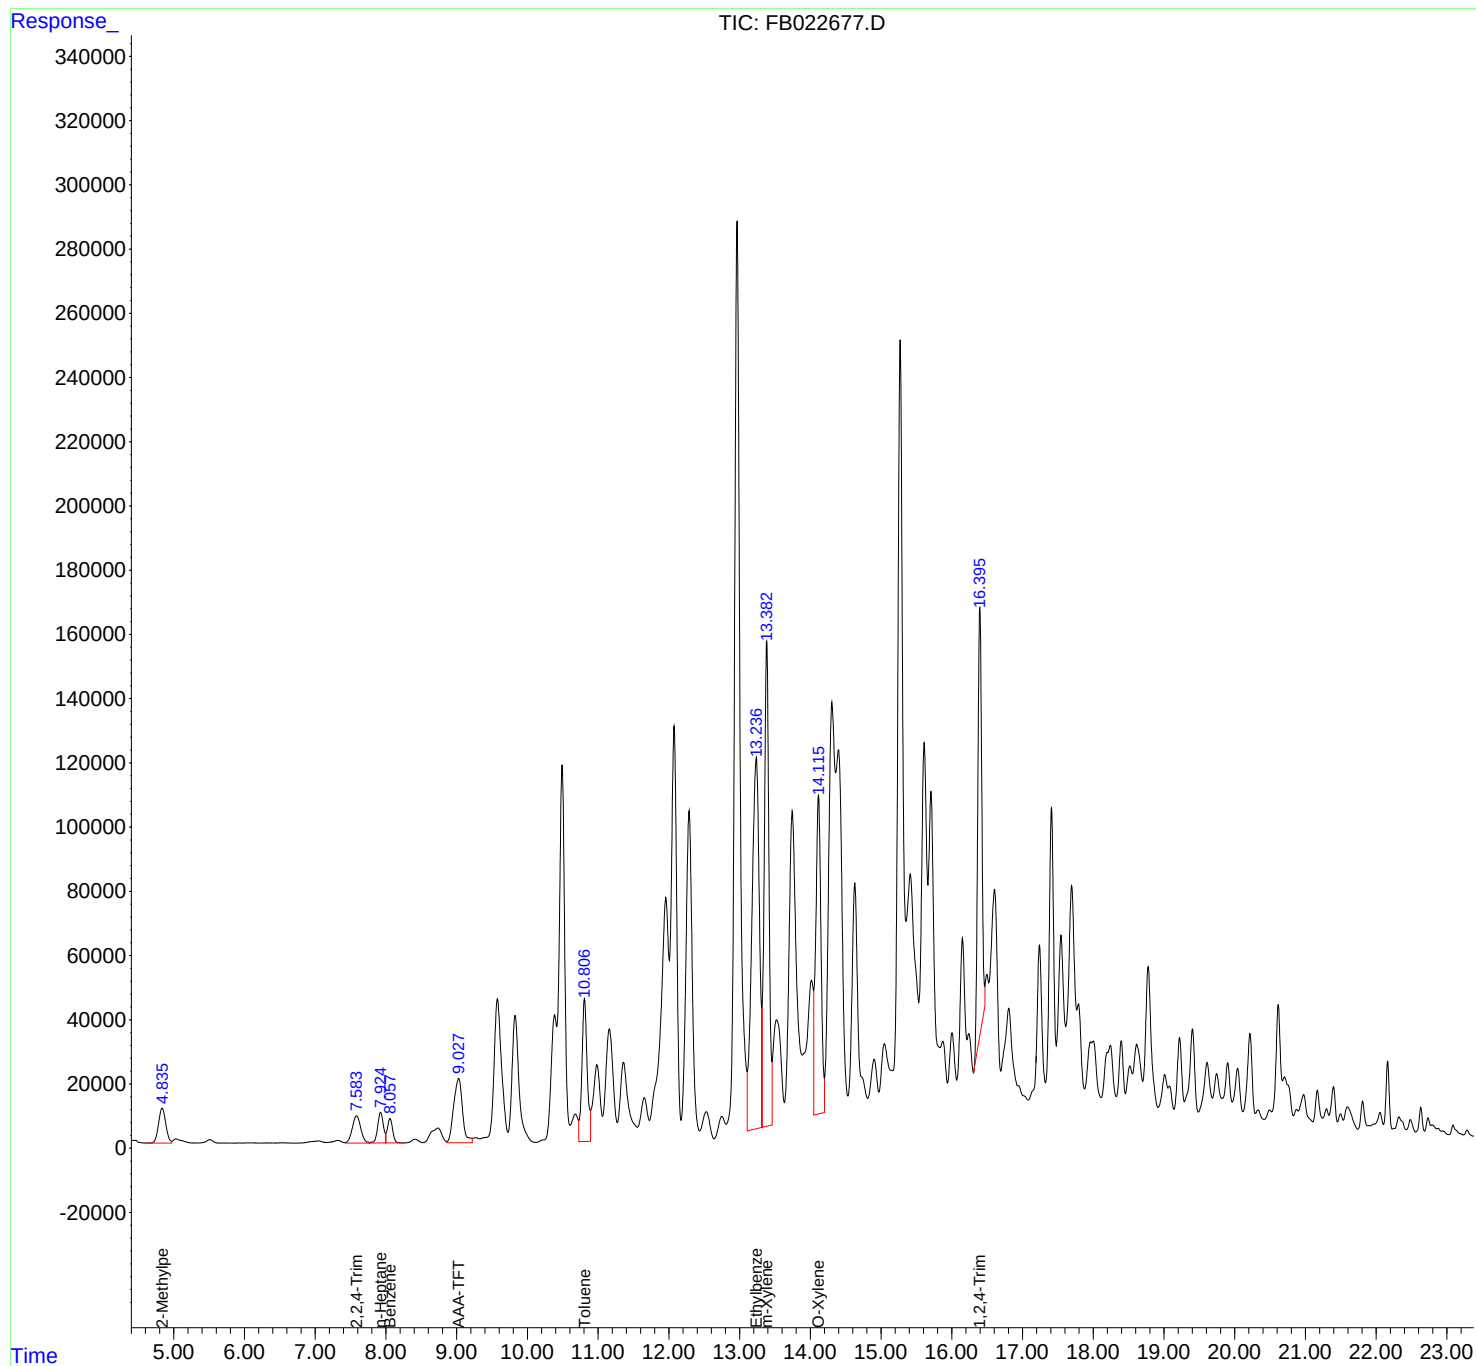

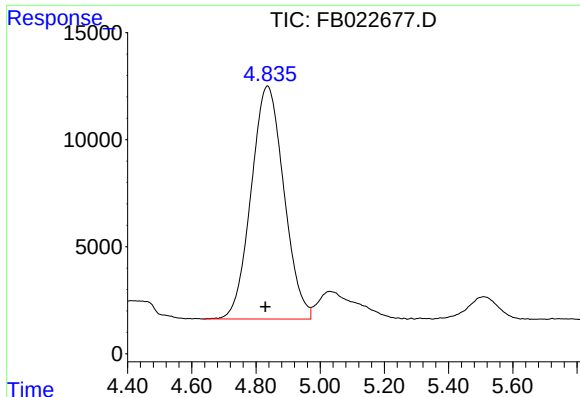


#1 2-Methylpentane

R.T.: 4.837 min
Delta R.T.: 0.007 min
Response: 771000
Conc: 23.12 ng/ml

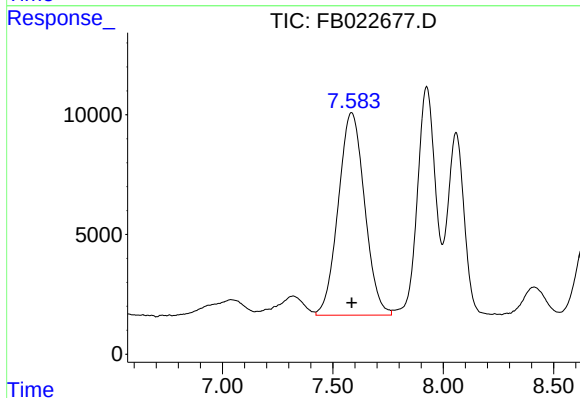


#2 2,2,4-Trimethylpentane

R.T.: 7.584 min
Delta R.T.: -0.001 min
Response: 701122
Conc: 20.21 ng/ml

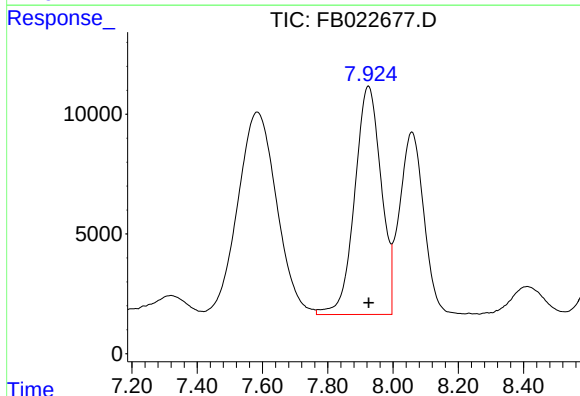


#3 n-Heptane

R.T.: 7.925 min
Delta R.T.: 0.000 min
Response: 536591
Conc: 15.85 ng/ml

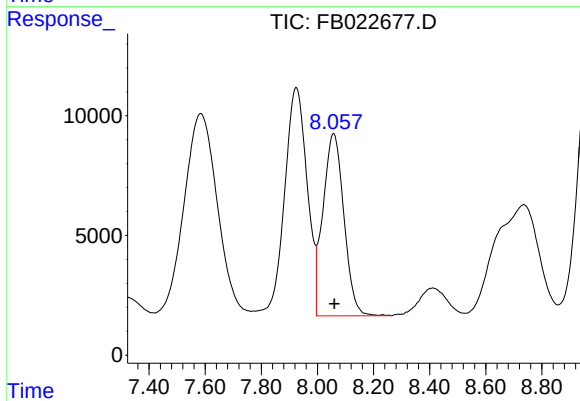


#4 Benzene

R.T.: 8.058 min
Delta R.T.: -0.002 min
Response: 394146
Conc: 9.46 ng/ml

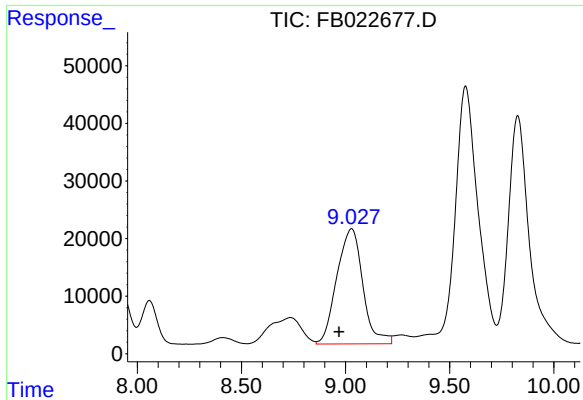


#5 AAA-TFT

R.T.: 9.029 min
Delta R.T.: 0.060 min
Response: 1734147
Conc: 71.97 ng/ml

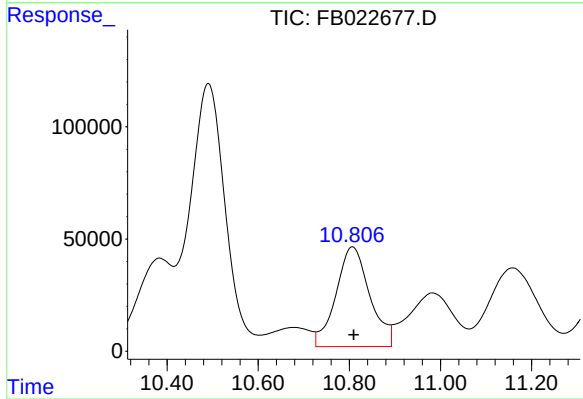


#6 Toluene

R.T.: 10.807 min
Delta R.T.: -0.002 min
Response: 2294109
Conc: 56.68 ng/ml

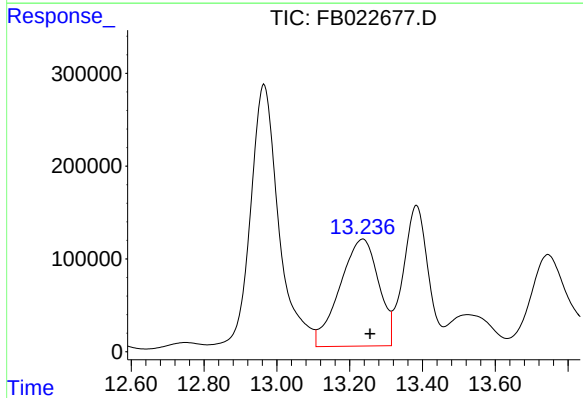


#7 Ethylbenzene

R.T.: 13.236 min
Delta R.T.: -0.020 min
Response: 8555079
Conc: 221.06 ng/ml

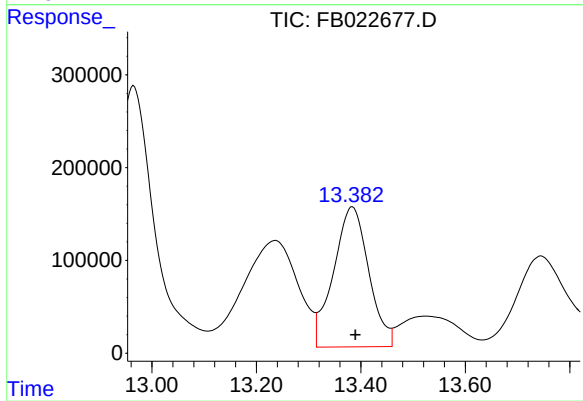


#8 m-Xylene

R.T.: 13.384 min
Delta R.T.: -0.006 min
Response: 7079798
Conc: 190.93 ng/ml

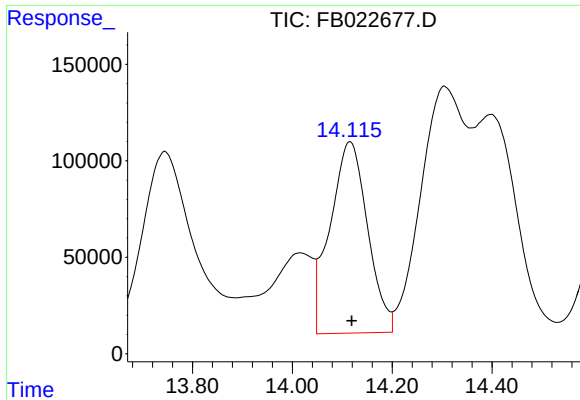

#9 O-Xylene

R.T.: 14.116 min
Delta R.T.: -0.003 min
Response: 5179973
Conc: 148.36 ng/ml

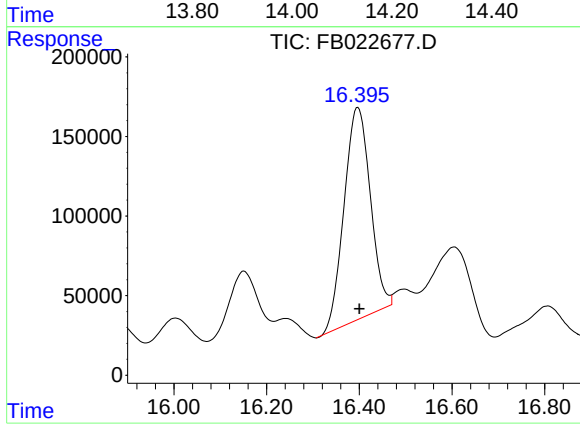

#10 1,2,4-Trimethylbenzene

R.T.: 16.397 min
Delta R.T.: -0.003 min
Response: 5225982
Conc: 210.92 ng/ml