

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100323\
 Data File : FB030375.D
 Signal(s) : FID2B.CH
 Acq On : 3 Oct 2023 12:10
 Operator : YP/AJ
 Sample : BSF1003S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 04 01:34:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
 Quant Title :
 QLast Update : Mon Sep 18 13:44:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	245376	17.740 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	534367	29.192 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	608587	30.083 ng/ml
3) t n-Heptane	7.748	202273	9.520 ng/ml
4) t Benzene	7.883	246741	9.693 ng/ml
6) t Toluene	10.616	719233	29.018 ng/ml
7) t Ethylbenzene	13.052	226725	9.740 ng/ml
8) t m-Xylene	13.185	445085	19.405 ng/ml
9) t O-Xylene	13.912	427631	19.259 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	415695	18.971 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100323\
Data File : FB030375.D
Signal(s) : FID2B.CH
Acq On : 3 Oct 2023 12:10
Operator : YP/AJ
Sample : BSF1003S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 04 01:34:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
Quant Title :
QLast Update : Mon Sep 18 13:44:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

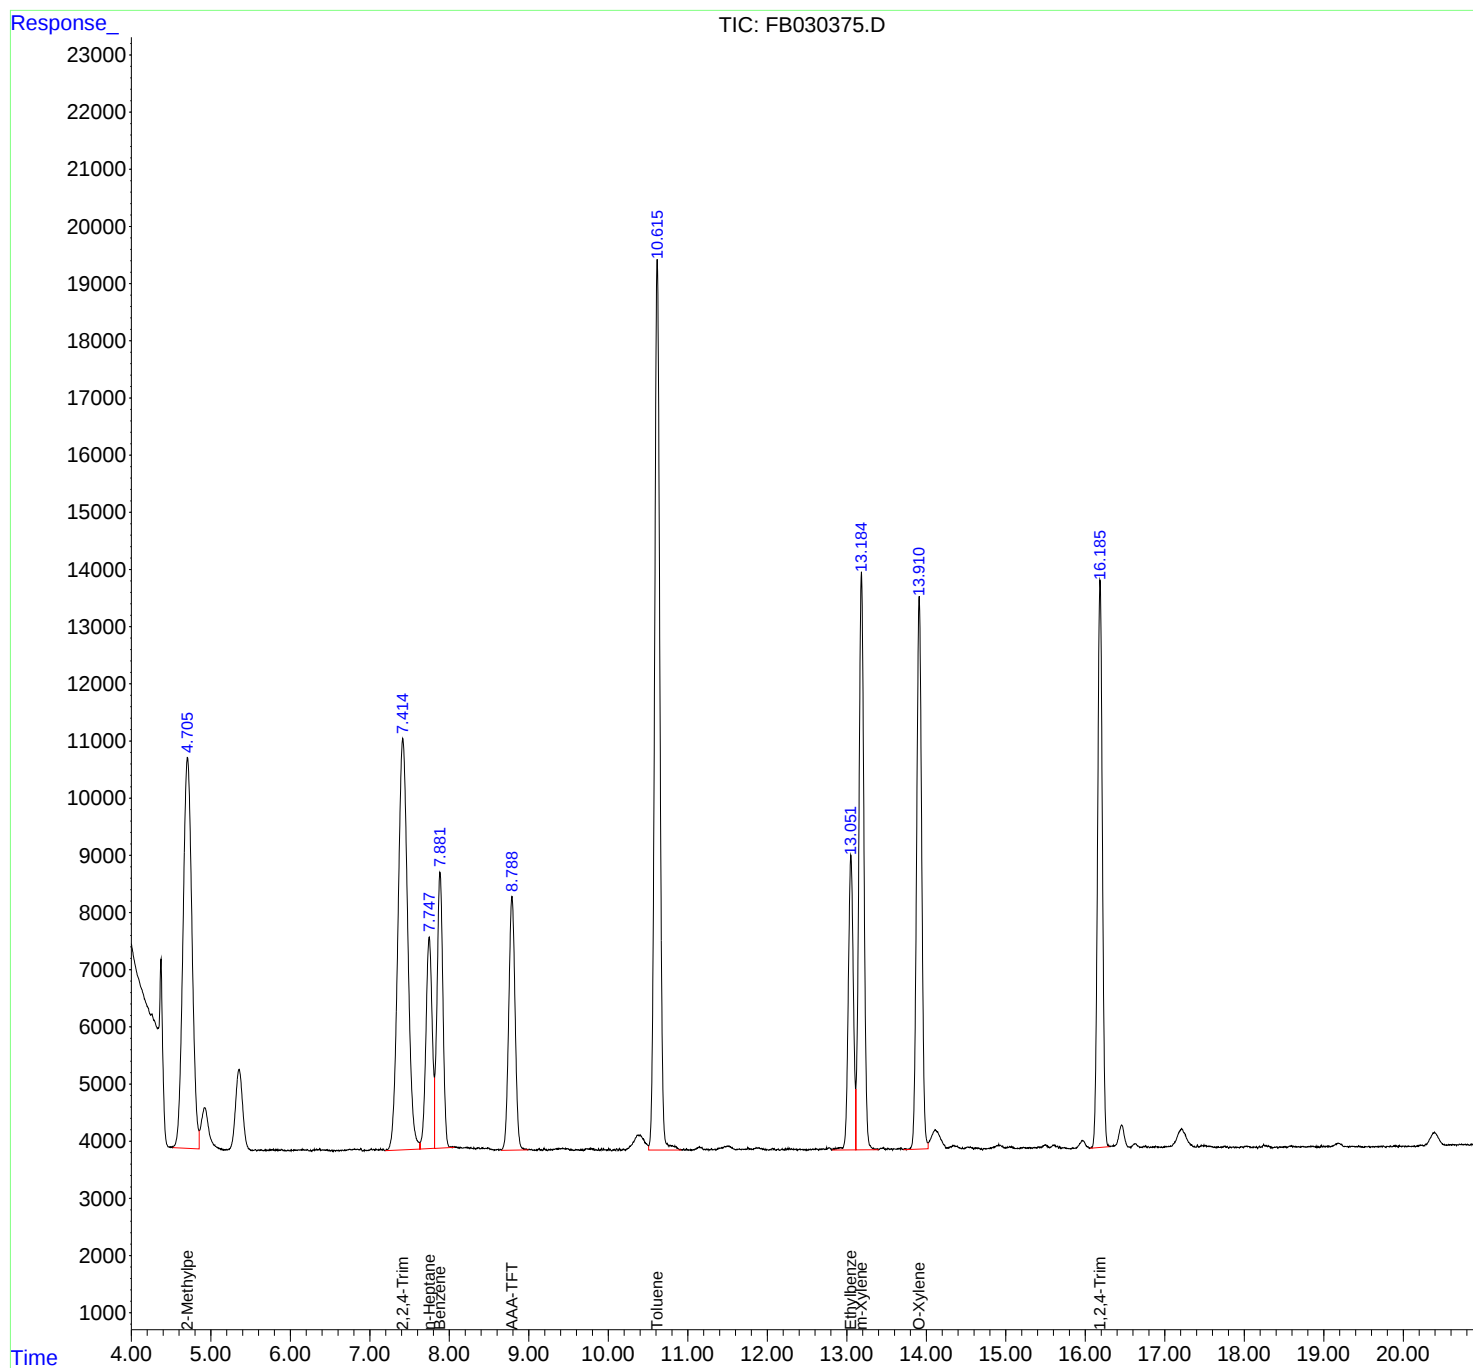


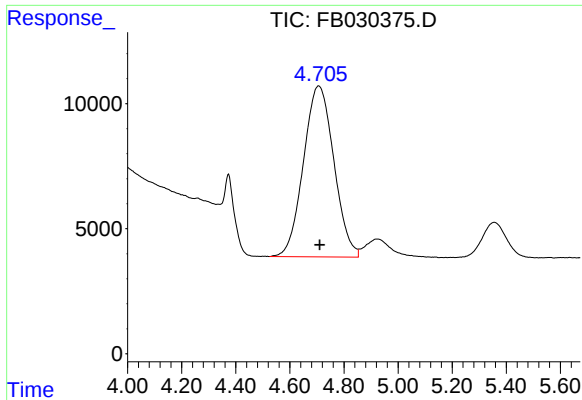

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: -0.003 min
Response: 534367
Conc: 29.19 ng/ml

Instrument :
FID_B
ClientSampleId :

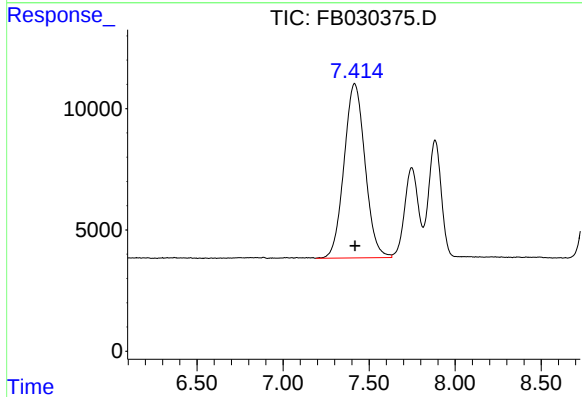


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 608587
Conc: 30.08 ng/ml

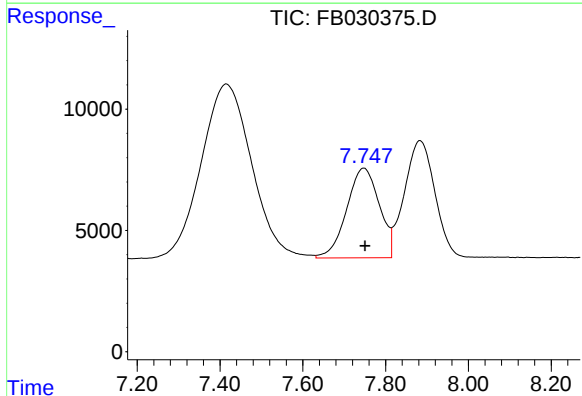


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.003 min
Response: 202273
Conc: 9.52 ng/ml

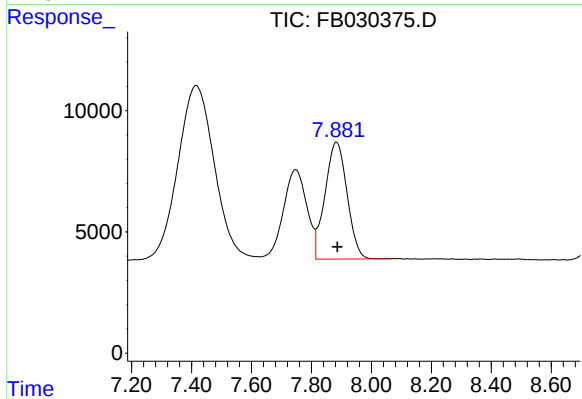

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.003 min
Response: 246741
Conc: 9.69 ng/ml

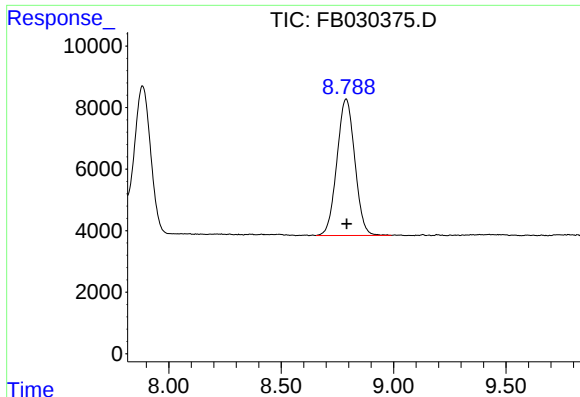

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.002 min
Response: 245376
Conc: 17.74 ng/ml

Instrument :
FID_B
ClientSampleId :

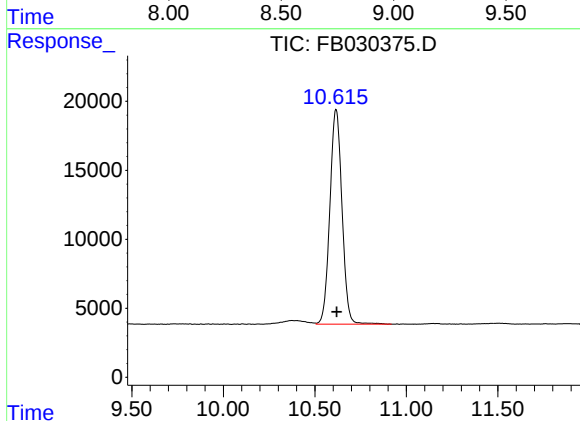


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.004 min
Response: 719233
Conc: 29.02 ng/ml

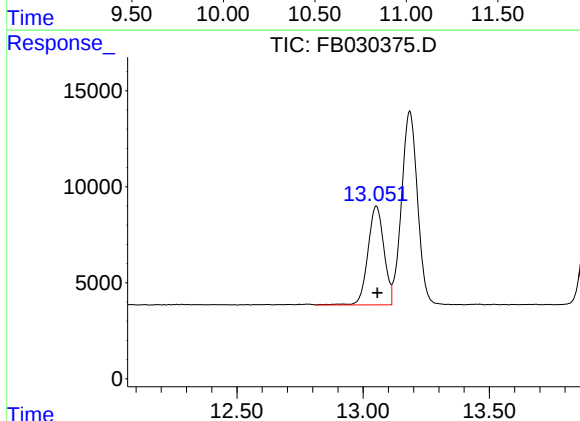


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.004 min
Response: 226725
Conc: 9.74 ng/ml

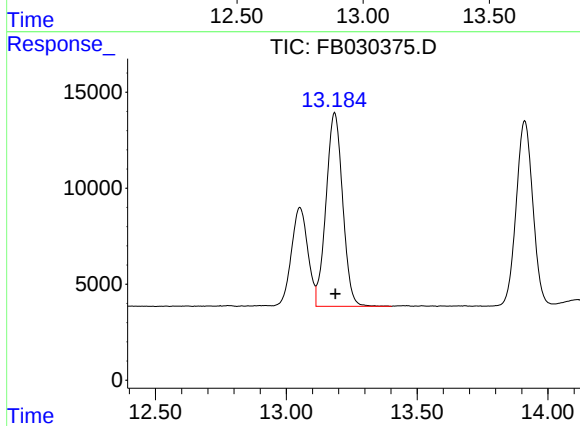

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.003 min
Response: 445085
Conc: 19.41 ng/ml

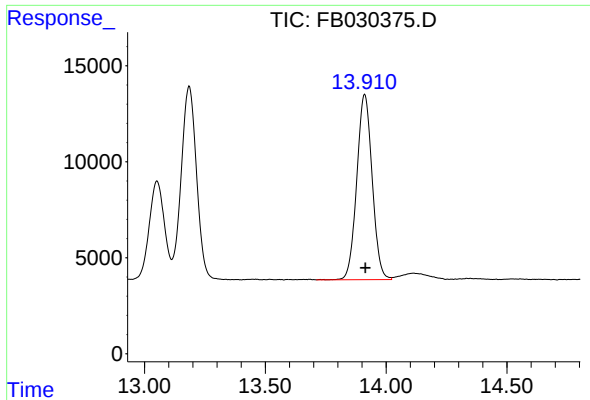

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.004 min
Response: 427631
Conc: 19.26 ng/ml

Instrument :
FID_B
ClientSampleId :

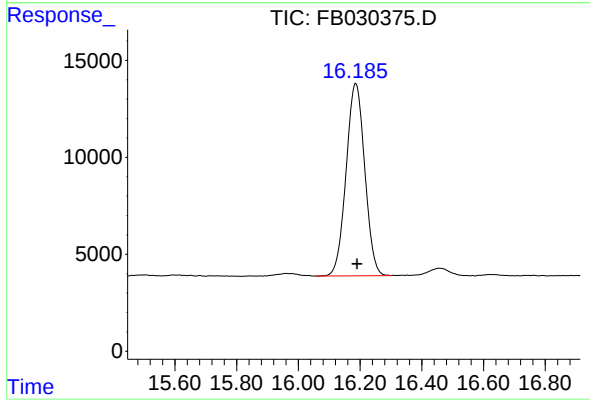

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: -0.004 min
Response: 415695
Conc: 18.97 ng/ml