

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100323\
 Data File : FB030377.D
 Signal(s) : FID2B.CH
 Acq On : 3 Oct 2023 13:28
 Operator : YP/AJ
 Sample : 04699-07
 Misc : 1 PPB WATER LOD
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 04 01:35:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
 Quant Title :
 QLast Update : Mon Sep 18 13:44:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	231364	16.727 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.715	23428	1.280 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	21930	1.084 ng/ml
3) t n-Heptane	7.747	8717	0.410 ng/ml
4) t Benzene	7.885	9767	0.384 ng/ml
6) t Toluene	10.622	28367	1.144 ng/ml
7) t Ethylbenzene	13.053	8381	0.360 ng/ml
8) t m-Xylene	13.187	16635	0.725 ng/ml
9) t O-Xylene	13.915	17792	0.801 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	20844	0.951 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100323\
Data File : FB030377.D
Signal(s) : FID2B.CH
Acq On : 3 Oct 2023 13:28
Operator : YP/AJ
Sample : 04699-07
Misc : 1 PPB WATER LOD
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 04 01:35:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
Quant Title :
QLast Update : Mon Sep 18 13:44:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

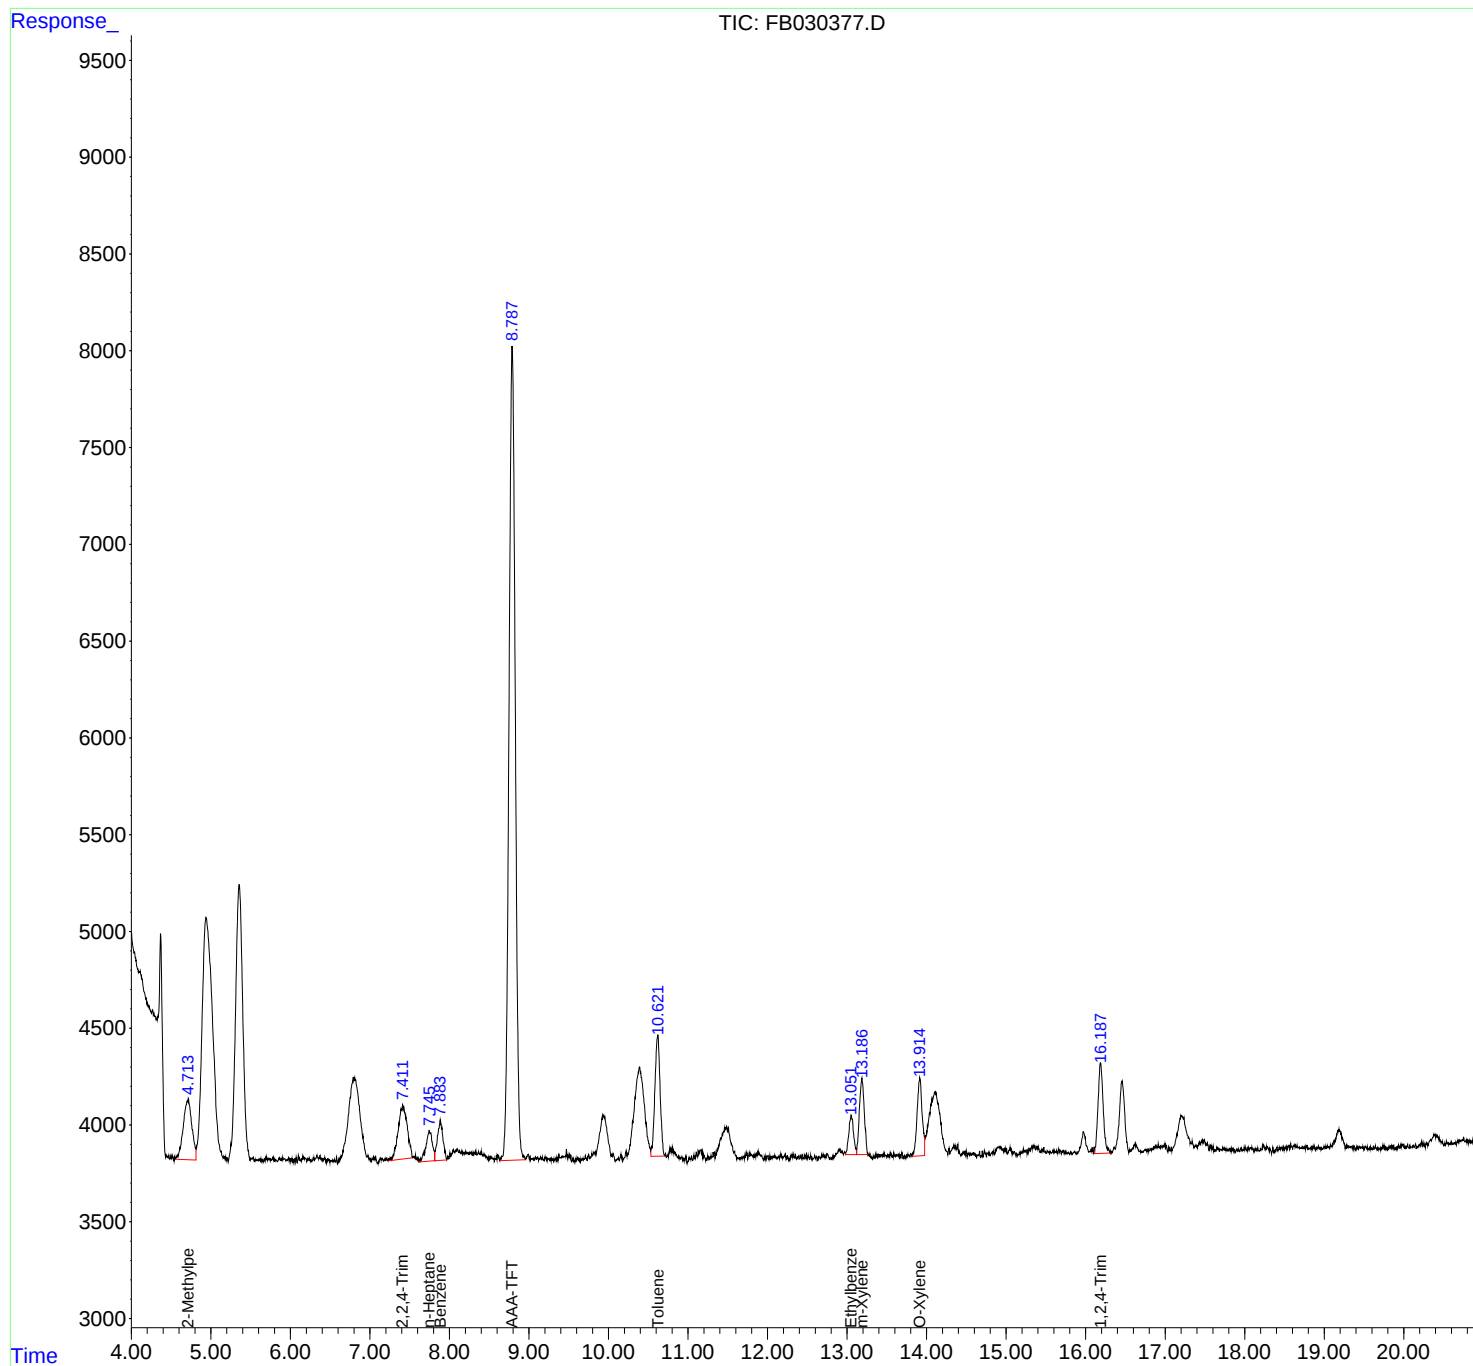


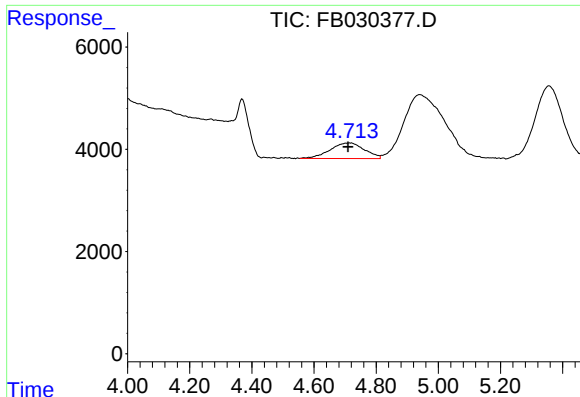

#1 2-Methylpentane


R.T.: 4.715 min
Delta R.T.: 0.005 min
Response: 23428
Conc: 1.28 ng/ml

Instrument :
FID_B
ClientSampleId :

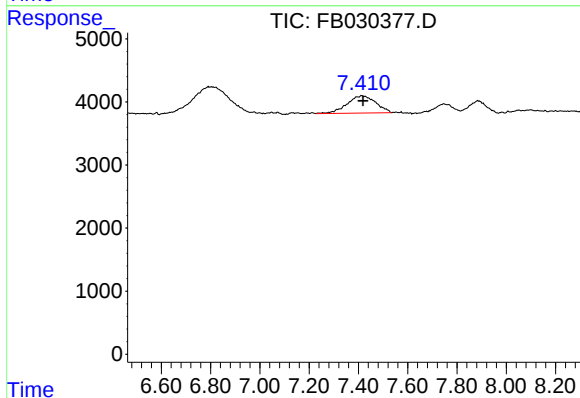


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.006 min
Response: 21930
Conc: 1.08 ng/ml

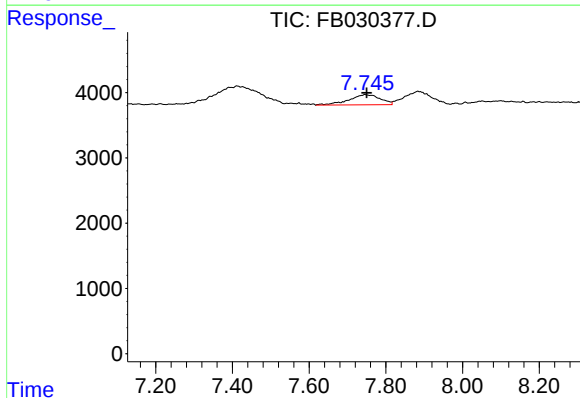


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.004 min
Response: 8717
Conc: 0.41 ng/ml

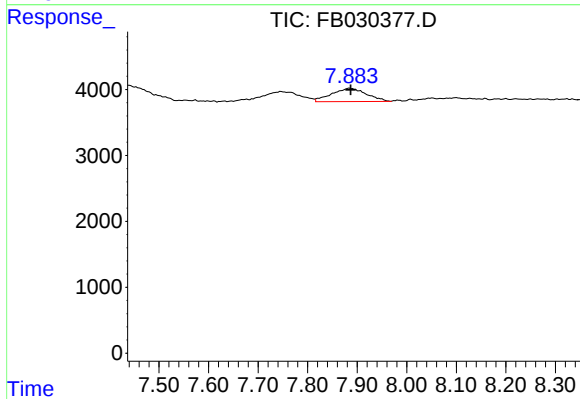

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.002 min
Response: 9767
Conc: 0.38 ng/ml

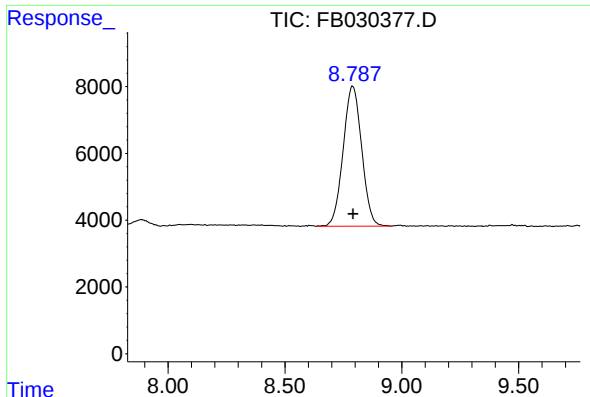

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.003 min
Response: 231364
Conc: 16.73 ng/ml

Instrument :
FID_B
ClientSampleId :

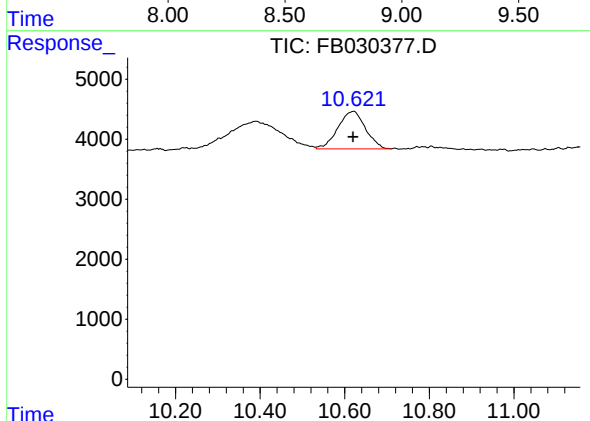


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.002 min
Response: 28367
Conc: 1.14 ng/ml

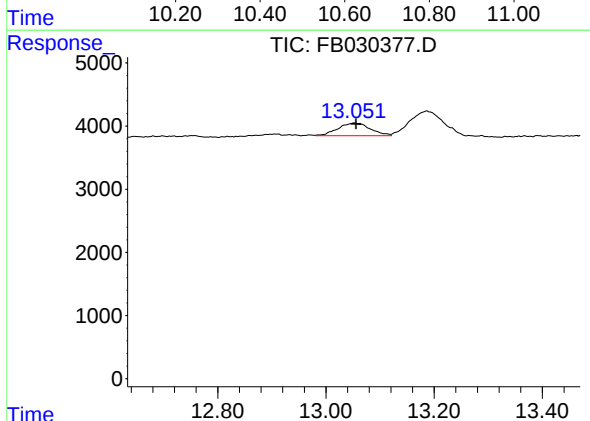


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.003 min
Response: 8381
Conc: 0.36 ng/ml

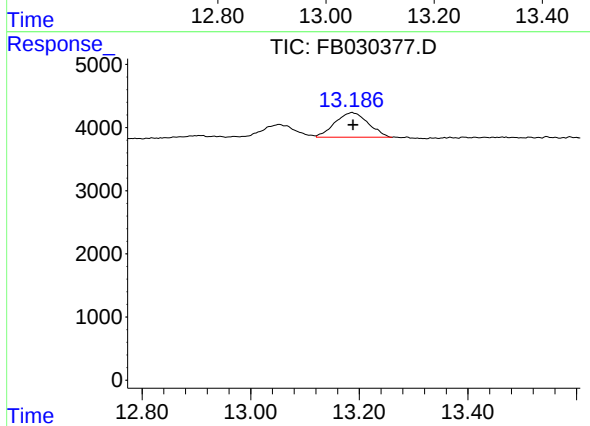

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.001 min
Response: 16635
Conc: 0.73 ng/ml

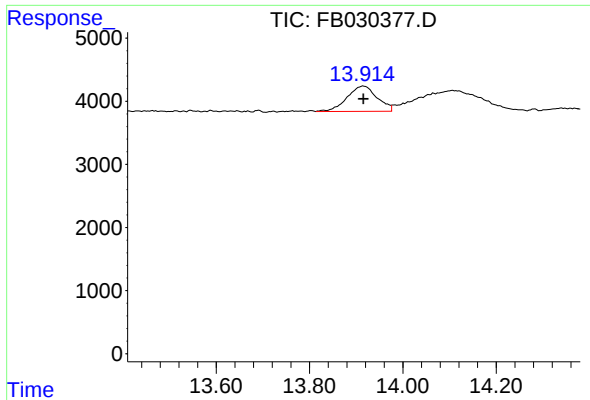

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: 0.000 min
Response: 17792
Conc: 0.80 ng/ml

Instrument :
FID_B
ClientSampleId :

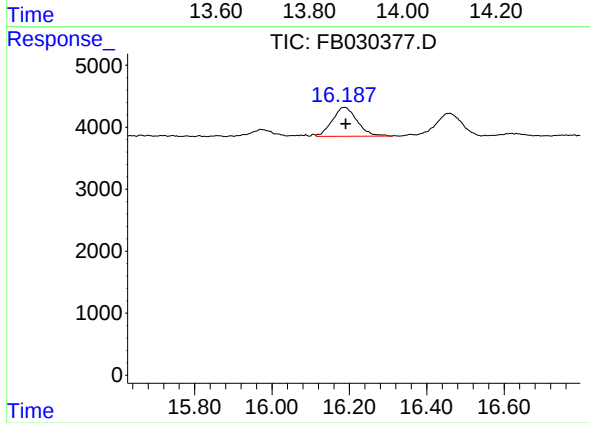

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.002 min
Response: 20844
Conc: 0.95 ng/ml