

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB100323\  
 Data File : FB030383.D  
 Signal(s) : FID2B.CH  
 Acq On : 3 Oct 2023 20:04  
 Operator : YP/AJ  
 Sample : BSF1003S3  
 Misc : 5 PPB WATER LOQ  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Oct 04 01:37:56 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB091823.M  
 Quant Title :  
 QLast Update : Mon Sep 18 13:44:02 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.794  | 270422   | 19.551 ng/ml |
| Target Compounds             |        |          |              |
| 1) t 2-Methylpentane         | 4.713  | 557272   | 30.444 ng/ml |
| 2) t 2,2,4-Trimethylpentane  | 7.423  | 652330   | 32.245 ng/ml |
| 3) t n-Heptane               | 7.753  | 221647   | 10.432 ng/ml |
| 4) t Benzene                 | 7.889  | 281832   | 11.071 ng/ml |
| 6) t Toluene                 | 10.622 | 823244   | 33.214 ng/ml |
| 7) t Ethylbenzene            | 13.057 | 254051   | 10.914 ng/ml |
| 8) t m-Xylene                | 13.190 | 504078   | 21.977 ng/ml |
| 9) t O-Xylene                | 13.917 | 482667   | 21.737 ng/ml |
| 10) t 1,2,4-Trimethylbenzene | 16.192 | 433462   | 19.782 ng/ml |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB100323\  
Data File : FB030383.D  
Signal(s) : FID2B.CH  
Acq On : 3 Oct 2023 20:04  
Operator : YP/AJ  
Sample : BSF1003S3  
Misc : 5 PPB WATER LOQ  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Oct 04 01:37:56 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB091823.M  
Quant Title :  
QLast Update : Mon Sep 18 13:44:02 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

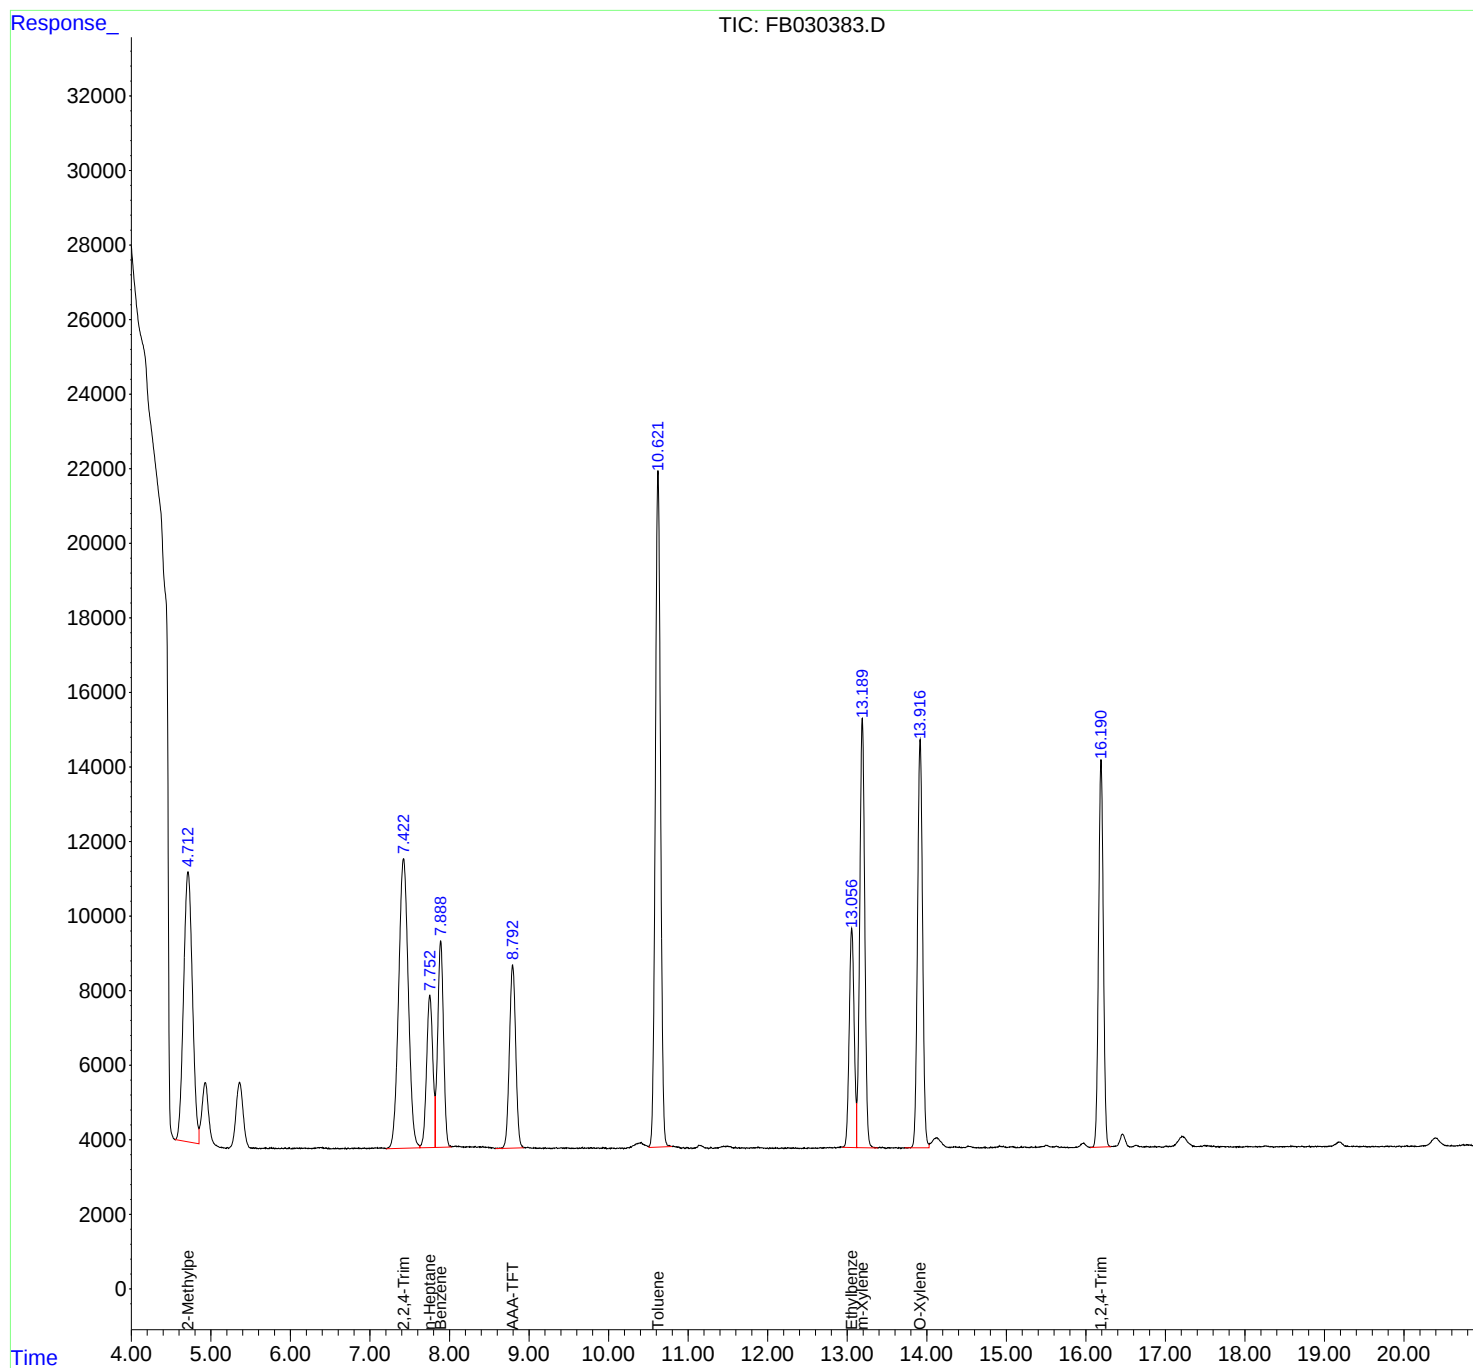


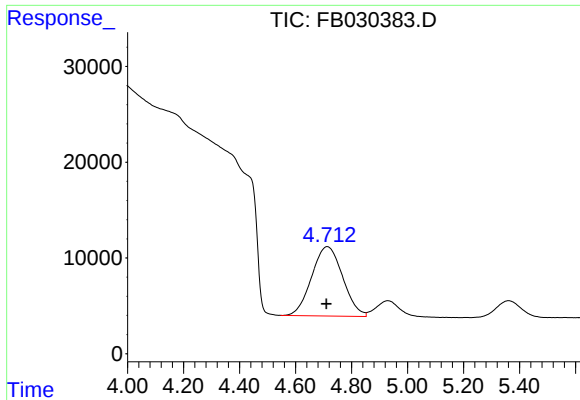

#1 2-Methylpentane


R.T.: 4.713 min  
Delta R.T.: 0.003 min  
Response: 557272  
Conc: 30.44 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

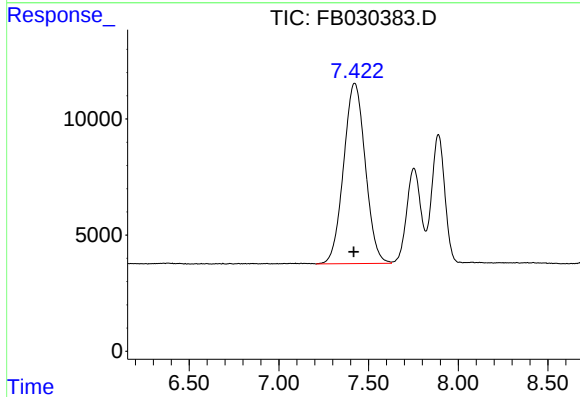


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min  
Delta R.T.: 0.004 min  
Response: 652330  
Conc: 32.24 ng/ml

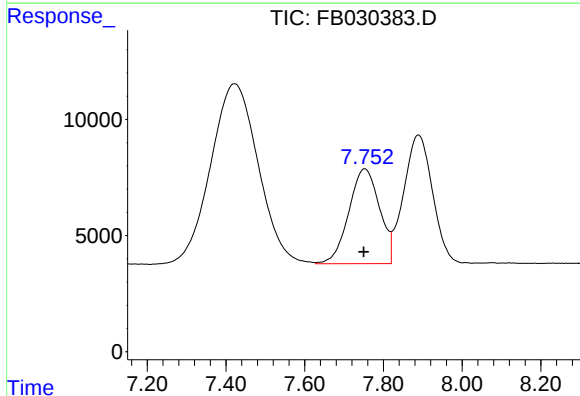


#3 n-Heptane

R.T.: 7.753 min  
Delta R.T.: 0.003 min  
Response: 221647  
Conc: 10.43 ng/ml

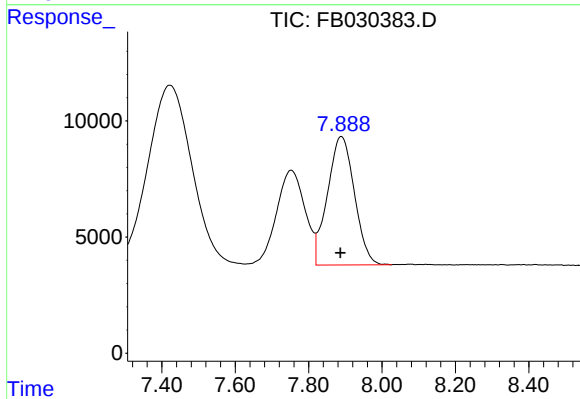

#4 Benzene


R.T.: 7.889 min  
Delta R.T.: 0.003 min  
Response: 281832  
Conc: 11.07 ng/ml

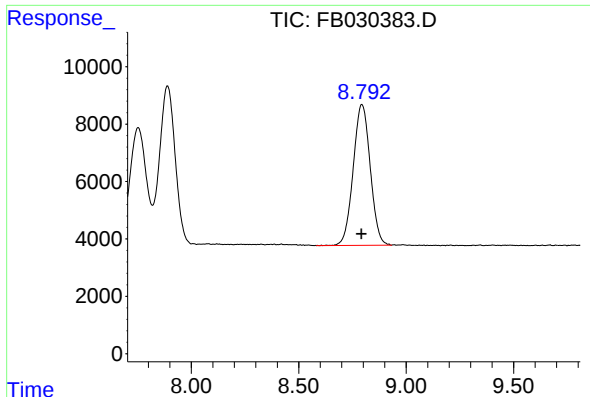

#5 AAA-TFT


R.T.: 8.794 min  
Delta R.T.: 0.002 min  
Response: 270422  
Conc: 19.55 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

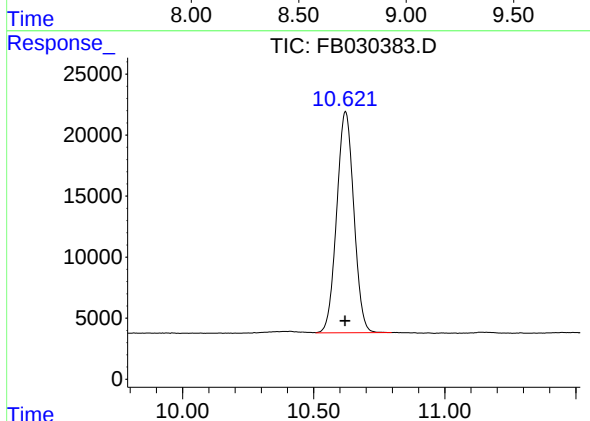


#6 Toluene

R.T.: 10.622 min  
Delta R.T.: 0.002 min  
Response: 823244  
Conc: 33.21 ng/ml

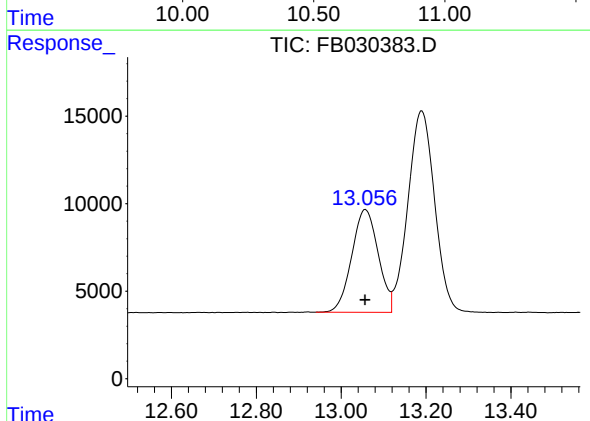


#7 Ethylbenzene

R.T.: 13.057 min  
Delta R.T.: 0.001 min  
Response: 254051  
Conc: 10.91 ng/ml

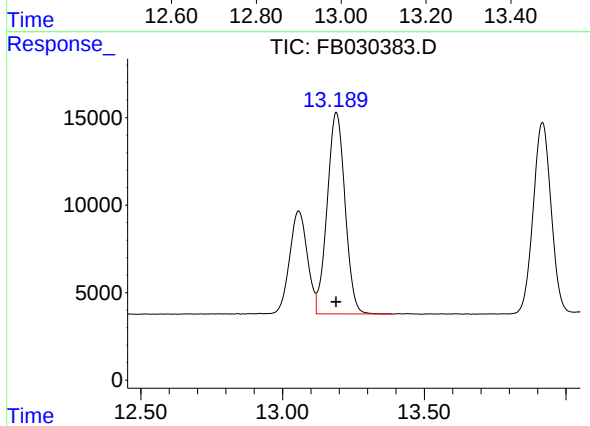

#8 m-Xylene


R.T.: 13.190 min  
Delta R.T.: 0.002 min  
Response: 504078  
Conc: 21.98 ng/ml

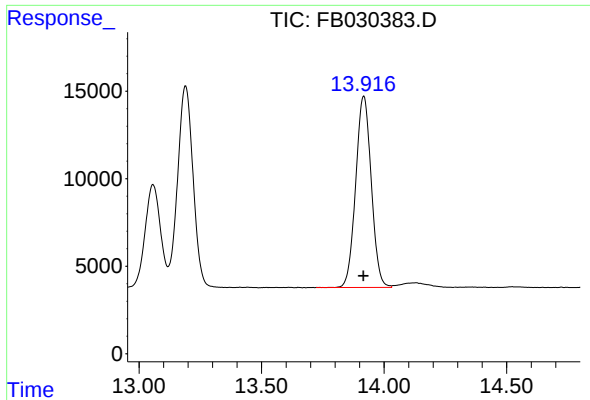

#9 O-Xylene

R.T.: 13.917 min  
Delta R.T.: 0.002 min  
Response: 482667  
Conc: 21.74 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

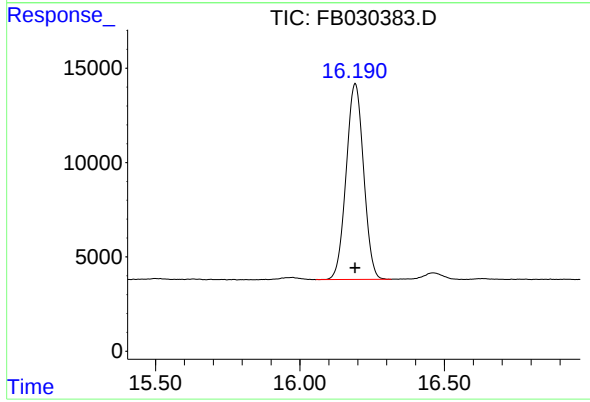

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min  
Delta R.T.: 0.000 min  
Response: 433462  
Conc: 19.78 ng/ml