

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100323\
 Data File : FB030374.D
 Signal(s) : FID2B.CH
 Acq On : 3 Oct 2023 11:31
 Operator : YP/AJ
 Sample : BSF1003W1
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1003W1

Integration File: Calibration.e
 Quant Time: Oct 04 01:34:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
 Quant Title :
 QLast Update : Mon Sep 18 13:44:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	285858	20.667 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	525191	28.691 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	568953	28.124 ng/ml
3) t n-Heptane	7.746	198444	9.340 ng/ml
4) t Benzene	7.882	239733	9.417 ng/ml
6) t Toluene	10.615	713545	28.788 ng/ml
7) t Ethylbenzene	13.051	222679	9.566 ng/ml
8) t m-Xylene	13.184	439110	19.145 ng/ml
9) t O-Xylene	13.911	422021	19.006 ng/ml
10) t 1,2,4-Trimethylbenzene	16.185	408545	18.645 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100323\
Data File : FB030374.D
Signal(s) : FID2B.CH
Acq On : 3 Oct 2023 11:31
Operator : YP/AJ
Sample : BSF1003W1
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1003W1

Integration File: Calibration.e
Quant Time: Oct 04 01:34:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
Quant Title :
QLast Update : Mon Sep 18 13:44:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

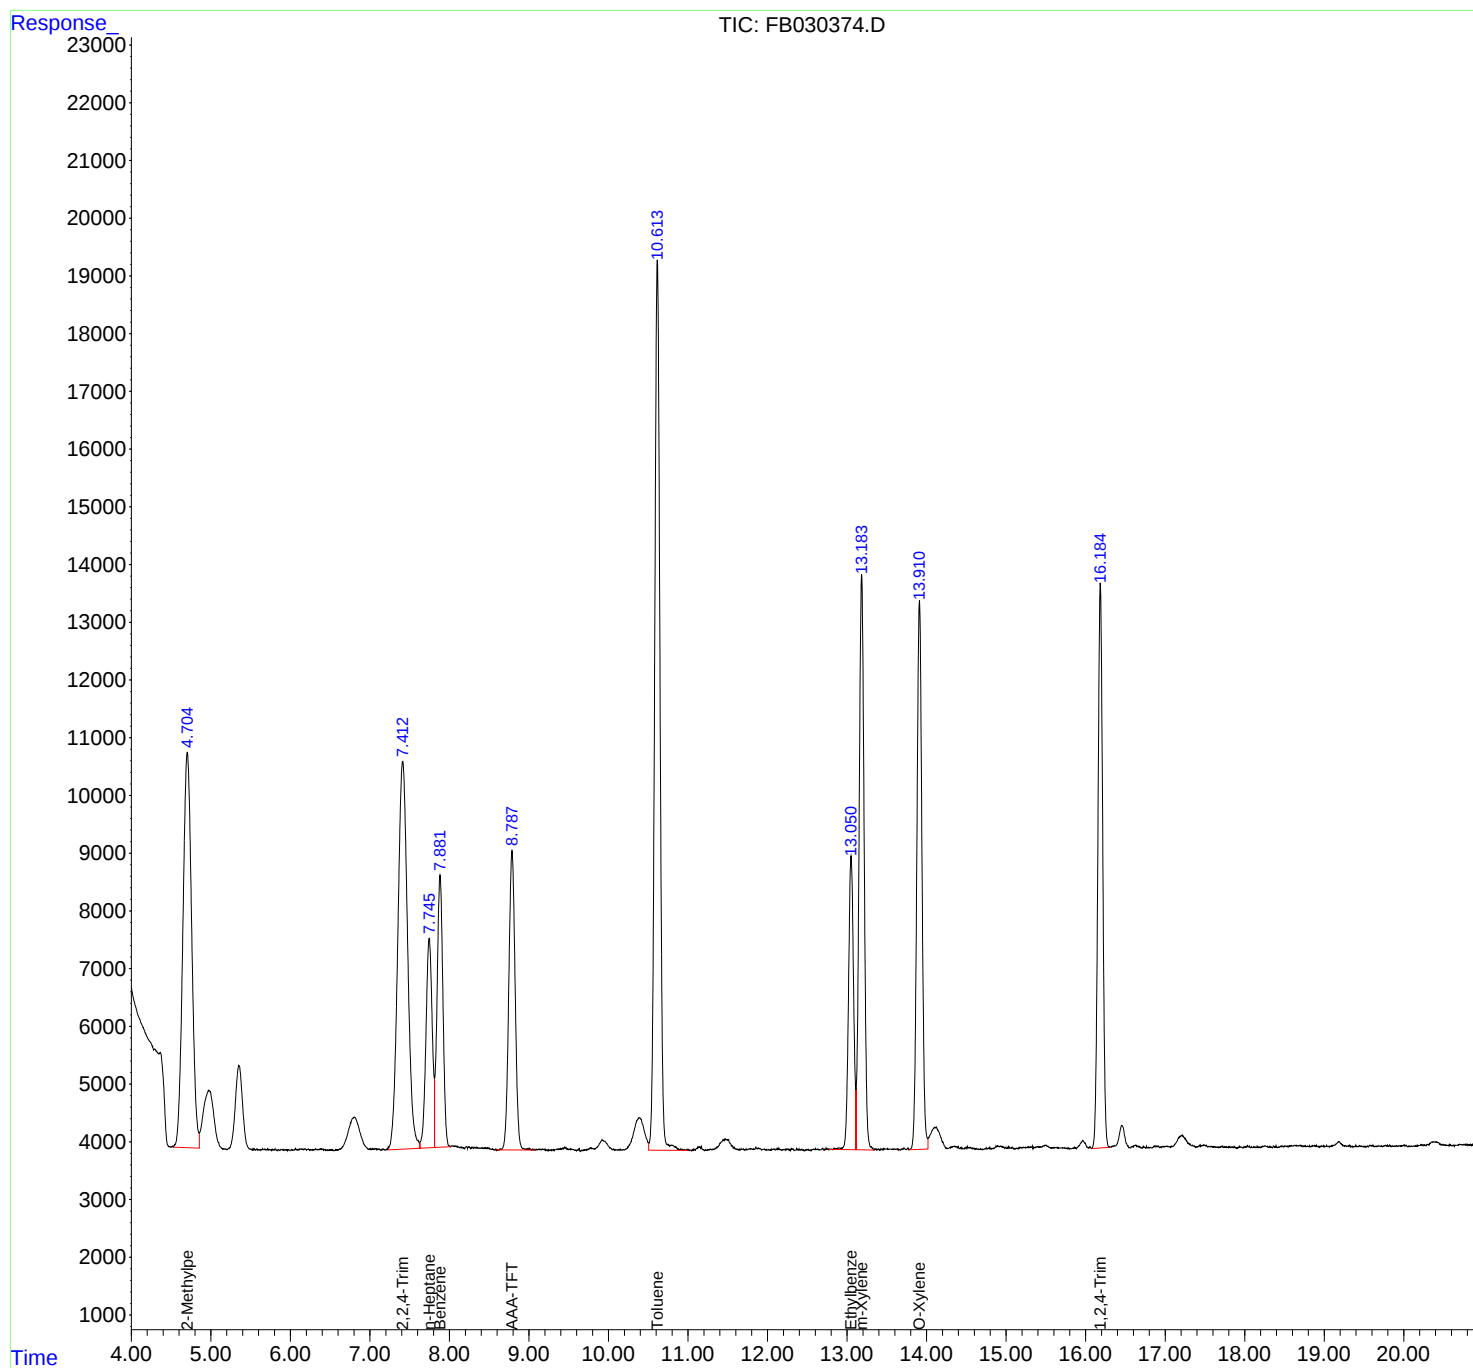


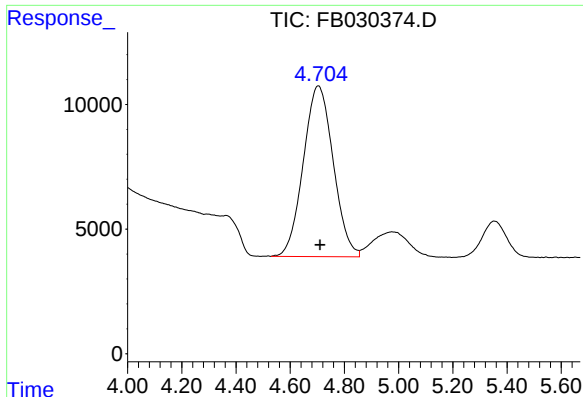

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.005 min
Response: 525191
Conc: 28.69 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1003W1

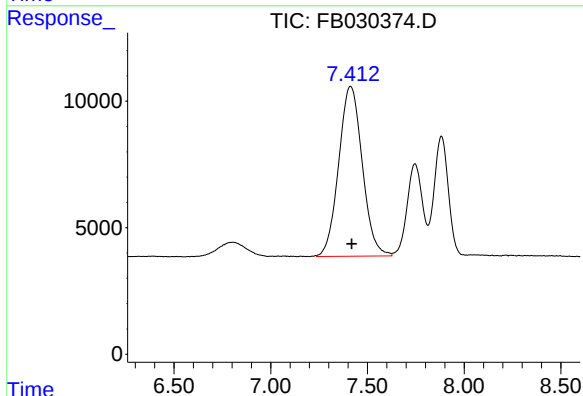


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.006 min
Response: 568953
Conc: 28.12 ng/ml

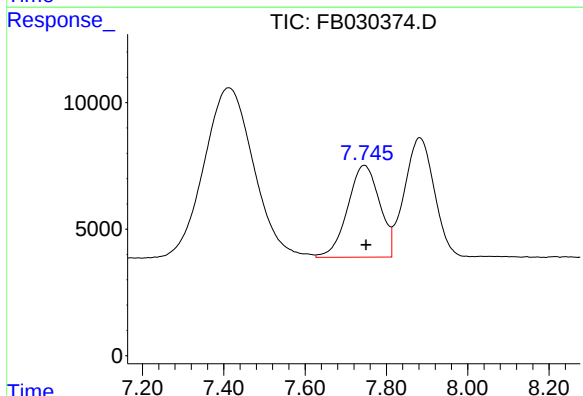


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.004 min
Response: 198444
Conc: 9.34 ng/ml

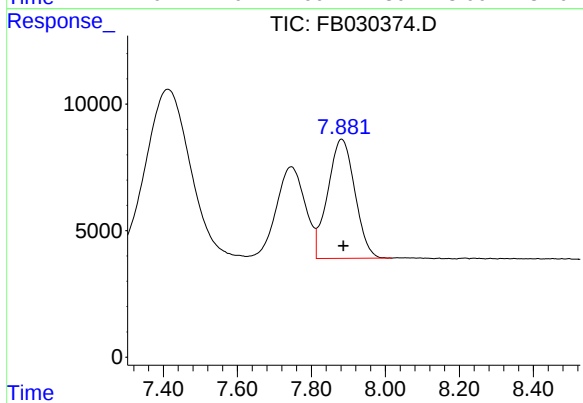

#4 Benzene


R.T.: 7.882 min
Delta R.T.: -0.005 min
Response: 239733
Conc: 9.42 ng/ml

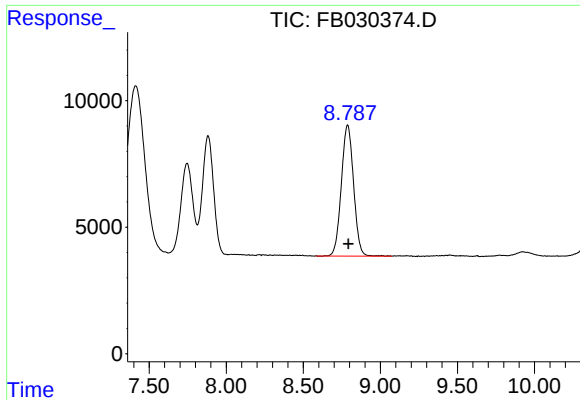

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: -0.004 min
Response: 285858
Conc: 20.67 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1003W1

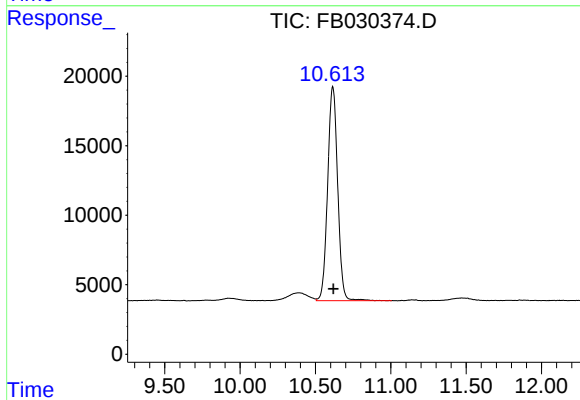


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.005 min
Response: 713545
Conc: 28.79 ng/ml

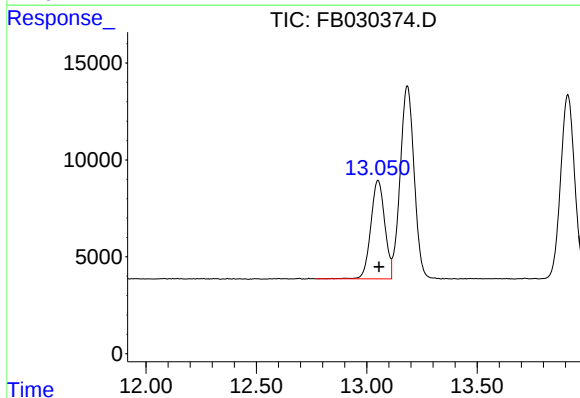


#7 Ethylbenzene

R.T.: 13.051 min
Delta R.T.: -0.005 min
Response: 222679
Conc: 9.57 ng/ml

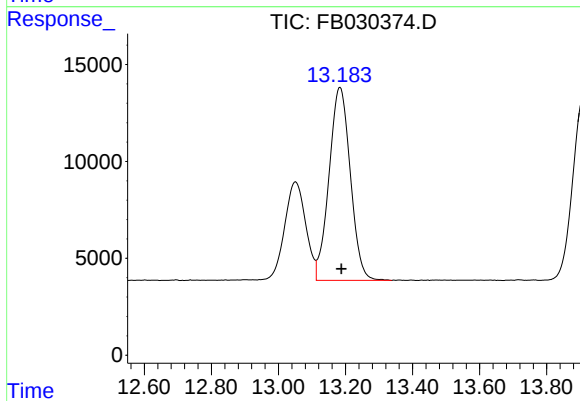

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: -0.004 min
Response: 439110
Conc: 19.14 ng/ml

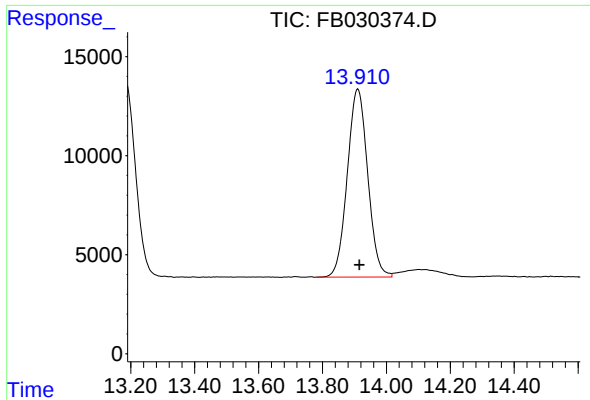

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: -0.004 min
Response: 422021
Conc: 19.01 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1003W1

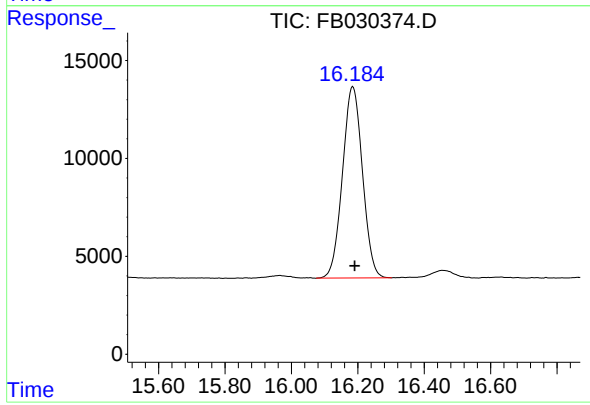

#10 1,2,4-Trimethylbenzene

R.T.: 16.185 min
Delta R.T.: -0.005 min
Response: 408545
Conc: 18.65 ng/ml