

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB100323\  
 Data File : FB030375.D  
 Signal(s) : FID2B.CH  
 Acq On : 3 Oct 2023 12:10  
 Operator : YP/AJ  
 Sample : BSF1003S1  
 Misc : 5.00G/5.00 ML DI WATER  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :  
 BSF1003S1

Integration File: Calibration.e  
 Quant Time: Oct 04 01:34:31 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB091823.M  
 Quant Title :  
 QLast Update : Mon Sep 18 13:44:02 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.789  | 245376   | 17.740 ng/ml |
| Target Compounds             |        |          |              |
| 1) t 2-Methylpentane         | 4.707  | 534367   | 29.192 ng/ml |
| 2) t 2,2,4-Trimethylpentane  | 7.415  | 608587   | 30.083 ng/ml |
| 3) t n-Heptane               | 7.748  | 202273   | 9.520 ng/ml  |
| 4) t Benzene                 | 7.883  | 246741   | 9.693 ng/ml  |
| 6) t Toluene                 | 10.616 | 719233   | 29.018 ng/ml |
| 7) t Ethylbenzene            | 13.052 | 226725   | 9.740 ng/ml  |
| 8) t m-Xylene                | 13.185 | 445085   | 19.405 ng/ml |
| 9) t O-Xylene                | 13.912 | 427631   | 19.259 ng/ml |
| 10) t 1,2,4-Trimethylbenzene | 16.186 | 415695   | 18.971 ng/ml |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB100323\  
Data File : FB030375.D  
Signal(s) : FID2B.CH  
Acq On : 3 Oct 2023 12:10  
Operator : YP/AJ  
Sample : BSF1003S1  
Misc : 5.00G/5.00 ML DI WATER  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
BSF1003S1

Integration File: Calibration.e  
Quant Time: Oct 04 01:34:31 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB091823.M  
Quant Title :  
QLast Update : Mon Sep 18 13:44:02 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

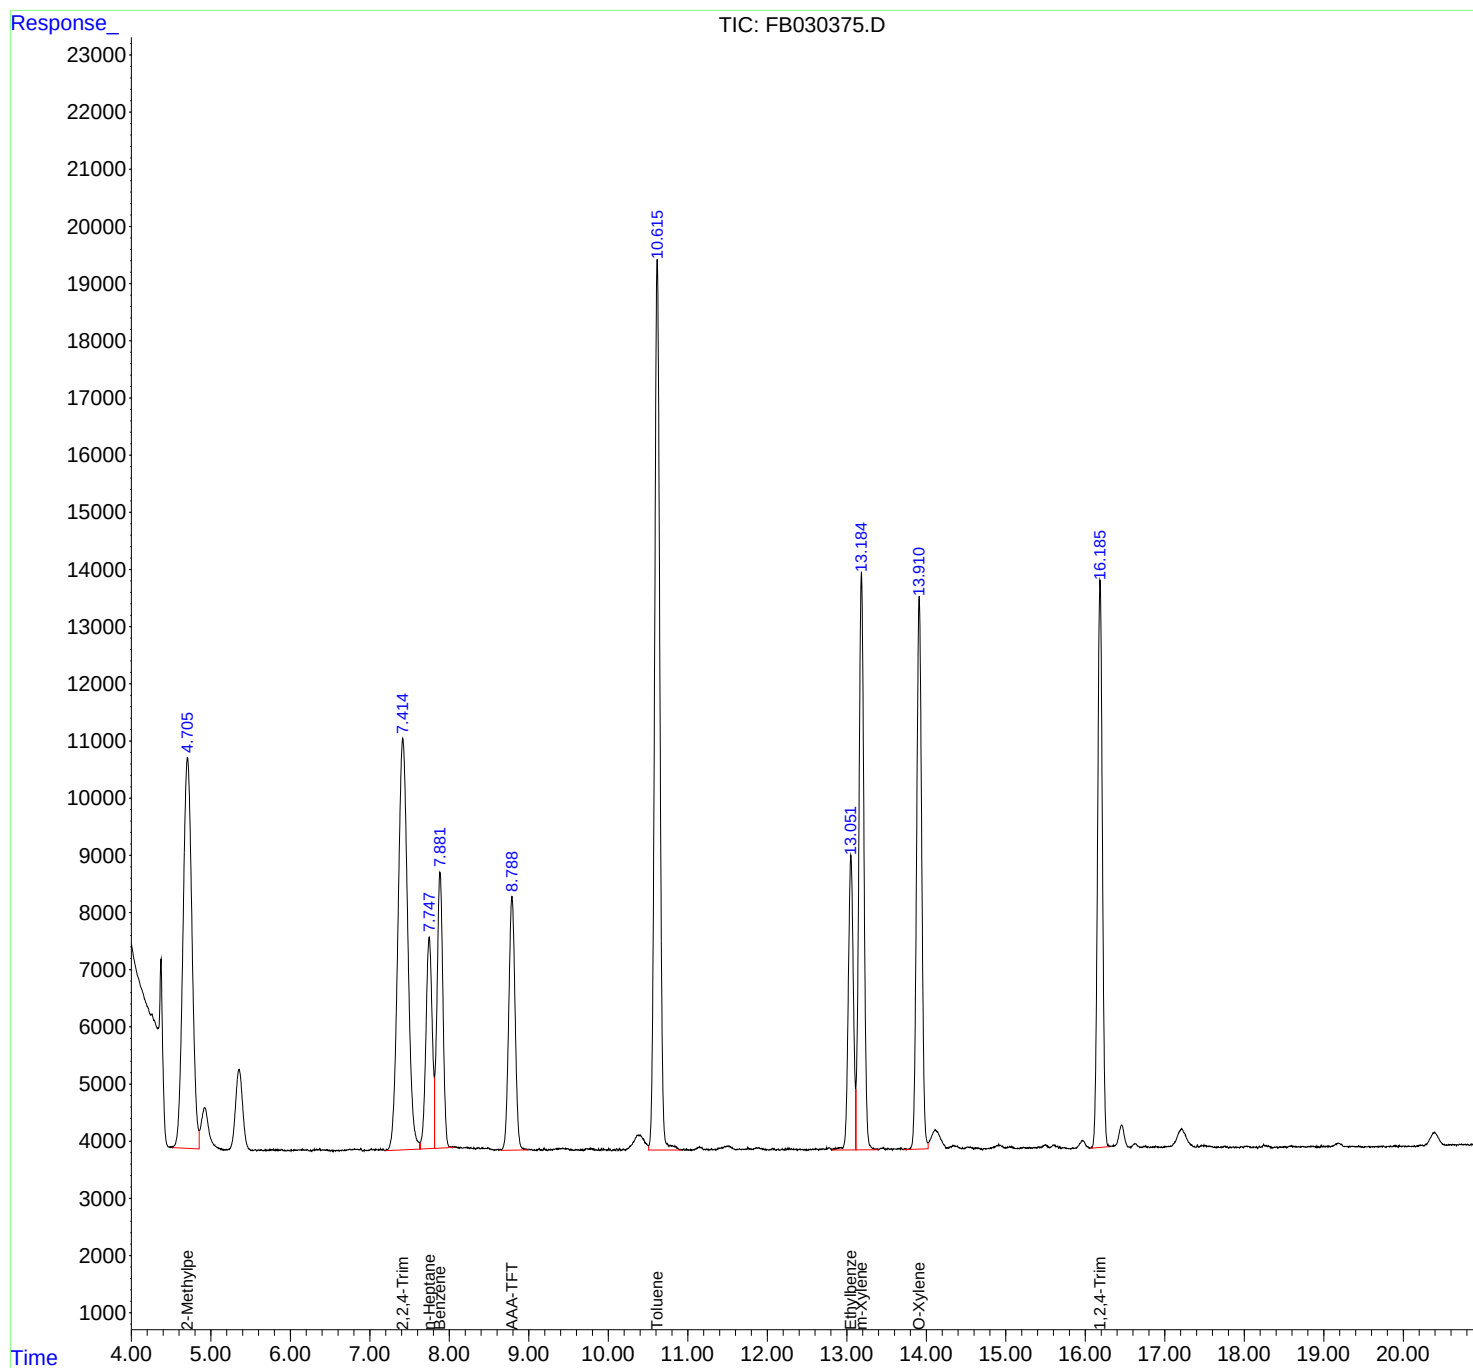


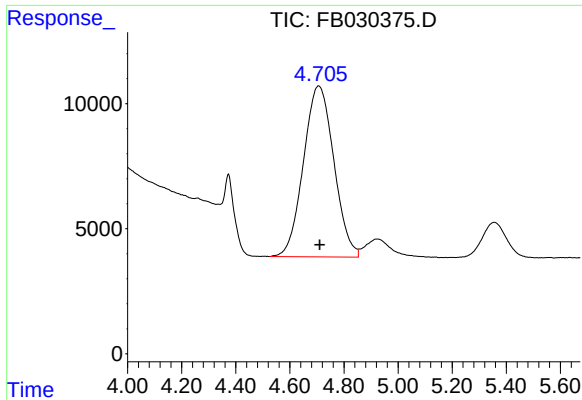

#1 2-Methylpentane


R.T.: 4.707 min  
Delta R.T.: -0.003 min  
Response: 534367  
Conc: 29.19 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF1003S1

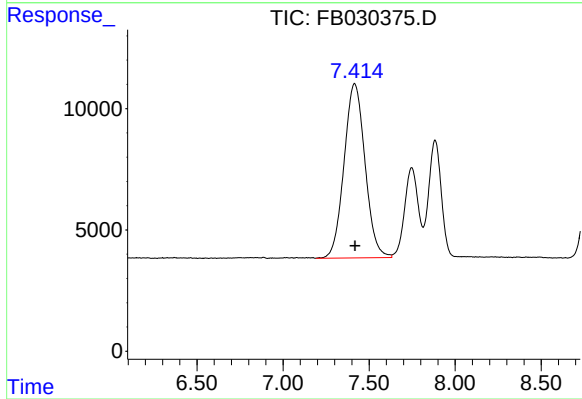


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min  
Delta R.T.: -0.003 min  
Response: 608587  
Conc: 30.08 ng/ml

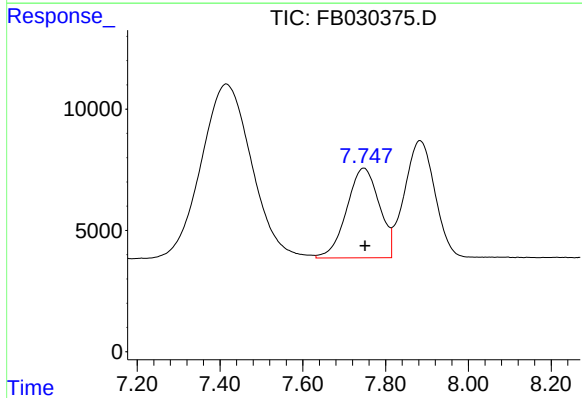


#3 n-Heptane

R.T.: 7.748 min  
Delta R.T.: -0.003 min  
Response: 202273  
Conc: 9.52 ng/ml

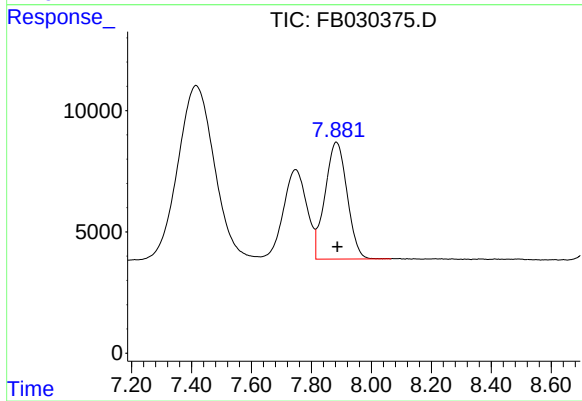

#4 Benzene


R.T.: 7.883 min  
Delta R.T.: -0.003 min  
Response: 246741  
Conc: 9.69 ng/ml

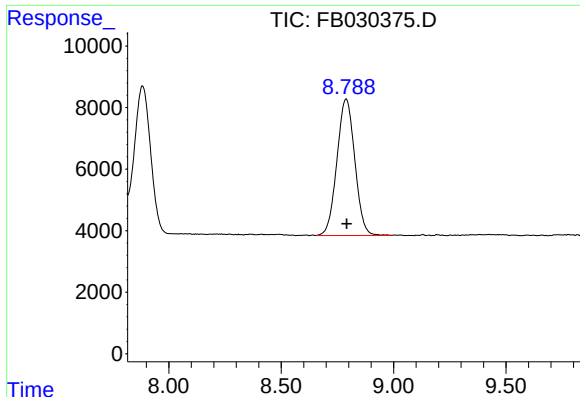

#5 AAA-TFT


R.T.: 8.789 min  
Delta R.T.: -0.002 min  
Response: 245376  
Conc: 17.74 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF1003S1

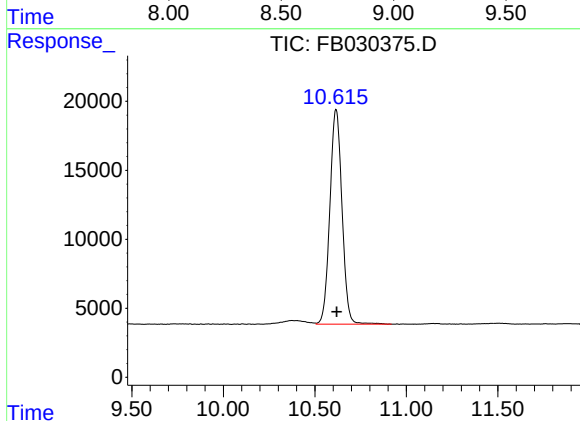


#6 Toluene

R.T.: 10.616 min  
Delta R.T.: -0.004 min  
Response: 719233  
Conc: 29.02 ng/ml

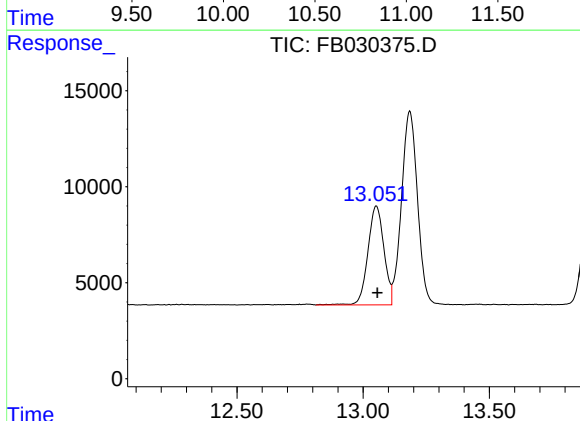


#7 Ethylbenzene

R.T.: 13.052 min  
Delta R.T.: -0.004 min  
Response: 226725  
Conc: 9.74 ng/ml

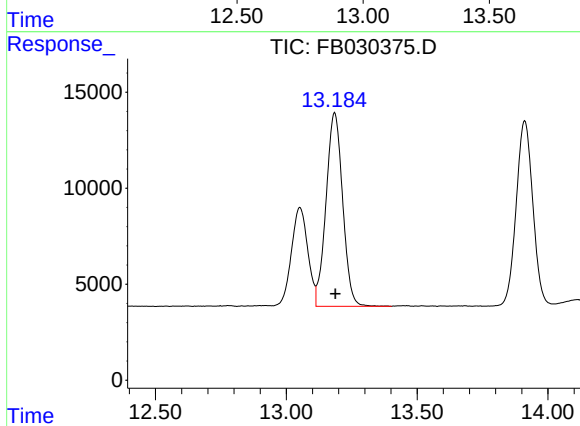

#8 m-Xylene


R.T.: 13.185 min  
Delta R.T.: -0.003 min  
Response: 445085  
Conc: 19.41 ng/ml

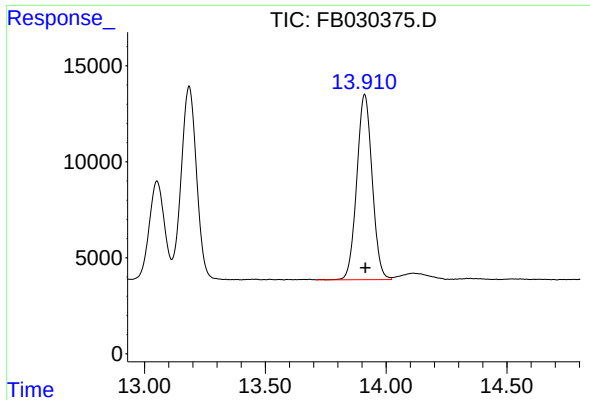

#9 O-Xylene

R.T.: 13.912 min  
Delta R.T.: -0.004 min  
Response: 427631  
Conc: 19.26 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF1003S1

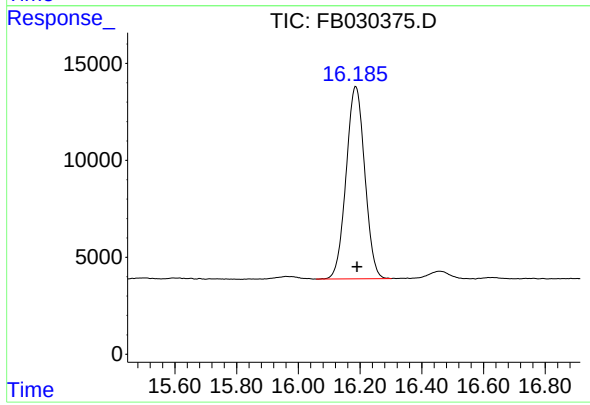

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min  
Delta R.T.: -0.004 min  
Response: 415695  
Conc: 18.97 ng/ml