

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100323\
 Data File : FB030378.D
 Signal(s) : FID2B.CH
 Acq On : 3 Oct 2023 14:10
 Operator : YP/AJ
 Sample : BSF1003W2
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1003W2

Integration File: Calibration.e
 Quant Time: Oct 04 01:35:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
 Quant Title :
 QLast Update : Mon Sep 18 13:44:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	245127	17.722 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	444344	24.274 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	561319	27.746 ng/ml
3) t n-Heptane	7.749	151833	7.146 ng/ml
4) t Benzene	7.885	200361	7.871 ng/ml
6) t Toluene	10.618	597401	24.102 ng/ml
7) t Ethylbenzene	13.055	197684	8.492 ng/ml
8) t m-Xylene	13.187	397275	17.321 ng/ml
9) t O-Xylene	13.914	400934	18.056 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	416306	18.999 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100323\
Data File : FB030378.D
Signal(s) : FID2B.CH
Acq On : 3 Oct 2023 14:10
Operator : YP/AJ
Sample : BSF1003W2
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1003W2

Integration File: Calibration.e
Quant Time: Oct 04 01:35:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
Quant Title :
QLast Update : Mon Sep 18 13:44:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

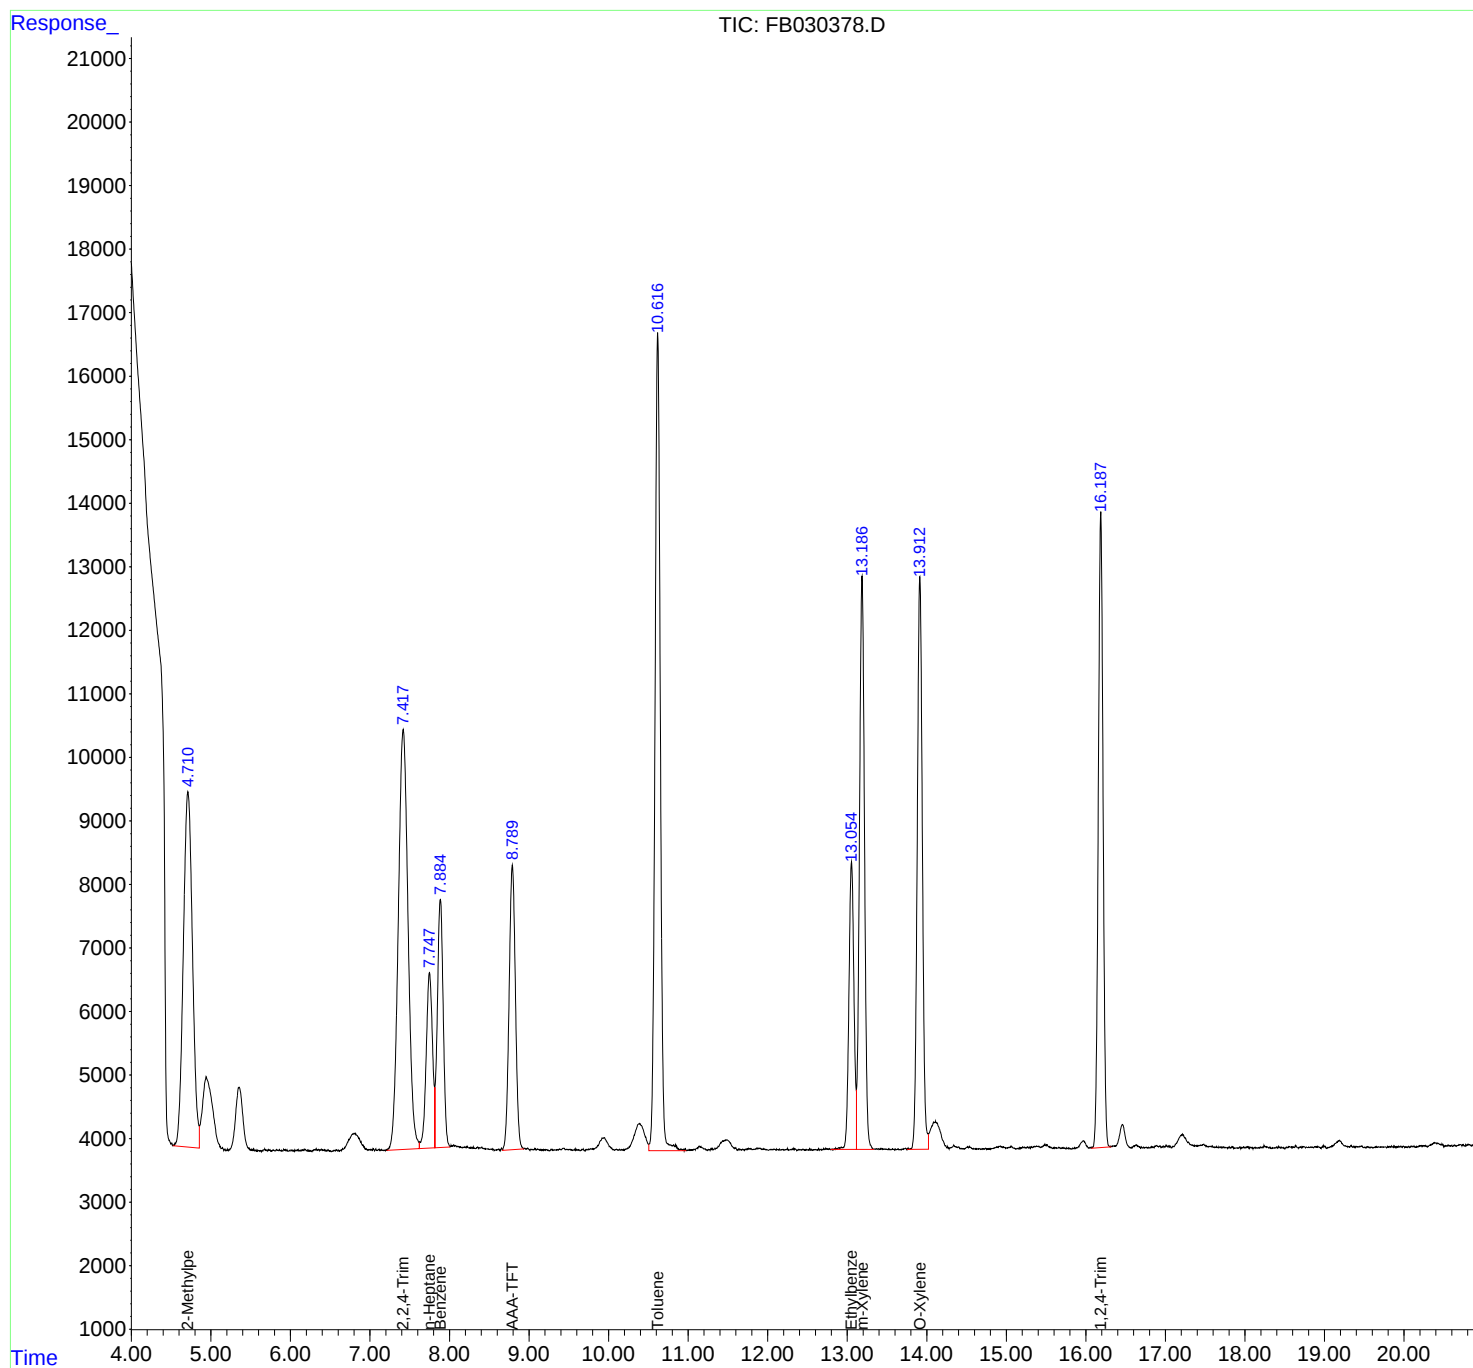


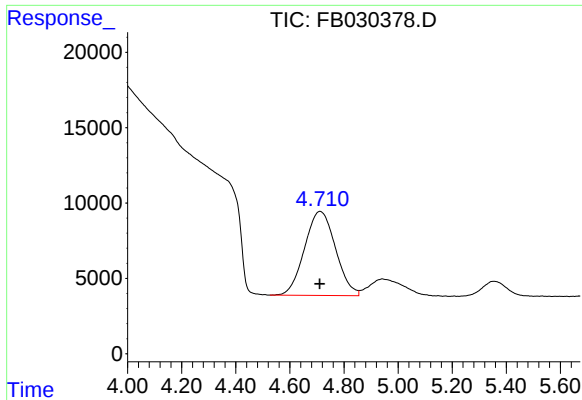

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.002 min
Response: 444344
Conc: 24.27 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1003W2

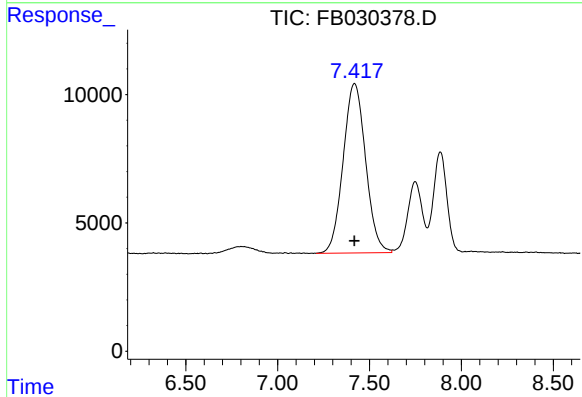


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 561319
Conc: 27.75 ng/ml

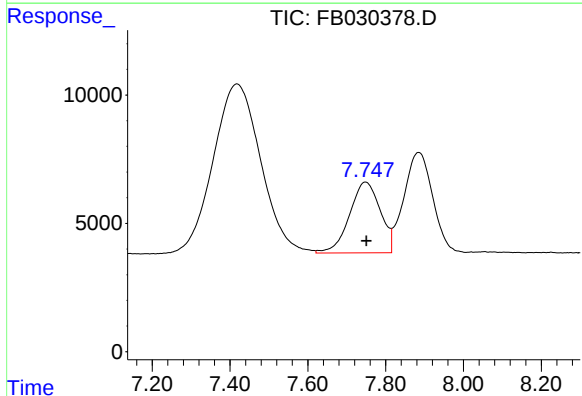


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.002 min
Response: 151833
Conc: 7.15 ng/ml

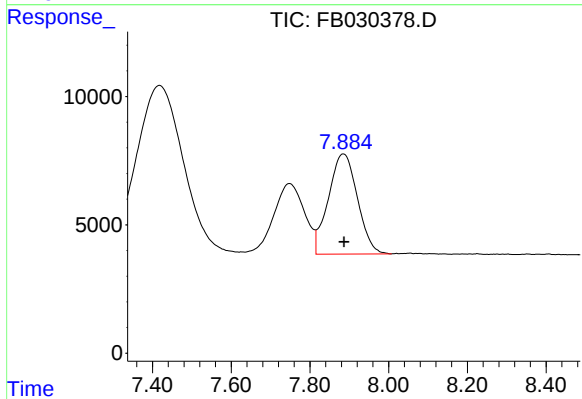

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.001 min
Response: 200361
Conc: 7.87 ng/ml

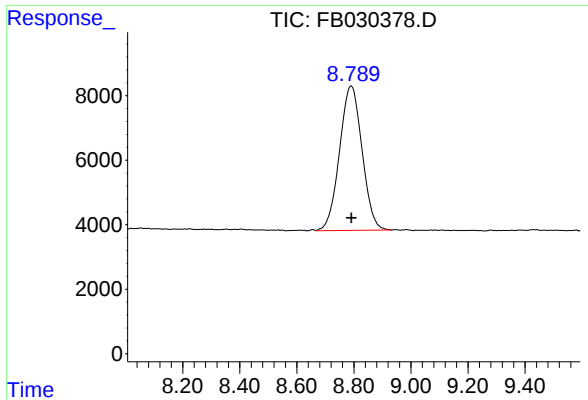

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: -0.001 min
Response: 245127
Conc: 17.72 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1003W2

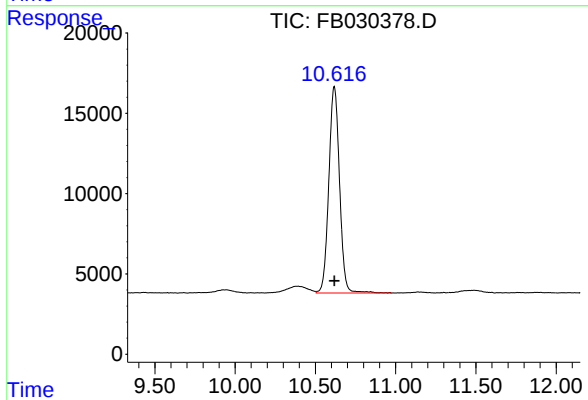


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.002 min
Response: 597401
Conc: 24.10 ng/ml

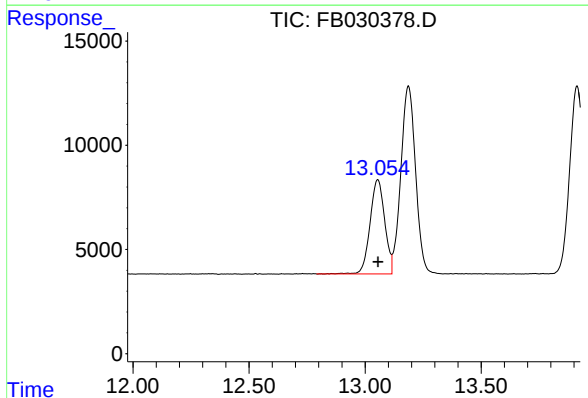


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.001 min
Response: 197684
Conc: 8.49 ng/ml

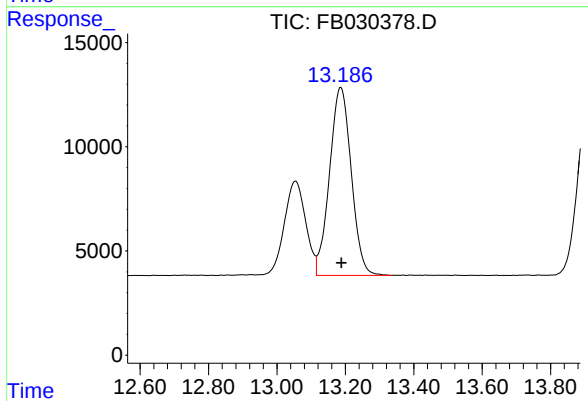

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.001 min
Response: 397275
Conc: 17.32 ng/ml

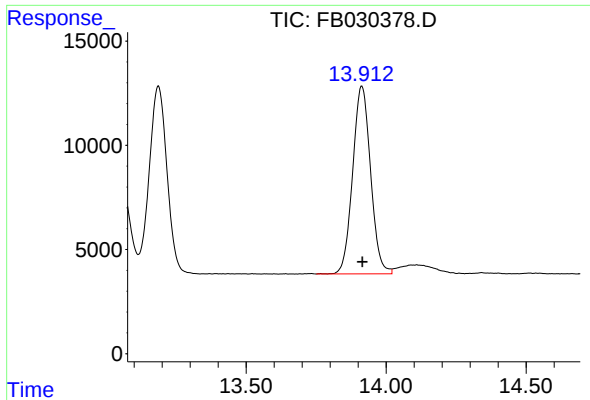

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.002 min
Response: 400934
Conc: 18.06 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1003W2

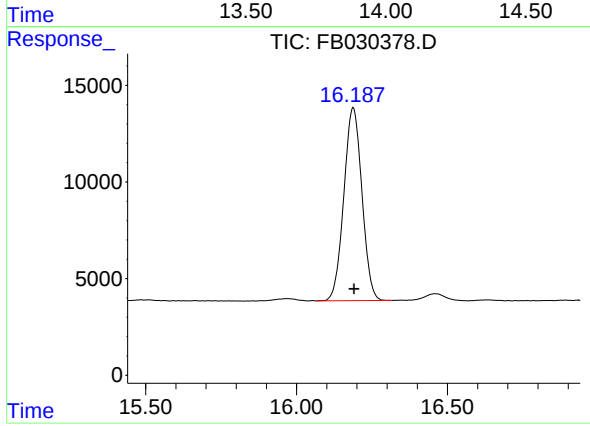

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.003 min
Response: 416306
Conc: 19.00 ng/ml