

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100323\
 Data File : FB030379.D
 Signal(s) : FID2B.CH
 Acq On : 3 Oct 2023 14:49
 Operator : YP/AJ
 Sample : BSF1003S2
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1003S2

Integration File: Calibration.e
 Quant Time: Oct 04 01:36:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
 Quant Title :
 QLast Update : Mon Sep 18 13:44:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	321361	23.233 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	479766	26.210 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	556982	27.532 ng/ml
3) t n-Heptane	7.749	185846	8.747 ng/ml
4) t Benzene	7.886	235641	9.257 ng/ml
6) t Toluene	10.618	680641	27.461 ng/ml
7) t Ethylbenzene	13.055	220749	9.483 ng/ml
8) t m-Xylene	13.187	429472	18.724 ng/ml
9) t O-Xylene	13.914	418971	18.869 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	389712	17.786 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100323\
Data File : FB030379.D
Signal(s) : FID2B.CH
Acq On : 3 Oct 2023 14:49
Operator : YP/AJ
Sample : BSF1003S2
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1003S2

Integration File: Calibration.e
Quant Time: Oct 04 01:36:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
Quant Title :
QLast Update : Mon Sep 18 13:44:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

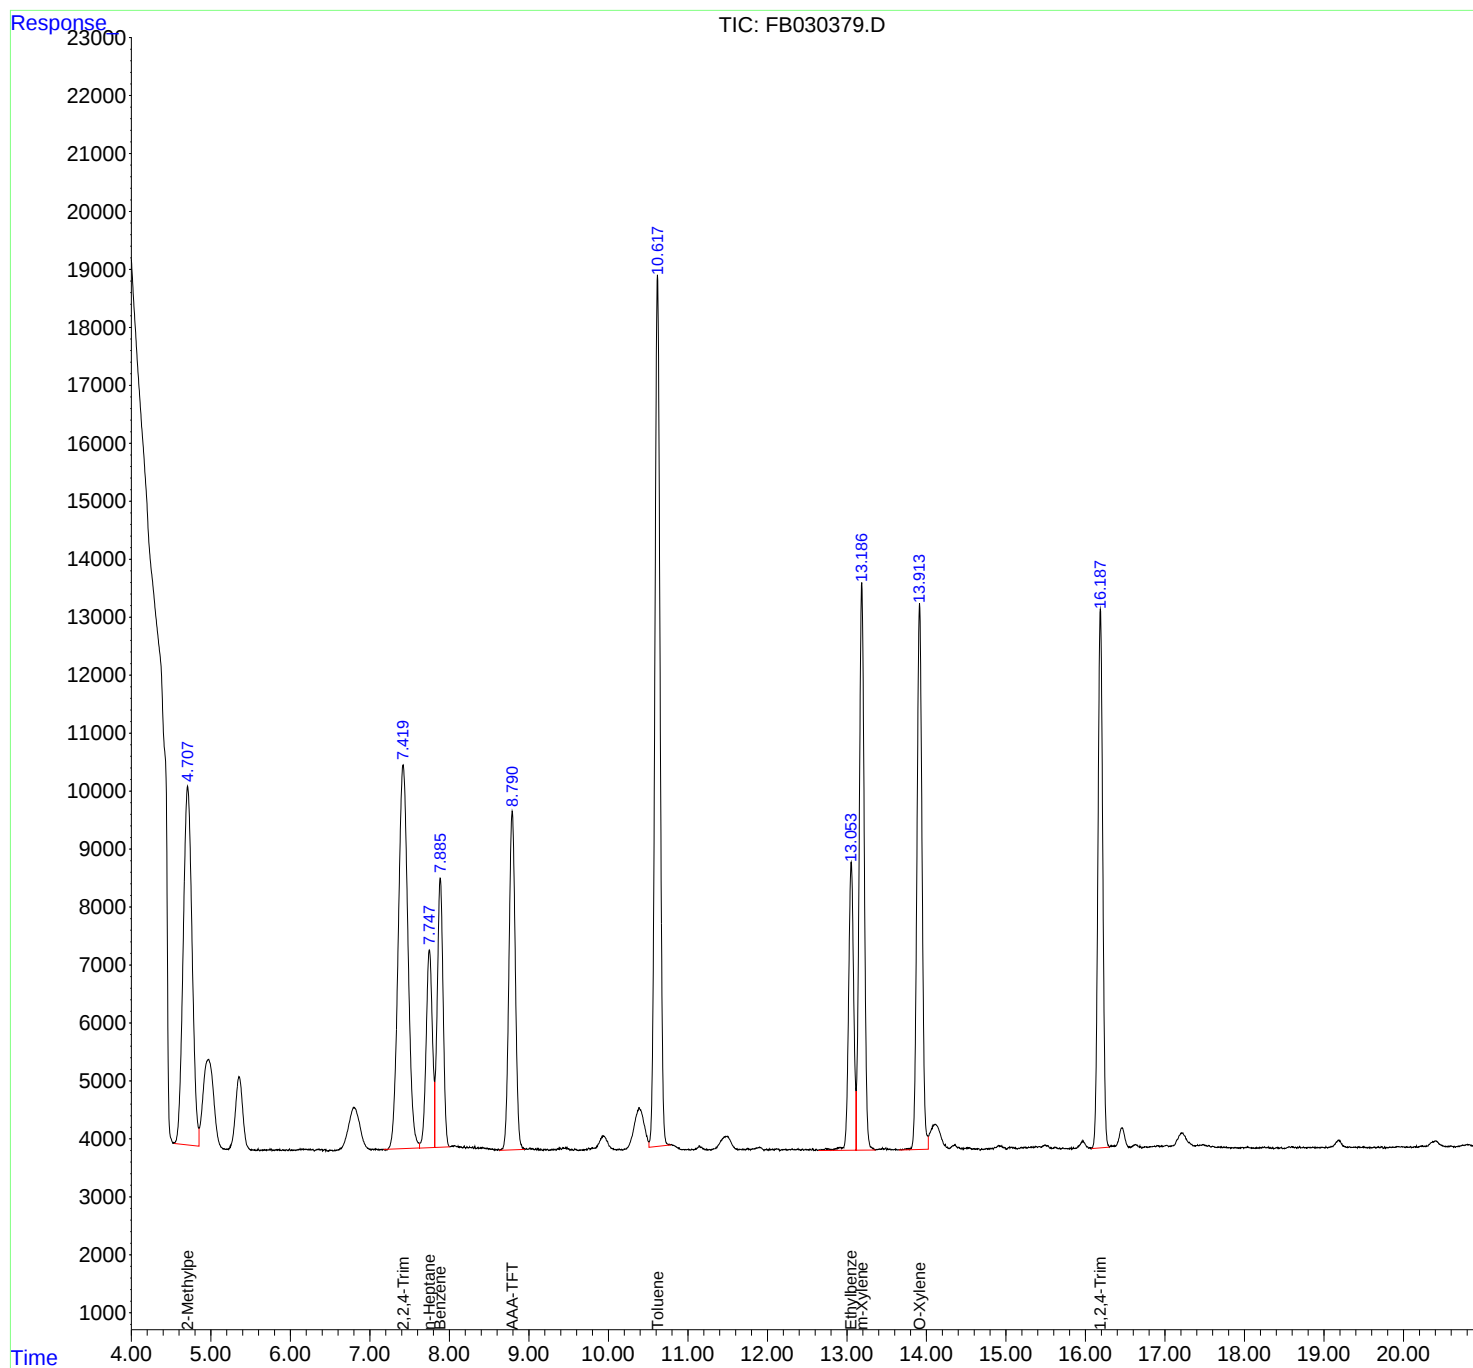


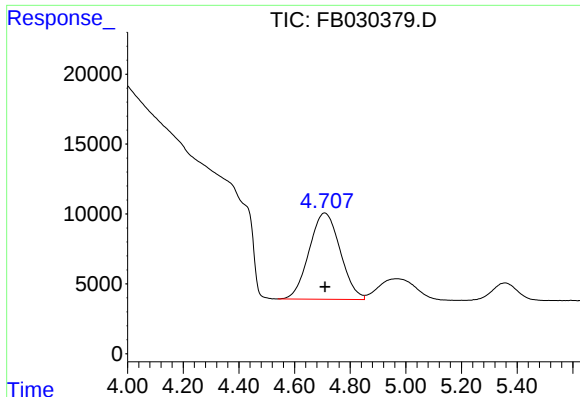

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: -0.002 min
Response: 479766
Conc: 26.21 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1003S2

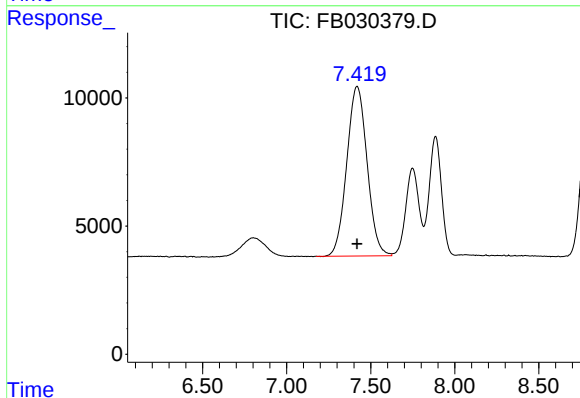


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.001 min
Response: 556982
Conc: 27.53 ng/ml

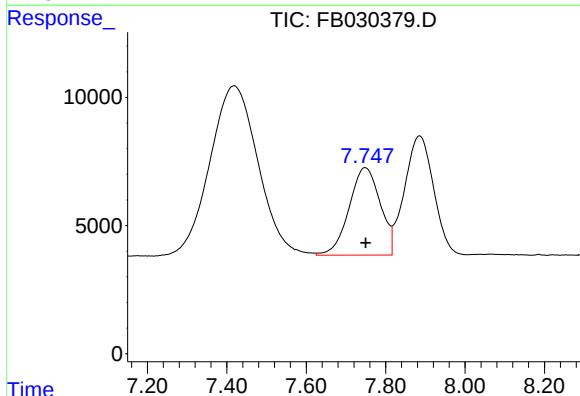


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.002 min
Response: 185846
Conc: 8.75 ng/ml

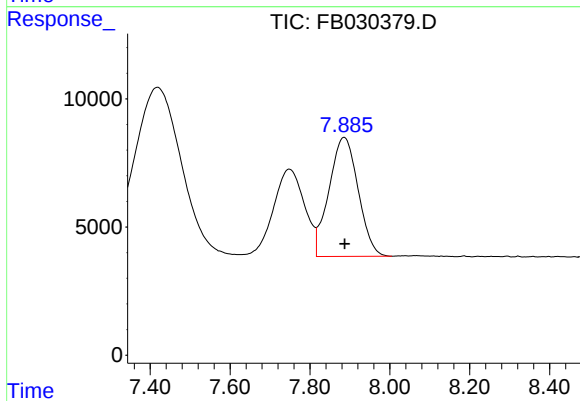

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 235641
Conc: 9.26 ng/ml

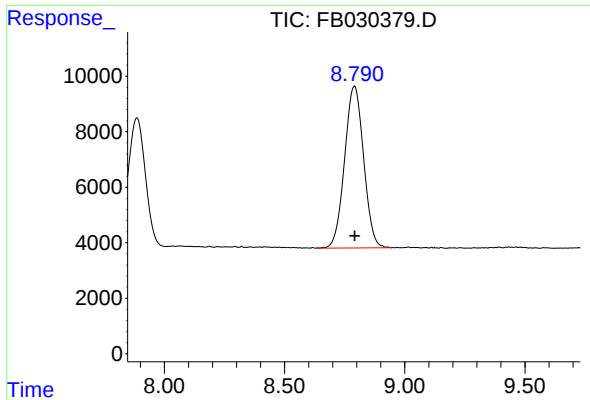

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 321361
Conc: 23.23 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1003S2

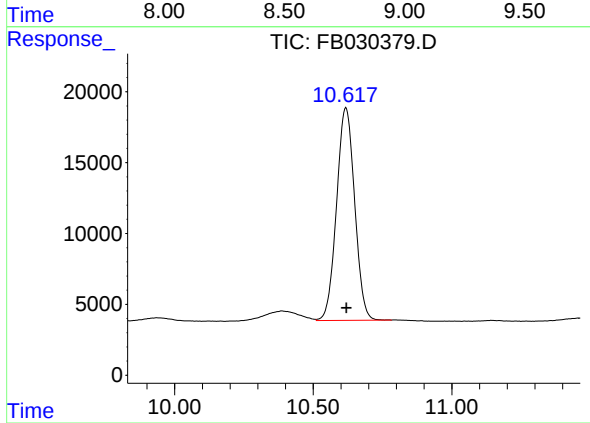


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.002 min
Response: 680641
Conc: 27.46 ng/ml

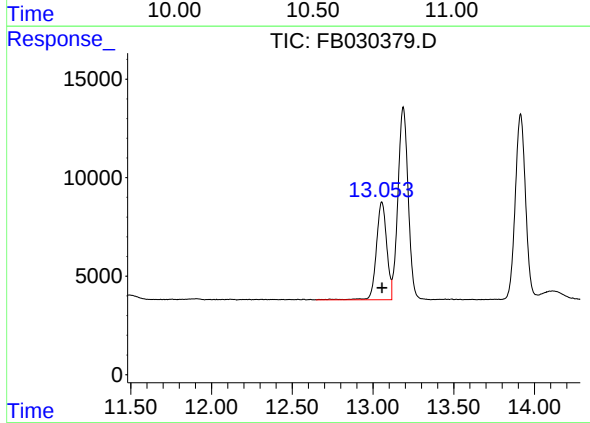


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.001 min
Response: 220749
Conc: 9.48 ng/ml

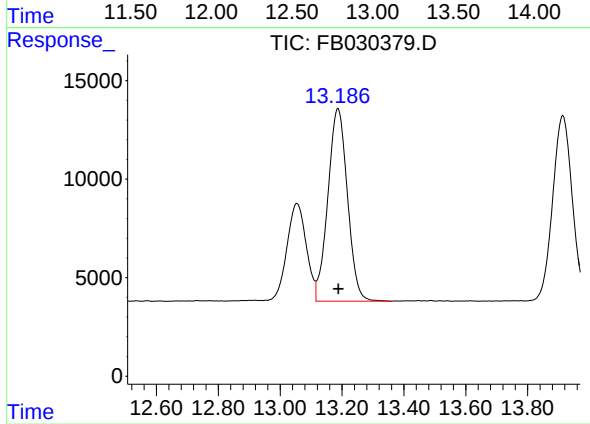

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.001 min
Response: 429472
Conc: 18.72 ng/ml

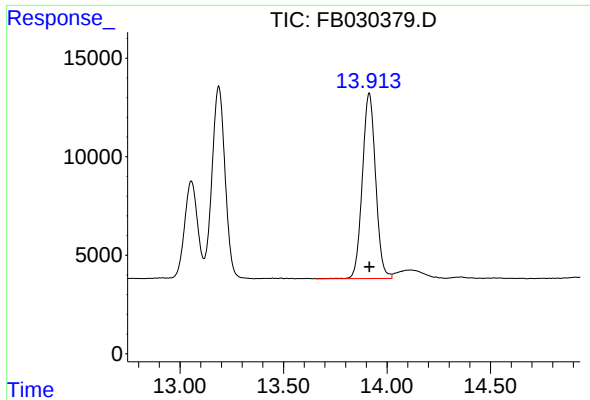

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.001 min
Response: 418971
Conc: 18.87 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1003S2

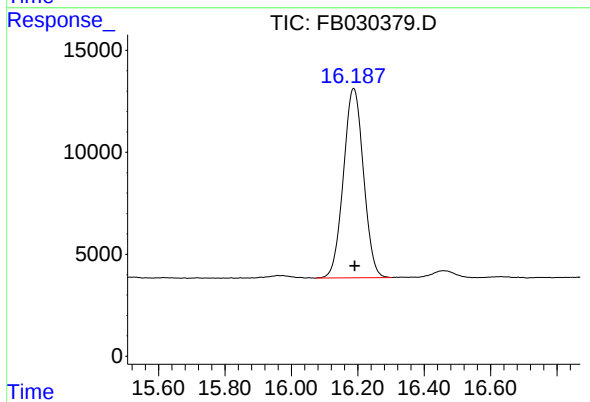

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.002 min
Response: 389712
Conc: 17.79 ng/ml