

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100323\
 Data File : FB030382.D
 Signal(s) : FID2B.CH
 Acq On : 3 Oct 2023 18:46
 Operator : YP/AJ
 Sample : 04699-08
 Misc : 5 PPB WATER LOQ
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 LOQ-WATER-02-QT4-2023

Integration File: Calibration.e
 Quant Time: Oct 04 01:37:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
 Quant Title :
 QLast Update : Mon Sep 18 13:44:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	207212	14.981 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	146863	8.023 ng/mlm
2) t 2,2,4-Trimethylpentane	7.419	176588	8.729 ng/ml
3) t n-Heptane	7.754	57793	2.720 ng/ml
4) t Benzene	7.889	72694	2.856 ng/ml
6) t Toluene	10.622	217965	8.794 ng/ml
7) t Ethylbenzene	13.058	66983	2.877 ng/ml
8) t m-Xylene	13.191	134597	5.868 ng/ml
9) t O-Xylene	13.918	132198	5.954 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	127140	5.802 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100323\
Data File : FB030382.D
Signal(s) : FID2B.CH
Acq On : 3 Oct 2023 18:46
Operator : YP/AJ
Sample : 04699-08
Misc : 5 PPB WATER LOQ
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
LOQ-WATER-02-QT4-2023

Integration File: Calibration.e
Quant Time: Oct 04 01:37:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
Quant Title :
QLast Update : Mon Sep 18 13:44:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

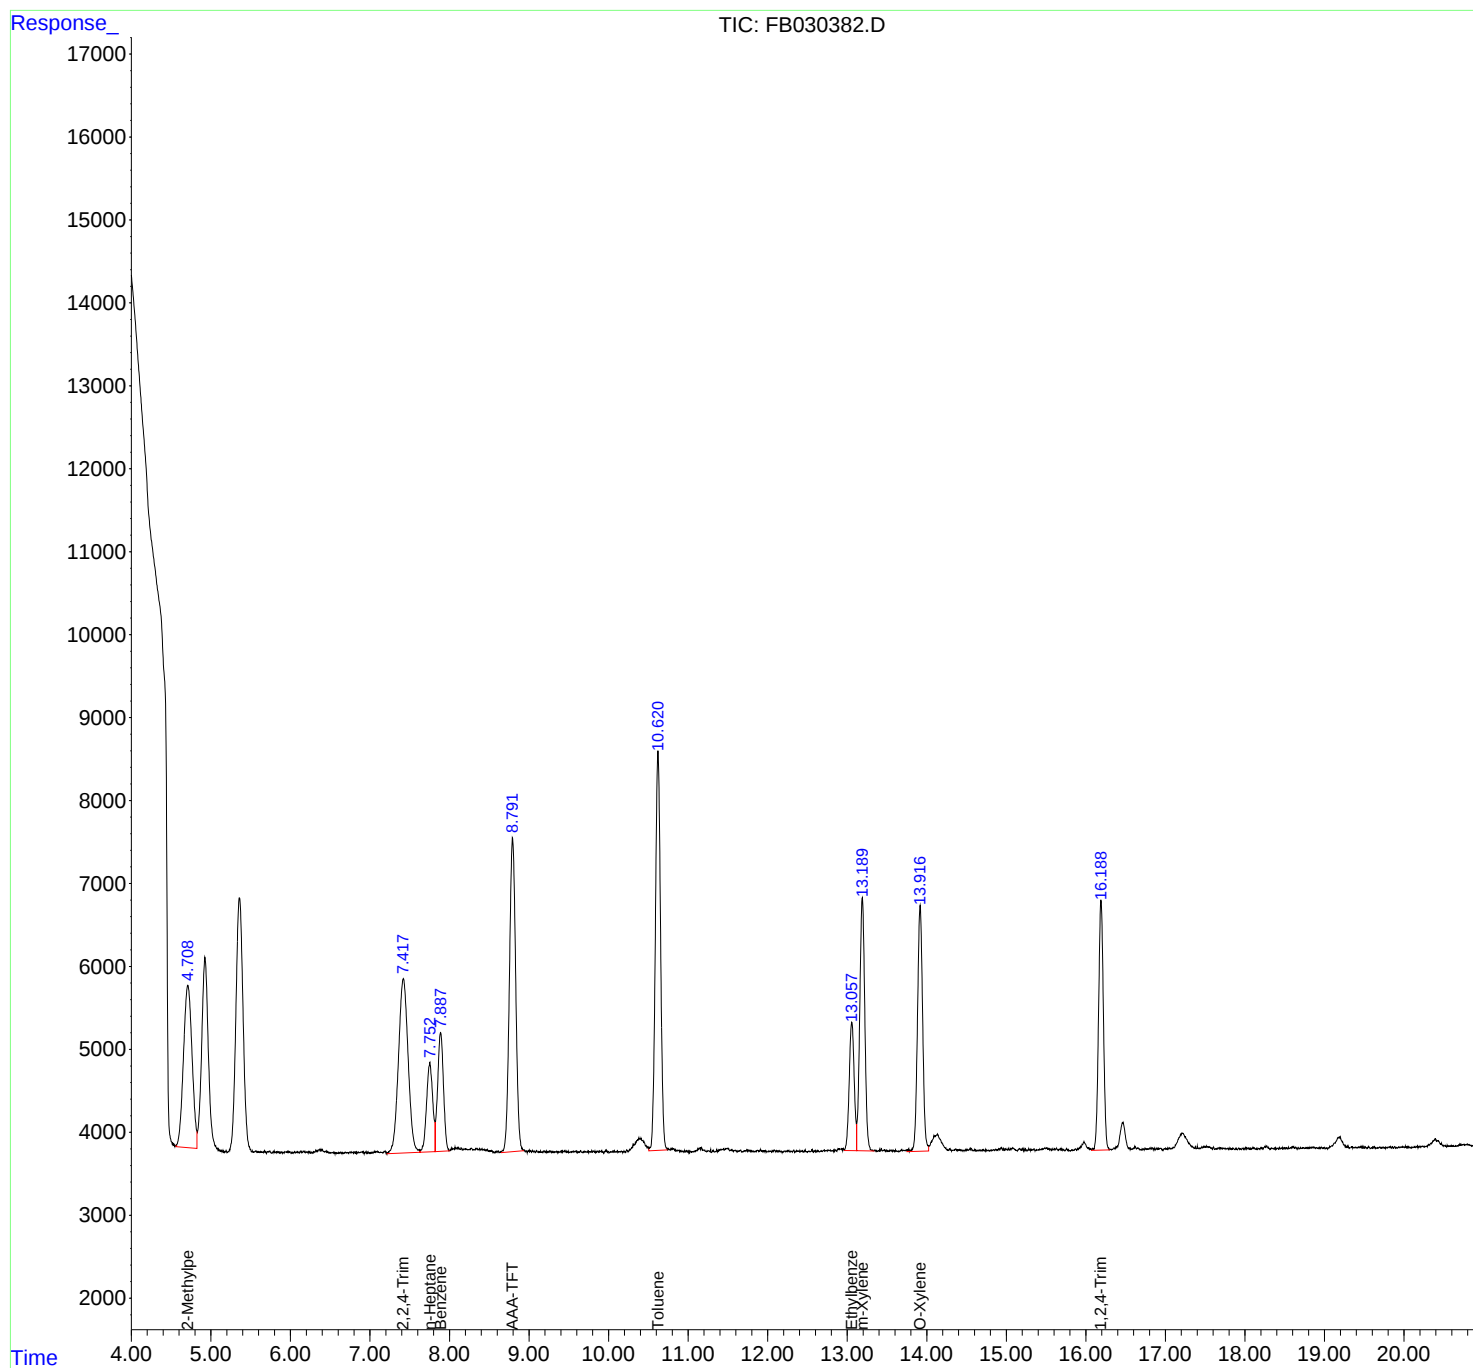


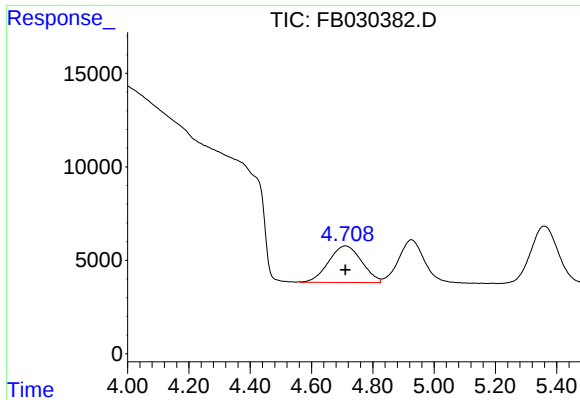

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: -0.002 min
Response: 146863
Conc: 8.02 ng/ml

Instrument :
FID_B
ClientSampleId :
LOQ-WATER-02-QT4-2023

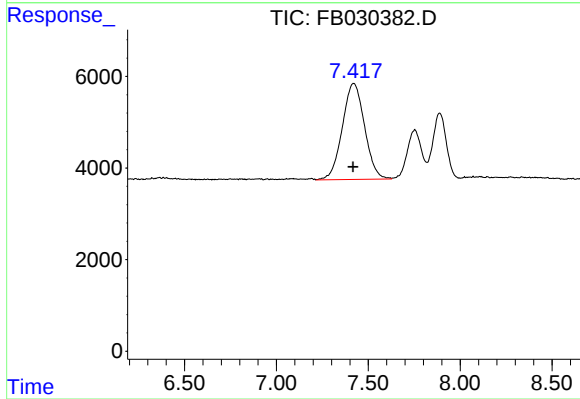


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 176588
Conc: 8.73 ng/ml

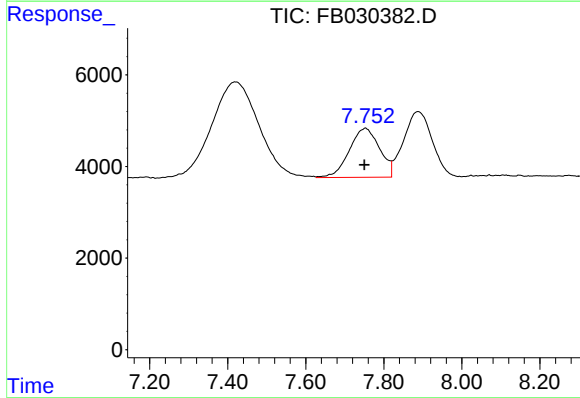


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.003 min
Response: 57793
Conc: 2.72 ng/ml

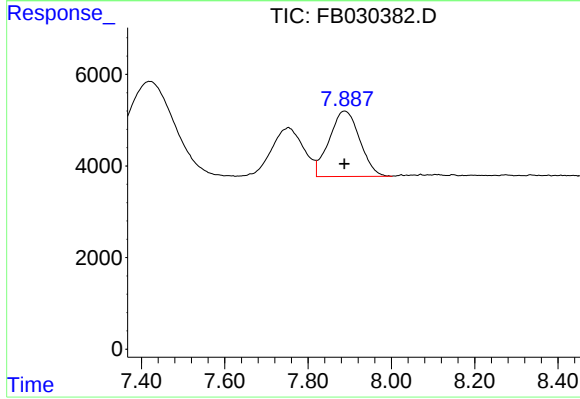

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.002 min
Response: 72694
Conc: 2.86 ng/ml

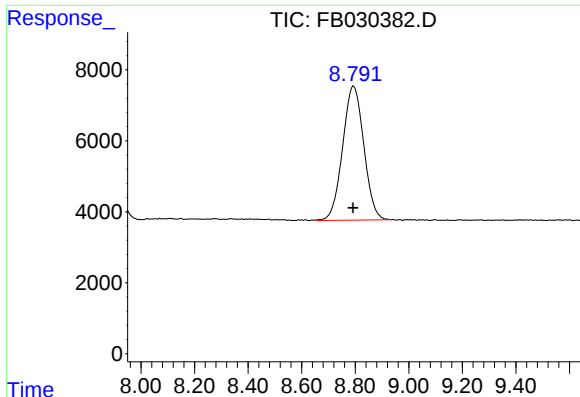

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.001 min
Response: 207212
Conc: 14.98 ng/ml

Instrument :
FID_B
ClientSampleId :
LOQ-WATER-02-QT4-2023

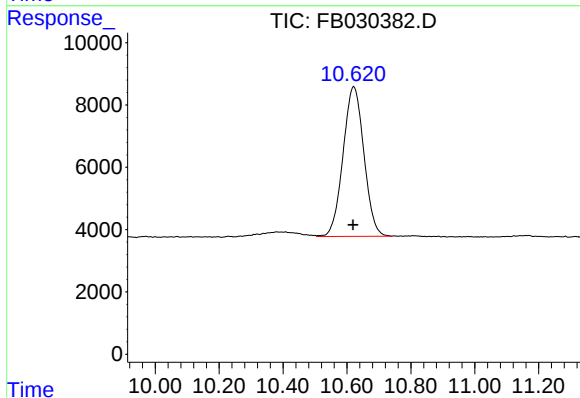


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.002 min
Response: 217965
Conc: 8.79 ng/ml

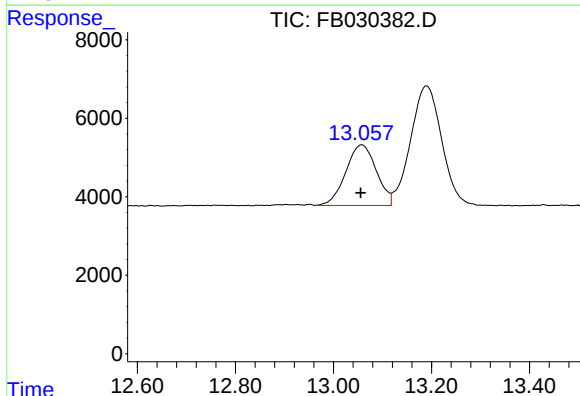


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.002 min
Response: 66983
Conc: 2.88 ng/ml

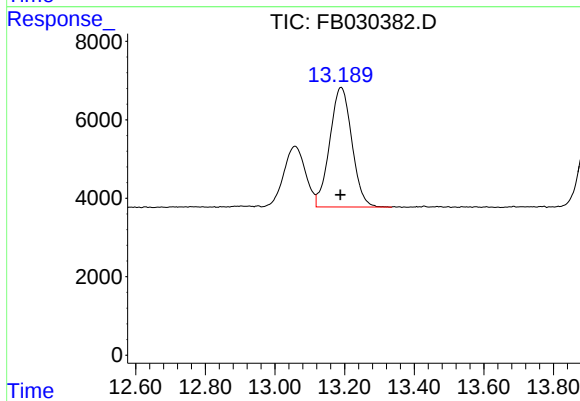

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.002 min
Response: 134597
Conc: 5.87 ng/ml

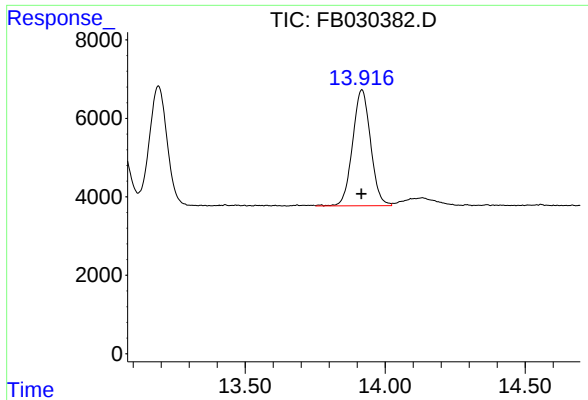

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.002 min
Response: 132198
Conc: 5.95 ng/ml

Instrument :
FID_B
ClientSampleId :
LOQ-WATER-02-QT4-2023

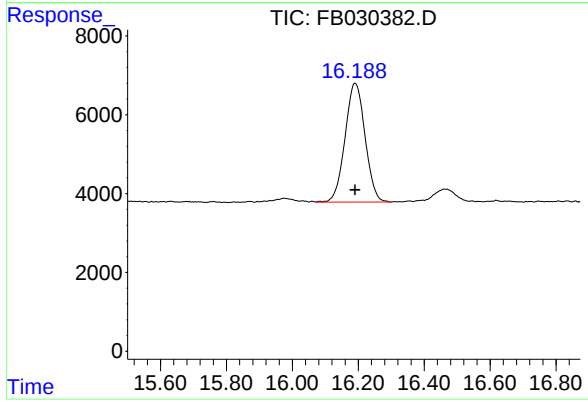

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 127140
Conc: 5.80 ng/ml