

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100323\
 Data File : FB030383.D
 Signal(s) : FID2B.CH
 Acq On : 3 Oct 2023 20:04
 Operator : YP/AJ
 Sample : BSF1003S3
 Misc : 5 PPB WATER LOQ
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1003S3

Integration File: Calibration.e
 Quant Time: Oct 04 01:37:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
 Quant Title :
 QLast Update : Mon Sep 18 13:44:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	270422	19.551 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	557272	30.444 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	652330	32.245 ng/ml
3) t n-Heptane	7.753	221647	10.432 ng/ml
4) t Benzene	7.889	281832	11.071 ng/ml
6) t Toluene	10.622	823244	33.214 ng/ml
7) t Ethylbenzene	13.057	254051	10.914 ng/ml
8) t m-Xylene	13.190	504078	21.977 ng/ml
9) t O-Xylene	13.917	482667	21.737 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	433462	19.782 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100323\
Data File : FB030383.D
Signal(s) : FID2B.CH
Acq On : 3 Oct 2023 20:04
Operator : YP/AJ
Sample : BSF1003S3
Misc : 5 PPB WATER LOQ
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1003S3

Integration File: Calibration.e
Quant Time: Oct 04 01:37:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
Quant Title :
QLast Update : Mon Sep 18 13:44:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

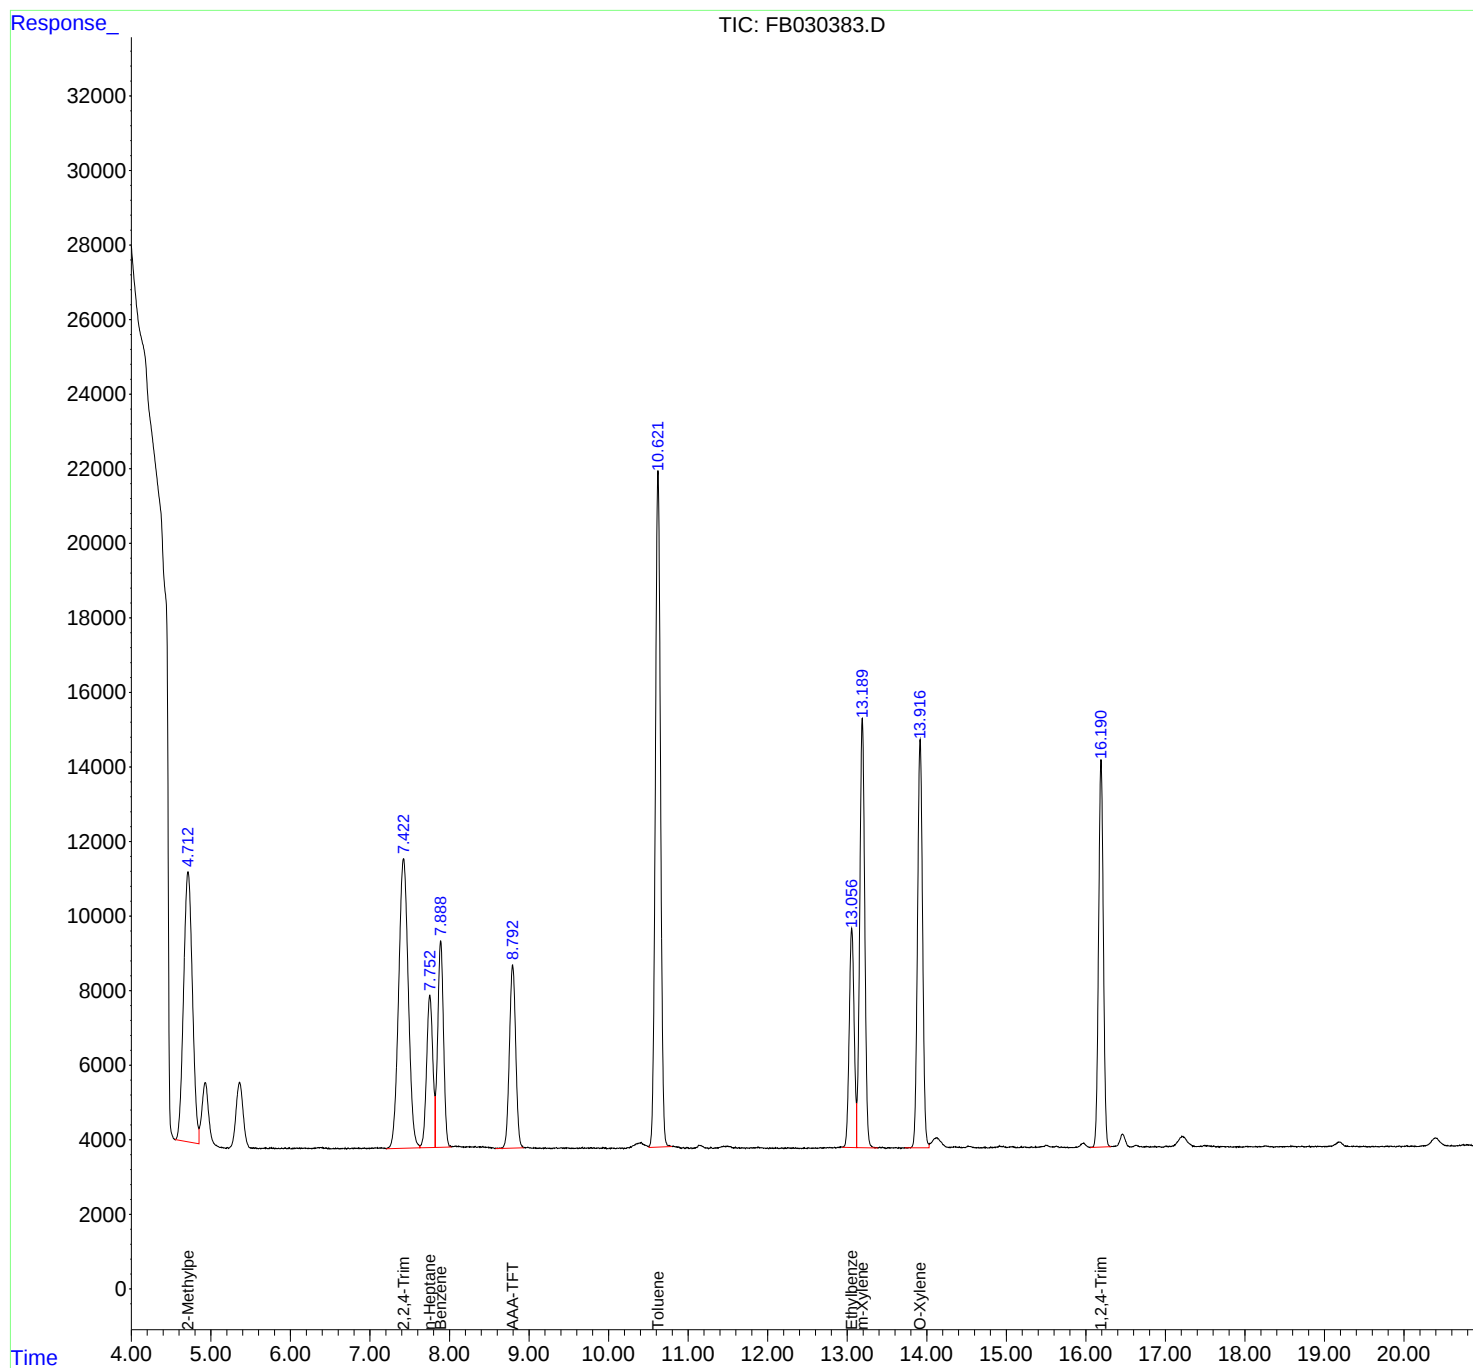


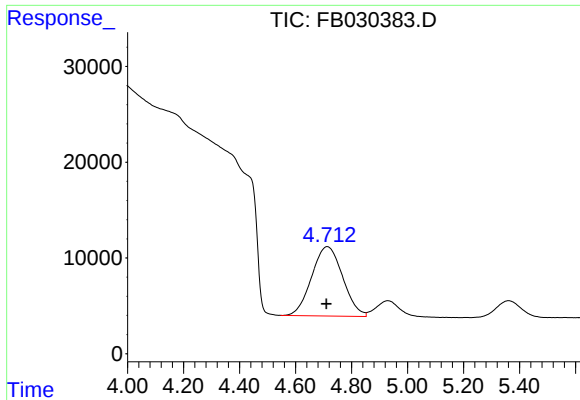

#1 2-Methylpentane


R.T.: 4.713 min
Delta R.T.: 0.003 min
Response: 557272
Conc: 30.44 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1003S3

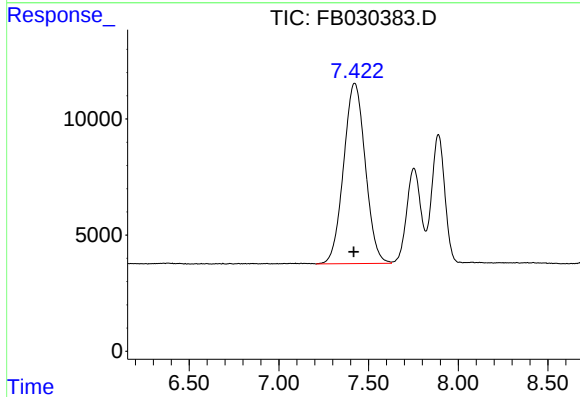


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: 0.004 min
Response: 652330
Conc: 32.24 ng/ml

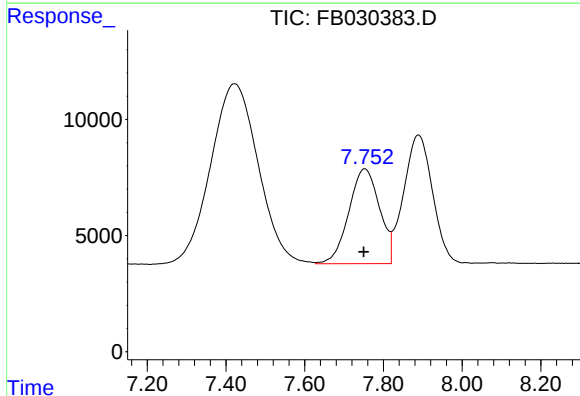


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.003 min
Response: 221647
Conc: 10.43 ng/ml

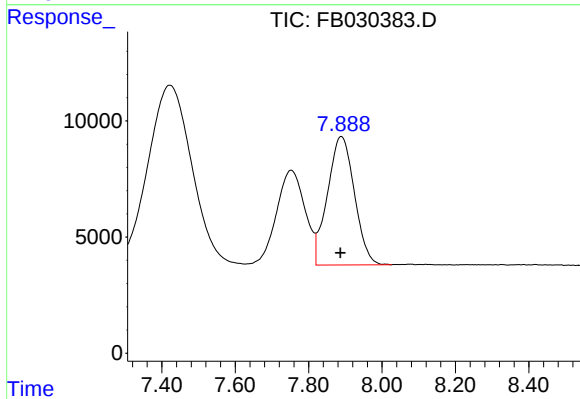

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.003 min
Response: 281832
Conc: 11.07 ng/ml

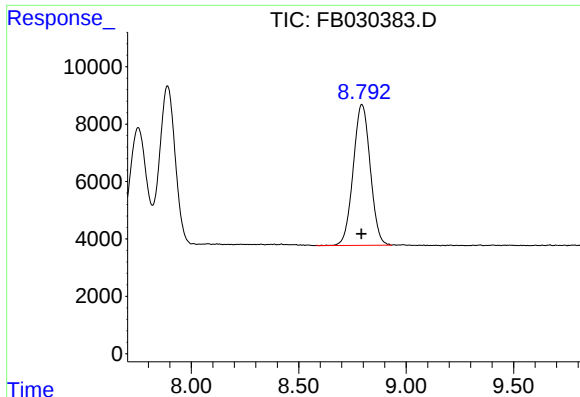

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.002 min
Response: 270422
Conc: 19.55 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1003S3

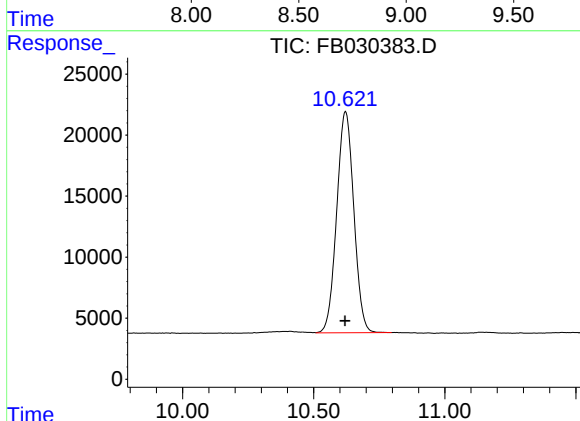


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.002 min
Response: 823244
Conc: 33.21 ng/ml

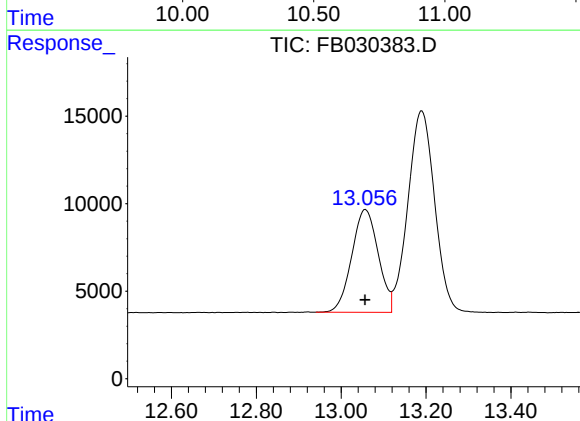


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.001 min
Response: 254051
Conc: 10.91 ng/ml

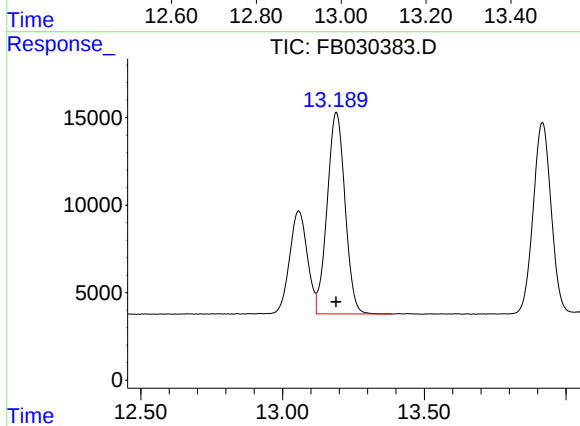

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.002 min
Response: 504078
Conc: 21.98 ng/ml

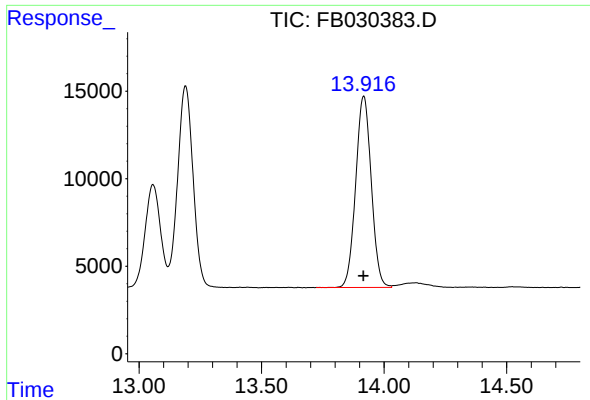

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.002 min
Response: 482667
Conc: 21.74 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1003S3

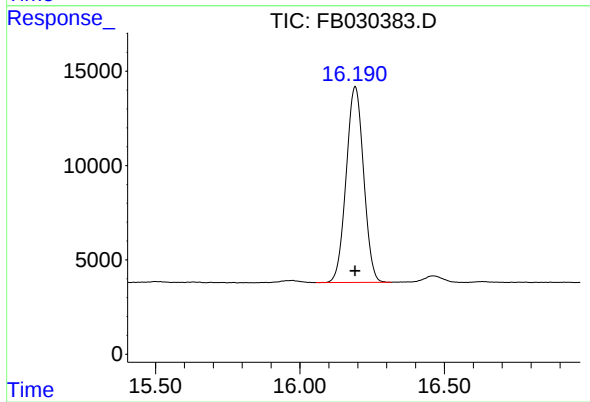

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 433462
Conc: 19.78 ng/ml