

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100418\
Data File : FB018104.D
Signal(s) : FID2B.CH
Acq On : 4 Oct 2018 9:54
Operator : MJ/SJ
Sample : BSF1004S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 04 16:45:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.109	183018	21.636 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.961	426781	26.799 ng/ml
2) t	2,2,4-Trimethylpentane	7.723	439581	27.623 ng/ml
3) t	n-Heptane	8.065	140312	9.105 ng/ml
4) t	Benzene	8.204	171964	9.033 ng/ml
6) t	Toluene	10.958	462603	29.230 ng/ml
7) t	Ethylbenzene	13.408	159926	9.787 ng/ml
8) t	m-Xylene	13.540	338513	19.567 ng/ml
9) t	O-Xylene	14.272	350623	19.294 ng/ml
10) t	1,2,4-Trimethylbenzene	16.555	410754	19.310 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100418\
Data File : FB018104.D
Signal(s) : FID2B.CH
Acq On : 4 Oct 2018 9:54
Operator : MJ/SJ
Sample : BSF1004S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 04 16:45:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

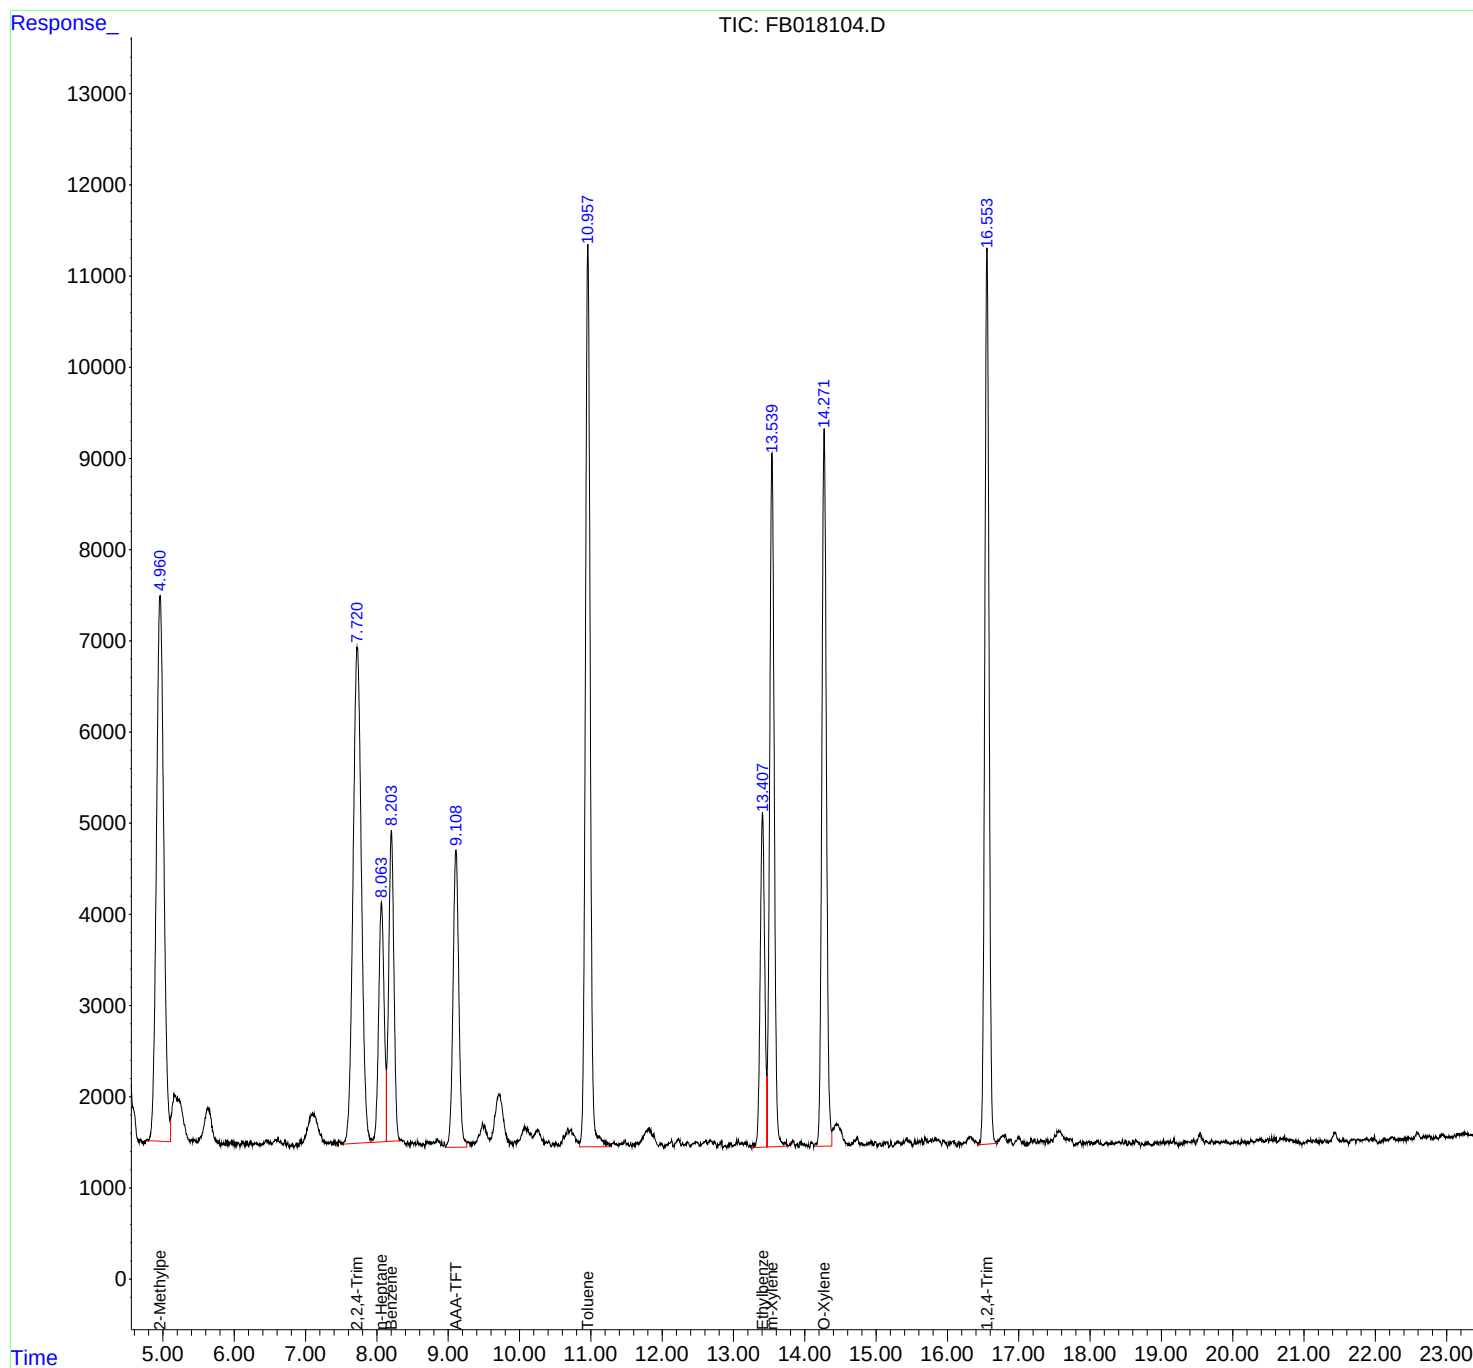

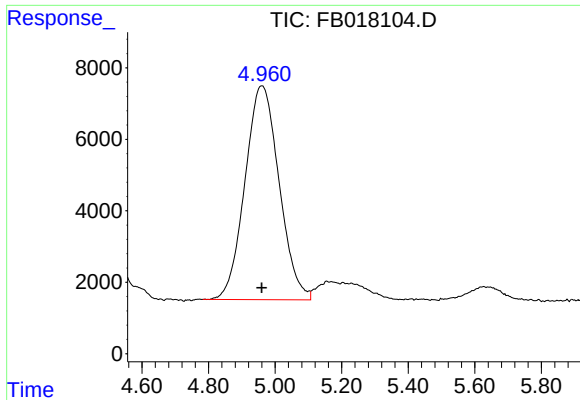


#1 2-Methylpentane

R.T.: 4.961 min
Delta R.T.: 0.000 min
Response: 426781
Conc: 26.80 ng/ml

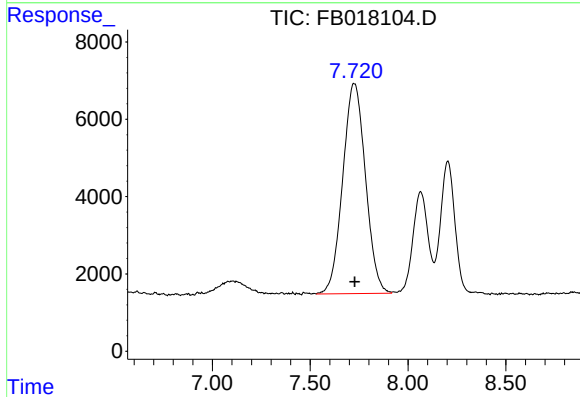


#2 2,2,4-Trimethylpentane

R.T.: 7.723 min
Delta R.T.: -0.005 min
Response: 439581
Conc: 27.62 ng/ml

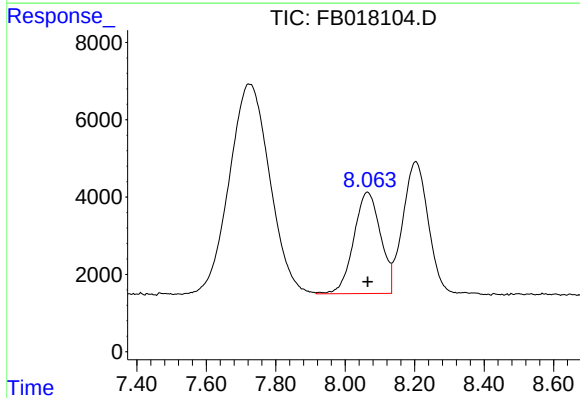


#3 n-Heptane

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 140312
Conc: 9.10 ng/ml

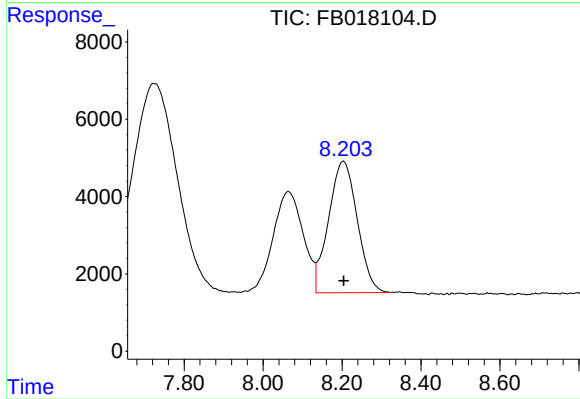


#4 Benzene

R.T.: 8.204 min
Delta R.T.: 0.000 min
Response: 171964
Conc: 9.03 ng/ml

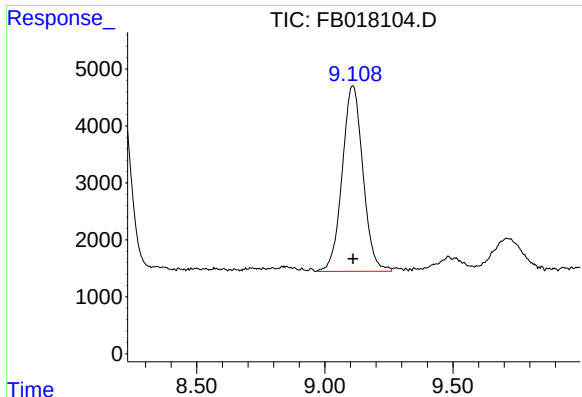


#5 AAA-TFT

R.T.: 9.109 min
Delta R.T.: 0.000 min
Response: 183018
Conc: 21.64 ng/ml

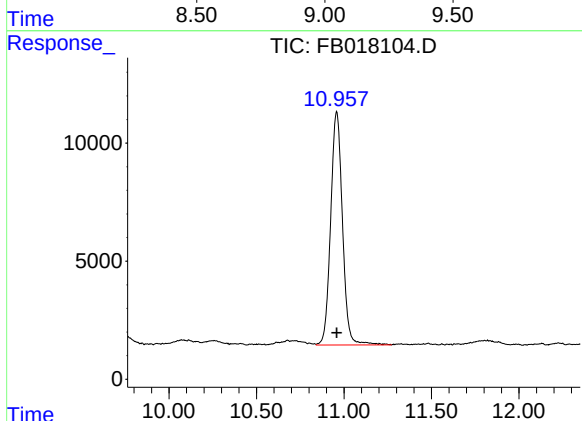


#6 Toluene

R.T.: 10.958 min
Delta R.T.: 0.000 min
Response: 462603
Conc: 29.23 ng/ml

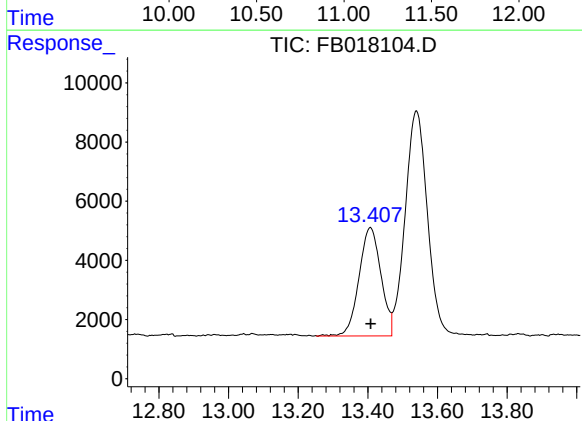


#7 Ethylbenzene

R.T.: 13.408 min
Delta R.T.: 0.000 min
Response: 159926
Conc: 9.79 ng/ml

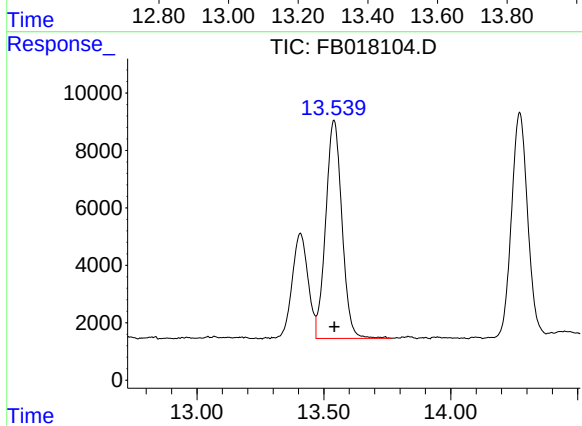


#8 m-Xylene

R.T.: 13.540 min
Delta R.T.: 0.000 min
Response: 338513
Conc: 19.57 ng/ml

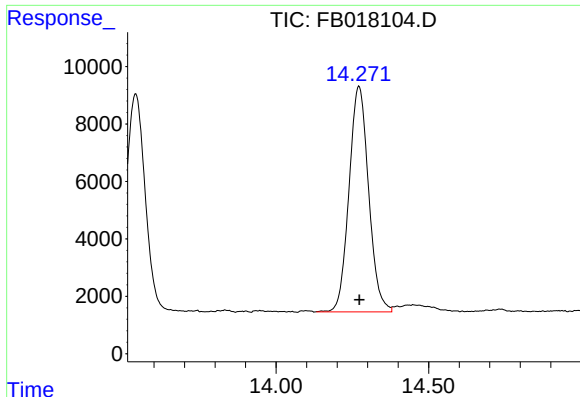

#9 O-Xylene

R.T.: 14.272 min
Delta R.T.: -0.001 min
Response: 350623
Conc: 19.29 ng/ml

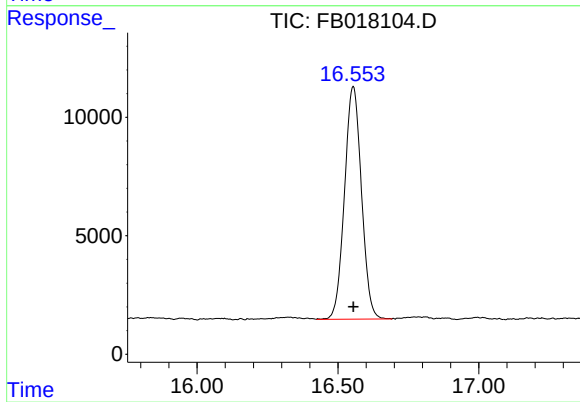

#10 1,2,4-Trimethylbenzene

R.T.: 16.555 min
Delta R.T.: 0.000 min
Response: 410754
Conc: 19.31 ng/ml