

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100419\
 Data File : FB022687.D
 Signal(s) : FID2B.CH
 Acq On : 4 Oct 2019 11:17
 Operator : DD/AJ
 Sample : K5205-02MSD
 Misc : 5.07g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 04 21:39:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
 Quant Title :
 QLast Update : Wed Oct 02 06:15:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.966	509966	21.165 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.834	920303	27.597 ng/ml
2) t	2,2,4-Trimethylpentane	7.586	915867	26.404 ng/ml
3) t	n-Heptane	7.925	274223	8.098 ng/ml
4) t	Benzene	8.059	412337	9.901 ng/ml
6) t	Toluene	10.807	1200293	29.653 ng/ml
7) t	Ethylbenzene	13.252	369693	9.553 ng/ml
8) t	m-Xylene	13.386	692405	18.673 ng/ml
9) t	O-Xylene	14.115	655799	18.783 ng/ml
10) t	1,2,4-Trimethylbenzene	16.396	474762	19.161 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100419\
Data File : FB022687.D
Signal(s) : FID2B.CH
Acq On : 4 Oct 2019 11:17
Operator : DD/AJ
Sample : K5205-02MSD
Misc : 5.07g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 04 21:39:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100119.M
Quant Title :
QLast Update : Wed Oct 02 06:15:33 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

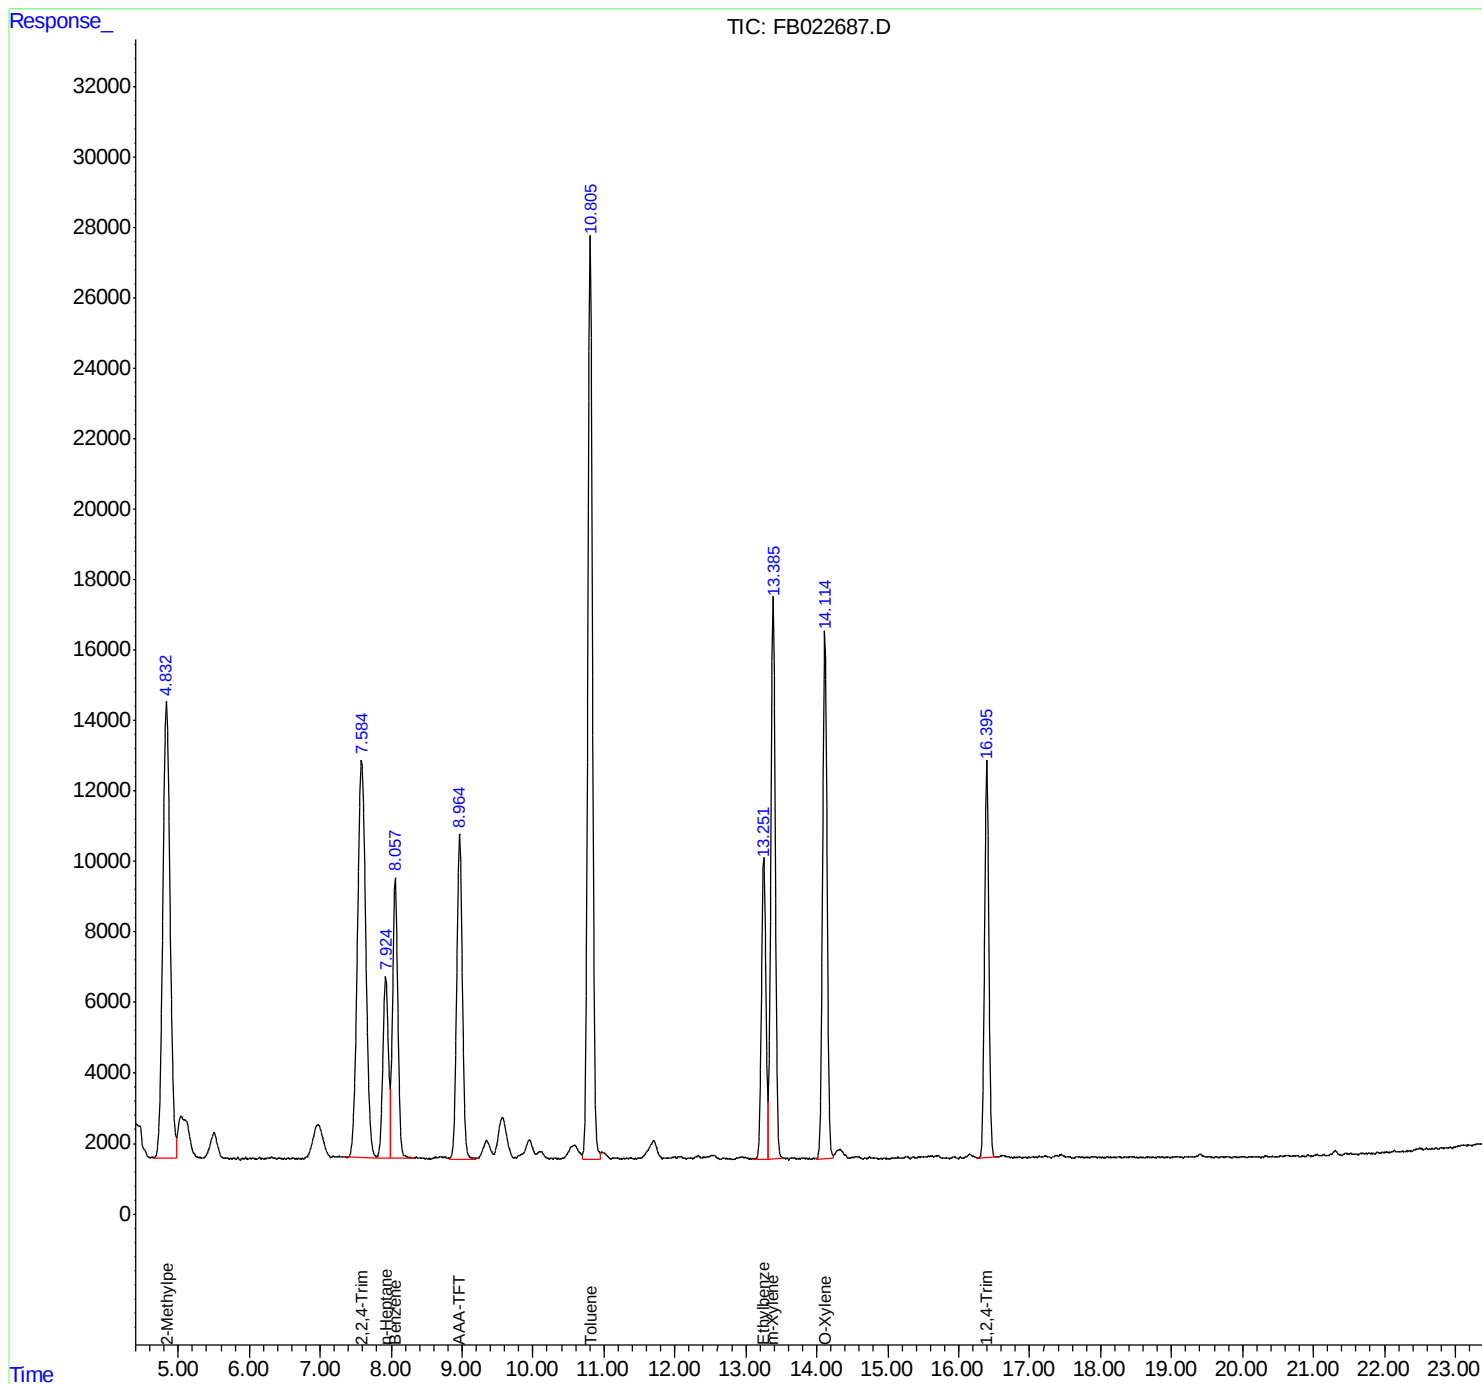

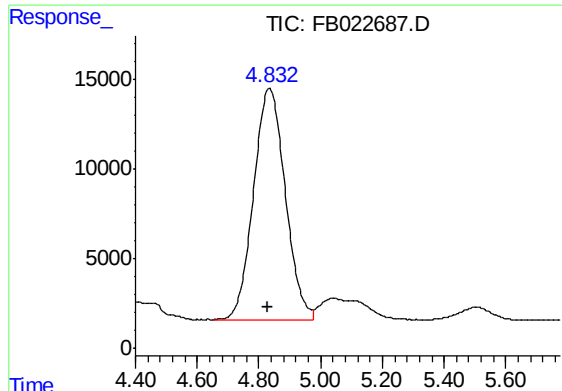


#1 2-Methylpentane

R.T.: 4.834 min
Delta R.T.: 0.004 min
Response: 920303
Conc: 27.60 ng/ml

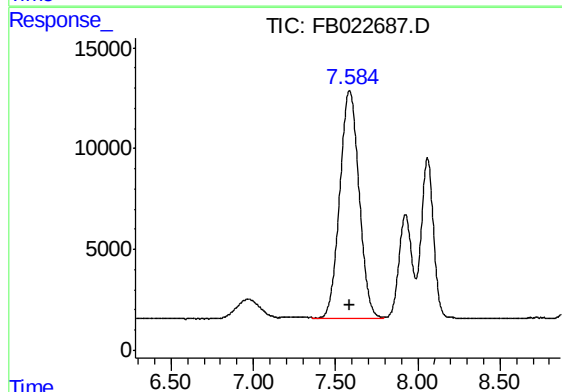


#2 2,2,4-Trimethylpentane

R.T.: 7.586 min
Delta R.T.: 0.000 min
Response: 915867
Conc: 26.40 ng/ml

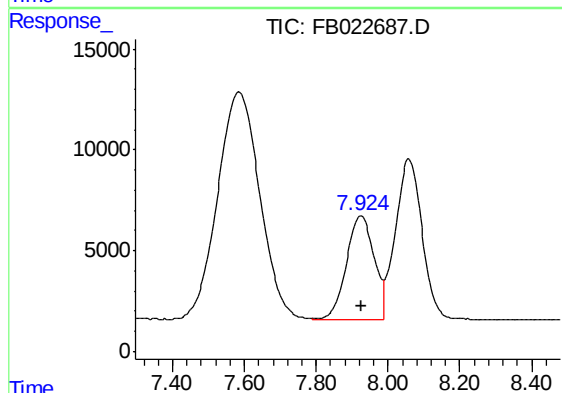


#3 n-Heptane

R.T.: 7.925 min
Delta R.T.: 0.000 min
Response: 274223
Conc: 8.10 ng/ml

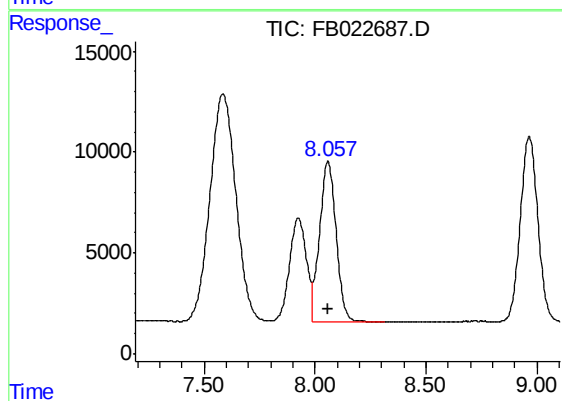


#4 Benzene

R.T.: 8.059 min
Delta R.T.: -0.002 min
Response: 412337
Conc: 9.90 ng/ml

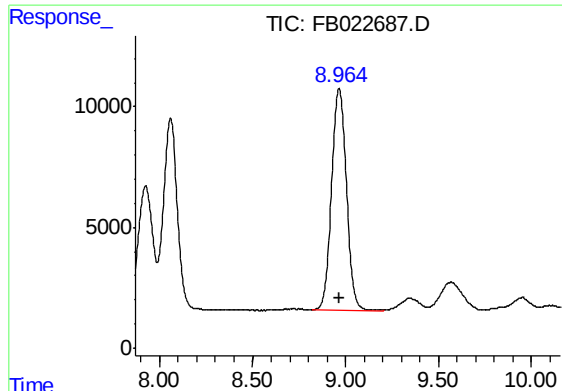


#5 AAA-TFT

R.T.: 8.966 min
Delta R.T.: -0.002 min
Response: 509966
Conc: 21.17 ng/ml

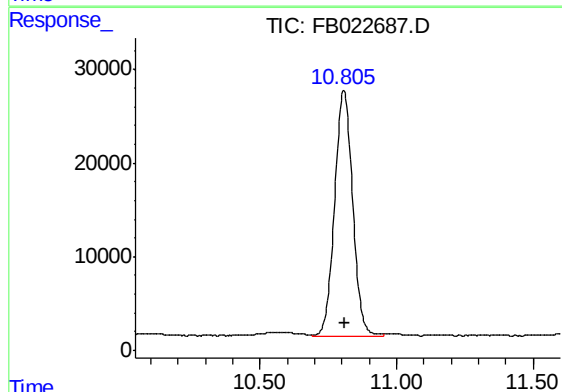


#6 Toluene

R.T.: 10.807 min
Delta R.T.: -0.003 min
Response: 1200293
Conc: 29.65 ng/ml

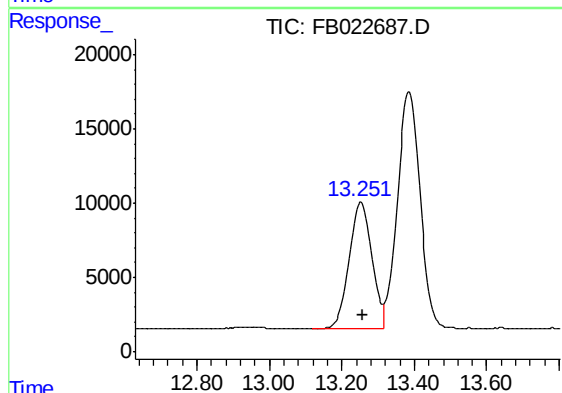


#7 Ethylbenzene

R.T.: 13.252 min
Delta R.T.: -0.004 min
Response: 369693
Conc: 9.55 ng/ml

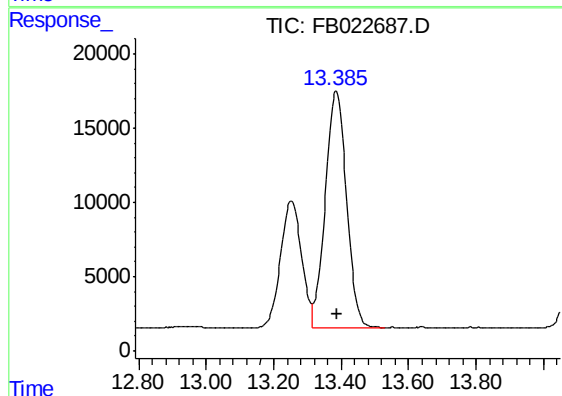

#8 m-Xylene

R.T.: 13.386 min
Delta R.T.: -0.004 min
Response: 692405
Conc: 18.67 ng/ml

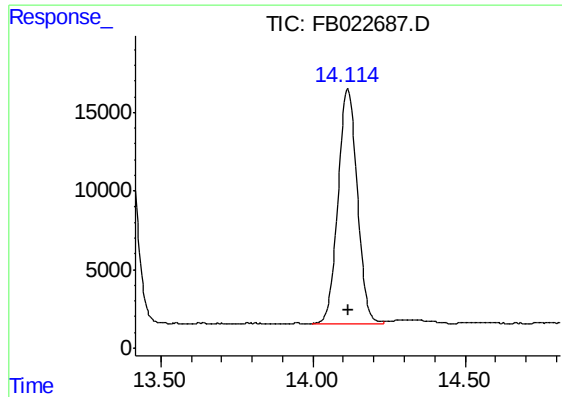


#9 O-Xylene

R.T.: 14.115 min

Delta R.T.: -0.004 min

Response: 655799

Conc: 18.78 ng/ml

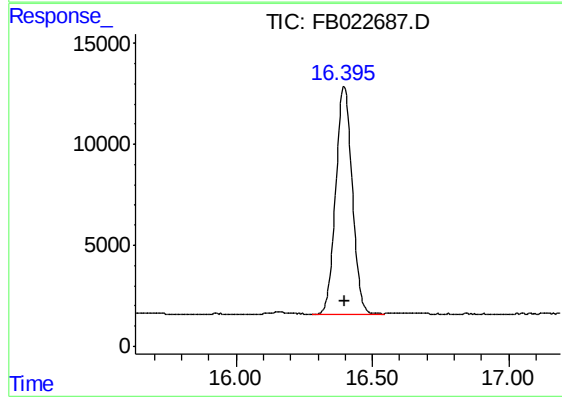

#10 1,2,4-Trimethylbenzene

R.T.: 16.396 min

Delta R.T.: -0.004 min

Response: 474762

Conc: 19.16 ng/ml