

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100422\
 Data File : FB028513.D
 Signal(s) : FID2B.CH
 Acq On : 4 Oct 2022 11:46
 Operator : AJ/MA
 Sample : BSF1004S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1004S1

Integration File: Calibration.e
 Quant Time: Oct 05 05:26:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	240811	20.120 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	575042	28.401 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	627339	29.822 ng/ml
3) t n-Heptane	7.750	200932	9.347 ng/ml
4) t Benzene	7.887	253897	10.320 ng/ml
6) t Toluene	10.620	735348	31.585 ng/ml
7) t Ethylbenzene	13.057	232672	10.463 ng/ml
8) t m-Xylene	13.190	455218	20.860 ng/ml
9) t O-Xylene	13.917	441324	21.064 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	426758	21.224 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100422\
Data File : FB028513.D
Signal(s) : FID2B.CH
Acq On : 4 Oct 2022 11:46
Operator : AJ/MA
Sample : BSF1004S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1004S1

Integration File: Calibration.e
Quant Time: Oct 05 05:26:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

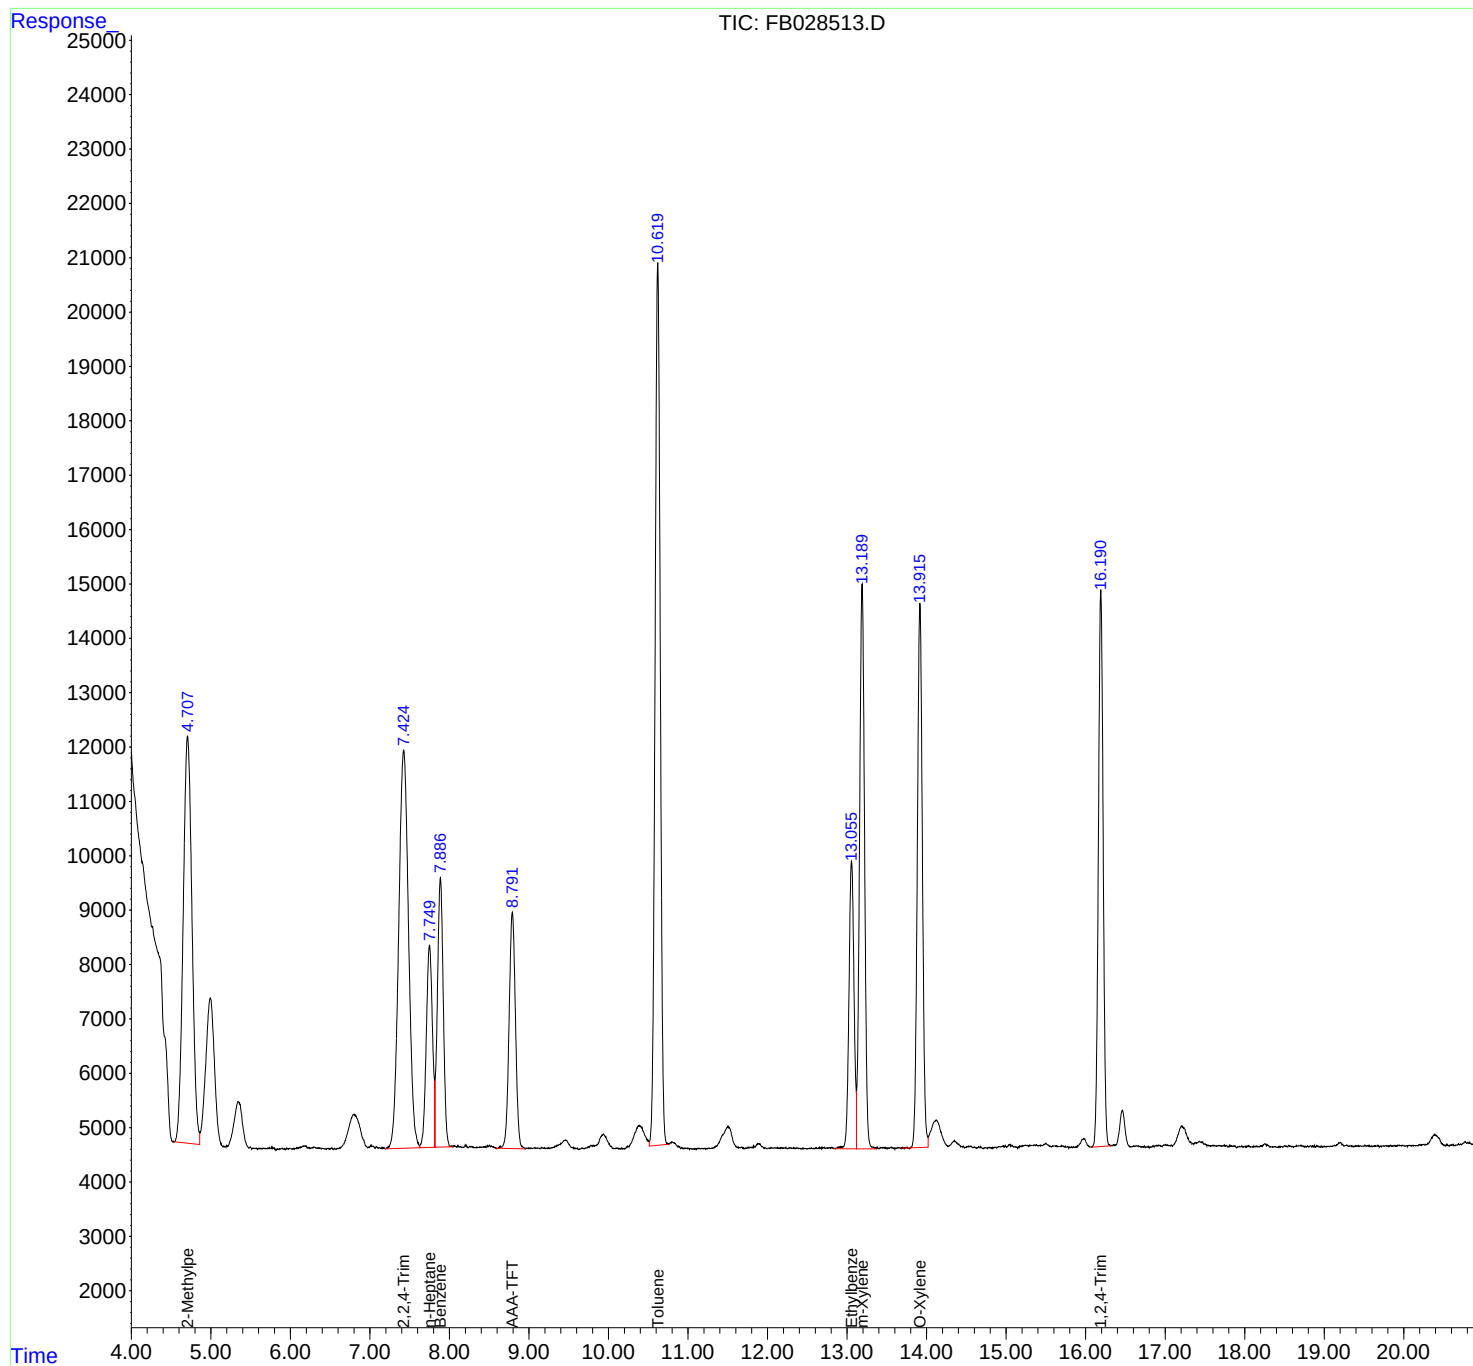


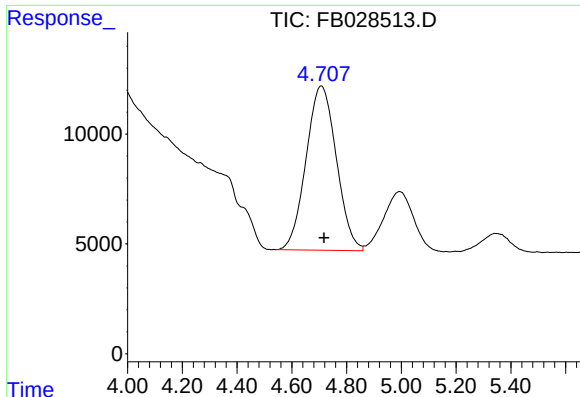

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: -0.010 min
Response: 575042
Conc: 28.40 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1004S1

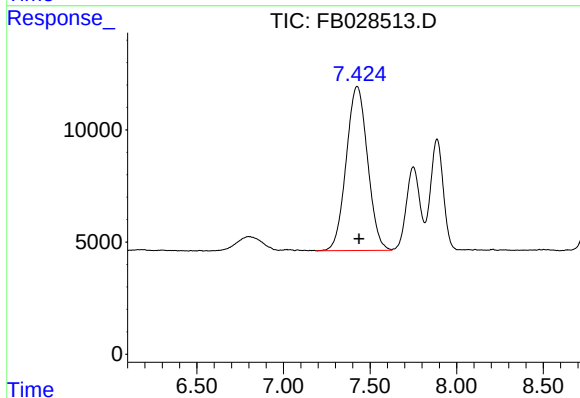


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: -0.011 min
Response: 627339
Conc: 29.82 ng/ml

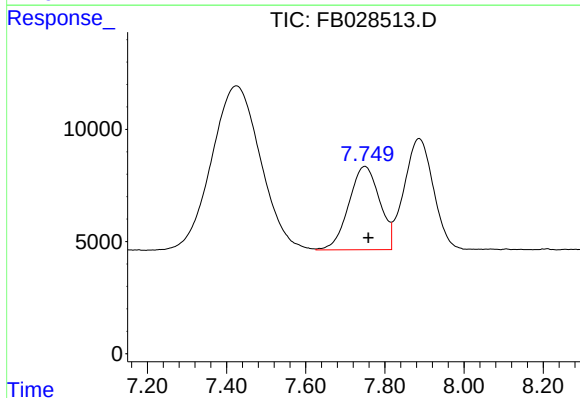


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.008 min
Response: 200932
Conc: 9.35 ng/ml

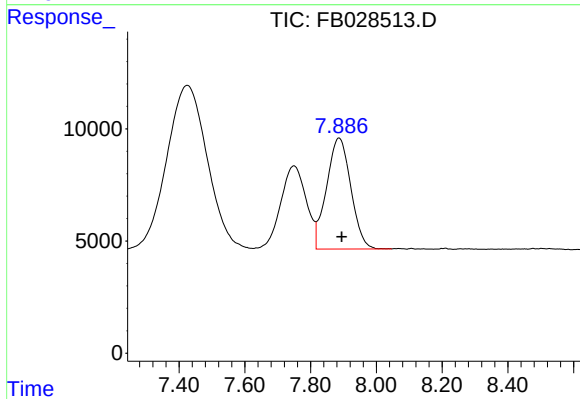

#4 Benzene


R.T.: 7.887 min
Delta R.T.: -0.008 min
Response: 253897
Conc: 10.32 ng/ml

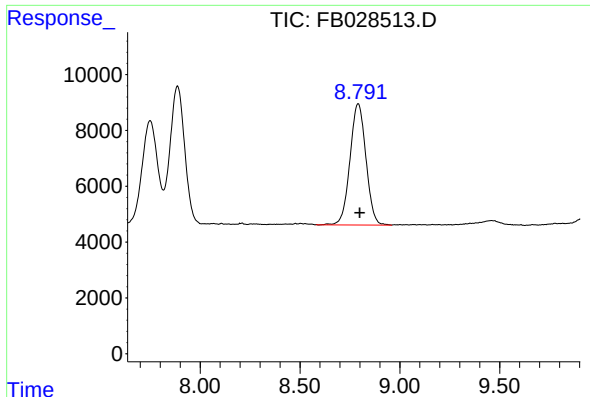

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: -0.008 min
Response: 240811
Conc: 20.12 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1004S1

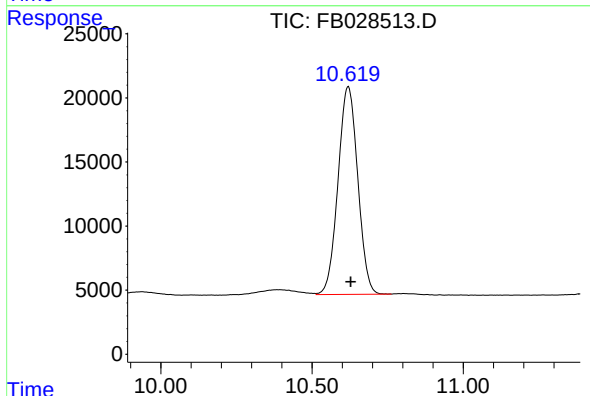


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.008 min
Response: 735348
Conc: 31.59 ng/ml

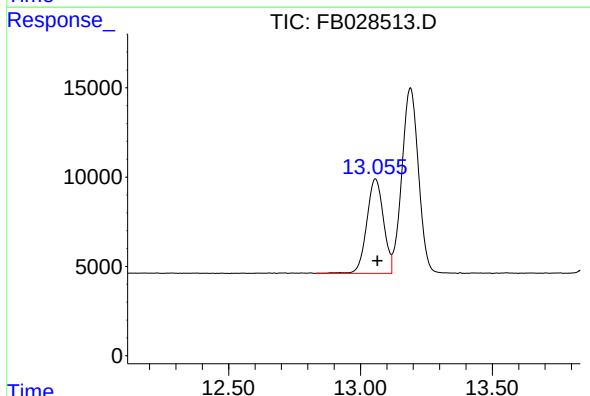


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: -0.008 min
Response: 232672
Conc: 10.46 ng/ml

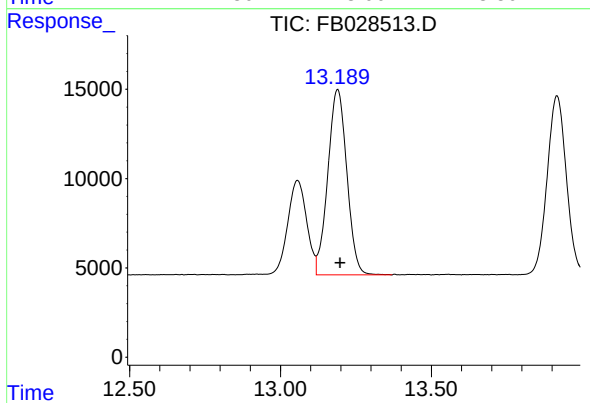

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: -0.007 min
Response: 455218
Conc: 20.86 ng/ml

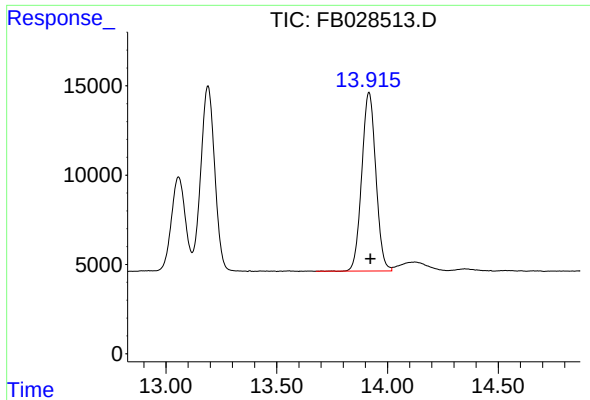

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.007 min
Response: 441324
Conc: 21.06 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1004S1

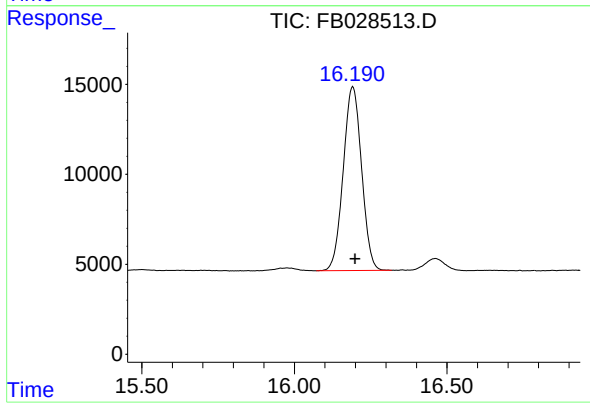

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.008 min
Response: 426758
Conc: 21.22 ng/ml