

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100422\
 Data File : FB028518.D
 Signal(s) : FID2B.CH
 Acq On : 4 Oct 2022 15:17
 Operator : AJ/MA
 Sample : 20 PPB GRO CCC
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO CCC

Integration File: Calibration.e
 Quant Time: Oct 05 05:27:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	245547	20.516 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	547949	27.063 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	609162	28.958 ng/ml
3) t n-Heptane	7.749	186788	8.689 ng/ml
4) t Benzene	7.886	238618	9.699 ng/ml
6) t Toluene	10.620	674674	28.979 ng/ml
7) t Ethylbenzene	13.057	216491	9.735 ng/ml
8) t m-Xylene	13.190	428604	19.640 ng/ml
9) t O-Xylene	13.917	420868	20.087 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	422671	21.021 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100422\
Data File : FB028518.D
Signal(s) : FID2B.CH
Acq On : 4 Oct 2022 15:17
Operator : AJ/MA
Sample : 20 PPB GRO CCC
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 PPB GRO CCC

Integration File: Calibration.e
Quant Time: Oct 05 05:27:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

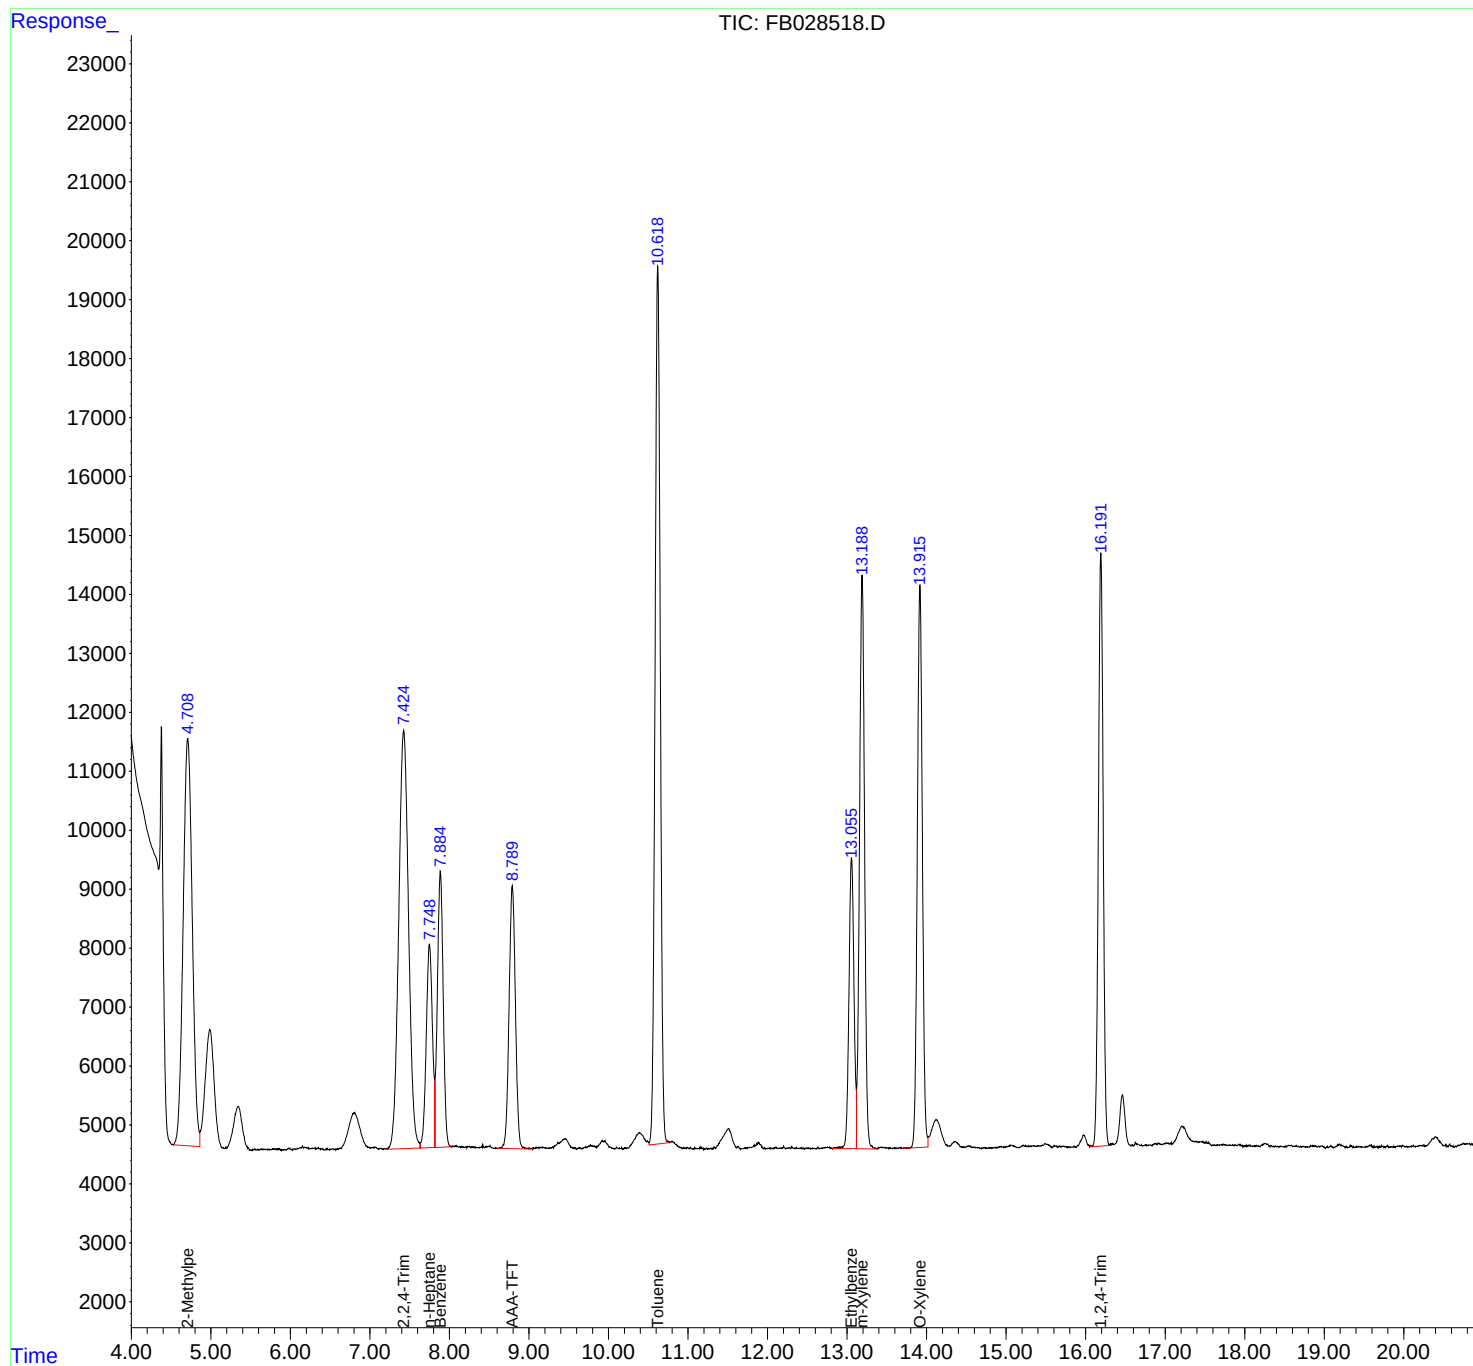


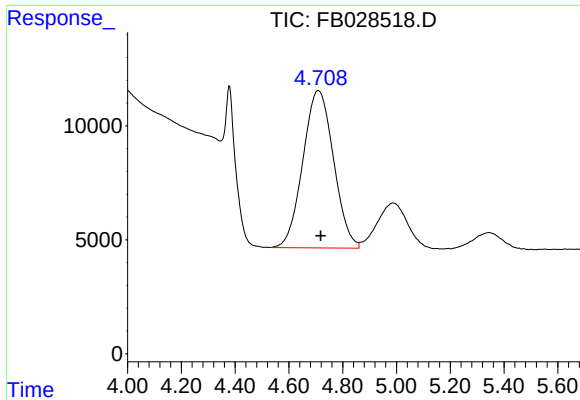

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: -0.008 min
Response: 547949
Conc: 27.06 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO CCC

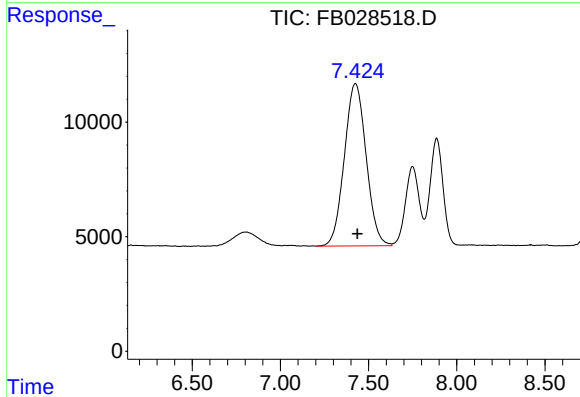


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: -0.012 min
Response: 609162
Conc: 28.96 ng/ml

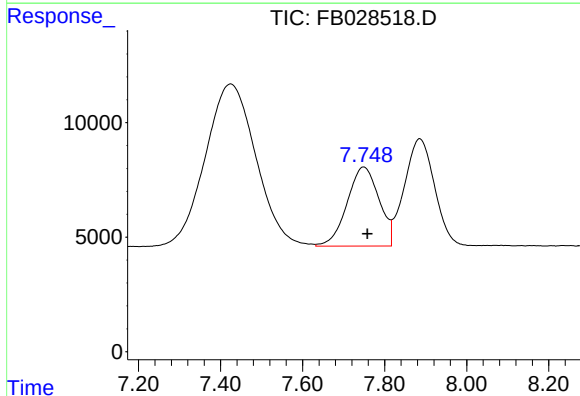


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.009 min
Response: 186788
Conc: 8.69 ng/ml

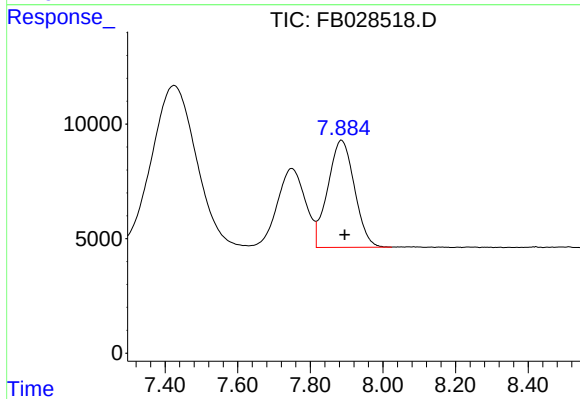

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.009 min
Response: 238618
Conc: 9.70 ng/ml

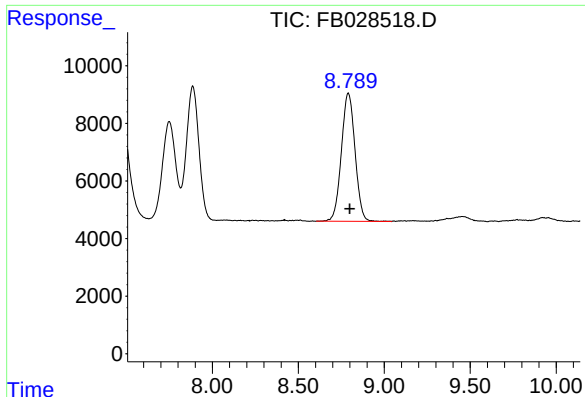

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: -0.009 min
Response: 245547
Conc: 20.52 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO CCC

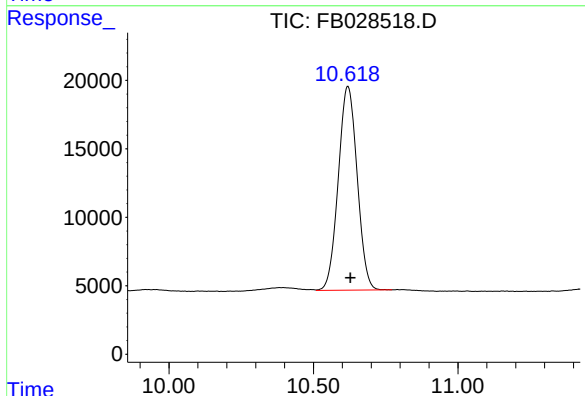


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.008 min
Response: 674674
Conc: 28.98 ng/ml

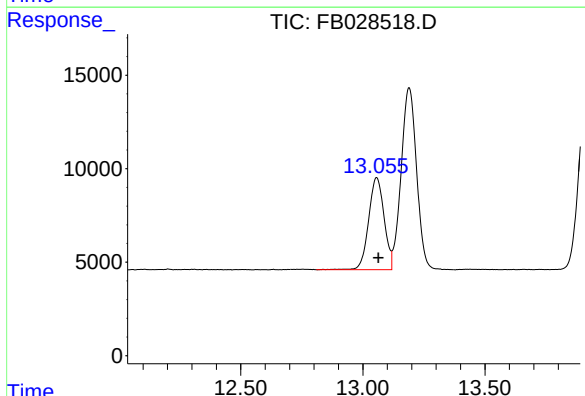


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: -0.008 min
Response: 216491
Conc: 9.73 ng/ml

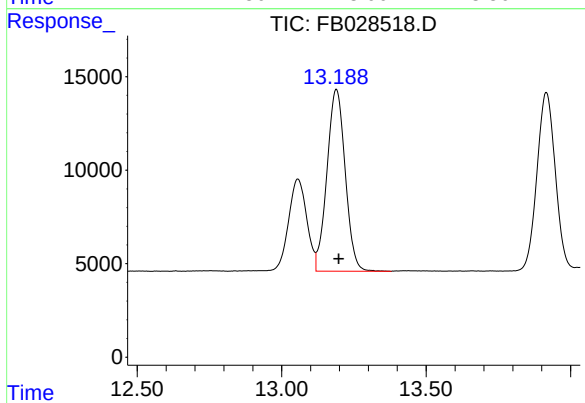

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: -0.008 min
Response: 428604
Conc: 19.64 ng/ml

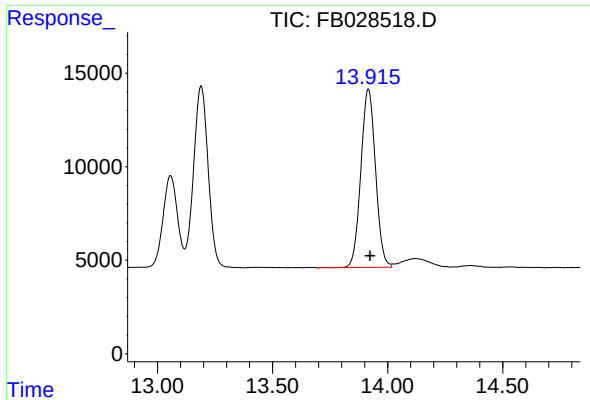

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.007 min
Response: 420868
Conc: 20.09 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO CCC

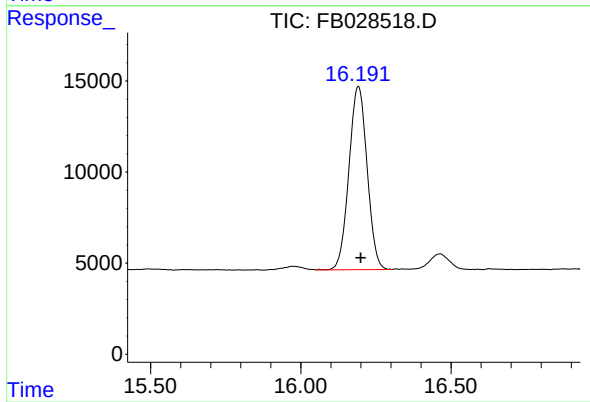

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.007 min
Response: 422671
Conc: 21.02 ng/ml