

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100422\
 Data File : FB028524.D
 Signal(s) : FID2B.CH
 Acq On : 4 Oct 2022 19:29
 Operator : AJ/MA
 Sample : N4936-03MS 50X
 Misc : 5.03G/5.00 ML MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SASP2-T-2-(16-22)MS

Integration File: Calibration.e
 Quant Time: Oct 05 05:27:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	213823	17.865 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.700	425364	21.009 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	550834	26.185 ng/ml
3) t n-Heptane	7.744	152822	7.109 ng/ml
4) t Benzene	7.883	234487	9.532 ng/ml
6) t Toluene	10.619	631876	27.141 ng/ml
7) t Ethylbenzene	13.057	194873	8.763 ng/ml
8) t m-Xylene	13.189	390754	17.906 ng/ml
9) t O-Xylene	13.917	402585	19.215 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	409735	20.378 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100422\
Data File : FB028524.D
Signal(s) : FID2B.CH
Acq On : 4 Oct 2022 19:29
Operator : AJ/MA
Sample : N4936-03MS 50X
Misc : 5.03G/5.00 ML MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SASP2-T-2-(16-22)MS

Integration File: Calibration.e
Quant Time: Oct 05 05:27:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

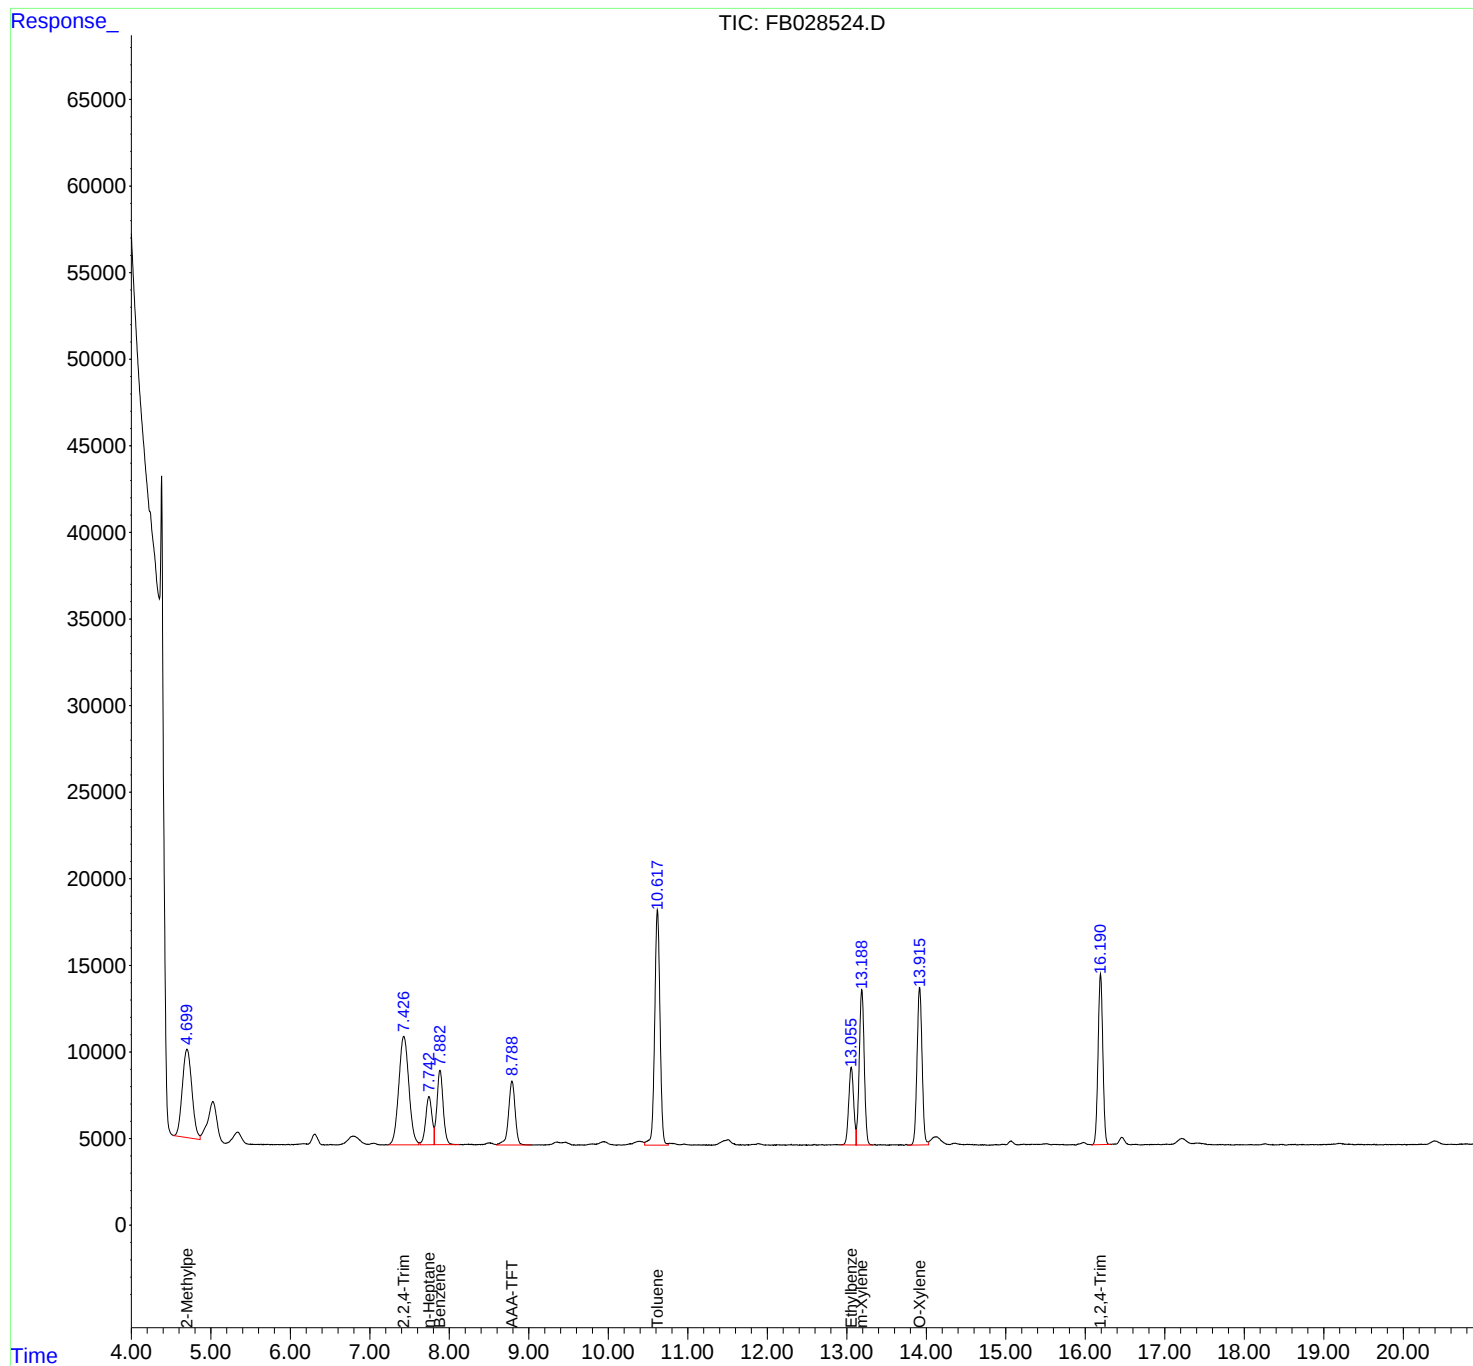


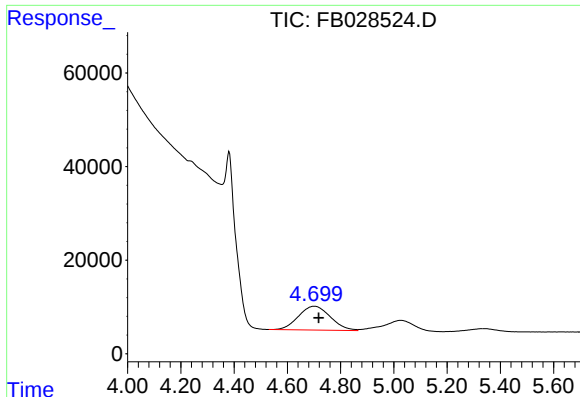

#1 2-Methylpentane


R.T.: 4.700 min
Delta R.T.: -0.018 min
Response: 425364
Conc: 21.01 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-2-(16-22)MS

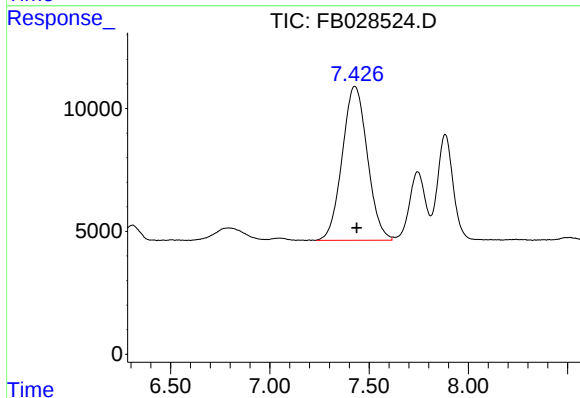


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: -0.010 min
Response: 550834
Conc: 26.19 ng/ml

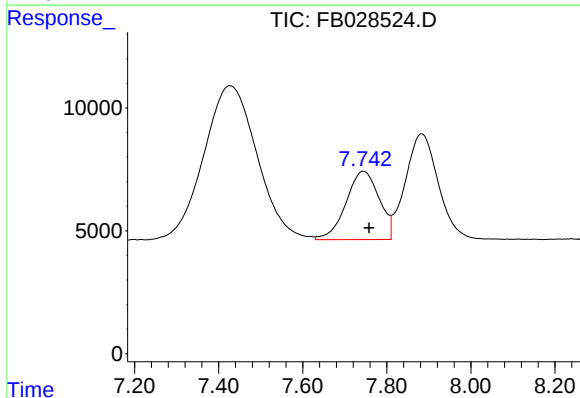


#3 n-Heptane

R.T.: 7.744 min
Delta R.T.: -0.014 min
Response: 152822
Conc: 7.11 ng/ml

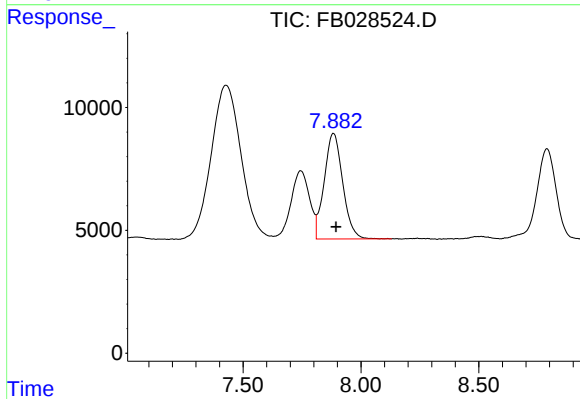

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.011 min
Response: 234487
Conc: 9.53 ng/ml

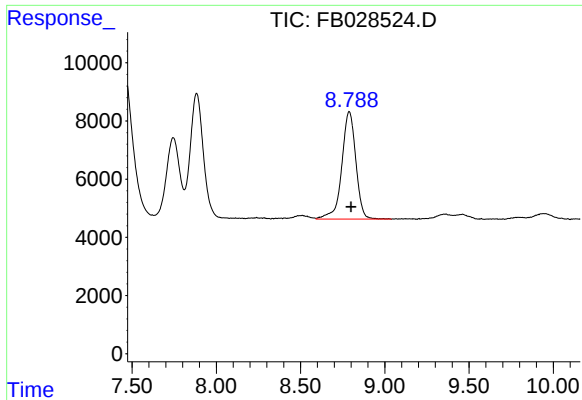

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.011 min
Response: 213823
Conc: 17.87 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-2-(16-22)MS

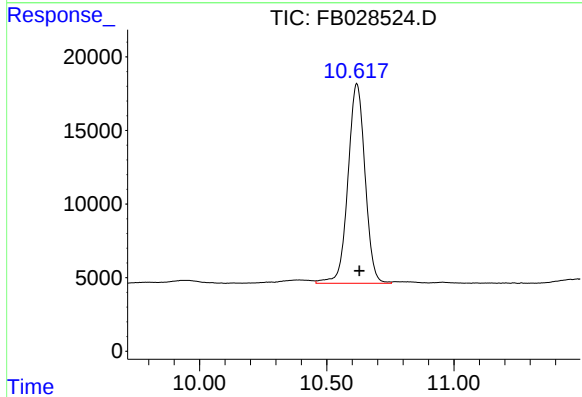


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.010 min
Response: 631876
Conc: 27.14 ng/ml

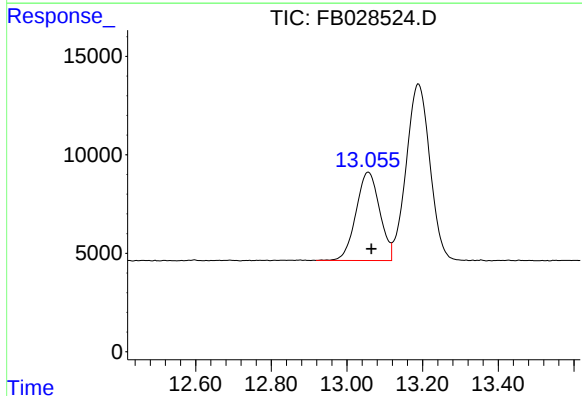


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: -0.008 min
Response: 194873
Conc: 8.76 ng/ml

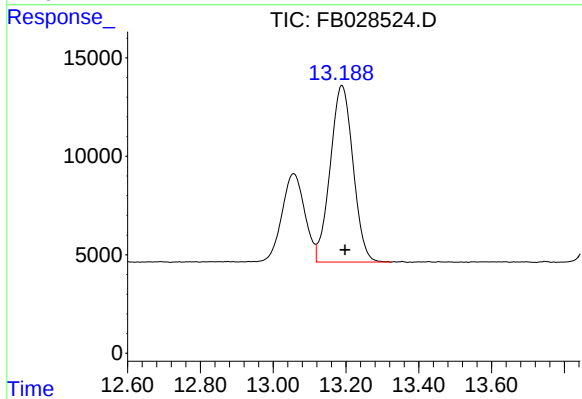

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: -0.008 min
Response: 390754
Conc: 17.91 ng/ml

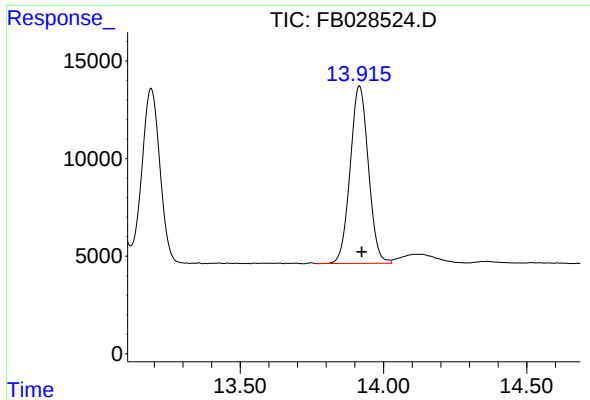

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.007 min
Response: 402585
Conc: 19.21 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-2-(16-22)MS

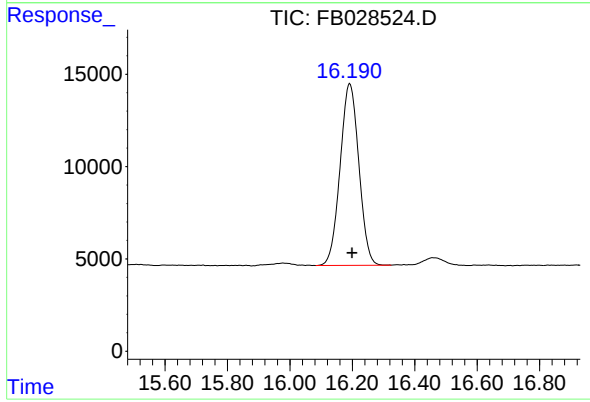

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.007 min
Response: 409735
Conc: 20.38 ng/ml