

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100422\
 Data File : FB028525.D
 Signal(s) : FID2B.CH
 Acq On : 4 Oct 2022 20:08
 Operator : AJ/MA
 Sample : N4936-03MSD 50X
 Misc : 5.08G/5.00 ML MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SASP2-T-2-(16-22)MSD

Integration File: Calibration.e
 Quant Time: Oct 05 05:27:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	214847	17.951 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.695	412234	20.360 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	547164	26.011 ng/ml
3) t n-Heptane	7.744	172337	8.017 ng/ml
4) t Benzene	7.883	247531	10.062 ng/ml
6) t Toluene	10.618	656946	28.218 ng/ml
7) t Ethylbenzene	13.056	199729	8.981 ng/ml
8) t m-Xylene	13.189	394551	18.080 ng/ml
9) t O-Xylene	13.916	390286	18.628 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	363093	18.058 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100422\
Data File : FB028525.D
Signal(s) : FID2B.CH
Acq On : 4 Oct 2022 20:08
Operator : AJ/MA
Sample : N4936-03MSD 50X
Misc : 5.08G/5.00 ML MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SASP2-T-2-(16-22)MSD

Integration File: Calibration.e
Quant Time: Oct 05 05:27:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

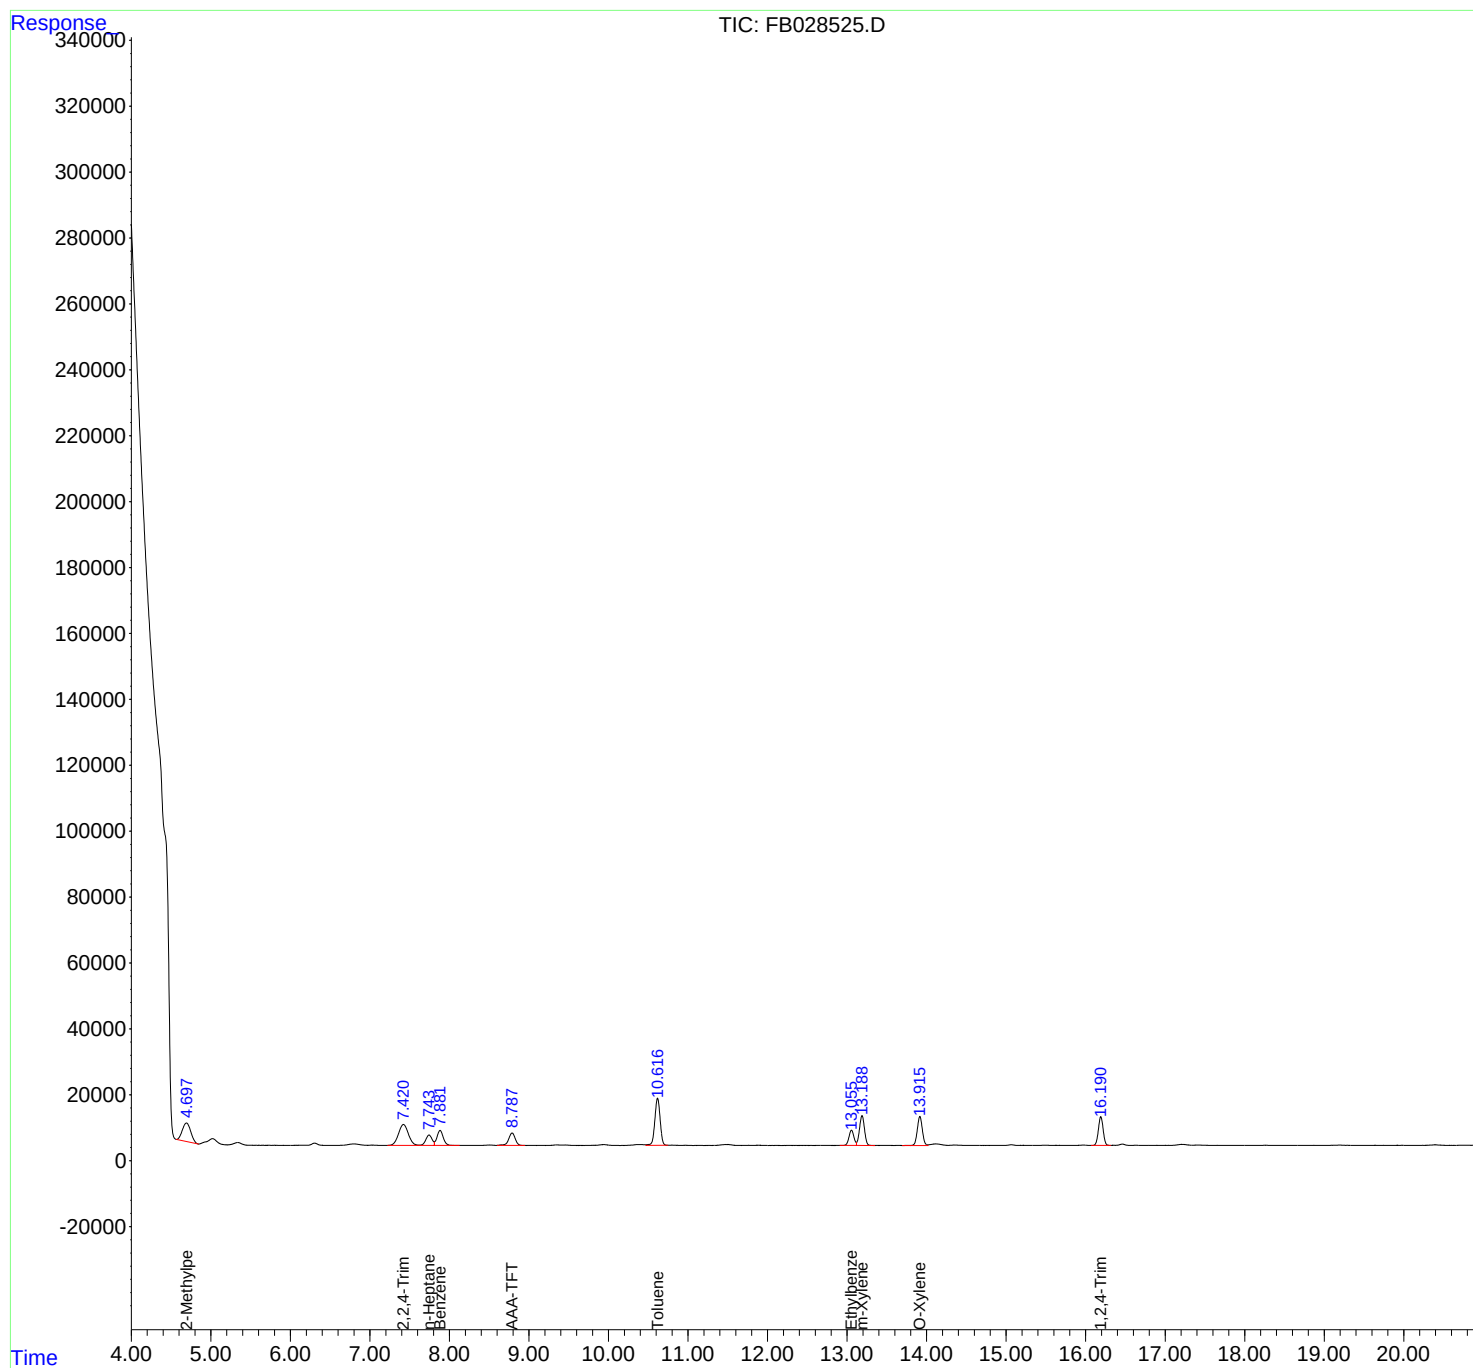


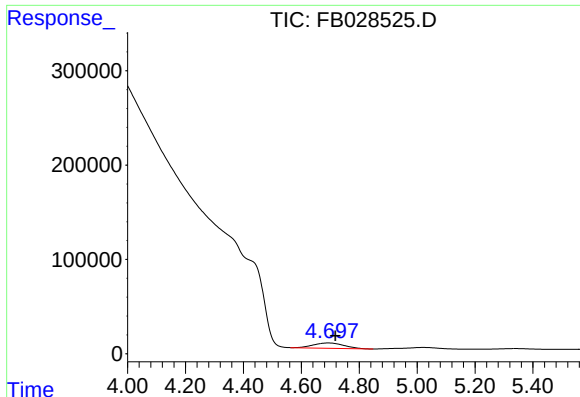

#1 2-Methylpentane


R.T.: 4.695 min
Delta R.T.: -0.023 min
Response: 412234
Conc: 20.36 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-2-(16-22)MSD

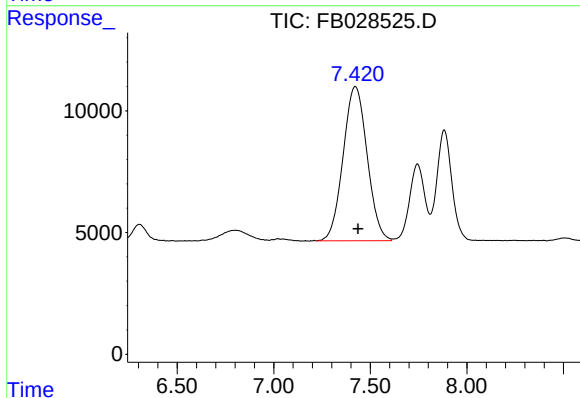


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: -0.016 min
Response: 547164
Conc: 26.01 ng/ml

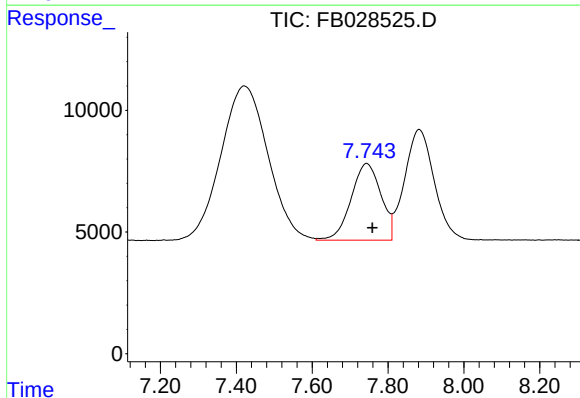


#3 n-Heptane

R.T.: 7.744 min
Delta R.T.: -0.014 min
Response: 172337
Conc: 8.02 ng/ml

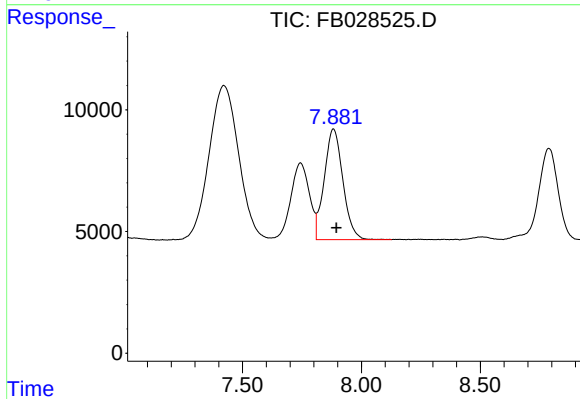

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.012 min
Response: 247531
Conc: 10.06 ng/ml

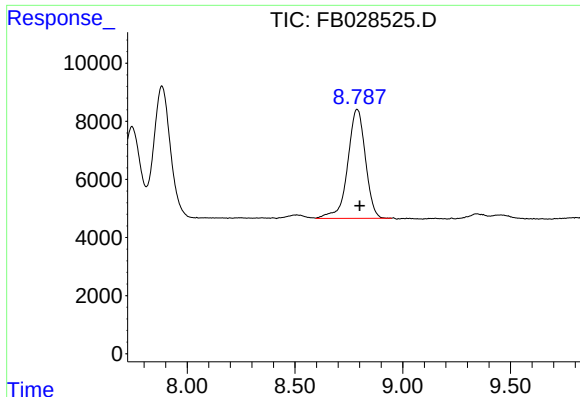

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: -0.011 min
Response: 214847
Conc: 17.95 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-2-(16-22)MSD

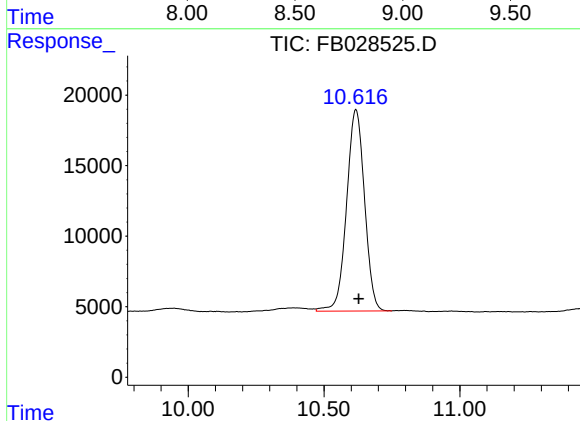


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.010 min
Response: 656946
Conc: 28.22 ng/ml

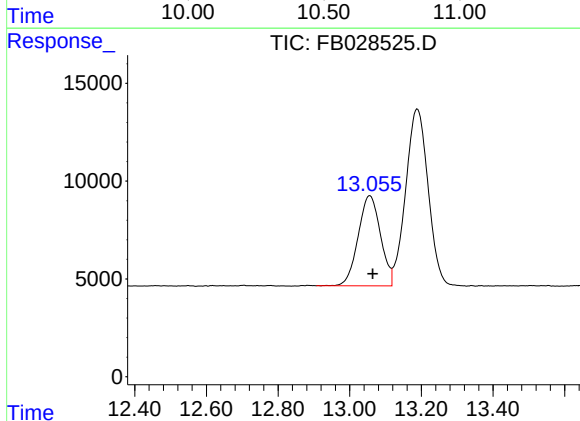


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.008 min
Response: 199729
Conc: 8.98 ng/ml

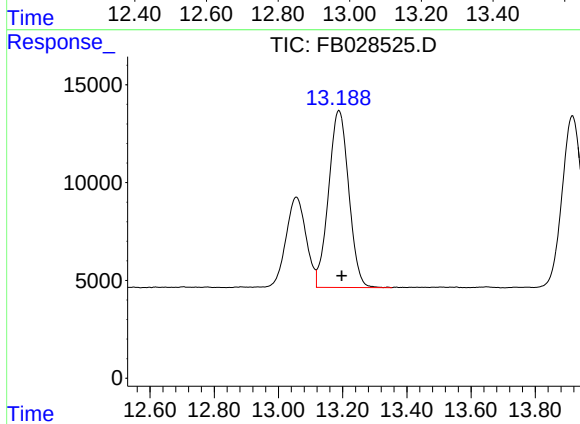

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: -0.008 min
Response: 394551
Conc: 18.08 ng/ml

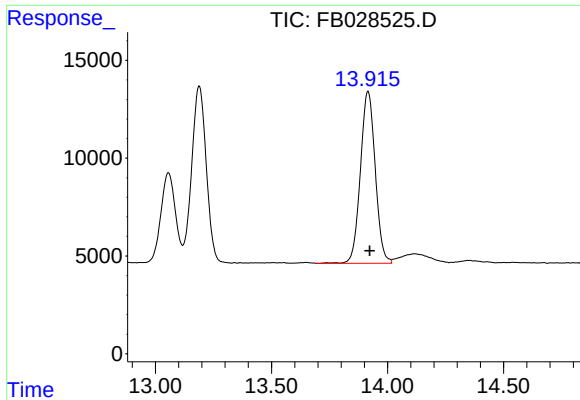

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.008 min
Response: 390286
Conc: 18.63 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-2-(16-22)MSD

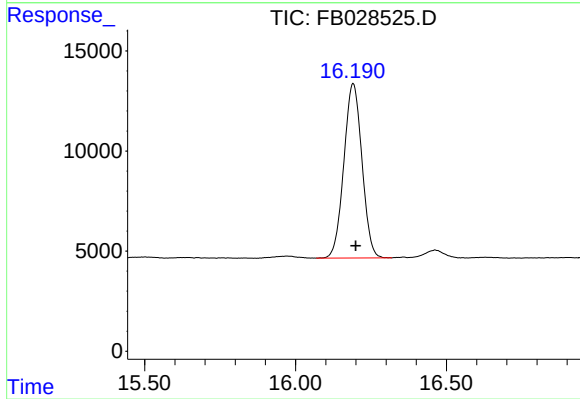

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.008 min
Response: 363093
Conc: 18.06 ng/ml