

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100422\
 Data File : FB028526.D
 Signal(s) : FID2B.CH
 Acq On : 4 Oct 2022 20:47
 Operator : AJ/MA
 Sample : BSF1004S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1004S2

Integration File: Calibration.e
 Quant Time: Oct 05 05:28:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	216719	18.107 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	526602	26.009 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	588044	27.954 ng/ml
3) t n-Heptane	7.750	178334	8.296 ng/ml
4) t Benzene	7.887	241142	9.802 ng/ml
6) t Toluene	10.620	691186	29.688 ng/ml
7) t Ethylbenzene	13.057	214816	9.660 ng/ml
8) t m-Xylene	13.189	427920	19.609 ng/ml
9) t O-Xylene	13.917	422610	20.170 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	415160	20.647 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100422\
Data File : FB028526.D
Signal(s) : FID2B.CH
Acq On : 4 Oct 2022 20:47
Operator : AJ/MA
Sample : BSF1004S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1004S2

Integration File: Calibration.e
Quant Time: Oct 05 05:28:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

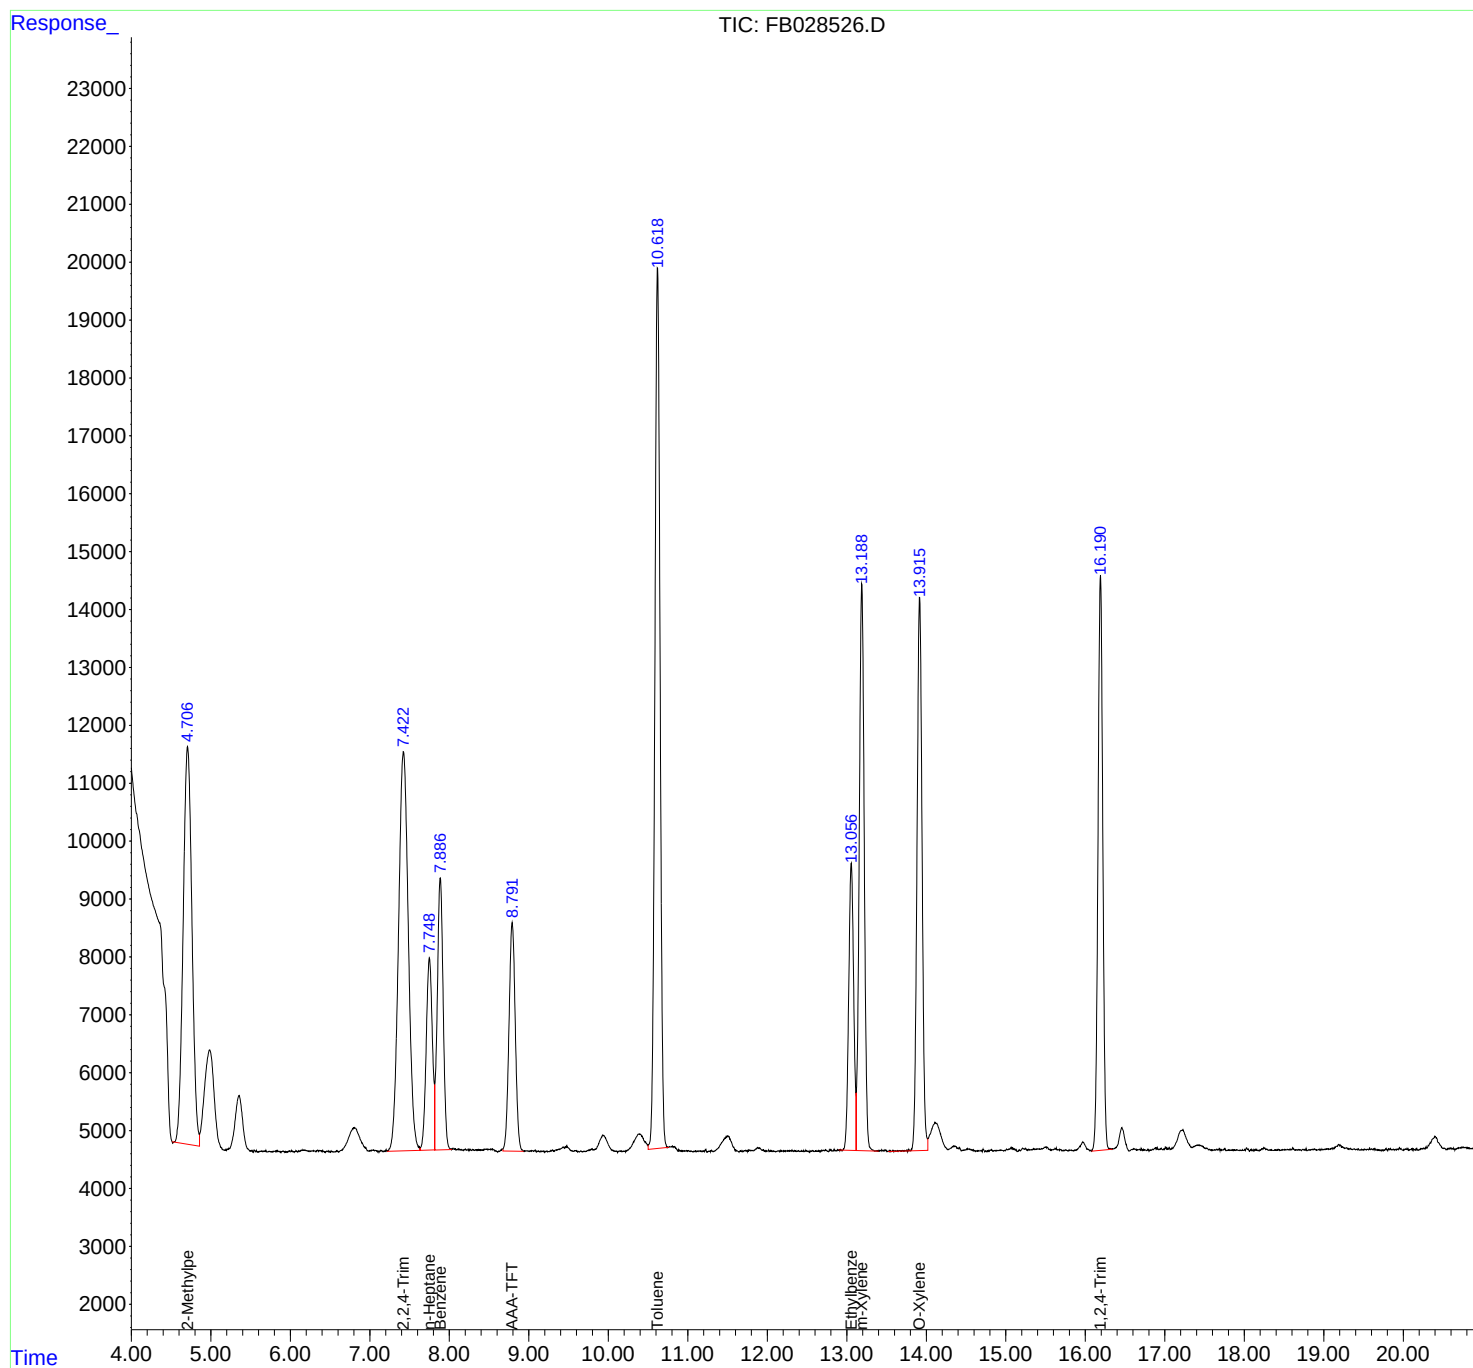


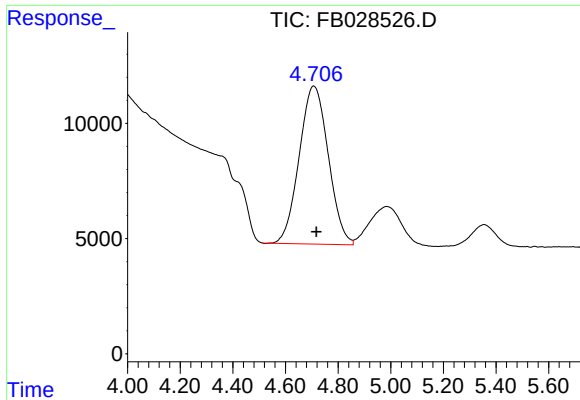

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: -0.011 min
Response: 526602
Conc: 26.01 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1004S2

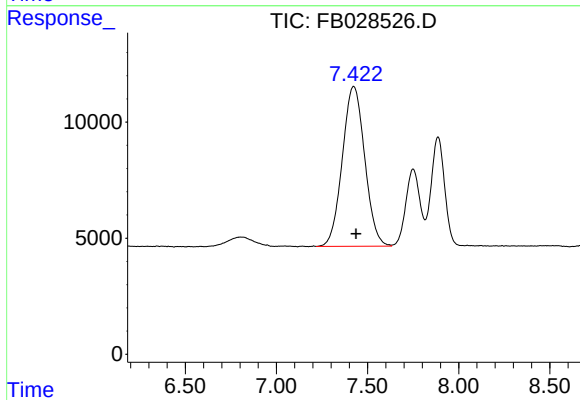


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: -0.014 min
Response: 588044
Conc: 27.95 ng/ml

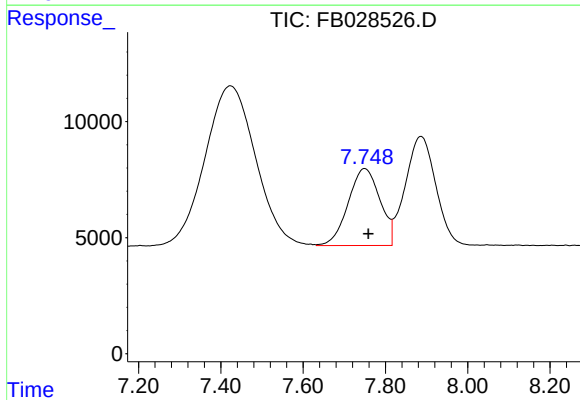


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.009 min
Response: 178334
Conc: 8.30 ng/ml

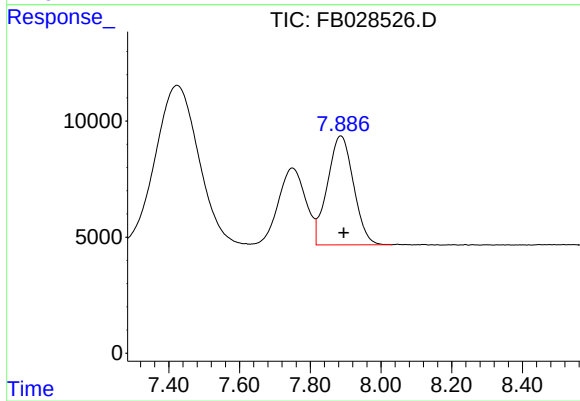

#4 Benzene


R.T.: 7.887 min
Delta R.T.: -0.008 min
Response: 241142
Conc: 9.80 ng/ml

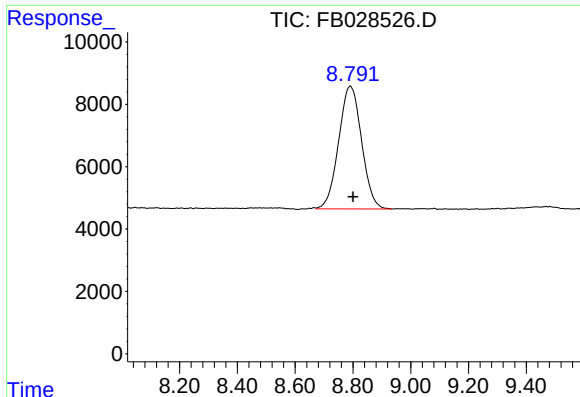

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: -0.008 min
Response: 216719
Conc: 18.11 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1004S2

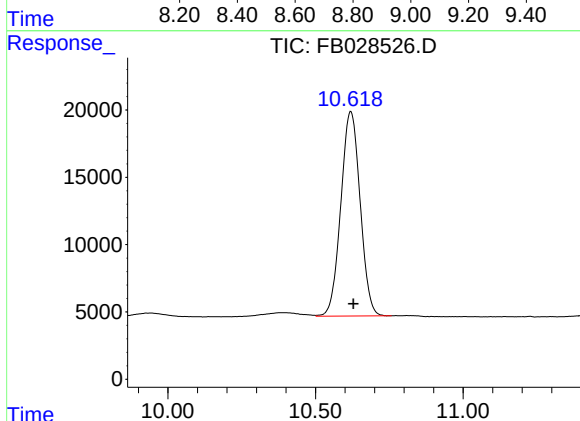


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.008 min
Response: 691186
Conc: 29.69 ng/ml

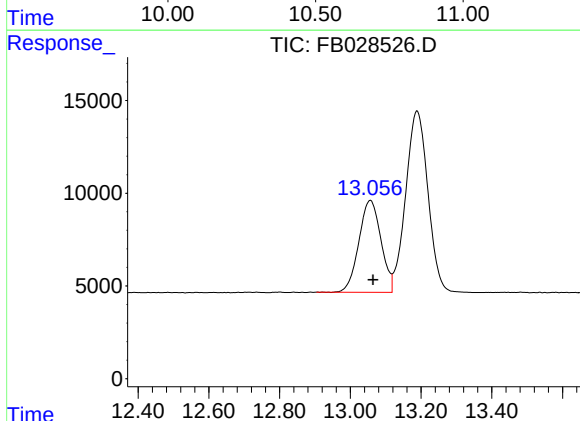


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: -0.008 min
Response: 214816
Conc: 9.66 ng/ml

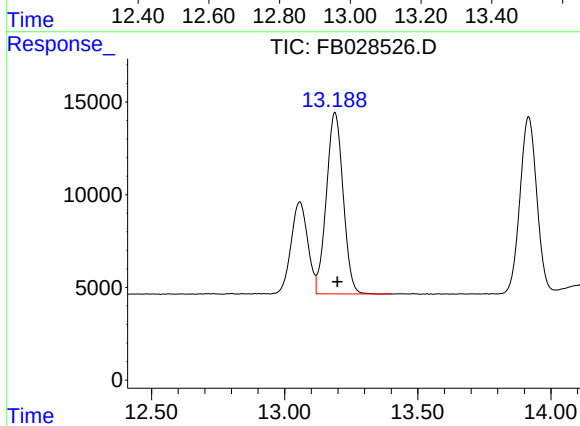

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: -0.008 min
Response: 427920
Conc: 19.61 ng/ml

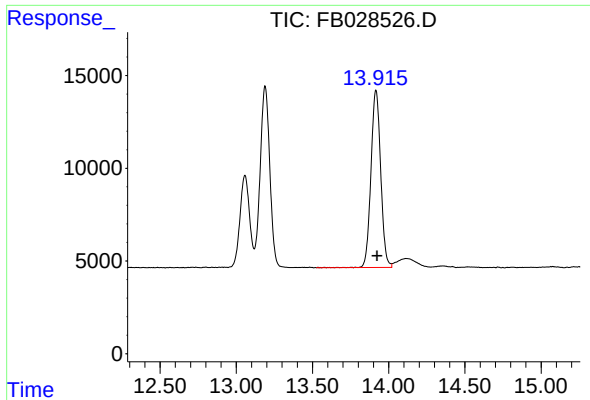

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.007 min
Response: 422610
Conc: 20.17 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1004S2

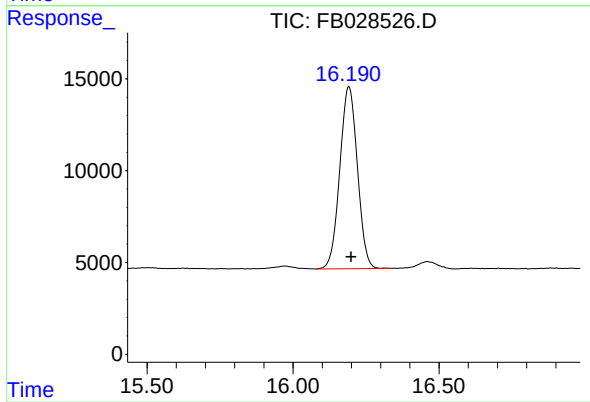

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.007 min
Response: 415160
Conc: 20.65 ng/ml