

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100423\
 Data File : FB030388.D
 Signal(s) : FID2B.CH
 Acq On : 4 Oct 2023 11:06
 Operator : YP/AJ
 Sample : BSF1004W2
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 05 00:15:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
 Quant Title :
 QLast Update : Mon Sep 18 13:44:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	199385	14.415 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	490904	26.818 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	546846	27.031 ng/ml
3) t n-Heptane	7.745	190904	8.985 ng/ml
4) t Benzene	7.883	235320	9.244 ng/ml
6) t Toluene	10.616	697315	28.134 ng/ml
7) t Ethylbenzene	13.052	218562	9.389 ng/ml
8) t m-Xylene	13.184	431004	18.791 ng/ml
9) t O-Xylene	13.911	414240	18.655 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	391855	17.883 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100423\
Data File : FB030388.D
Signal(s) : FID2B.CH
Acq On : 4 Oct 2023 11:06
Operator : YP/AJ
Sample : BSF1004W2
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 05 00:15:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
Quant Title :
QLast Update : Mon Sep 18 13:44:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

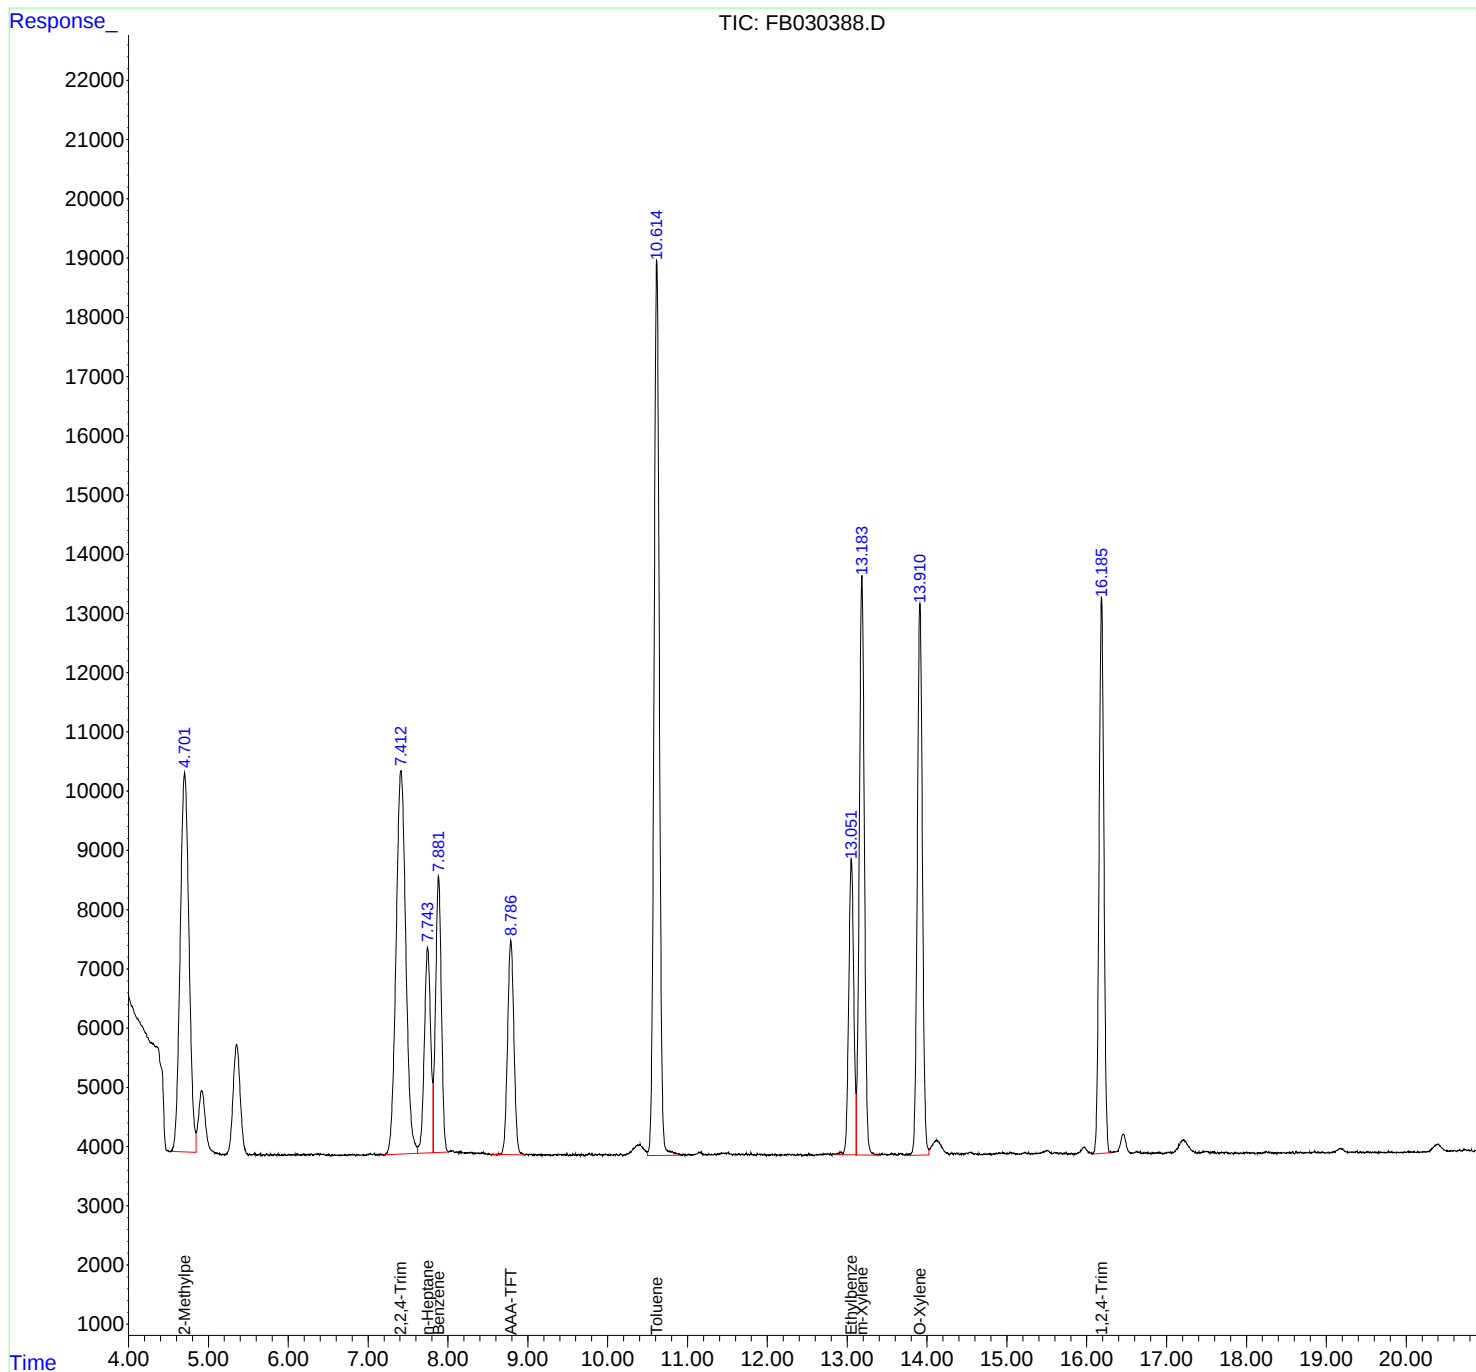


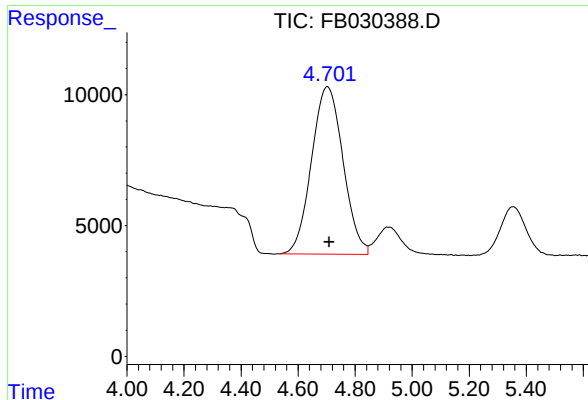

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: -0.007 min
Response: 490904
Conc: 26.82 ng/ml

Instrument :
FID_B
ClientSampleId :

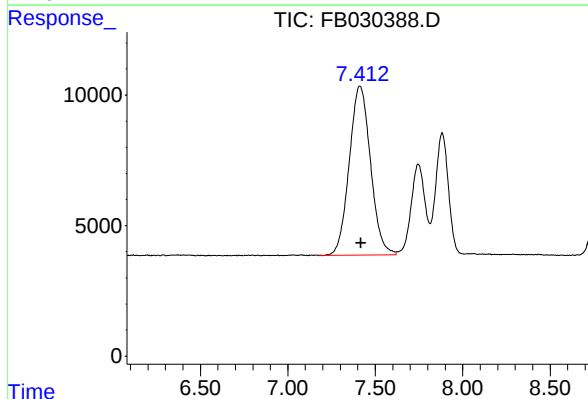


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.006 min
Response: 546846
Conc: 27.03 ng/ml

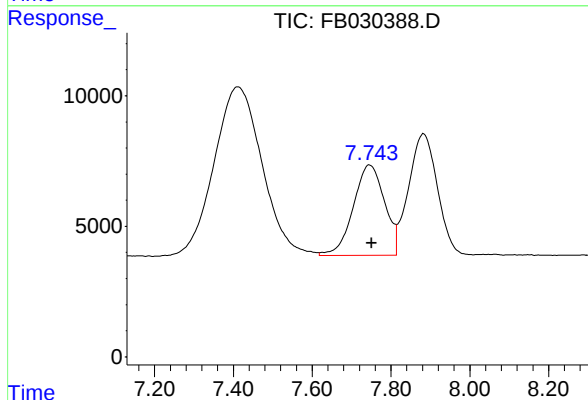


#3 n-Heptane

R.T.: 7.745 min
Delta R.T.: -0.005 min
Response: 190904
Conc: 8.99 ng/ml

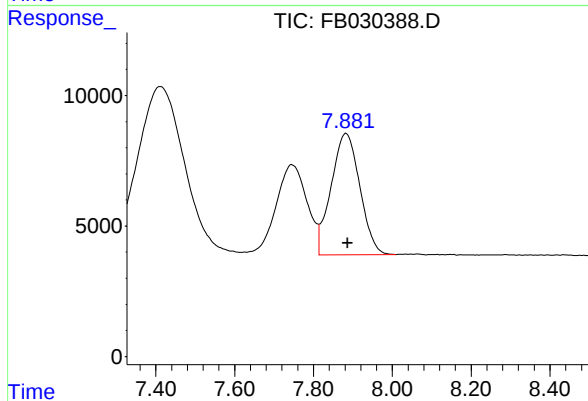

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.004 min
Response: 235320
Conc: 9.24 ng/ml

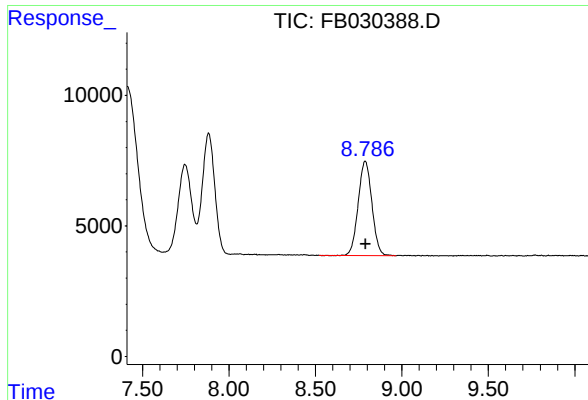

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: -0.004 min
Response: 199385
Conc: 14.41 ng/ml

Instrument :
FID_B
ClientSampleId :

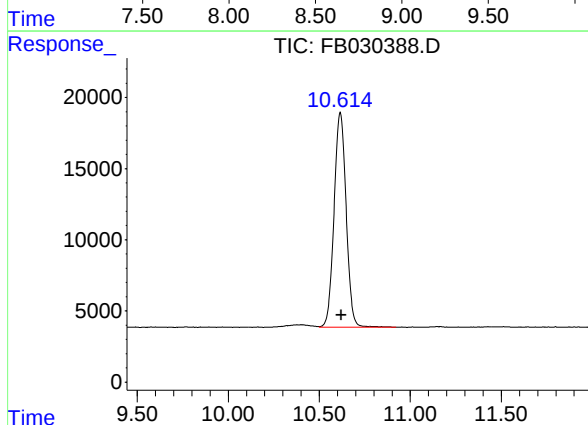


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.004 min
Response: 697315
Conc: 28.13 ng/ml

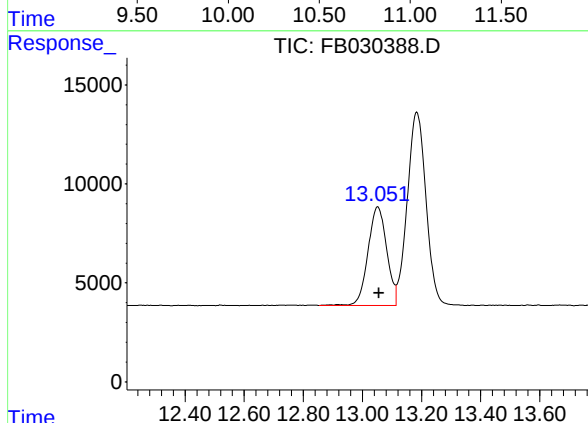


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.004 min
Response: 218562
Conc: 9.39 ng/ml

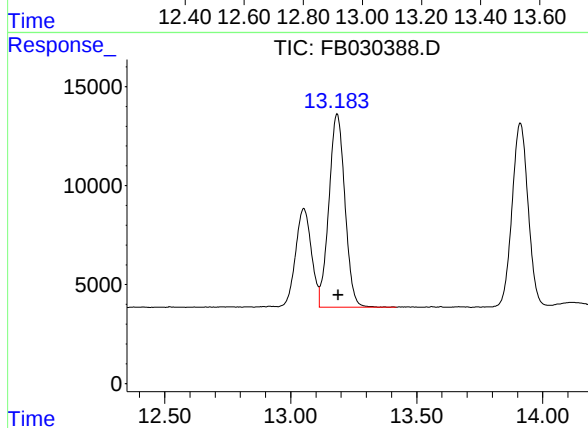

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: -0.004 min
Response: 431004
Conc: 18.79 ng/ml

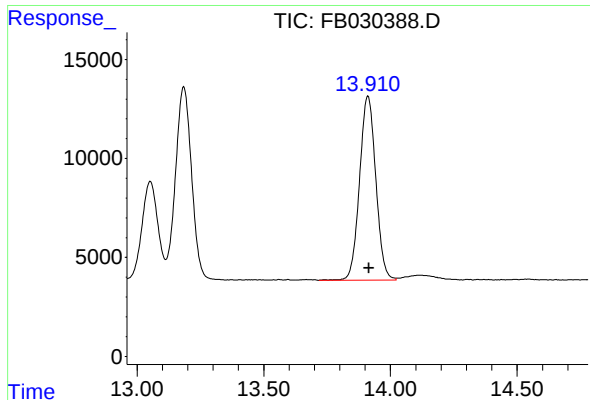

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: -0.004 min
Response: 414240
Conc: 18.66 ng/ml

Instrument :
FID_B
ClientSampleId :

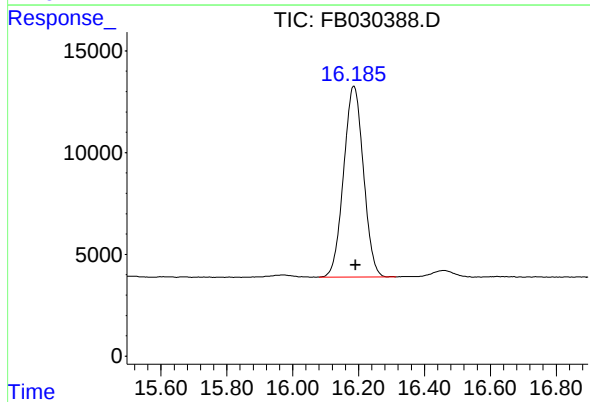

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: -0.005 min
Response: 391855
Conc: 17.88 ng/ml