

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100423\
 Data File : FB030387.D
 Signal(s) : FID2B.CH
 Acq On : 4 Oct 2023 10:27
 Operator : YP/AJ
 Sample : BSF1004W1
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1004W1

Integration File: Calibration.e
 Quant Time: Oct 05 00:15:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
 Quant Title :
 QLast Update : Mon Sep 18 13:44:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	263443	19.046 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	475325	25.967 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	558268	27.595 ng/ml
3) t n-Heptane	7.746	178228	8.388 ng/ml
4) t Benzene	7.883	220420	8.659 ng/ml
6) t Toluene	10.614	652424	26.322 ng/ml
7) t Ethylbenzene	13.051	208695	8.965 ng/ml
8) t m-Xylene	13.184	414042	18.052 ng/ml
9) t O-Xylene	13.910	399918	18.010 ng/ml
10) t 1,2,4-Trimethylbenzene	16.185	402265	18.359 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100423\
Data File : FB030387.D
Signal(s) : FID2B.CH
Acq On : 4 Oct 2023 10:27
Operator : YP/AJ
Sample : BSF1004W1
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1004W1

Integration File: Calibration.e
Quant Time: Oct 05 00:15:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091823.M
Quant Title :
QLast Update : Mon Sep 18 13:44:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

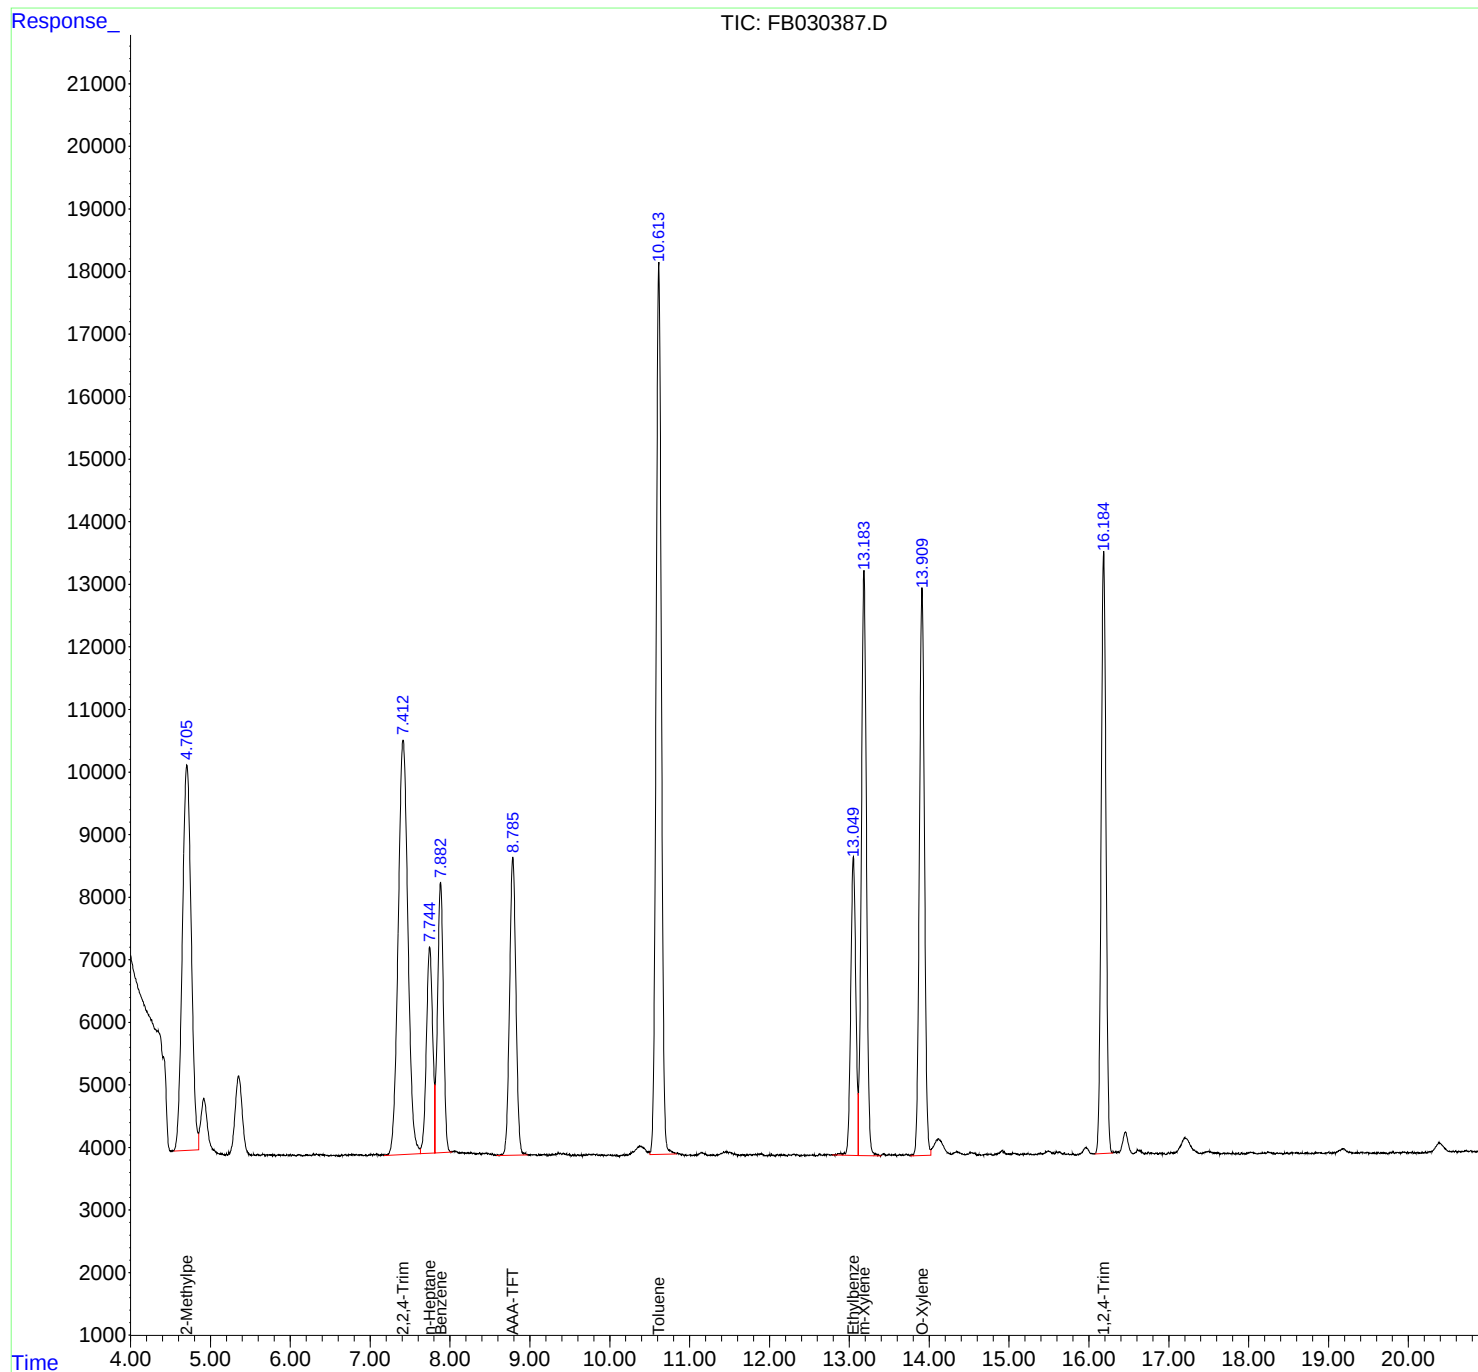


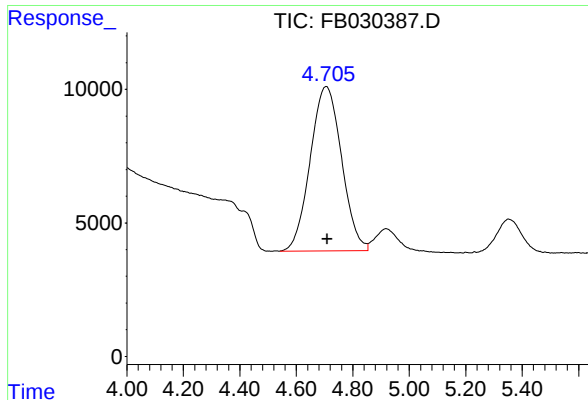

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: -0.004 min
Response: 475325
Conc: 25.97 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1004W1

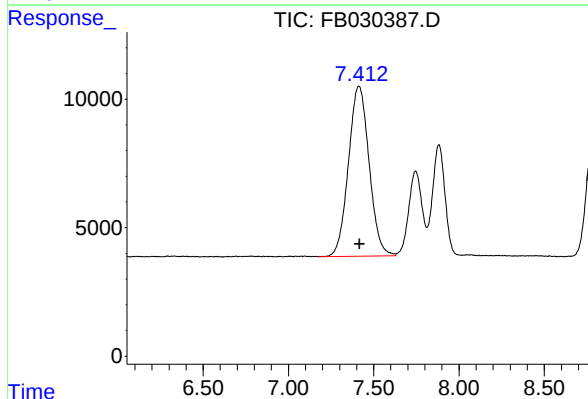


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.005 min
Response: 558268
Conc: 27.60 ng/ml

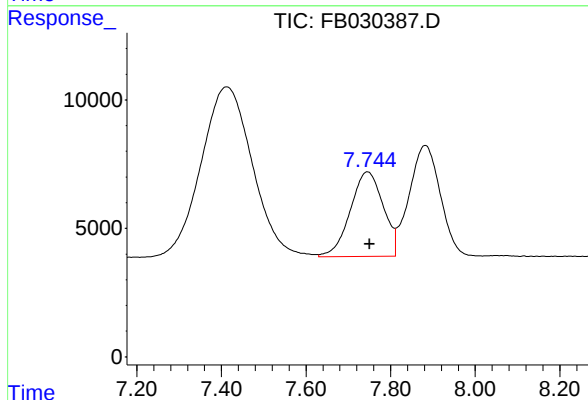


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.004 min
Response: 178228
Conc: 8.39 ng/ml

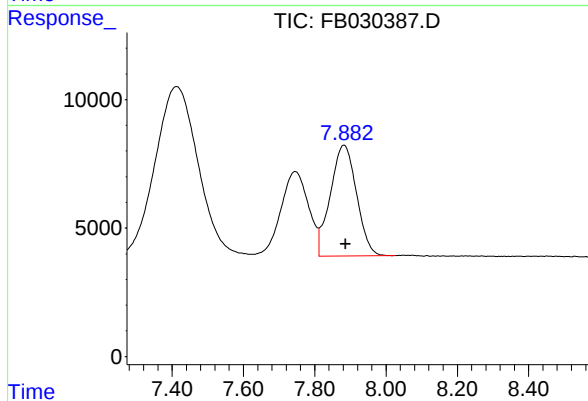

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.004 min
Response: 220420
Conc: 8.66 ng/ml

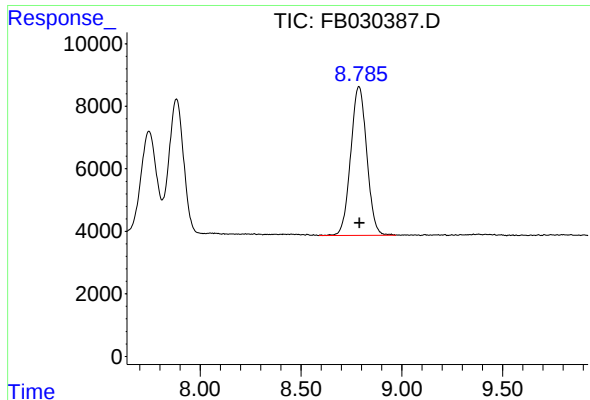

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: -0.005 min
Response: 263443
Conc: 19.05 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1004W1

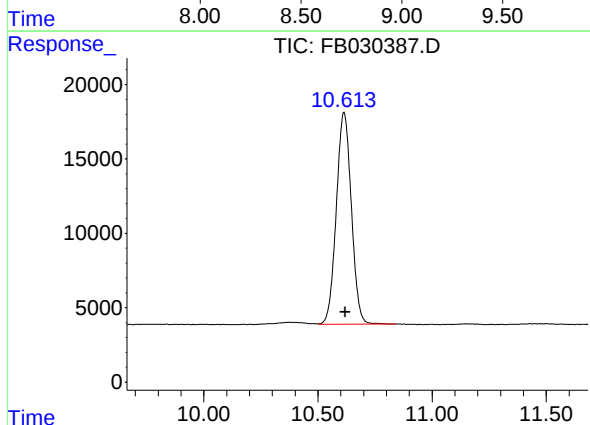


#6 Toluene

R.T.: 10.614 min
Delta R.T.: -0.005 min
Response: 652424
Conc: 26.32 ng/ml

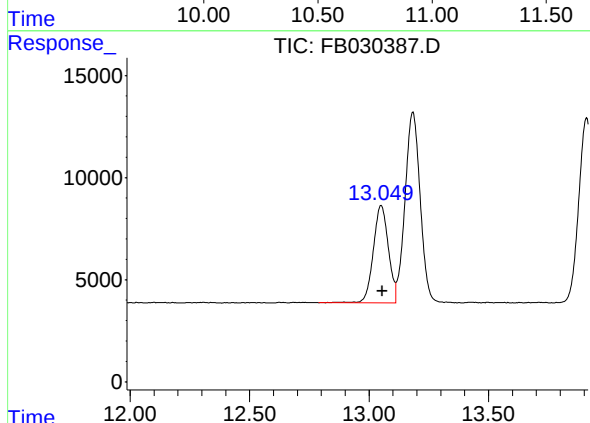


#7 Ethylbenzene

R.T.: 13.051 min
Delta R.T.: -0.005 min
Response: 208695
Conc: 8.97 ng/ml

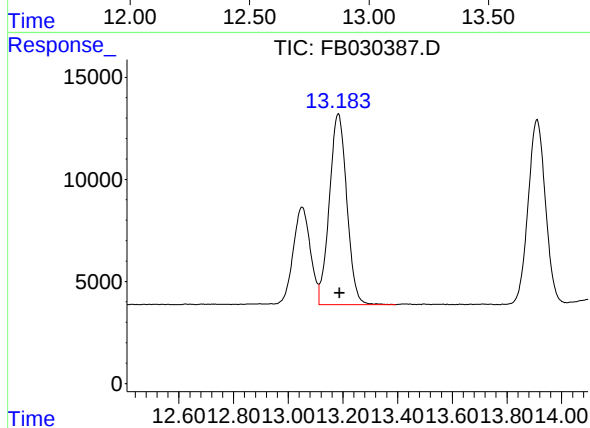

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: -0.005 min
Response: 414042
Conc: 18.05 ng/ml

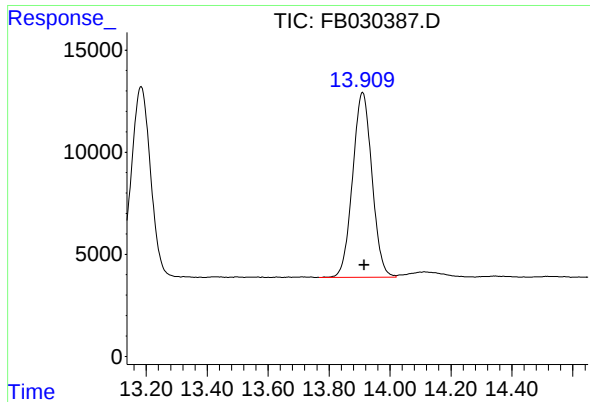

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: -0.005 min
Response: 399918
Conc: 18.01 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1004W1

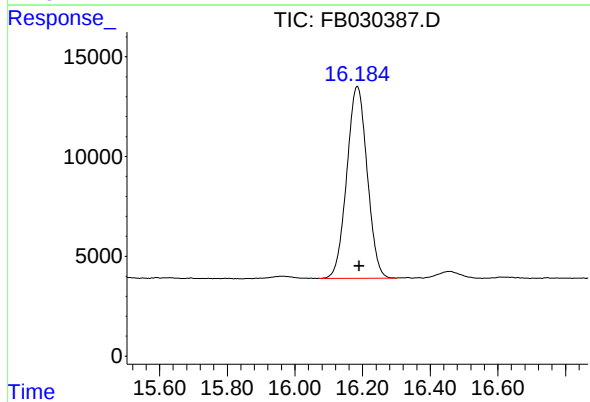

#10 1,2,4-Trimethylbenzene

R.T.: 16.185 min
Delta R.T.: -0.006 min
Response: 402265
Conc: 18.36 ng/ml