

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100424\
 Data File : FB030972.D
 Signal(s) : FID2B.CH
 Acq On : 4 Oct 2024 14:08
 Operator : YP/AJ
 Sample : BSF1004S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 05 04:15:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
 Quant Title :
 QLast Update : Fri Oct 04 11:53:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	667747	22.275 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.730	1164172	32.262 ng/ml
2) t 2,2,4-Trimethylpentane	7.432	1492629	31.323 ng/ml
3) t n-Heptane	7.757	487905	10.817 ng/ml
4) t Benzene	7.899	569764	10.366 ng/ml
6) t Toluene	10.626	1676639	31.038 ng/ml
7) t Ethylbenzene	13.062	492834	10.397 ng/ml
8) t m-Xylene	13.196	1079664	20.696 ng/ml
9) t O-Xylene	13.924	1004235	20.644 ng/ml
10) t 1,2,4-Trimethylbenzene	16.200	683705	20.865 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100424\
Data File : FB030972.D
Signal(s) : FID2B.CH
Acq On : 4 Oct 2024 14:08
Operator : YP/AJ
Sample : BSF1004S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 05 04:15:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

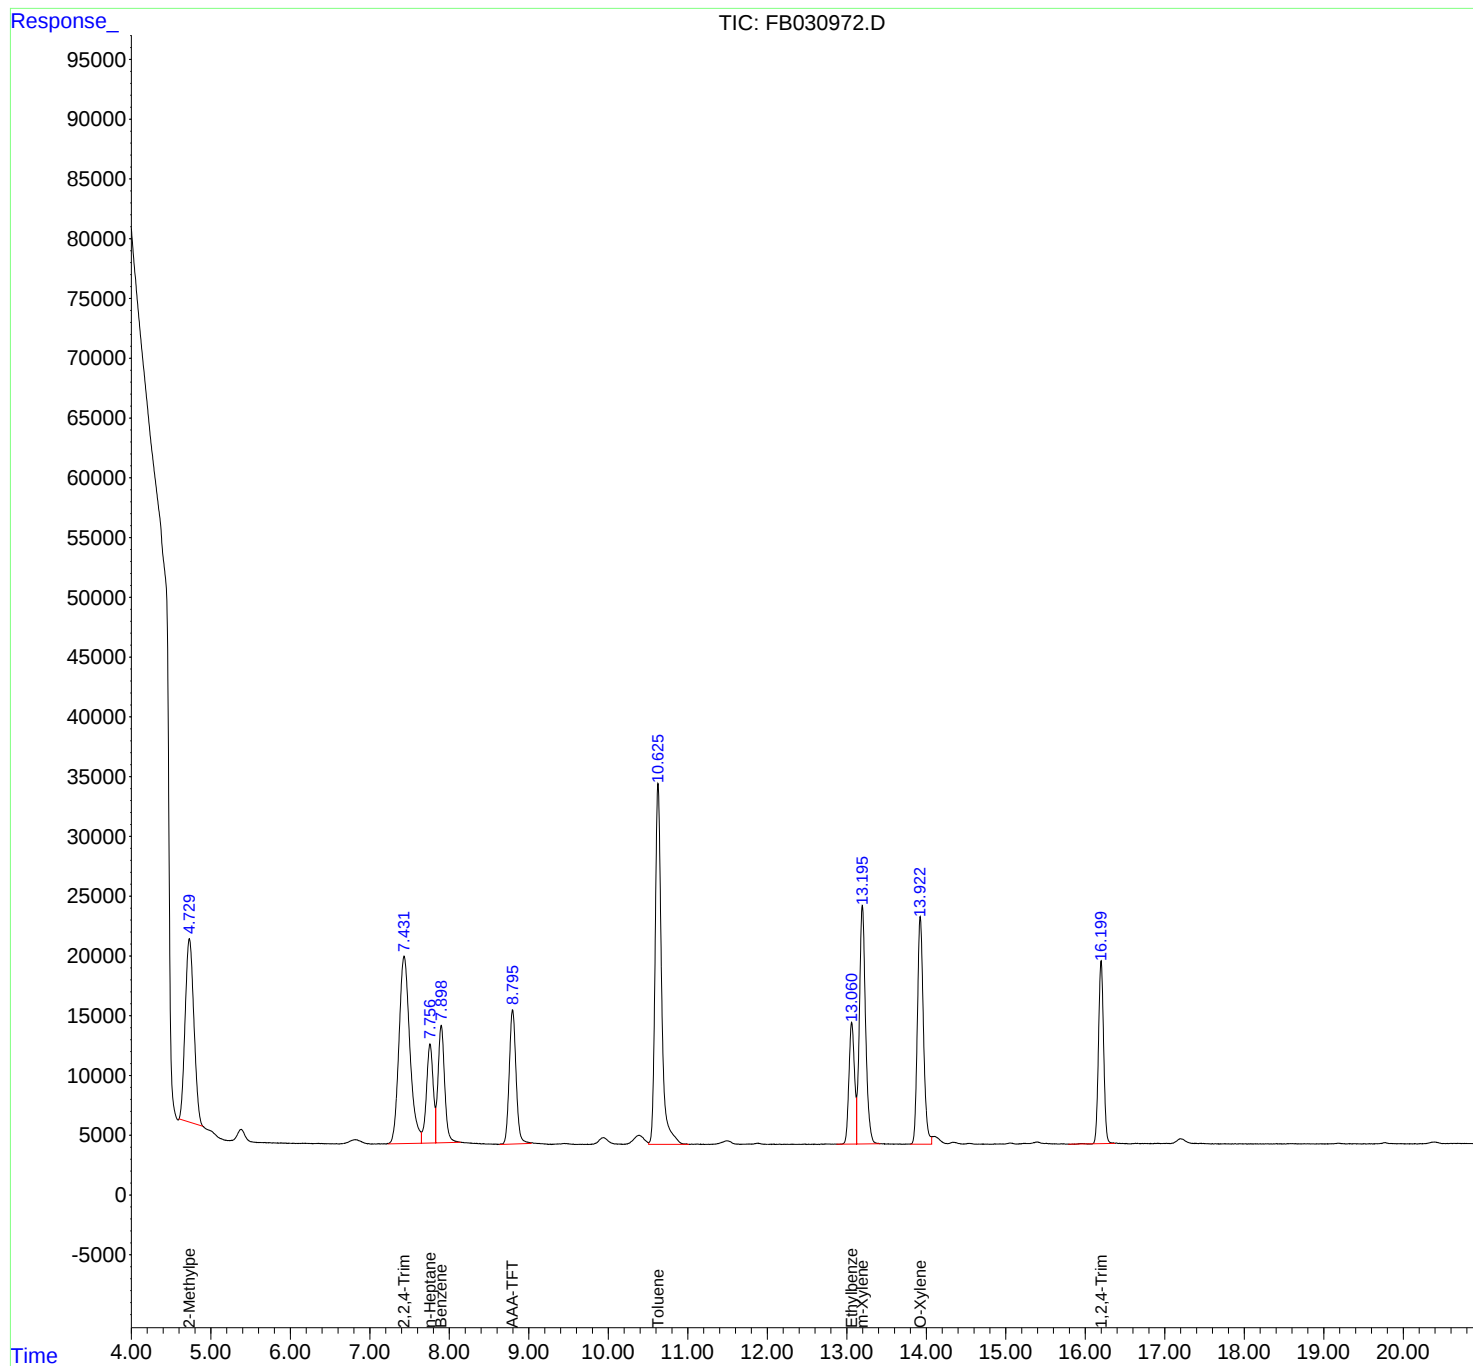


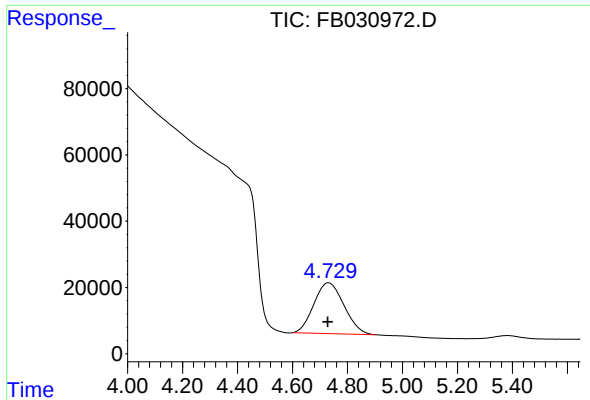

#1 2-Methylpentane


R.T.: 4.730 min
Delta R.T.: 0.002 min
Response: 1164172
Conc: 32.26 ng/ml

Instrument :
FID_B
ClientSampleId :

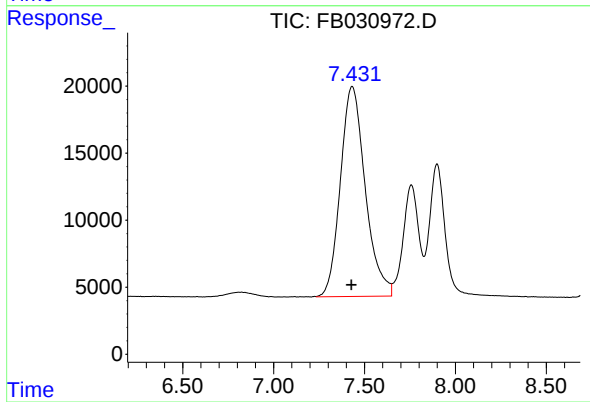


#2 2,2,4-Trimethylpentane

R.T.: 7.432 min
Delta R.T.: 0.005 min
Response: 1492629
Conc: 31.32 ng/ml

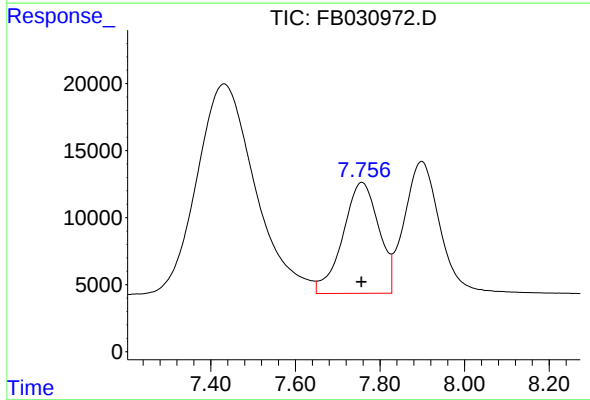


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 487905
Conc: 10.82 ng/ml

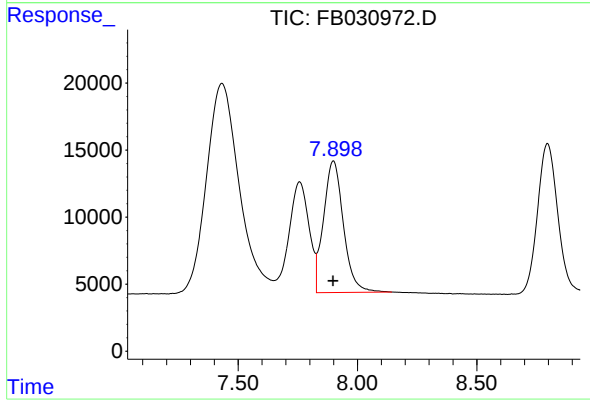

#4 Benzene


R.T.: 7.899 min
Delta R.T.: 0.002 min
Response: 569764
Conc: 10.37 ng/ml

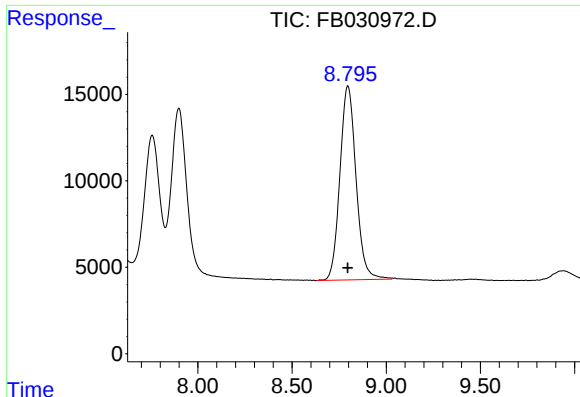

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.001 min
Response: 667747
Conc: 22.27 ng/ml

Instrument :
FID_B
ClientSampleId :

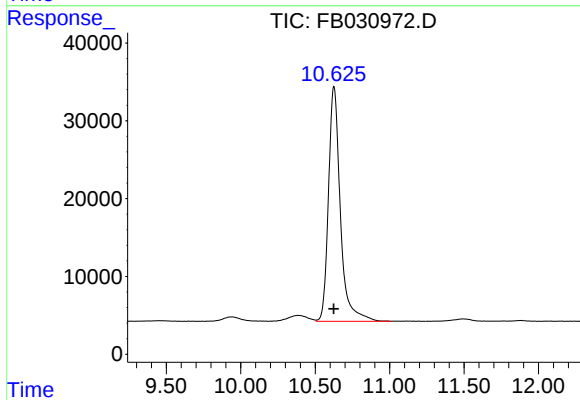


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.001 min
Response: 1676639
Conc: 31.04 ng/ml

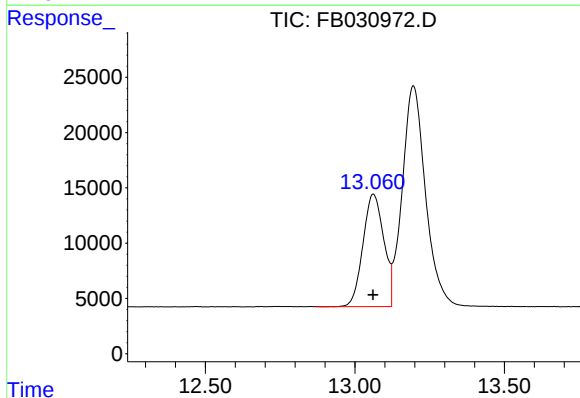


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: 0.001 min
Response: 492834
Conc: 10.40 ng/ml

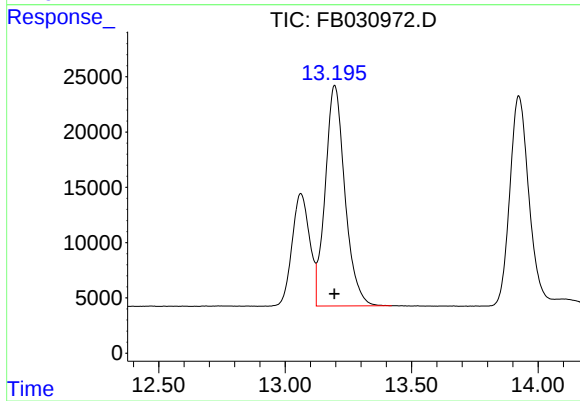

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: 0.001 min
Response: 1079664
Conc: 20.70 ng/ml

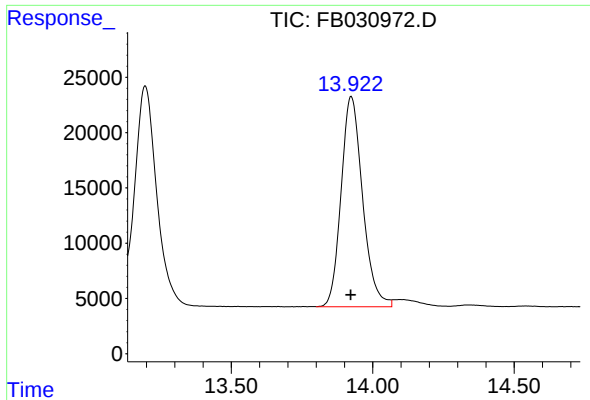

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.000 min
Response: 1004235
Conc: 20.64 ng/ml

Instrument :
FID_B
ClientSampleId :

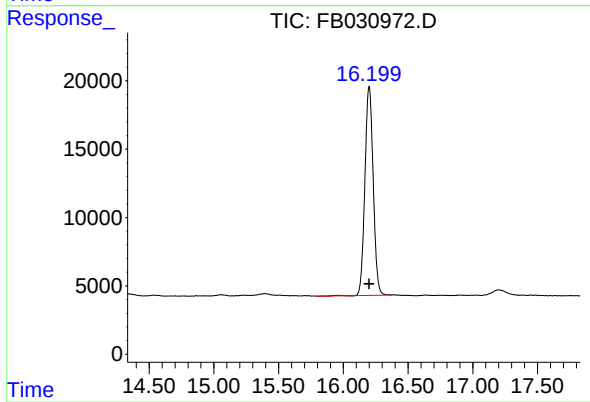

#10 1,2,4-Trimethylbenzene

R.T.: 16.200 min
Delta R.T.: 0.001 min
Response: 683705
Conc: 20.86 ng/ml