

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100424\
Data File : FB030973.D
Signal(s) : FID2B.CH
Acq On : 4 Oct 2024 14:35
Operator : YP/AJ
Sample : P4273-01
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 05 04:15:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	249040	8.308 ng/ml
Target Compounds			
8) t m-Xylene	13.199	7377	0.141 ng/ml
9) t O-Xylene	13.924	8803	0.181 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	15257	0.466 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100424\
Data File : FB030973.D
Signal(s) : FID2B.CH
Acq On : 4 Oct 2024 14:35
Operator : YP/AJ
Sample : P4273-01
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 05 04:15:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

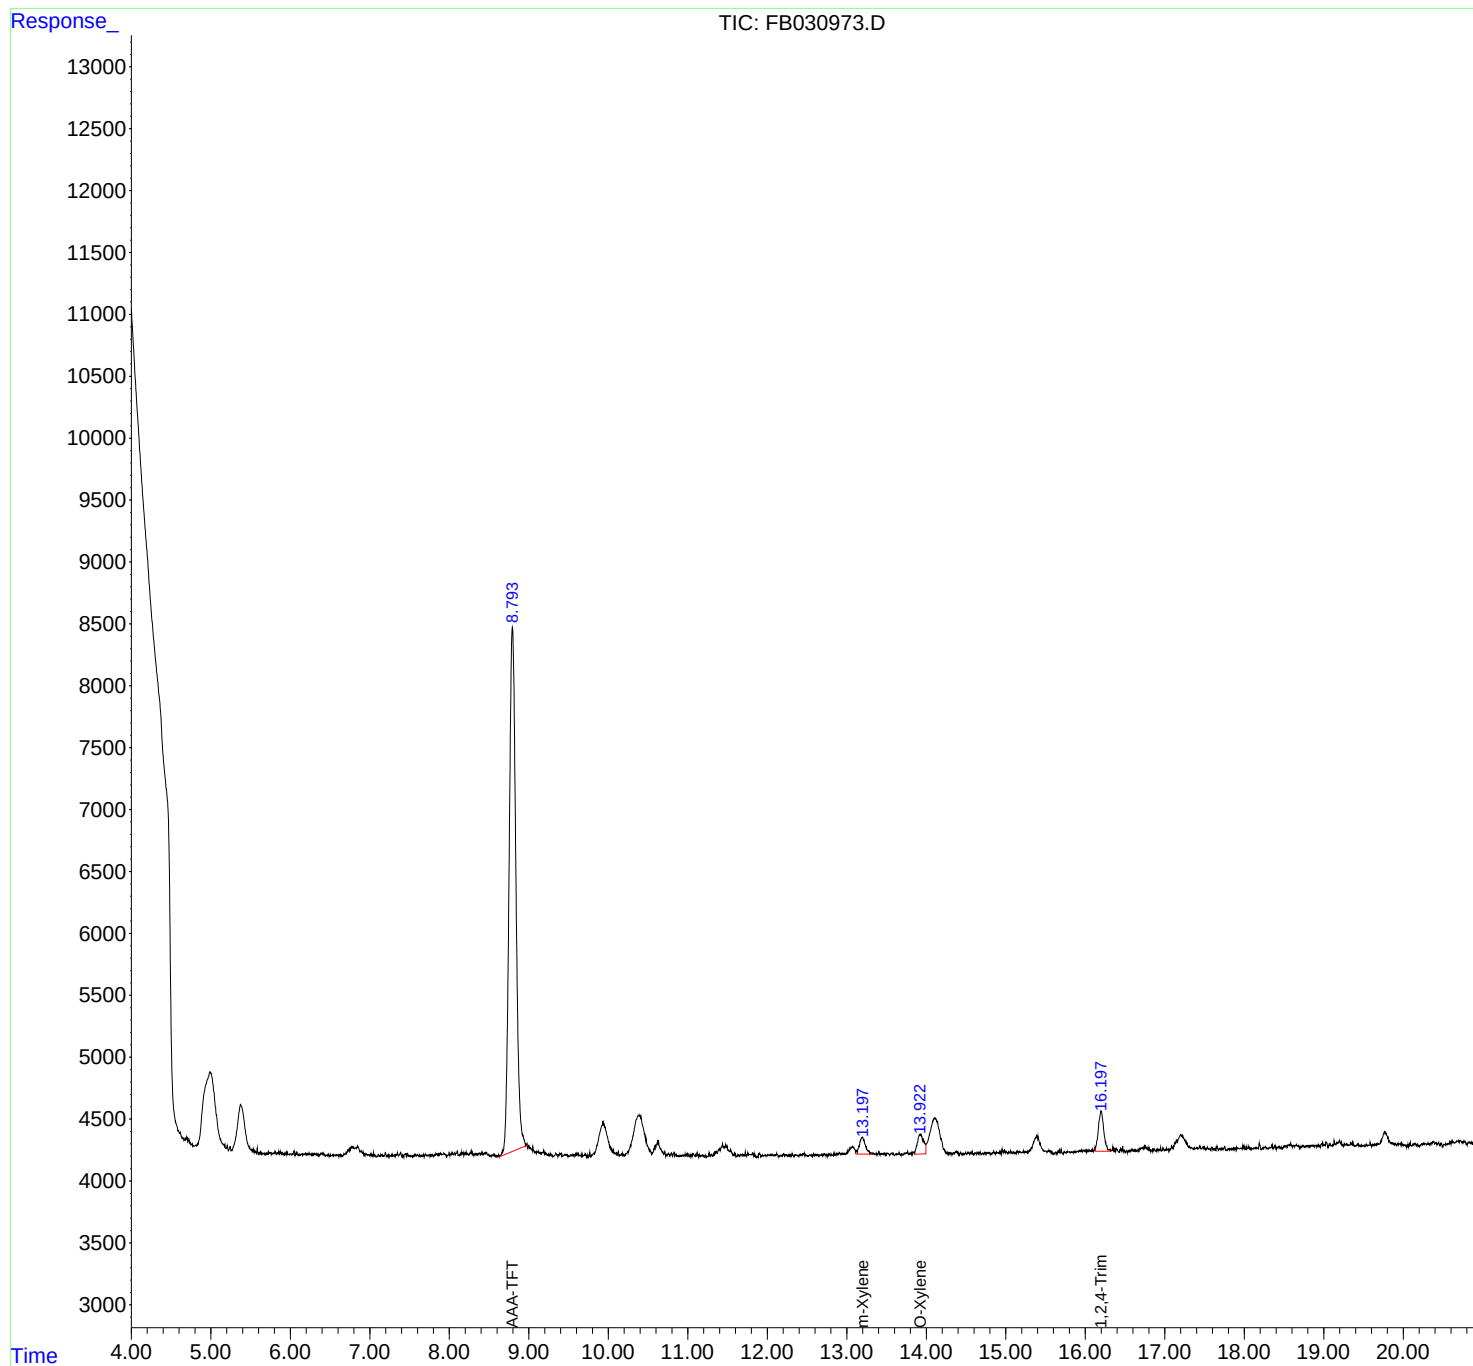


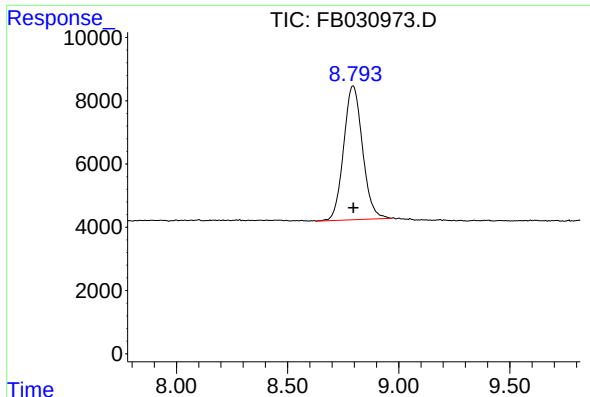

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 249040
Conc: 8.31 ng/ml

Instrument :
FID_B
ClientSampleId :

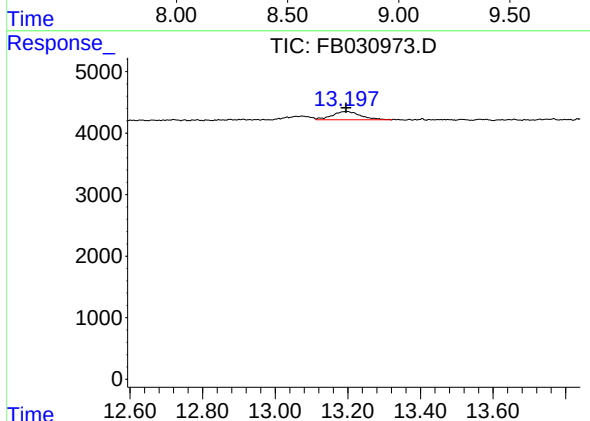


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: 0.004 min
Response: 7377
Conc: 0.14 ng/ml

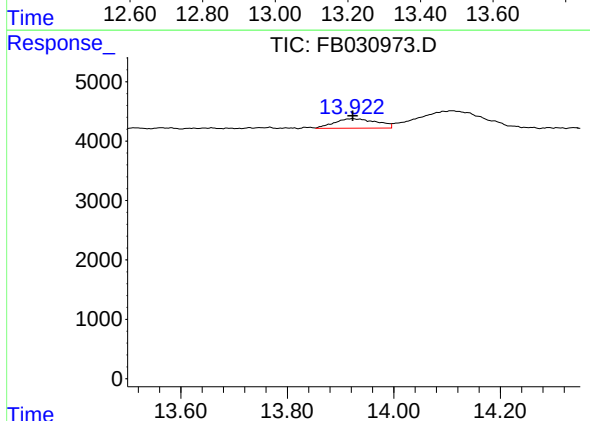

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.000 min
Response: 8803
Conc: 0.18 ng/ml

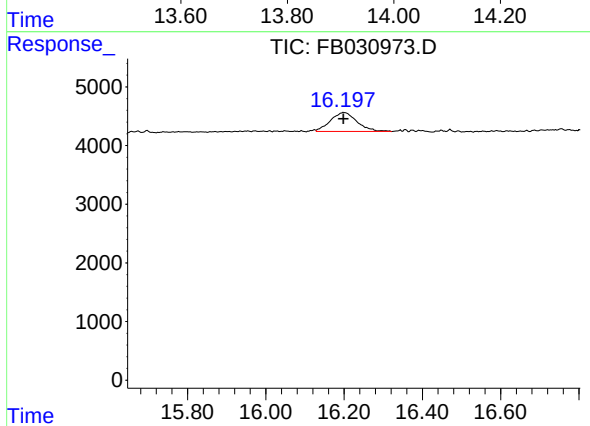

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.000 min
Response: 15257
Conc: 0.47 ng/ml