

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100424\
 Data File : FB030979.D
 Signal(s) : FID2B.CH
 Acq On : 4 Oct 2024 17:16
 Operator : YP/AJ
 Sample : P4277-01 50X
 Misc : 4.99G/5.00 ML MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 05 04:16:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
 Quant Title :
 QLast Update : Fri Oct 04 11:53:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	577103	19.251 ng/ml
Target Compounds			
6) t Toluene	10.628	4825	0.089 ng/ml
7) t Ethylbenzene	13.054	5845	0.123 ng/ml
8) t m-Xylene	13.192	10533	0.202 ng/ml
9) t O-Xylene	13.929	10360	0.213 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	19850	0.606 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100424\
Data File : FB030979.D
Signal(s) : FID2B.CH
Acq On : 4 Oct 2024 17:16
Operator : YP/AJ
Sample : P4277-01 50X
Misc : 4.99G/5.00 ML MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 05 04:16:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

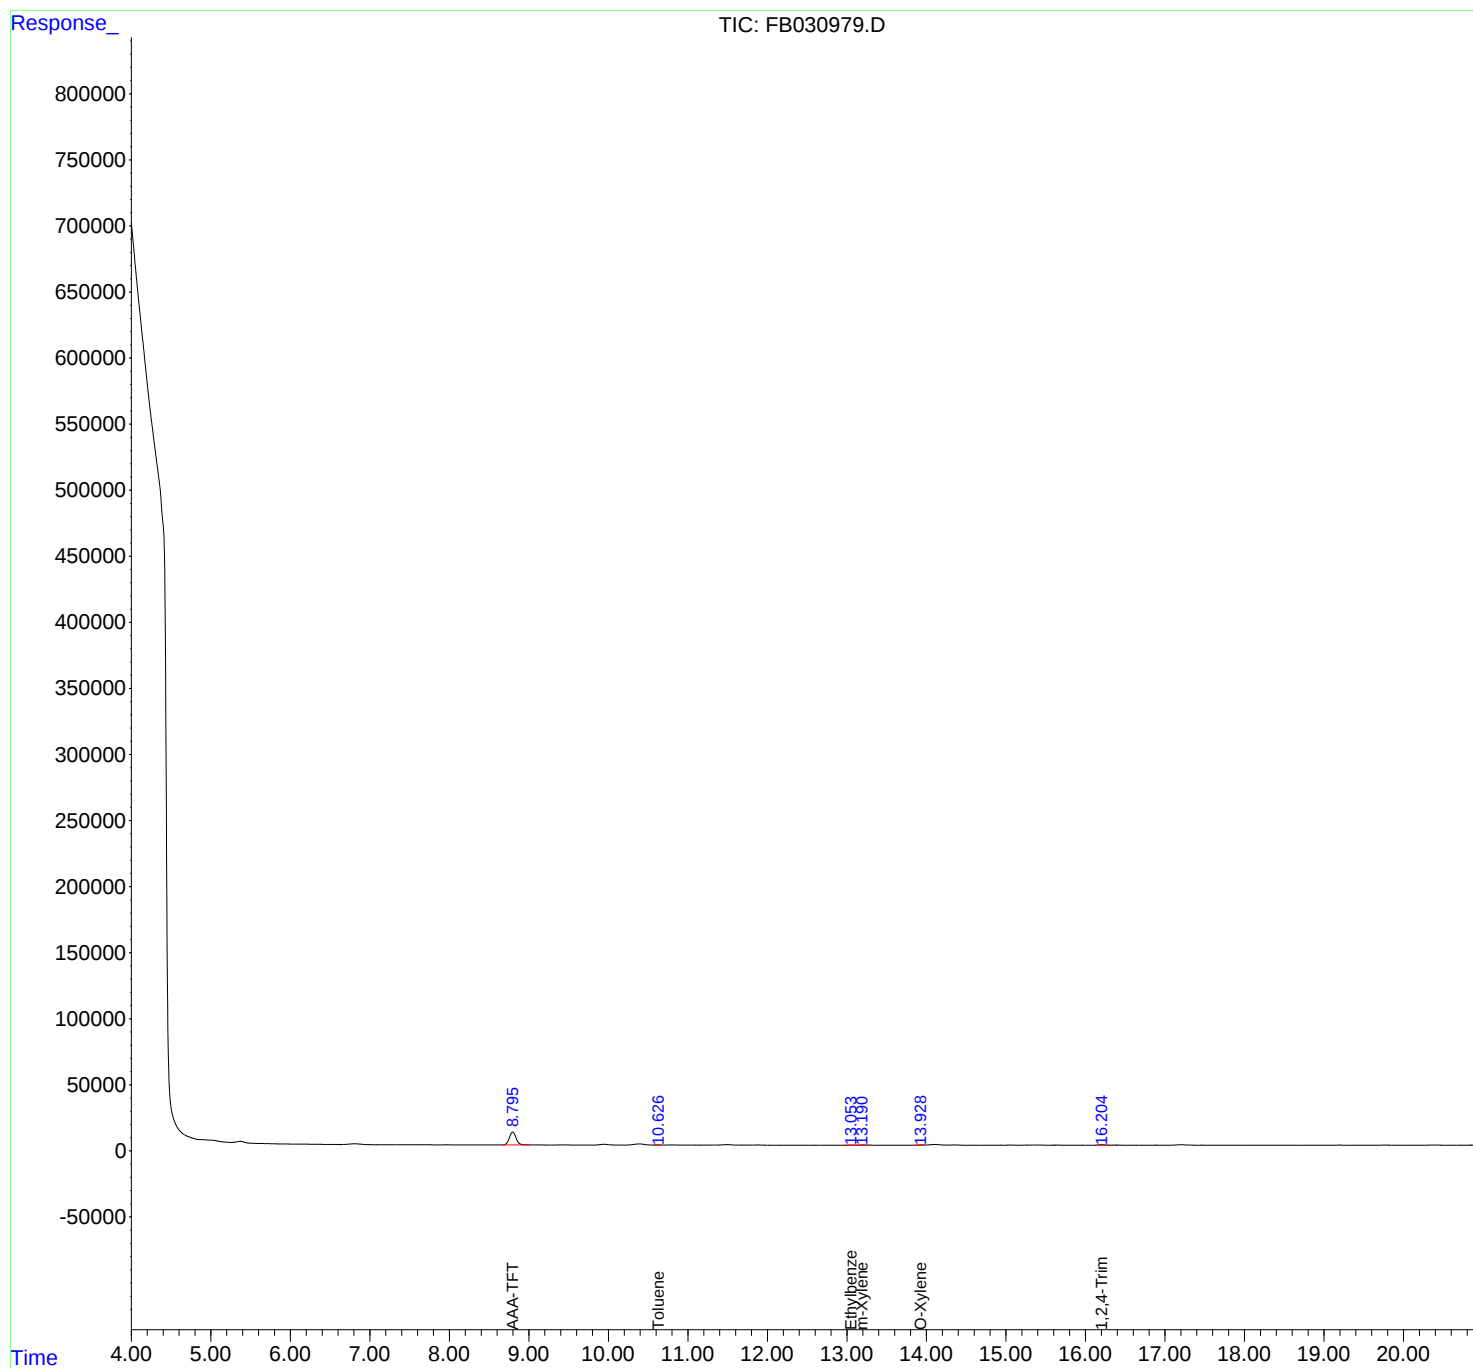


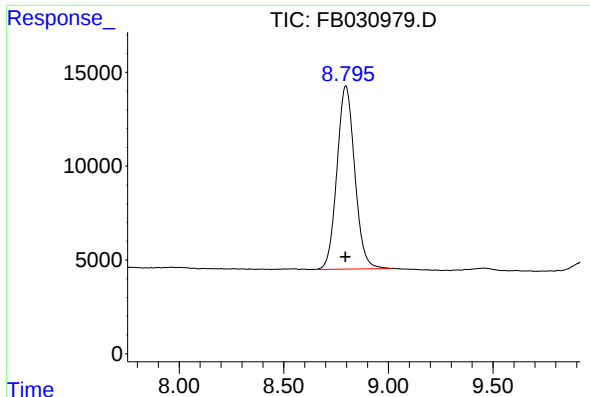

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.001 min
Response: 577103
Conc: 19.25 ng/ml

Instrument :
FID_B
ClientSampleId :

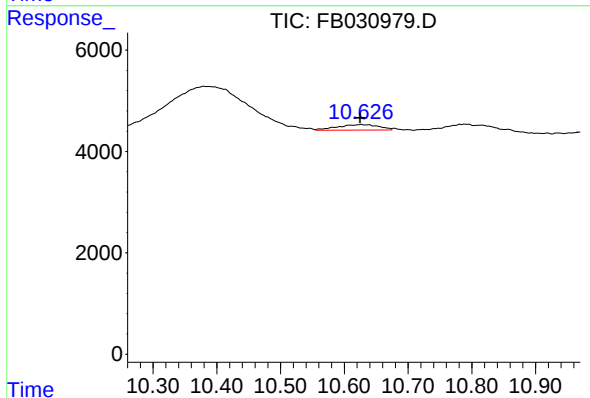


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.003 min
Response: 4825
Conc: 0.09 ng/ml

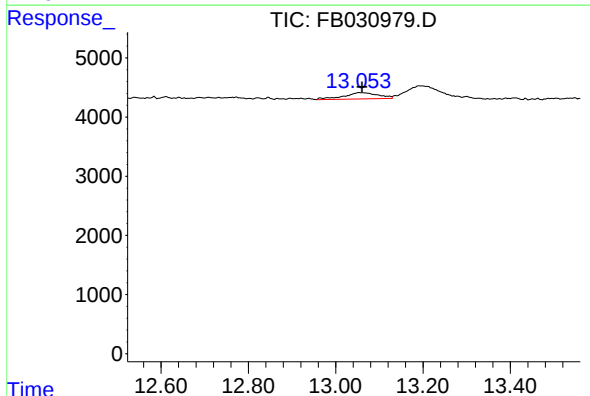


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.006 min
Response: 5845
Conc: 0.12 ng/ml

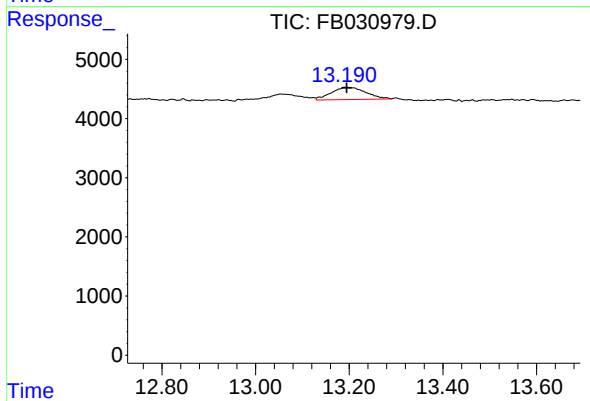

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: -0.003 min
Response: 10533
Conc: 0.20 ng/ml

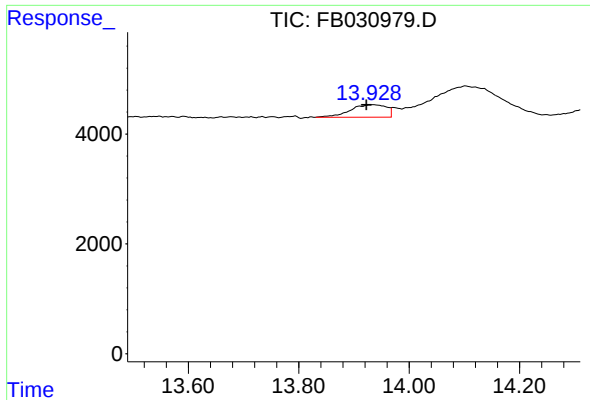

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.007 min
Response: 10360
Conc: 0.21 ng/ml

Instrument :
FID_B
ClientSampleId :

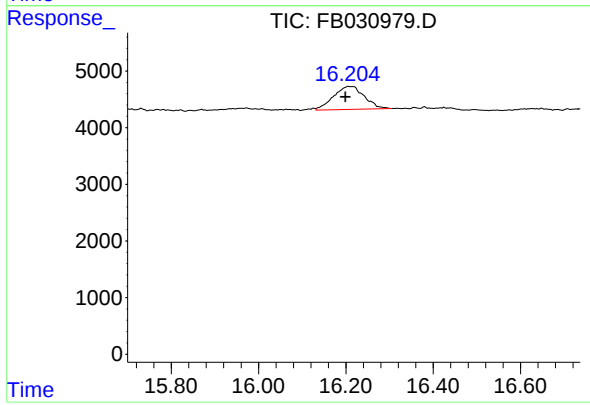

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.008 min
Response: 19850
Conc: 0.61 ng/ml