

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100424\
 Data File : FB030980.D
 Signal(s) : FID2B.CH
 Acq On : 4 Oct 2024 17:42
 Operator : YP/AJ
 Sample : BSF1004S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1004S2

Integration File: Calibration.e
 Quant Time: Oct 05 04:16:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
 Quant Title :
 QLast Update : Fri Oct 04 11:53:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	585521	19.532 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.731	1018334	28.221 ng/ml
2) t 2,2,4-Trimethylpentane	7.433	1357229	28.481 ng/ml
3) t n-Heptane	7.758	435914	9.664 ng/ml
4) t Benzene	7.900	532936	9.696 ng/ml
6) t Toluene	10.627	1531029	28.342 ng/ml
7) t Ethylbenzene	13.063	449115	9.475 ng/ml
8) t m-Xylene	13.197	986557	18.911 ng/ml
9) t O-Xylene	13.925	920464	18.922 ng/ml
10) t 1,2,4-Trimethylbenzene	16.200	639728	19.523 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100424\
Data File : FB030980.D
Signal(s) : FID2B.CH
Acq On : 4 Oct 2024 17:42
Operator : YP/AJ
Sample : BSF1004S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1004S2

Integration File: Calibration.e
Quant Time: Oct 05 04:16:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

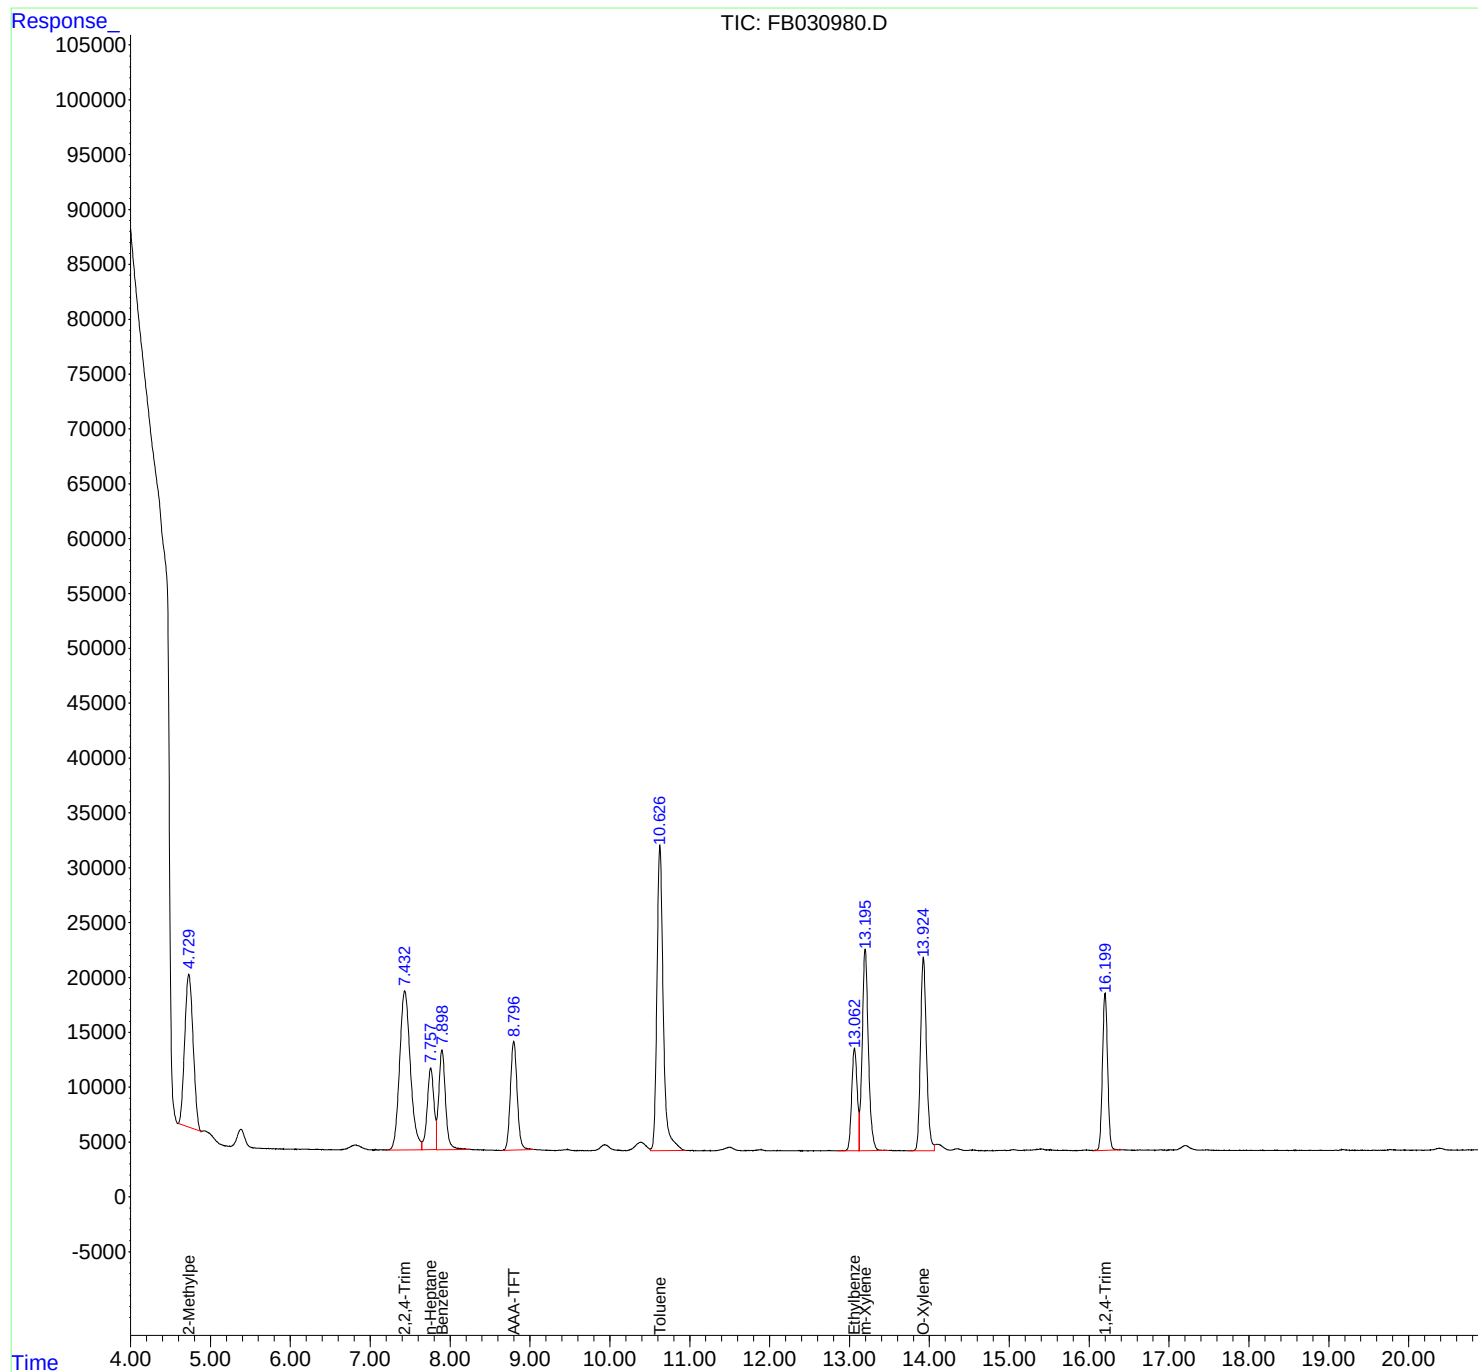


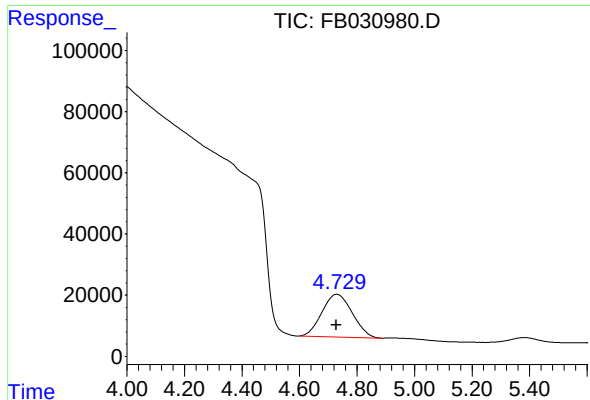

#1 2-Methylpentane


R.T.: 4.731 min
Delta R.T.: 0.003 min
Response: 1018334
Conc: 28.22 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1004S2

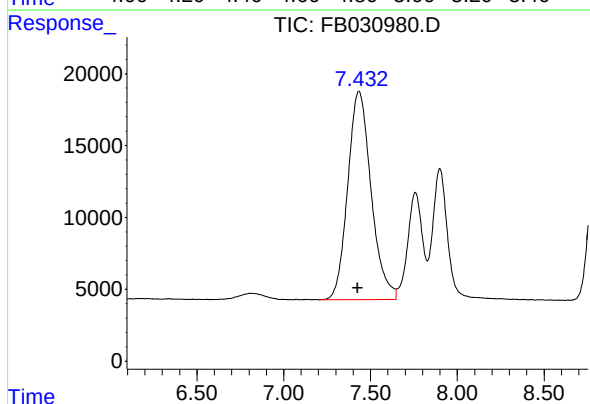


#2 2,2,4-Trimethylpentane

R.T.: 7.433 min
Delta R.T.: 0.005 min
Response: 1357229
Conc: 28.48 ng/ml

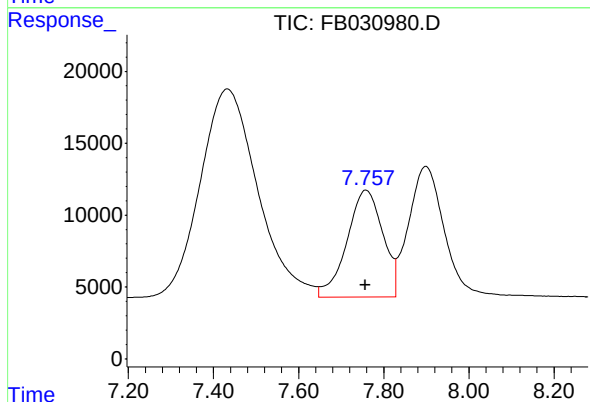


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.002 min
Response: 435914
Conc: 9.66 ng/ml

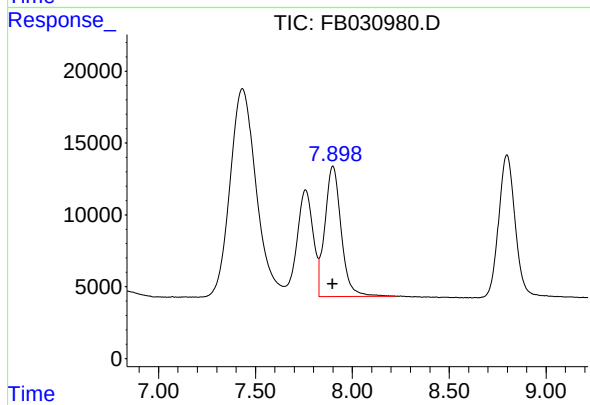

#4 Benzene


R.T.: 7.900 min
Delta R.T.: 0.002 min
Response: 532936
Conc: 9.70 ng/ml

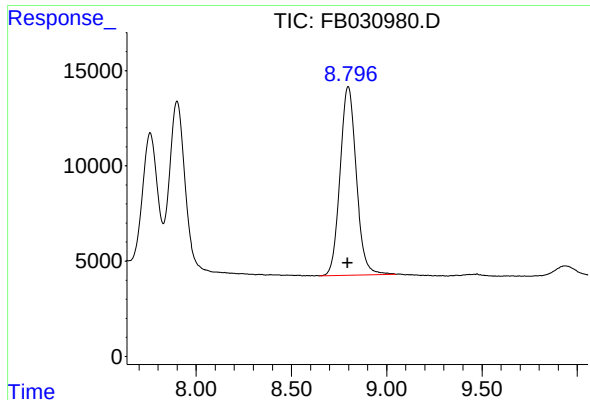

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.002 min
Response: 585521
Conc: 19.53 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1004S2

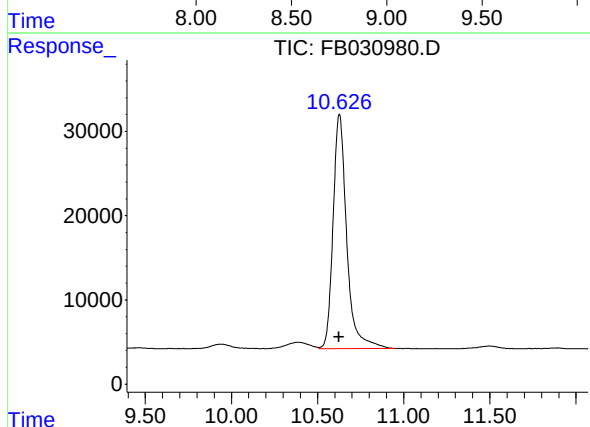


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.002 min
Response: 1531029
Conc: 28.34 ng/ml

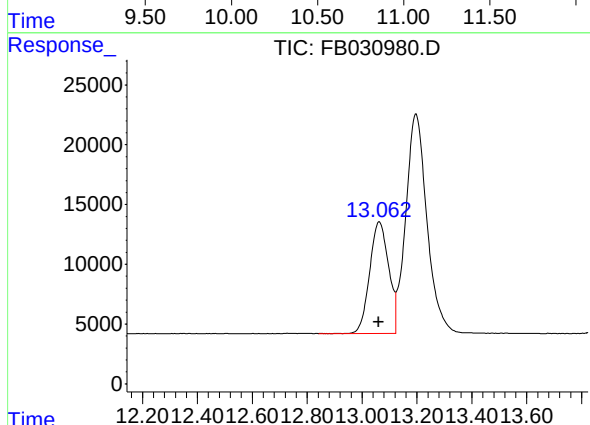


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.002 min
Response: 449115
Conc: 9.47 ng/ml

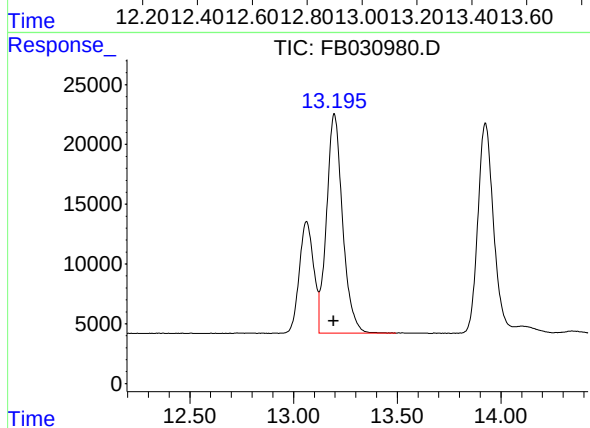

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.002 min
Response: 986557
Conc: 18.91 ng/ml

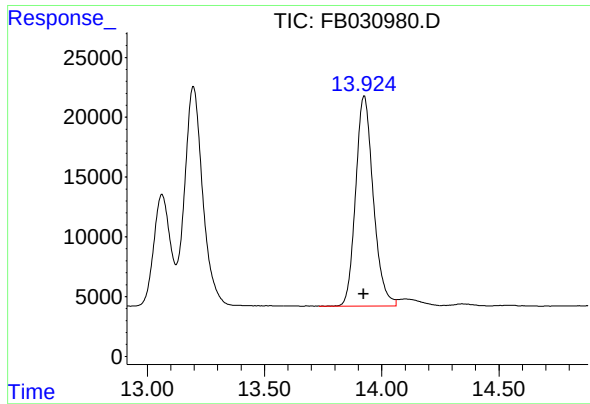

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: 0.002 min
Response: 920464
Conc: 18.92 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1004S2

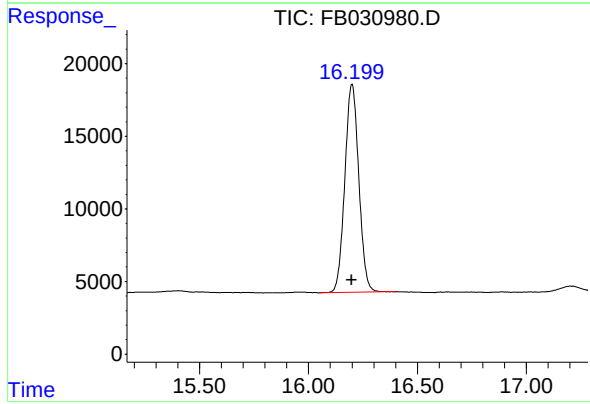

#10 1,2,4-Trimethylbenzene

R.T.: 16.200 min
Delta R.T.: 0.002 min
Response: 639728
Conc: 19.52 ng/ml