

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100518\
 Data File : FB018117.D
 Signal(s) : FID2B.CH
 Acq On : 5 Oct 2018 8:57
 Operator : MJ/SJ
 Sample : BSF1005S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 05 10:19:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
 Quant Title :
 QLast Update : Fri Sep 14 13:09:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.111	179748	21.250 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.963	425167	26.698 ng/ml
2) t 2,2,4-Trimethylpentane	7.726	438339	27.545 ng/ml
3) t n-Heptane	8.066	141386	9.175 ng/ml
4) t Benzene	8.206	188189	9.886 ng/ml
6) t Toluene	10.960	461763	29.177 ng/ml
7) t Ethylbenzene	13.409	159923	9.787 ng/ml
8) t m-Xylene	13.541	336153	19.431 ng/ml
9) t O-Xylene	14.273	353101	19.431 ng/ml
10) t 1,2,4-Trimethylbenzene	16.556	401666	18.883 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100518\
Data File : FB018117.D
Signal(s) : FID2B.CH
Acq On : 5 Oct 2018 8:57
Operator : MJ/SJ
Sample : BSF1005S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 05 10:19:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

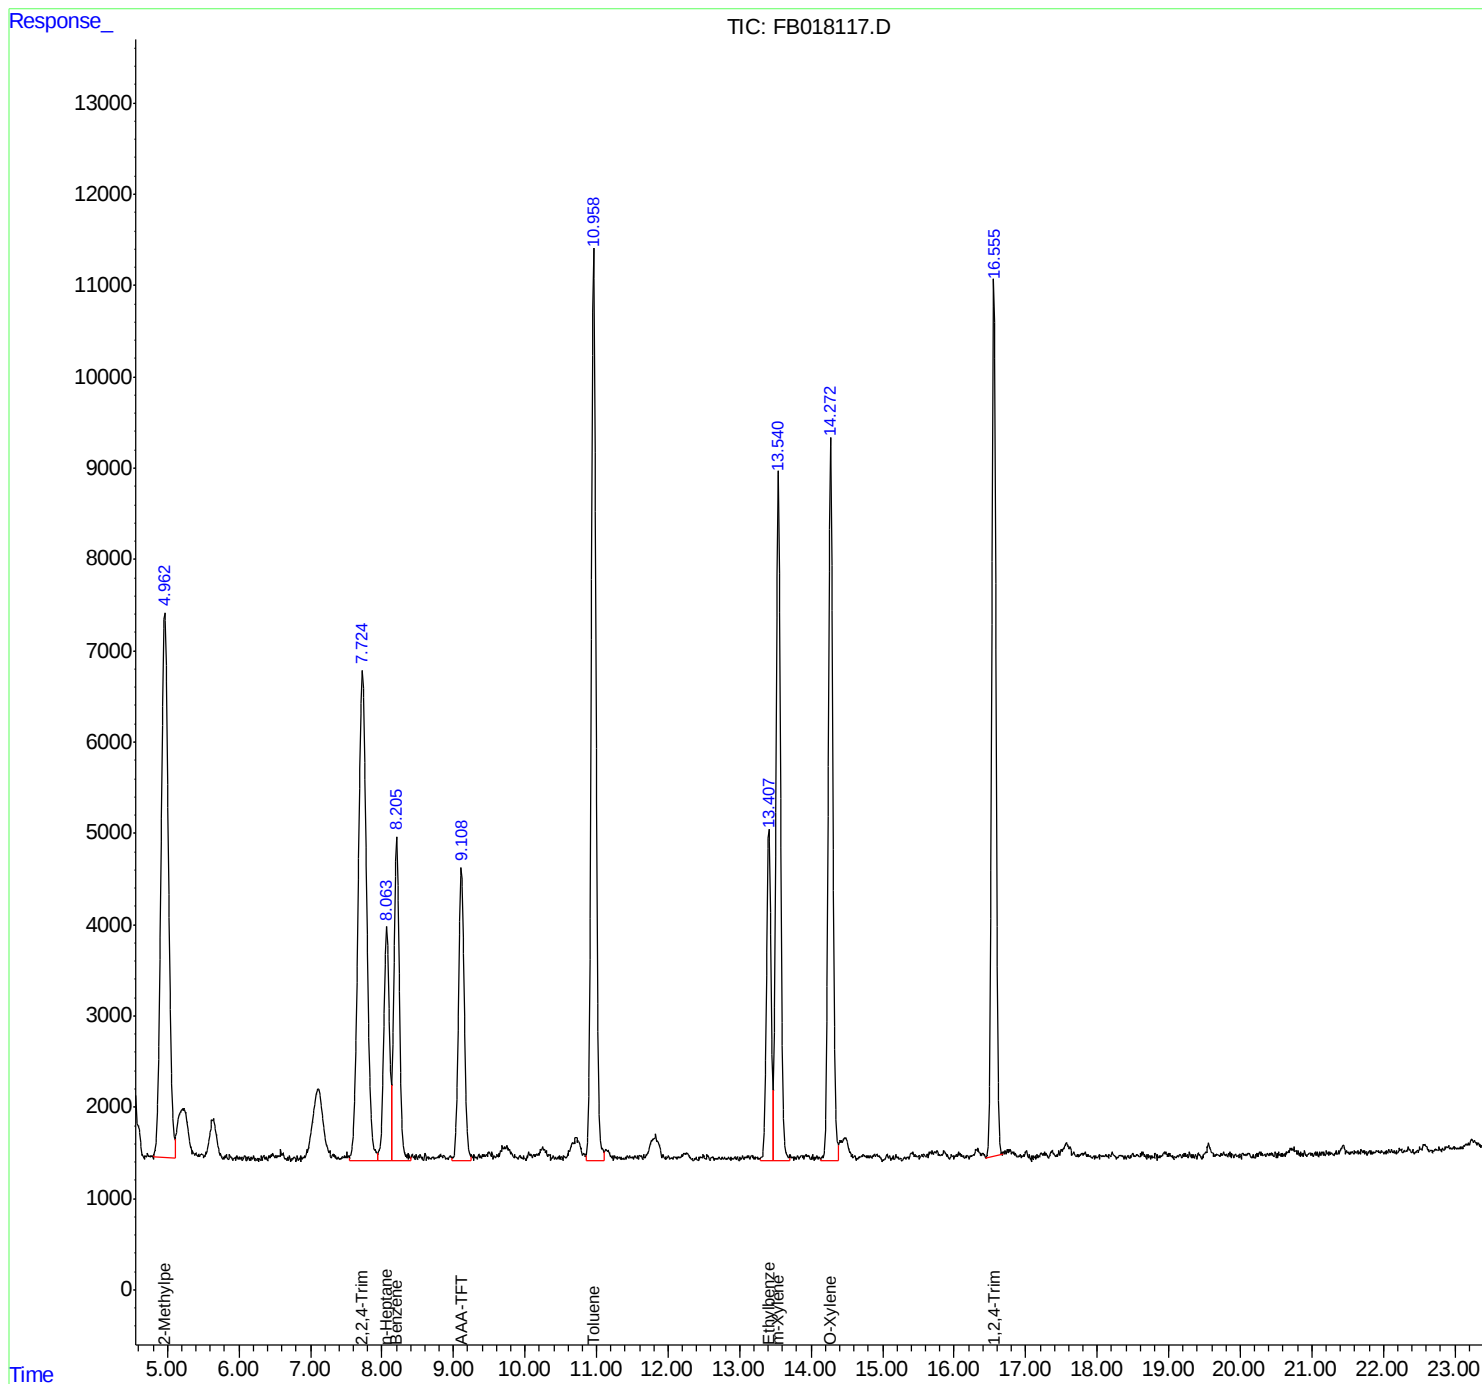

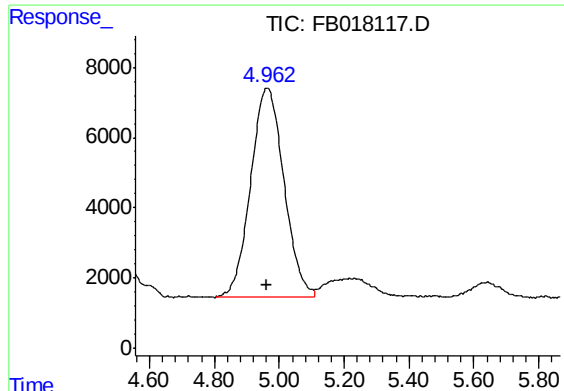


#1 2-Methylpentane

R.T.: 4.963 min
Delta R.T.: 0.003 min
Response: 425167
Conc: 26.70 ng/ml

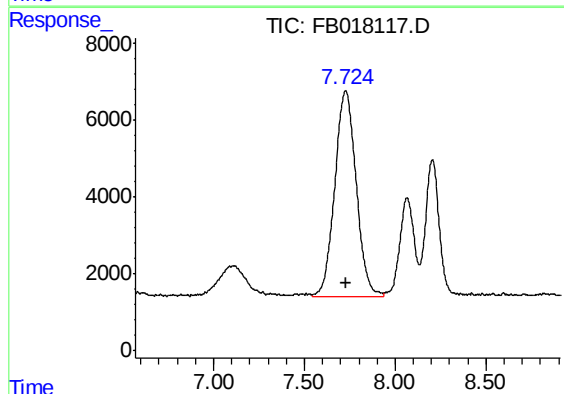


#2 2,2,4-Trimethylpentane

R.T.: 7.726 min
Delta R.T.: -0.001 min
Response: 438339
Conc: 27.54 ng/ml

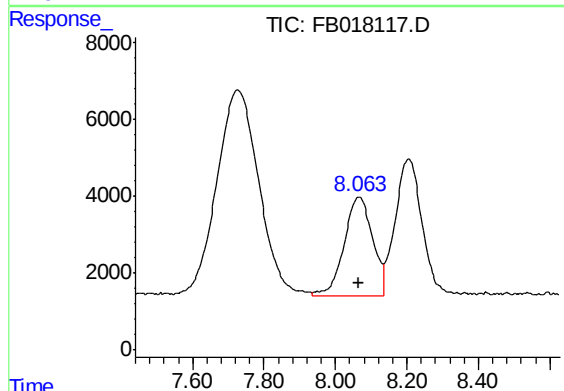


#3 n-Heptane

R.T.: 8.066 min
Delta R.T.: 0.000 min
Response: 141386
Conc: 9.17 ng/ml

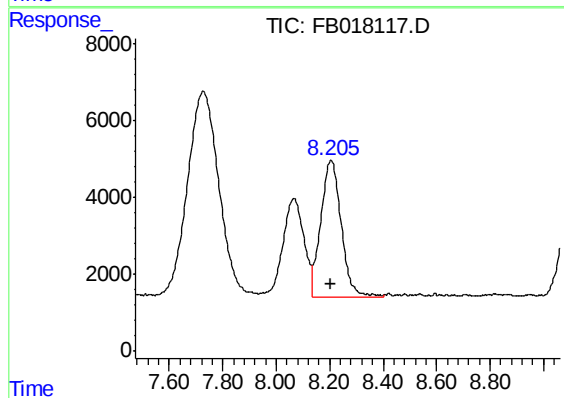


#4 Benzene

R.T.: 8.206 min
Delta R.T.: 0.001 min
Response: 188189
Conc: 9.89 ng/ml

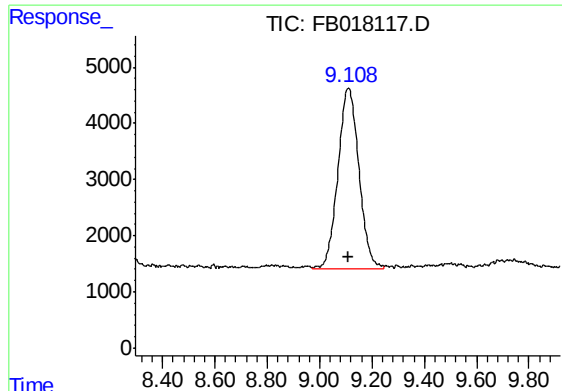


#5 AAA-TFT

R.T.: 9.111 min
Delta R.T.: 0.000 min
Response: 179748
Conc: 21.25 ng/ml

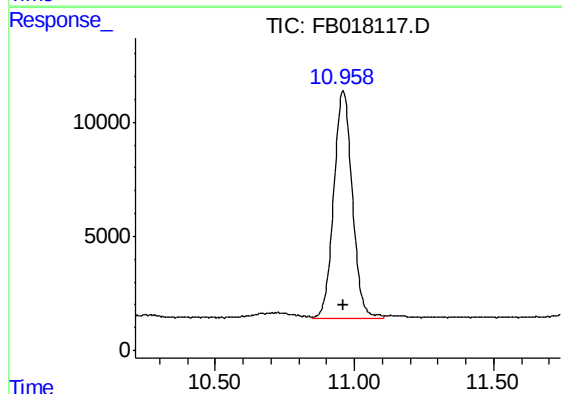


#6 Toluene

R.T.: 10.960 min
Delta R.T.: 0.000 min
Response: 461763
Conc: 29.18 ng/ml

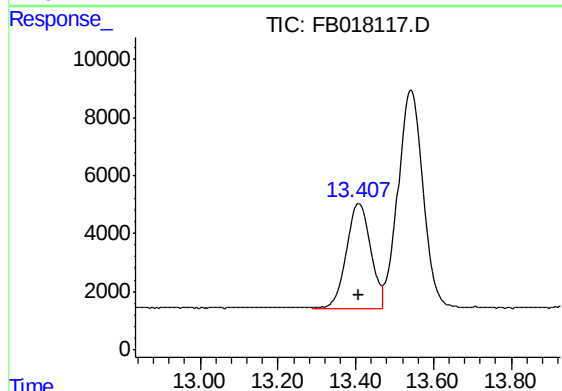


#7 Ethylbenzene

R.T.: 13.409 min
Delta R.T.: 0.000 min
Response: 159923
Conc: 9.79 ng/ml

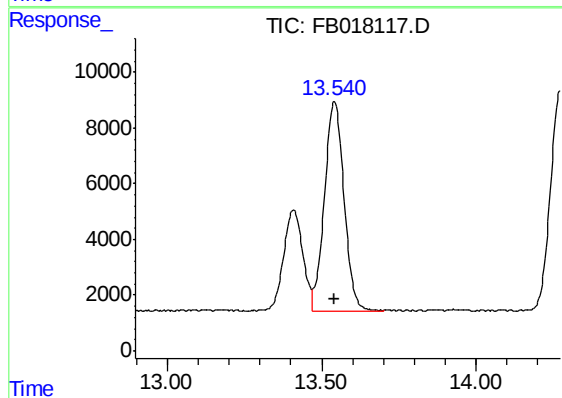


#8 m-Xylene

R.T.: 13.541 min
Delta R.T.: 0.000 min
Response: 336153
Conc: 19.43 ng/ml

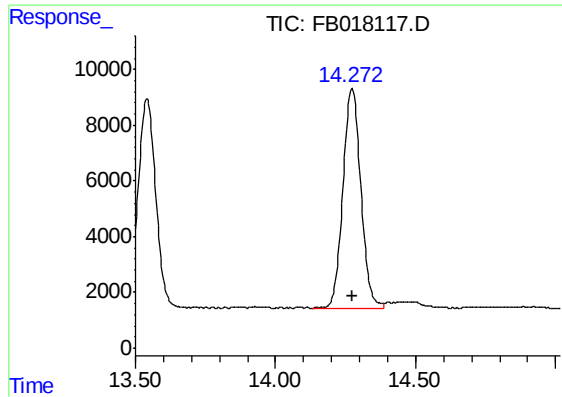

#9 O-Xylene

R.T.: 14.273 min
Delta R.T.: 0.000 min
Response: 353101
Conc: 19.43 ng/ml

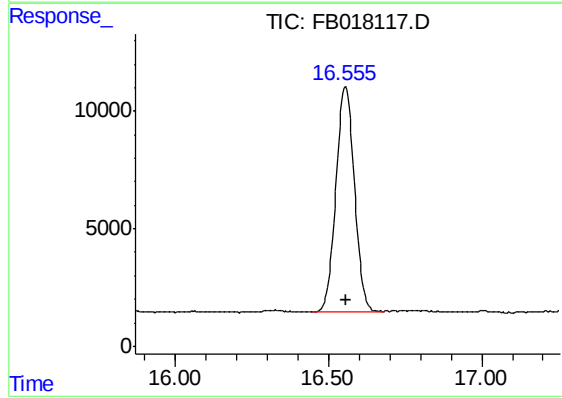

#10 1,2,4-Trimethylbenzene

R.T.: 16.556 min
Delta R.T.: 0.000 min
Response: 401666
Conc: 18.88 ng/ml